

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043532.D
 Acq On : 25 Oct 2024 18:43
 Operator : JC/MD
 Sample : VIBLK670
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK670

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

Signal : TIC: VX043532.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	33	rBV	49751	66344	7.54%	1.036%
2	1.368	43	46	57	rVB	81355	112637	12.80%	1.758%
3	1.642	89	91	100	rBV	35498	55070	6.26%	0.860%
4	2.294	191	198	210	rVB	175139	274898	31.24%	4.291%
5	2.575	242	244	245	rBV	589	479	0.05%	0.007%
6	2.709	262	266	267	rBV3	578	568	0.06%	0.009%
7	2.776	275	277	279	rBV3	809	911	0.10%	0.014%
8	2.940	299	304	307	rBV4	1115	2619	0.30%	0.041%
9	3.014	314	316	318	rVB	455	327	0.04%	0.005%
10	3.038	318	320	322	rVB2	404	311	0.04%	0.005%
11	3.099	328	330	333	rVB2	483	416	0.05%	0.006%
12	3.142	333	337	338	rBV	427	427	0.05%	0.007%
13	3.184	341	344	346	rBV3	475	556	0.06%	0.009%
14	3.294	359	362	365	rVB3	405	490	0.06%	0.008%
15	3.428	376	384	395	rVB3	8359	19920	2.26%	0.311%
16	3.666	421	423	425	rBV	563	352	0.04%	0.005%
17	3.721	429	432	433	rBV	328	329	0.04%	0.005%
18	3.843	450	452	454	rBV2	378	345	0.04%	0.005%
19	3.989	475	476	477	rBV	606	299	0.03%	0.005%
20	4.032	482	483	485	rBV	331	308	0.04%	0.005%
21	4.148	501	502	506	rVB2	486	531	0.06%	0.008%
22	4.361	534	537	539	rBV3	340	367	0.04%	0.006%
23	4.471	546	555	579	rBV2	55475	204523	23.25%	3.193%
24	4.873	619	621	624	rBV2	302	450	0.05%	0.007%
25	5.056	638	651	663	rBV	117223	352313	40.04%	5.500%
26	5.391	703	706	708	rBV2	646	575	0.07%	0.009%
27	5.464	715	718	720	rBV2	340	455	0.05%	0.007%
28	5.531	726	729	730	rBV2	476	428	0.05%	0.007%
29	5.958	789	799	814	rBV2	296268	879819	100.00%	13.734%
30	6.184	835	836	840	rVB2	379	395	0.04%	0.006%
31	6.367	860	866	867	rBV4	414	516	0.06%	0.008%
32	6.422	873	875	879	rVB2	570	555	0.06%	0.009%
33	6.464	879	882	883	rBV	478	496	0.06%	0.008%
34	6.507	887	889	891	rBV2	316	393	0.04%	0.006%
35	6.757	920	930	945	rBV	207641	510350	58.01%	7.967%
36	7.068	980	981	985	rBV3	448	465	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043532.D
 Acq On : 25 Oct 2024 18:43
 Operator : JC/MD
 Sample : VIBLK670
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK670

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

37	7.110	985	988	991	rBV4	847	1303	0.15%	0.020%
38	7.184	998	1000	1002	rBV3	378	331	0.04%	0.005%
39	7.306	1012	1020	1035	rBV	179754	397029	45.13%	6.198%
40	7.476	1047	1048	1049	rBV	554	352	0.04%	0.005%
41	7.610	1068	1070	1074	rVB3	349	355	0.04%	0.006%
42	7.745	1089	1092	1093	rVB2	424	420	0.05%	0.007%
43	7.757	1093	1094	1097	rBV	598	485	0.06%	0.008%
44	7.787	1097	1099	1100	rVV	344	329	0.04%	0.005%
45	7.927	1120	1122	1123	rBV2	343	341	0.04%	0.005%
46	8.153	1155	1159	1160	rBV2	399	560	0.06%	0.009%
47	8.244	1172	1174	1177	rVB	414	317	0.04%	0.005%
48	8.324	1181	1187	1198	rBV	102906	172121	19.56%	2.687%
49	8.482	1210	1213	1214	rBV2	408	415	0.05%	0.006%
50	8.543	1221	1223	1226	rVB2	633	540	0.06%	0.008%
51	8.647	1233	1240	1255	rBV	429744	688719	78.28%	10.751%
52	8.952	1284	1290	1301	rBV	71203	111043	12.62%	1.733%
53	9.080	1309	1311	1314	rBV2	490	548	0.06%	0.009%
54	9.275	1341	1343	1344	rVV2	567	329	0.04%	0.005%
55	9.354	1353	1356	1357	rBV2	593	737	0.08%	0.012%
56	9.391	1357	1362	1381	rVV	280303	460238	52.31%	7.184%
57	9.653	1403	1405	1407	rVB	559	345	0.04%	0.005%
58	9.781	1424	1426	1429	rBV2	476	604	0.07%	0.009%
59	10.055	1465	1471	1489	rVV	407857	586070	66.61%	9.149%
60	10.281	1506	1508	1510	rBV	302	326	0.04%	0.005%
61	10.366	1519	1522	1523	rBV2	502	548	0.06%	0.009%
62	10.384	1524	1525	1528	rVV2	605	532	0.06%	0.008%
63	10.421	1529	1531	1536	rVB3	420	645	0.07%	0.010%
64	10.671	1570	1572	1574	rBV2	340	377	0.04%	0.006%
65	10.762	1584	1587	1588	rBV2	273	323	0.04%	0.005%
66	10.811	1594	1595	1598	rBV2	377	415	0.05%	0.006%
67	10.878	1604	1606	1609	rBV2	395	458	0.05%	0.007%
68	10.933	1612	1615	1616	rVB2	446	345	0.04%	0.005%
69	10.970	1619	1621	1625	rVB3	522	626	0.07%	0.010%
70	11.006	1625	1627	1631	rVB	486	511	0.06%	0.008%
71	11.189	1652	1657	1669	rBV	327020	446066	50.70%	6.963%
72	11.323	1676	1679	1680	rVB3	731	643	0.07%	0.010%
73	11.439	1696	1698	1699	rBV	495	349	0.04%	0.005%
74	11.457	1699	1701	1702	rBV	541	304	0.03%	0.005%
75	11.610	1724	1726	1728	rVB3	457	436	0.05%	0.007%
76	11.725	1742	1745	1746	rBV	410	337	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043532.D
 Acq On : 25 Oct 2024 18:43
 Operator : JC/MD
 Sample : VIBLK670
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK670

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

77	11.762	1748	1751	1753	rBV2	956	827	0.09%	0.013%
78	11.793	1753	1756	1757	rBV	331	370	0.04%	0.006%
79	11.975	1783	1786	1788	rBV2	802	907	0.10%	0.014%
80	12.018	1788	1793	1805	rVV	361930	477865	54.31%	7.459%
81	12.317	1837	1842	1855	rBV	426194	549504	62.46%	8.578%
82	12.670	1897	1900	1901	rBV3	287	315	0.04%	0.005%
83	12.859	1929	1931	1935	rVB2	496	491	0.06%	0.008%
84	13.231	1991	1992	1994	rBV	472	411	0.05%	0.006%
85	13.298	2001	2003	2006	rBV2	570	620	0.07%	0.010%
86	13.542	2042	2043	2044	rBV	611	326	0.04%	0.005%
87	13.591	2048	2051	2055	rVV3	743	1310	0.15%	0.020%
88	13.780	2079	2082	2085	rBV2	592	747	0.08%	0.012%
89	13.920	2103	2105	2107	rBV2	387	394	0.04%	0.006%
90	14.036	2122	2124	2126	rBV	262	302	0.03%	0.005%
91	14.060	2126	2128	2129	rBV2	409	376	0.04%	0.006%
92	14.140	2139	2141	2143	rVB	422	302	0.03%	0.005%
93	14.469	2194	2195	2200	rVB4	661	868	0.10%	0.014%
94	14.505	2200	2201	2202	rBV	588	350	0.04%	0.005%
95	14.652	2223	2225	2227	rBV2	397	342	0.04%	0.005%
96	14.951	2272	2274	2276	rBV2	701	561	0.06%	0.009%
97	15.249	2322	2323	2325	rBV2	452	432	0.05%	0.007%
98	15.572	2374	2376	2378	rBV2	525	571	0.06%	0.009%
99	16.487	2524	2526	2528	rBV2	589	403	0.05%	0.006%
100	16.511	2528	2530	2532	rBV2	695	574	0.07%	0.009%




Sum of corrected areas: 6406177

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043532.D
Acq On : 25 Oct 2024 18:43
Operator : JC/MD
Sample : VIBLK670
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK670

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

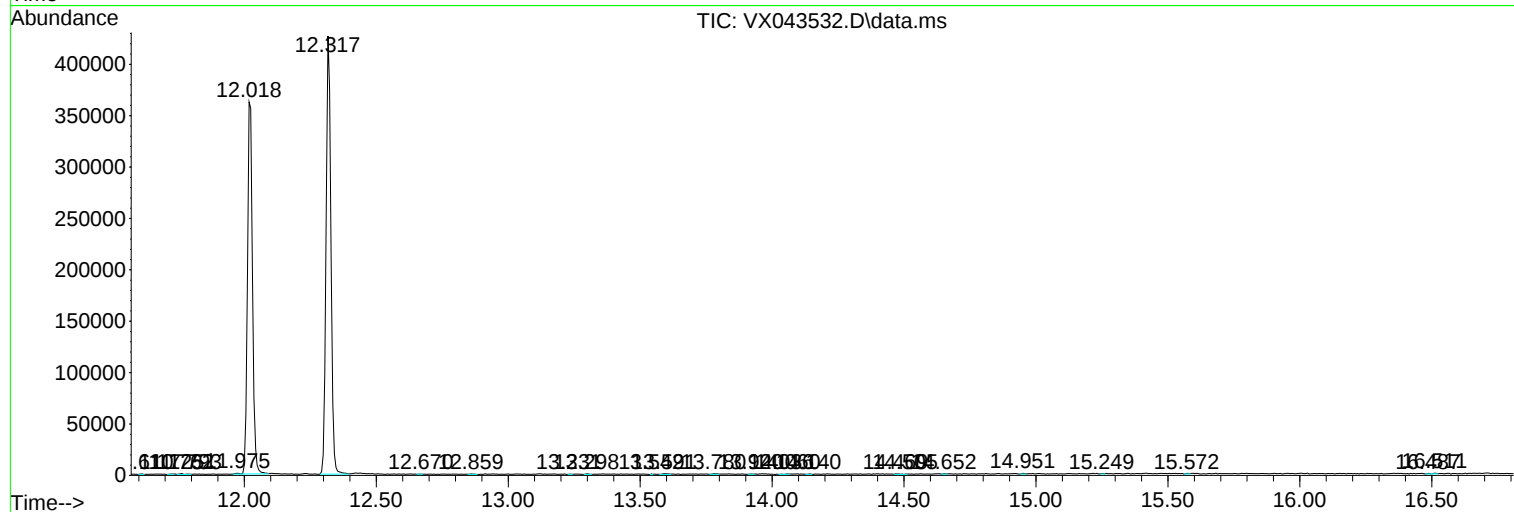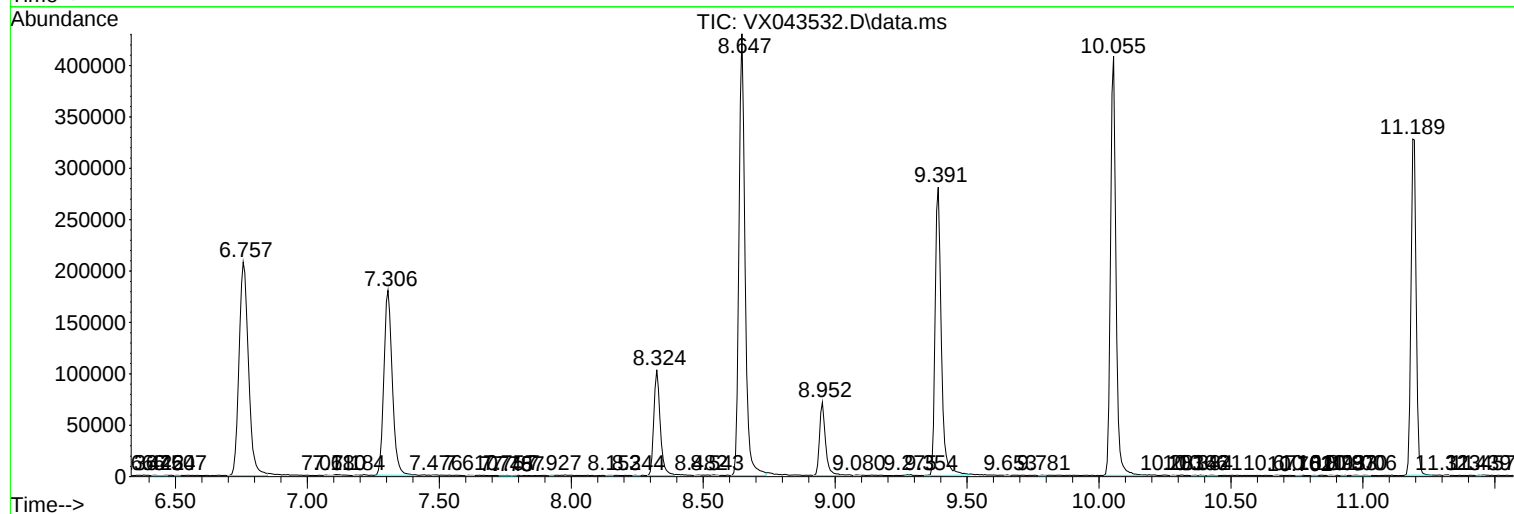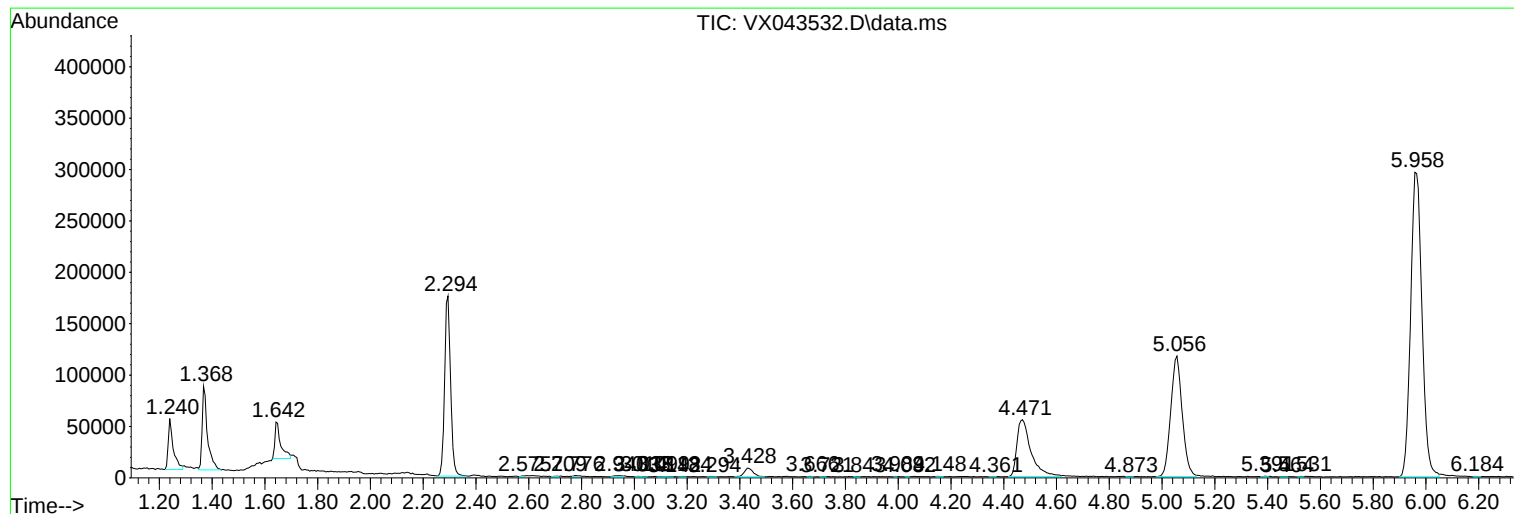

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043532.D
Acq On : 25 Oct 2024 18:43
Operator : JC/MD
Sample : VIBLK670
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK670

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043532.D
Acq On : 25 Oct 2024 18:43
Operator : JC/MD
Sample : VIBLK670
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK670

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------