
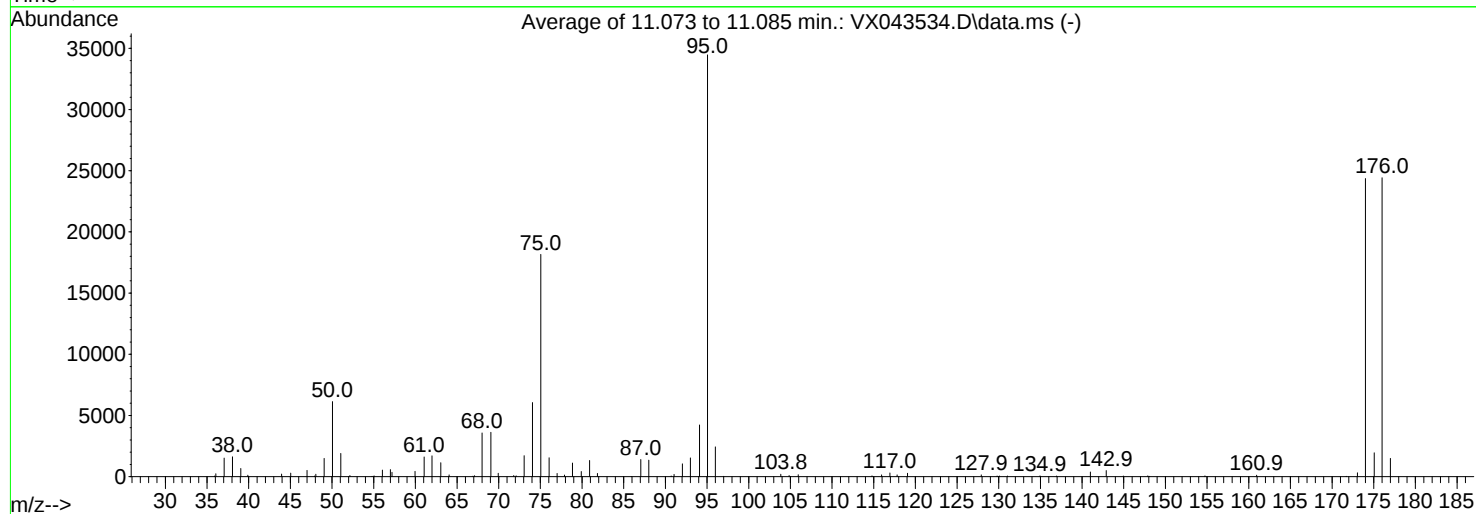


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102624\
Data File : VX043534.D
Acq On : 25 Oct 2024 21:50
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102624W.M
Title : SW846 8260
Last Update : Sat Oct 26 04:43:47 2024

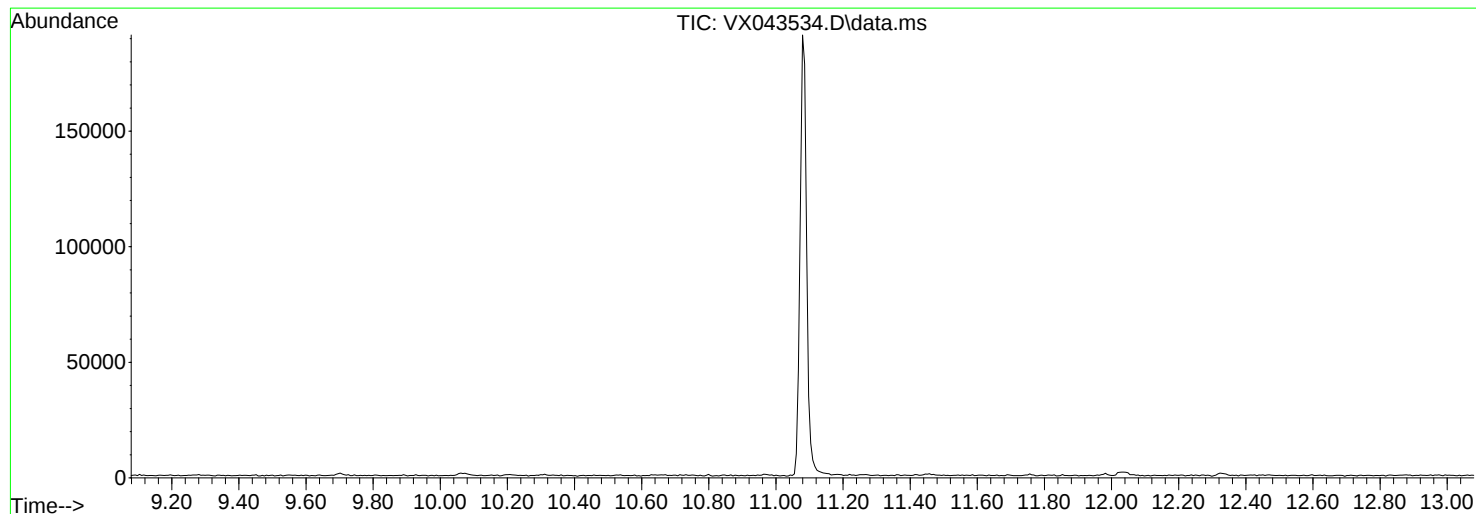

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	6131	PASS
75	95	30	60	52.7	18161	PASS
95	95	100	100	100.0	34469	PASS
96	95	5	9	7.1	2439	PASS
173	174	0.00	2	1.3	313	PASS
174	95	50	100	70.7	24363	PASS
175	174	5	9	8.0	1952	PASS
176	174	95	101	100.3	24425	PASS
177	176	5	9	6.1	1490	PASS