

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102824\
 Data File : VX043568.D
 Acq On : 28 Oct 2024 17:14
 Operator : JC/MD
 Sample : PB164394TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Oct 29 03:26:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 28 13:41:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	157154	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	298510	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	260799	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	116240	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	123854	49.426	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	98.860%
35) Dibromofluoromethane	5.385	113	97712	48.272	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.540%
50) Toluene-d8	8.647	98	351010	50.094	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.180%
62) 4-Bromofluorobenzene	11.079	95	125219	48.227	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	96.460%


Target Compounds			Qvalue			
3) Chloromethane	1.288	50	496	0.231	ug/l #	42
5) Bromomethane	1.593	94	411	0.506	ug/l	97
6) Chloroethane	1.636	64	325	0.463	ug/l #	43
11) Tert butyl alcohol	2.946	59	3644	7.791	ug/l #	100
13) Acrolein	2.239	56	146	0.399	ug/l	99
15) Acrylonitrile	3.081	53	375	0.355	ug/l #	30
16) Acetone	2.392	43	26778	26.910	ug/l	97
17) Carbon Disulfide	2.501	76	741	0.211	ug/l #	74
18) Methyl Acetate	2.715	43	2291	0.788	ug/l	93
20) Methylene Chloride	2.788	84	4022	1.875	ug/l #	96
25) 2-Butanone	4.593	43	1640	1.130	ug/l #	79
29) Tetrahydrofuran	5.050	42	1070	1.134	ug/l #	67
31) Cyclohexane	5.544	56	3188	1.205	ug/l #	1
36) 1,1-Dichloropropene	5.550	75	12824	5.343	ug/l #	49
37) Ethyl Acetate	4.739	43	1648	0.566	ug/l #	80
38) Carbon Tetrachloride	5.544	117	17016	6.416	ug/l #	17
43) Isopropyl Acetate	6.342	43	113795	23.614	ug/l	100
48) Methyl methacrylate	7.622	41	3426	1.500	ug/l #	13
49) 1,4-Dioxane	7.665	88	19	0.405	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	86503	29.451	ug/l #	50
53) t-1,3-Dichloropropene	8.958	75	854	0.299	ug/l #	42
54) cis-1,3-Dichloropropene	8.549	75	39965	13.113	ug/l #	59
57) 1,3-Dichloropropane	9.482	76	5263	1.565	ug/l #	42
59) 2-Hexanone	9.482	43	66718	29.908	ug/l #	53
68) m/p-Xylenes	10.305	106	733	0.209	ug/l	91
76) 1,2,3-Trichloropropane	11.079	75	64869	26.100	ug/l #	33
81) trans-1,4-Dichloro-2-b...	11.079	75	64869	71.803	ug/l #	7
87) 1,3-Dichlorobenzene	11.981	146	876	0.230	ug/l	91
88) 1,4-Dichlorobenzene	11.981	146	876	0.222	ug/l	91
93) 1,2,4-Trichlorobenzene	13.591	180	651	0.275	ug/l	91
95) Naphthalene	13.780	128	2548	0.282	ug/l	98
96) 1,2,3-Trichlorobenzene	13.963	180	563	0.226	ug/l	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102824\
Data File : VX043568.D
Acq On : 28 Oct 2024 17:14
Operator : JC/MD
Sample : PB164394TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Oct 29 03:26:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
Quant Title : SW846 8260
QLast Update : Mon Oct 28 13:41:34 2024
Response via : Initial Calibration




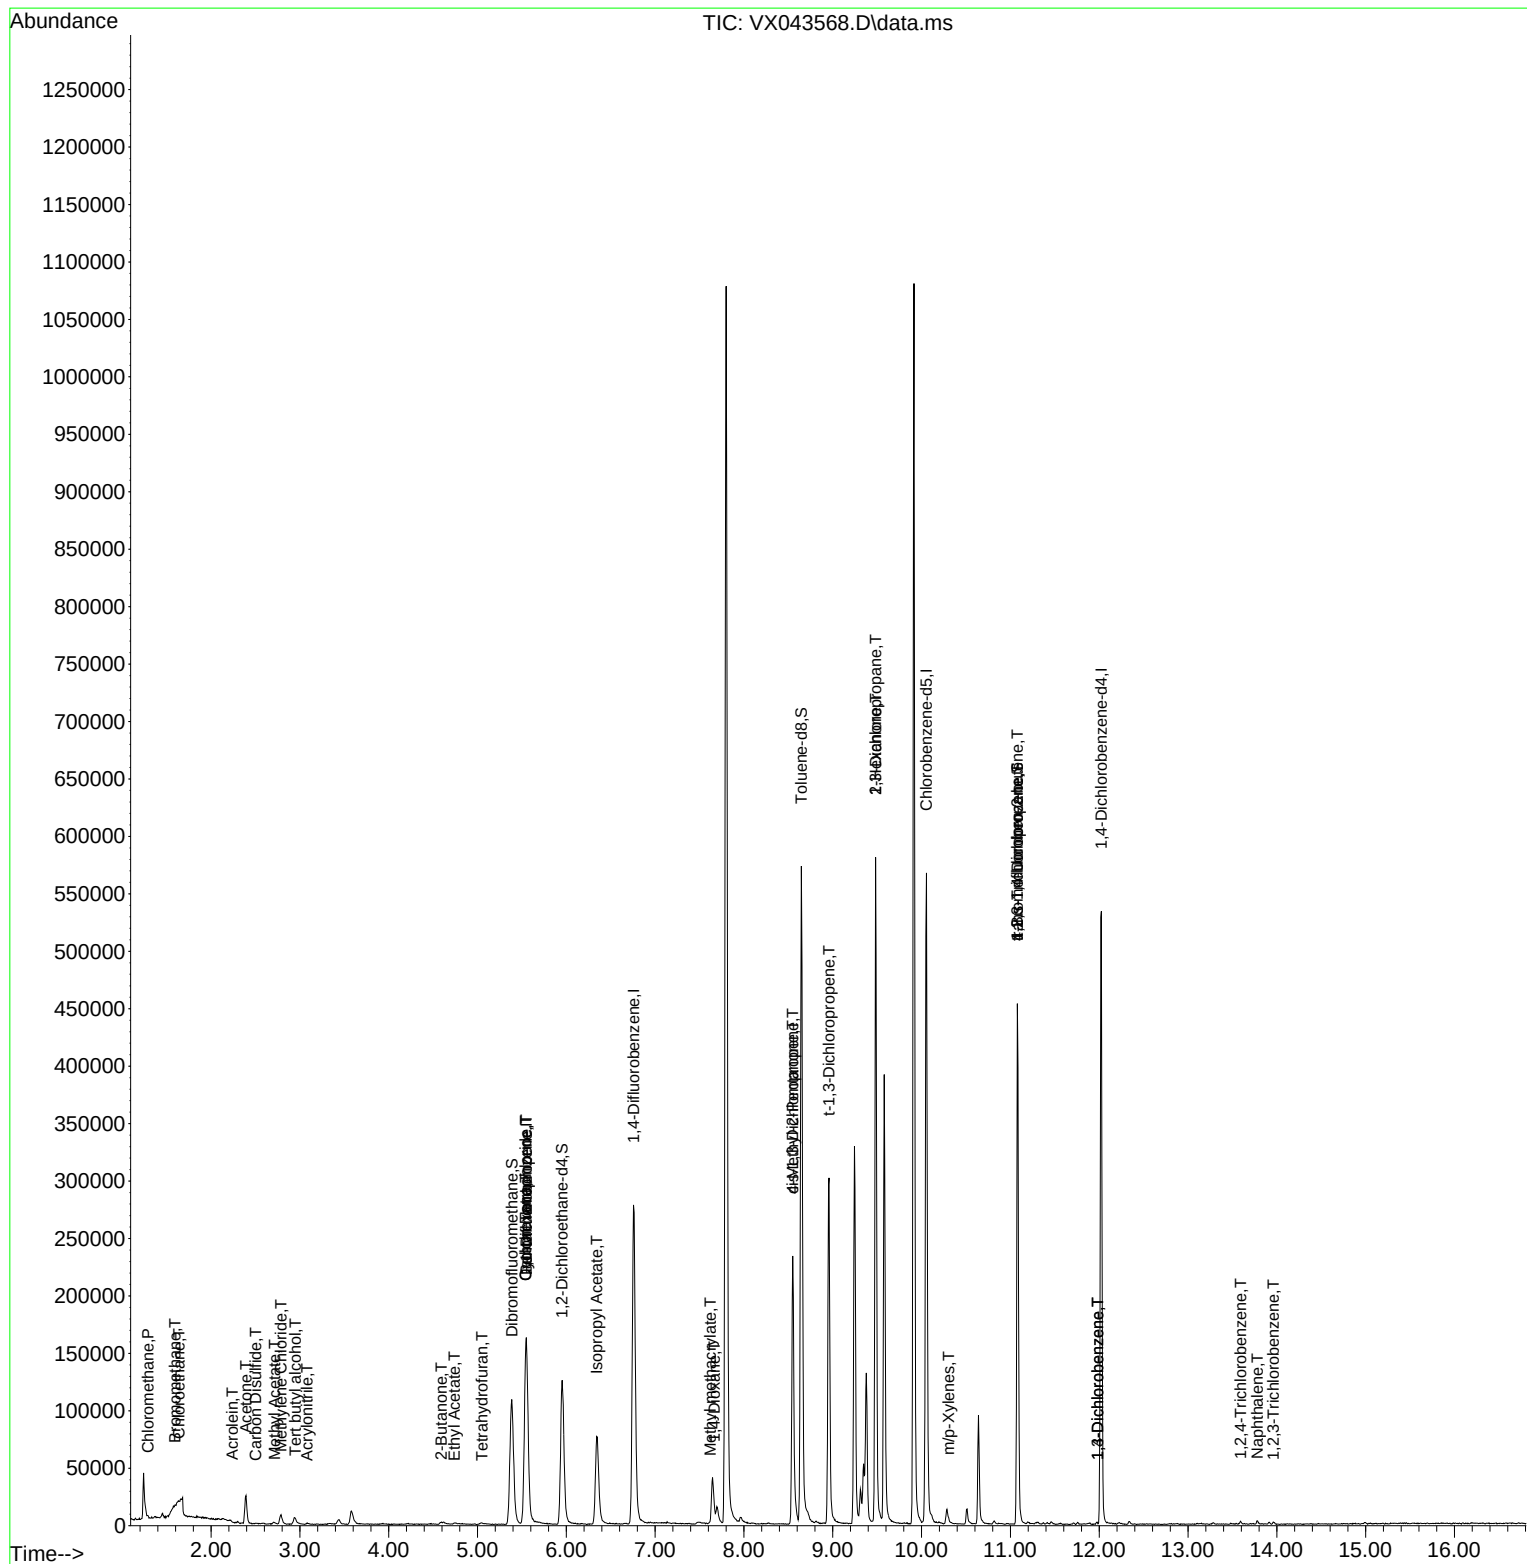




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 157154
Ion Ratio Lower Upper
168 100
99 61.2 52.6 78.8

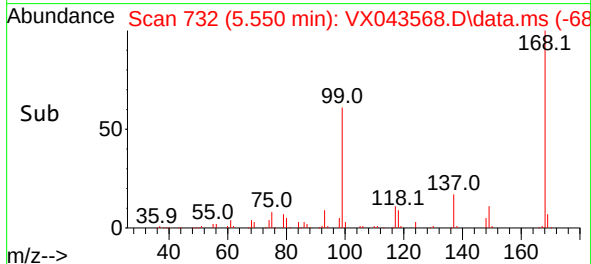

#3
Chloromethane
Concen: 0.231 ug/l
RT: 1.288 min Scan# 33
Delta R.T. -0.006 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14

Tgt Ion: 50 Resp: 496
Ion Ratio Lower Upper
50 100
52 0.0 26.3 39.5#


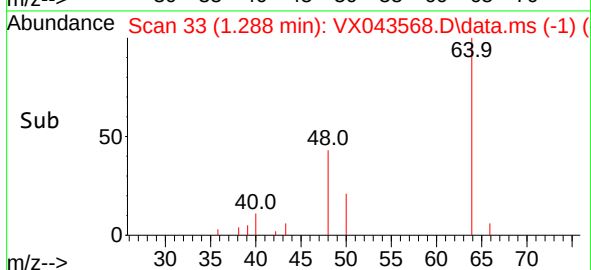

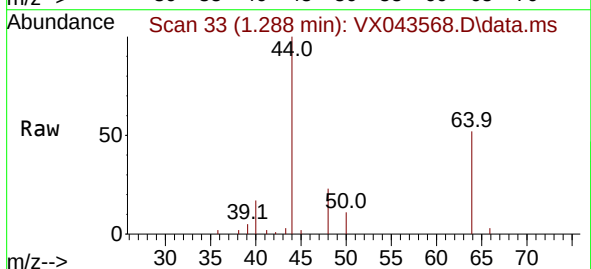


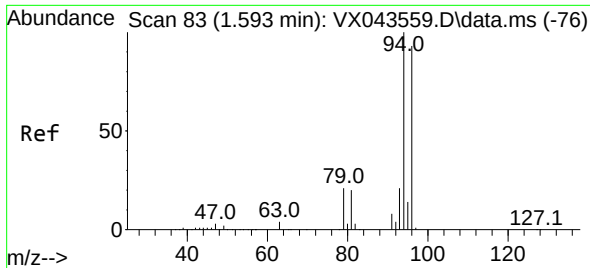

#5
Bromomethane
Concen: 0.506 ug/l
RT: 1.593 min Scan# 81
Delta R.T. 0.000 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 94 Resp: 411
Ion Ratio Lower Upper
94 100
96 98.1 75.9 113.9

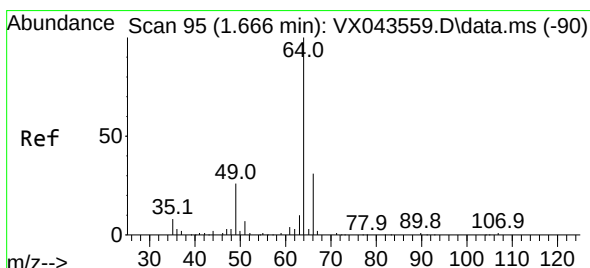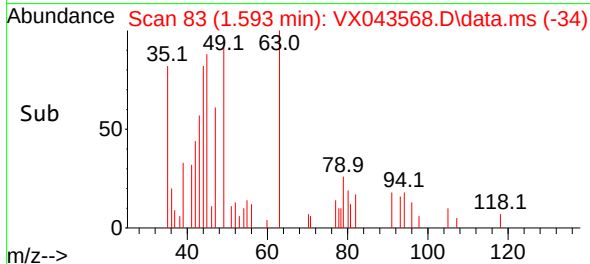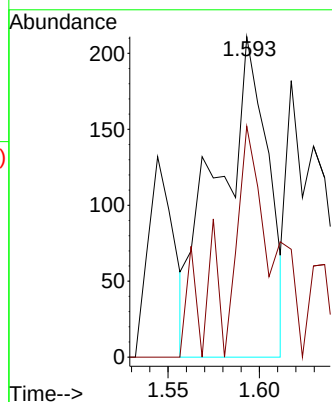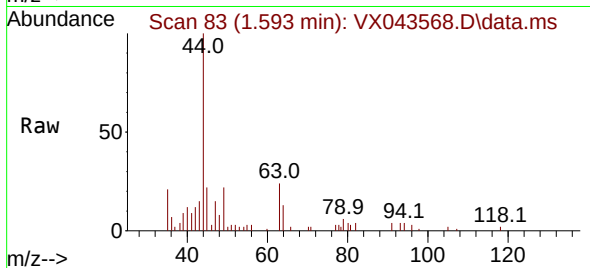

#6
Chloroethane
Concen: 0.463 ug/l
RT: 1.636 min Scan# 90
Delta R.T. -0.024 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14

Tgt Ion: 64 Resp: 325
Ion Ratio Lower Upper
64 100
66 0.0 25.1 37.7#


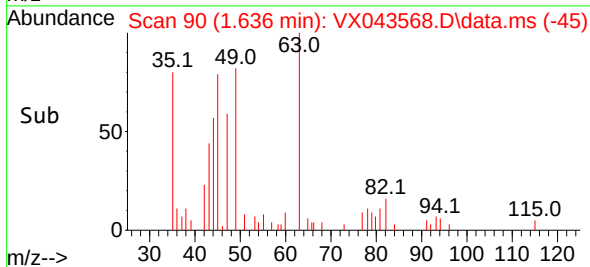
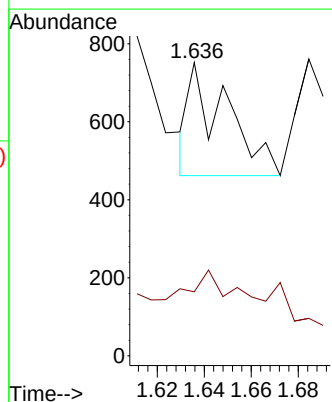
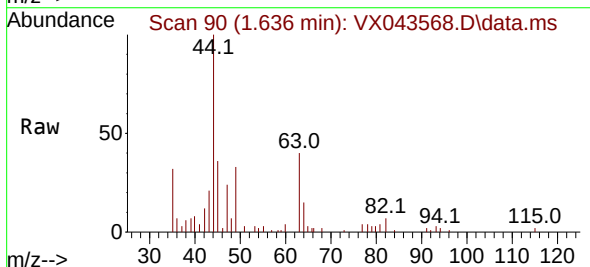




#11
Tert butyl alcohol
Concen: 7.791 ug/l
RT: 2.946 min Scan# 305
Delta R.T. -0.104 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 59 Resp: 3644
Ion Ratio Lower Upper
59 100
57 0.0 0.0 0.0

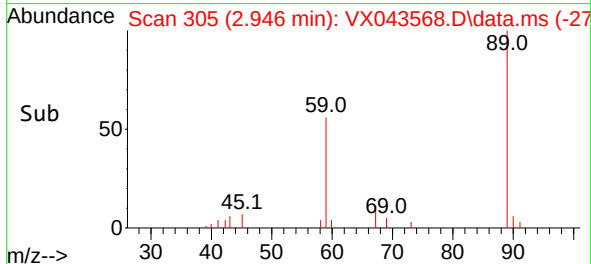

#13
Acrolein
Concen: 0.399 ug/l
RT: 2.239 min Scan# 189
Delta R.T. 0.000 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14

Tgt Ion: 56 Resp: 146
Ion Ratio Lower Upper
56 100
55 68.5 55.3 82.9





#15

Acrylonitrile

Concen: 0.355 ug/l

RT: 3.081 min Scan# 31

Delta R.T. 0.006 min

Lab File: VX043568.D





Acq: 28 Oct 2024 17:14

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 53	Resp:	375
Ion Ratio	Lower	Upper
53	100	
52	15.7	65.8 98.6#
51	0.0	28.5 42.7#

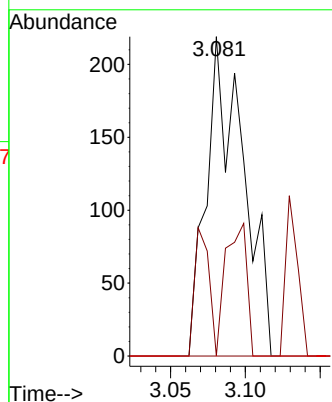

#16

Acetone

Concen: 26.910 ug/l




RT: 2.392 min Scan# 214


Delta R.T. -0.006 min

Lab File: VX043568.D

Acq: 28 Oct 2024 17:14

Tgt Ion: 43	Resp:	26778
Ion Ratio	Lower	Upper
43	100	
58	29.9	25.1 37.7


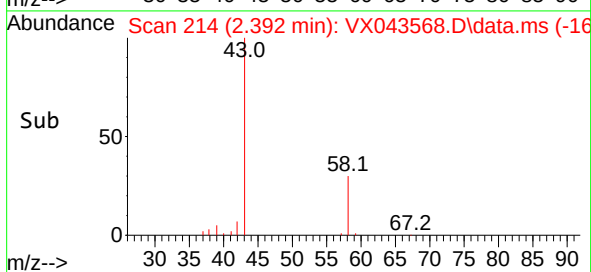
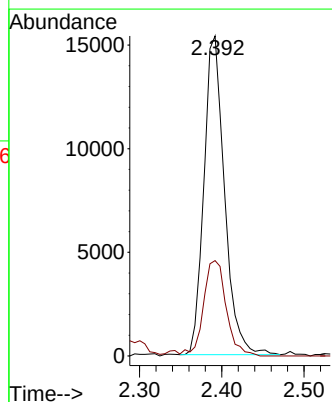





#17
Carbon Disulfide
Concen: 0.211 ug/l
RT: 2.501 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 76 Resp: 741
Ion Ratio Lower Upper
76 100
78 18.2 7.1 10.7#

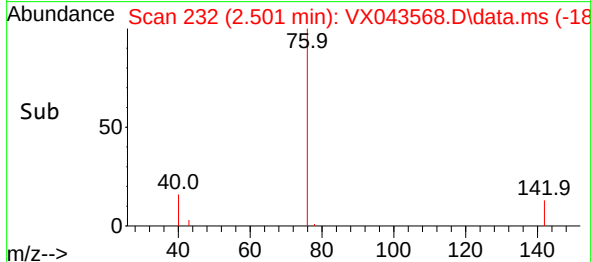

#18
Methyl Acetate
Concen: 0.788 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.006 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14


Tgt Ion: 43 Resp: 2291
Ion Ratio Lower Upper
43 100
74 20.5 19.1 28.7

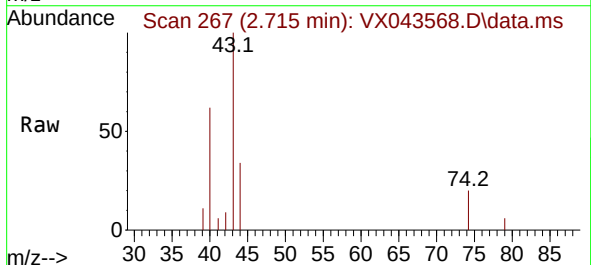






#20
Methylene Chloride
Concen: 1.875 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:	84	Resp:	4022
Ion	Ratio	Lower	Upper
84	100		
49	122.6	97.0	145.6
51	45.7	29.8	44.8#
86	62.5	53.1	79.7

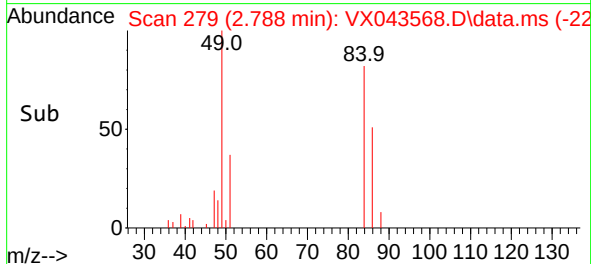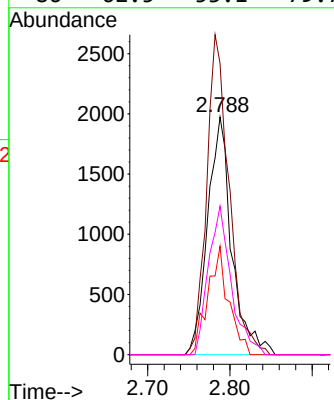

#25
2-Butanone
Concen: 1.130 ug/l
RT: 4.593 min Scan# 575
Delta R.T. 0.024 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14

Tgt Ion:	43	Resp:	1640
Ion	Ratio	Lower	Upper
43	100		
72	37.3	21.1	31.7#

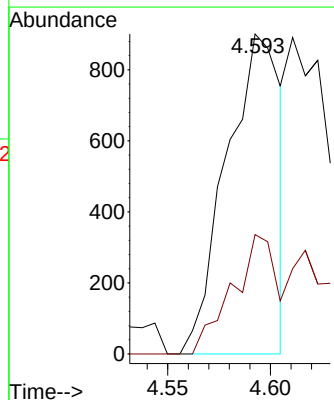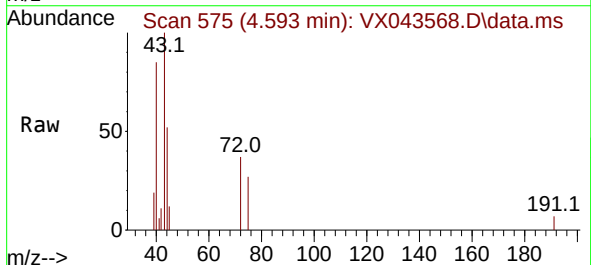



#29

Tetrahydrofuran

Concen: 1.134 ug/l

RT: 5.050 min Scan# 61

Delta R.T. 0.037 min

Lab File: VX043568.D





Acq: 28 Oct 2024 17:14

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion:	42	Resp:	1070
Ion	Ratio	Lower	Upper
42	100		
72	26.3	36.6	55.0#
71	20.1	34.2	51.4#

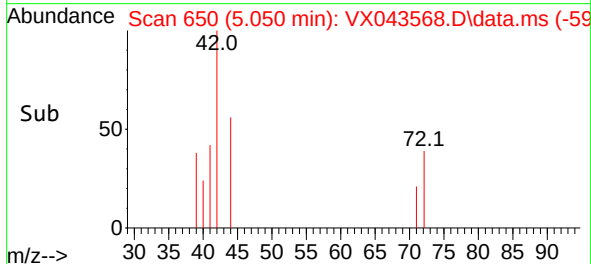

#31

Cyclohexane

Concen: 1.205 ug/l




RT: 5.544 min Scan# 731


Delta R.T. 0.085 min

Lab File: VX043568.D

Acq: 28 Oct 2024 17:14

Tgt Ion:	56	Resp:	3188
Ion	Ratio	Lower	Upper
56	100		
69	209.2	24.9	37.3#
84	113.3	73.3	109.9#





#33

1,2-Dichloroethane-d4

Concen: 49.426 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.000 min

Lab File: VX043568.D

Acq: 28 Oct 2024 17:14

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 123854

Ion Ratio Lower Upper

65 100

67 52.2 0.0 103.4

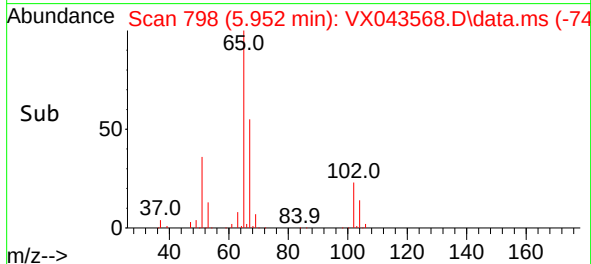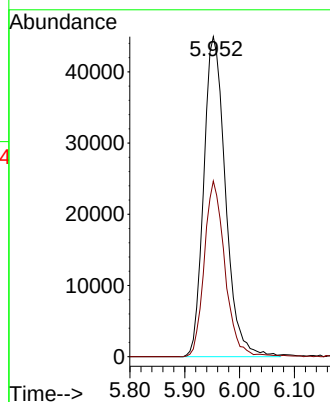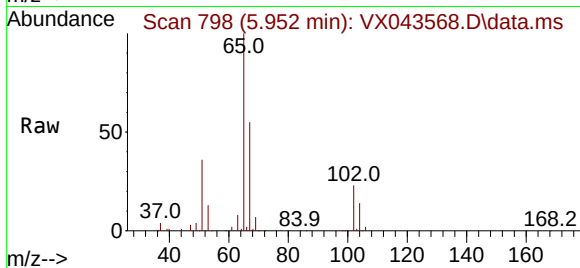

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. 0.000 min

Lab File: VX043568.D

Acq: 28 Oct 2024 17:14




Tgt Ion: 114 Resp: 298510


Ion Ratio Lower Upper

114 100

63 21.0 0.0 41.2

88 16.2 0.0 34.0


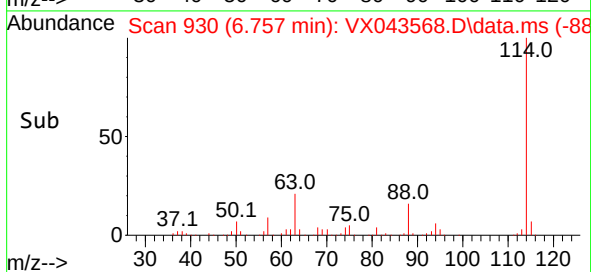
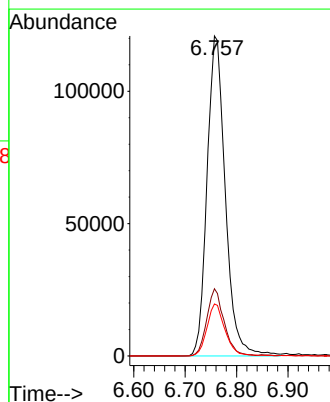
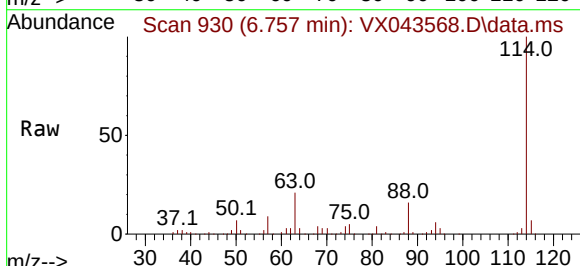


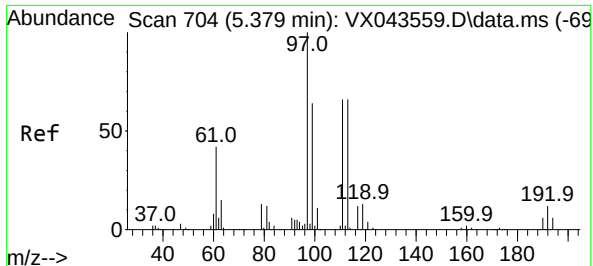

#35
Dibromofluoromethane
Concen: 48.272 ug/l
RT: 5.385 min Scan# 704
Delta R.T. 0.000 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:113 Resp: 97712
Ion Ratio Lower Upper
113 100
111 101.4 81.4 122.0
192 18.2 14.1 21.1

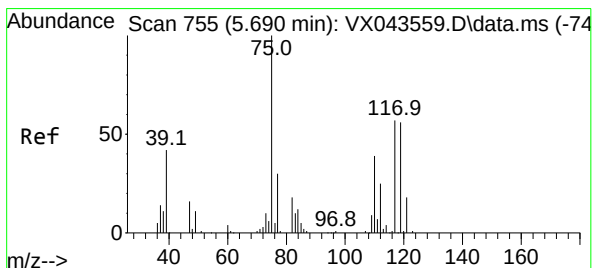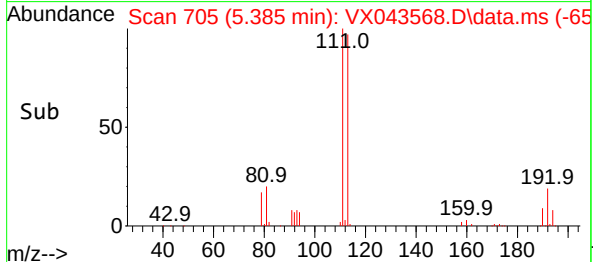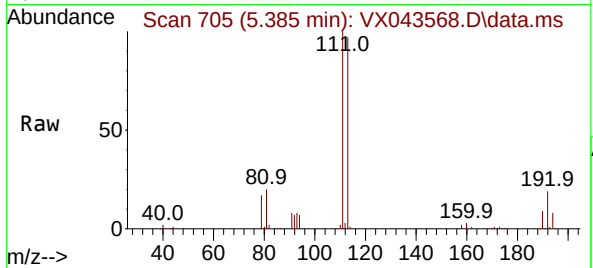

#36
1,1-Dichloropropene
Concen: 5.343 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.134 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14


Tgt Ion: 75 Resp: 12824
Ion Ratio Lower Upper
75 100
110 9.0 17.9 53.7#
77 0.0 25.0 37.4#

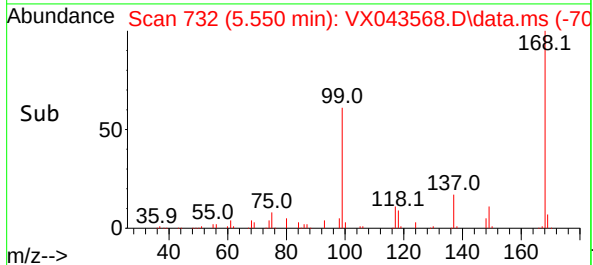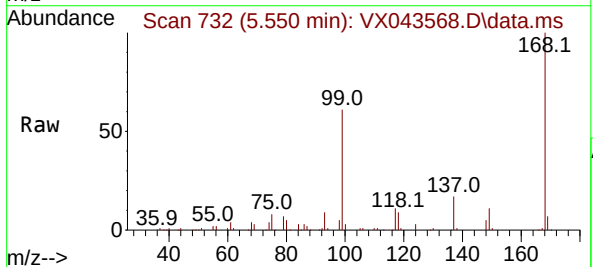






#37
Ethyl Acetate
Concen: 0.566 ug/l
RT: 4.739 min Scan# 595
Delta R.T. 0.018 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 43 Resp: 1648
Ion Ratio Lower Upper
43 100
61 4.0 11.0 16.6#
70 5.8 8.9 13.3#

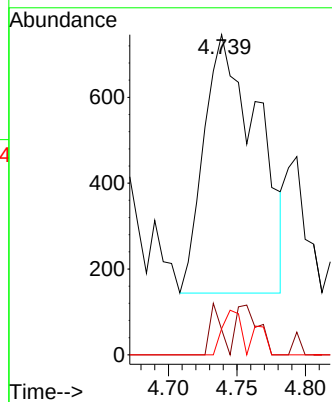

#38
Carbon Tetrachloride
Concen: 6.416 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.128 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14


Tgt Ion: 117 Resp: 17016
Ion Ratio Lower Upper
117 100
119 6.4 77.0 115.6#
121 0.0 24.7 37.1#

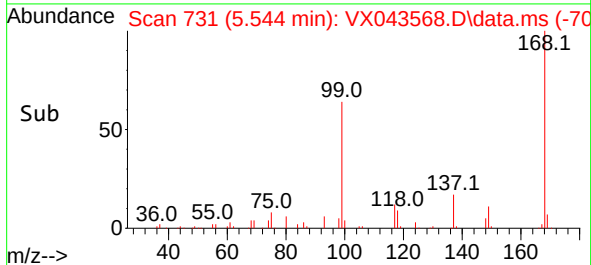






#43
Isopropyl Acetate
Concen: 23.614 ug/l
RT: 6.342 min Scan# 862
Delta R.T. 0.000 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 43 Resp: 113795
Ion Ratio Lower Upper
43 100
61 20.4 16.2 24.4
87 13.5 11.0 16.6

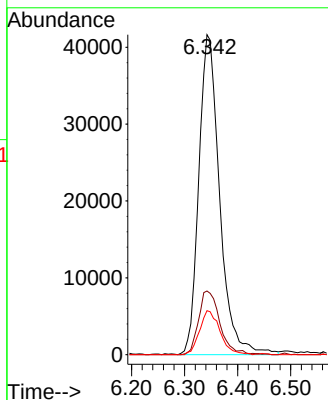

#48
Methyl methacrylate
Concen: 1.500 ug/l
RT: 7.622 min Scan# 1072
Delta R.T. -0.073 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14

Tgt Ion: 41 Resp: 3426
Ion Ratio Lower Upper
41 100
69 0.0 67.7 101.5#
39 0.0 46.3 69.5#

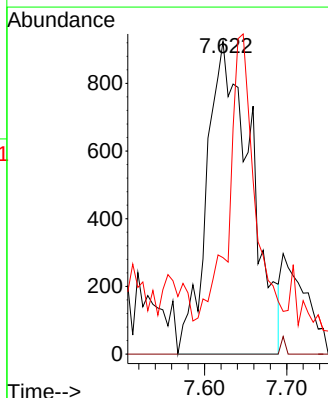



#49

1,4-Dioxane

Concen: 0.405 ug/l

RT: 7.665 min Scan# 1080

Delta R.T. -0.006 min

Lab File: VX043568.D

Acq: 28 Oct 2024 17:14





Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 88 Resp: 19

Ion	Ratio	Lower	Upper
88	100		
43	0.0	25.3	37.9#
58	10136.8	53.9	80.9#



#50

Toluene-d8

Concen: 50.094 ug/l

RT: 8.647 min Scan# 1240




Delta R.T. 0.000 min


Lab File: VX043568.D

Acq: 28 Oct 2024 17:14

Tgt Ion: 98 Resp: 351010

Ion	Ratio	Lower	Upper
98	100		
100	66.9	53.4	80.2


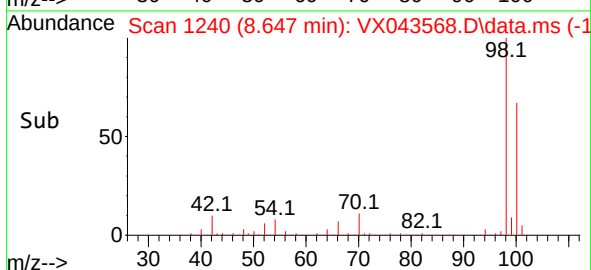






#51
4-Methyl-2-Pentanone
Concen: 29.451 ug/l
RT: 8.549 min Scan# 11
Delta R.T. -0.030 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 86503
Ion Ratio Lower Upper
43 100
58 9.2 31.7 47.5#

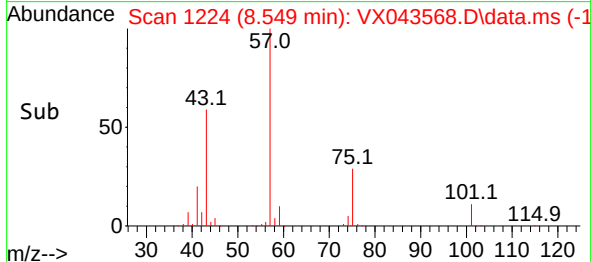

#53
t-1,3-Dichloropropene
Concen: 0.299 ug/l
RT: 8.958 min Scan# 1291
Delta R.T. -0.018 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14

Tgt Ion: 75 Resp: 854
Ion Ratio Lower Upper
75 100
77 0.0 26.0 39.0#




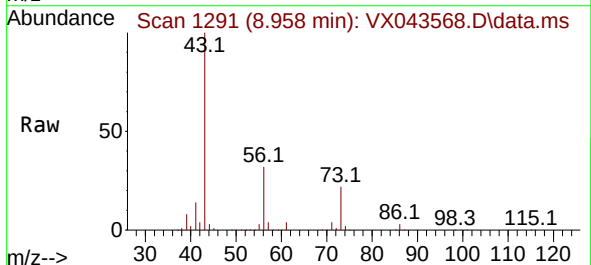


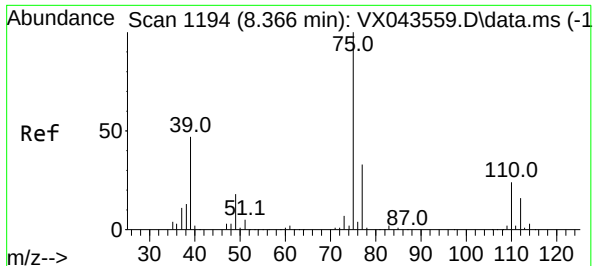

#54
 cis-1,3-Dichloropropene
 Concen: 13.113 ug/l
 RT: 8.549 min Scan# 1194
 Delta R.T. 0.183 min
 Lab File: VX043568.D
 Acq: 28 Oct 2024 17:14




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 75 Resp: 39965
 Ion Ratio Lower Upper
 75 100
 77 0.7 24.8 37.2#
 39 25.7 37.7 56.5#

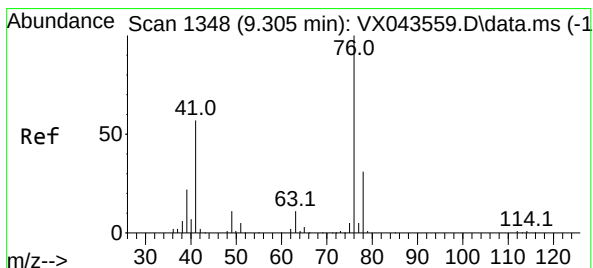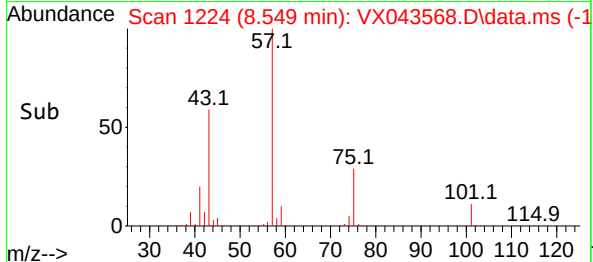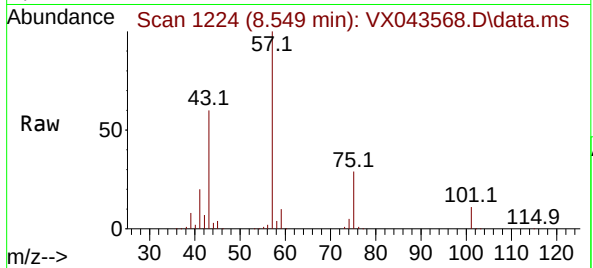

#57
 1,3-Dichloropropane
 Concen: 1.565 ug/l
 RT: 9.482 min Scan# 1377
 Delta R.T. 0.177 min
 Lab File: VX043568.D
 Acq: 28 Oct 2024 17:14

Tgt Ion: 76 Resp: 5263
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.9 38.9#

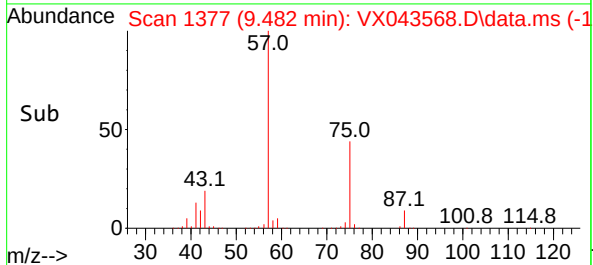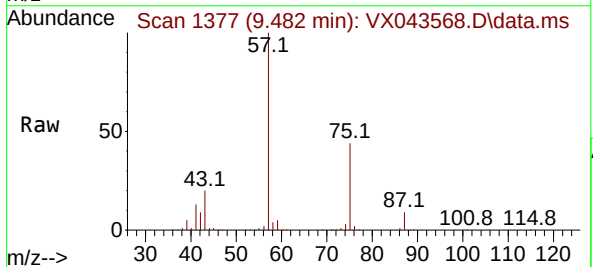



#59

2-Hexanone

Concen: 29.908 ug/l

RT: 9.482 min Scan# 1

Delta R.T. 0.049 min

Lab File: VX043568.D

Acq: 28 Oct 2024 17:14

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 66718

Ion Ratio Lower Upper

43 100

58 21.4 27.5 82.5#

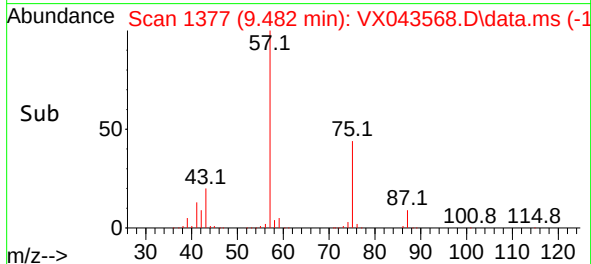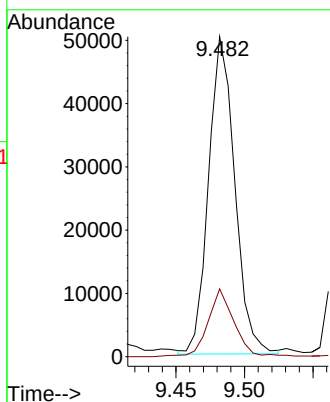

#62

4-Bromofluorobenzene

Concen: 48.227 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX043568.D

Acq: 28 Oct 2024 17:14




Tgt Ion: 95 Resp: 125219


Ion Ratio Lower Upper

95 100

174 75.6 0.0 146.6

176 74.2 0.0 139.6









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 260799
Ion Ratio Lower Upper
117 100
82 54.8 42.1 63.1
119 32.5 25.4 38.2

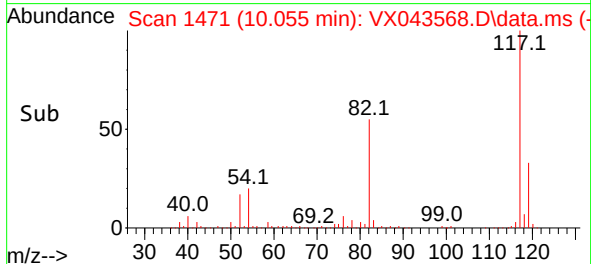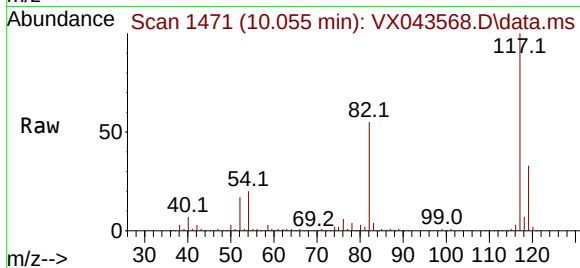

#68
m/p-Xylenes
Concen: 0.209 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14

Tgt Ion:106 Resp: 733
Ion Ratio Lower Upper
106 100
91 220.2 164.7 247.1

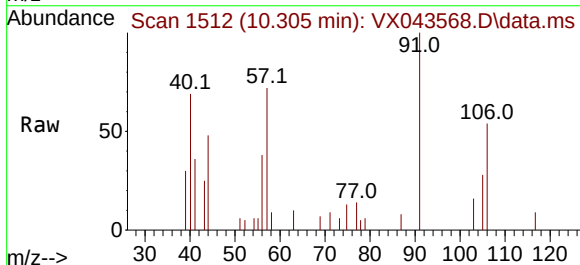



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX043568.D

Acq: 28 Oct 2024 17:14

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:152 Resp: 116240

Ion Ratio Lower Upper

152 100

115 61.9 42.9 128.7

150 159.3 0.0 343.6

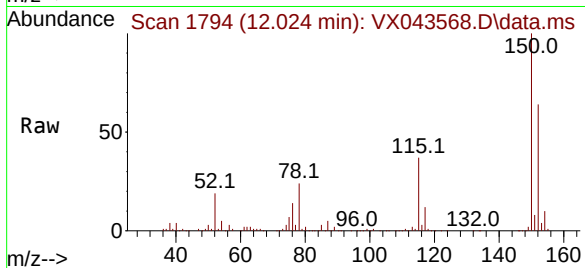

#76

1,2,3-Trichloropropane

Concen: 26.100 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX043568.D




Acq: 28 Oct 2024 17:14


Tgt Ion: 75 Resp: 64869

Ion Ratio Lower Upper

75 100

77 1.1 22.4 67.2#


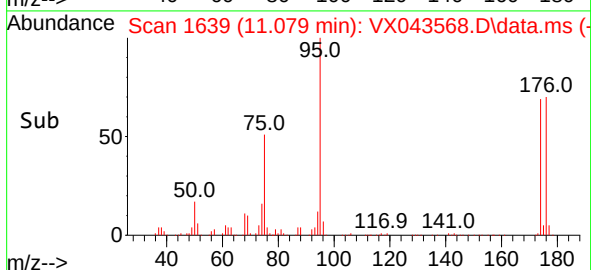

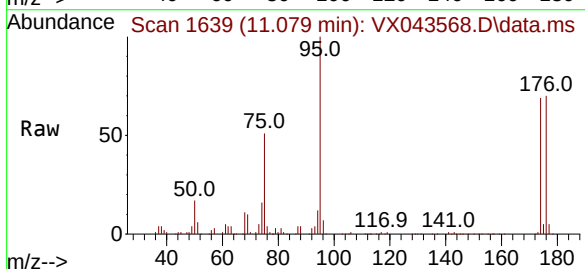




#81
trans-1,4-Dichloro-2-butene
Concen: 71.803 ug/l
RT: 11.079 min Scan# 1629
Delta R.T. 0.061 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 64869
Ion Ratio Lower Upper
75 100
53 0.0 84.6 126.8#
89 0.0 38.6 58.0#

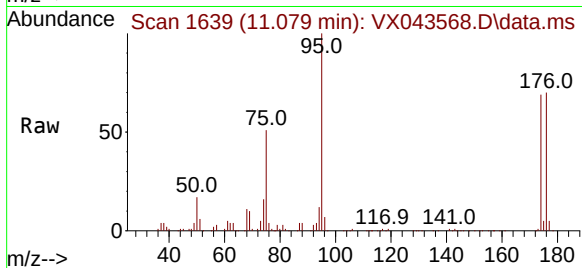

#87
1,3-Dichlorobenzene
Concen: 0.230 ug/l
RT: 11.981 min Scan# 1787
Delta R.T. 0.012 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14


Tgt Ion:146 Resp: 876
Ion Ratio Lower Upper
146 100
111 37.1 21.1 63.4
148 55.8 31.6 94.8

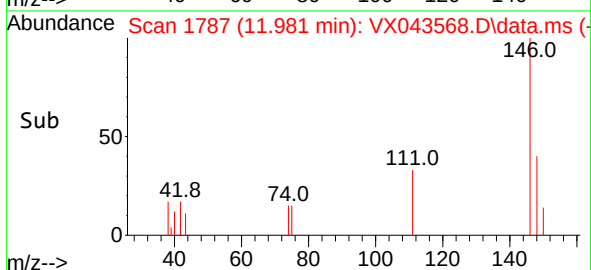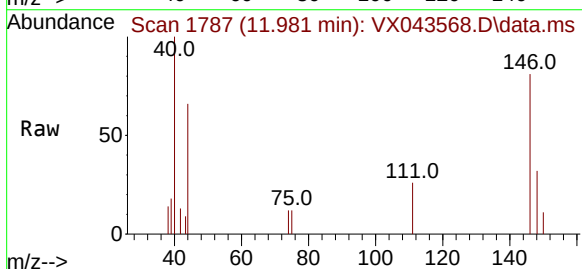






#88
1,4-Dichlorobenzene
Concen: 0.222 ug/l
RT: 11.981 min Scan# 11
Delta R.T. -0.061 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14

Instrument :
MSVOA_X
ClientSampleId :



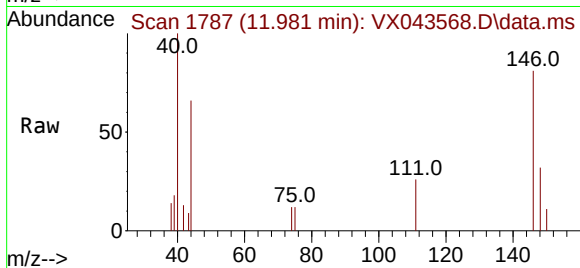



Tgt Ion:146 Resp: 876
Ion Ratio Lower Upper
146 100
111 37.1 20.4 61.3
148 55.8 31.9 95.9

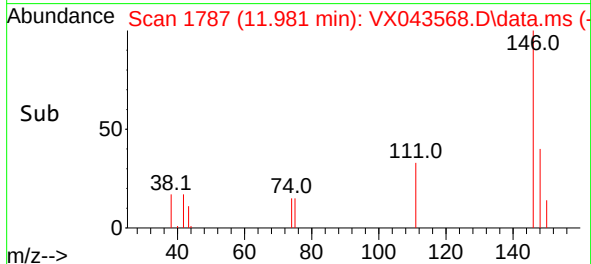

#93
1,2,4-Trichlorobenzene
Concen: 0.275 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.006 min
Lab File: VX043568.D
Acq: 28 Oct 2024 17:14

Tgt Ion:180 Resp: 651
Ion Ratio Lower Upper
180 100
182 85.9 46.8 140.4
145 26.3 16.1 48.3

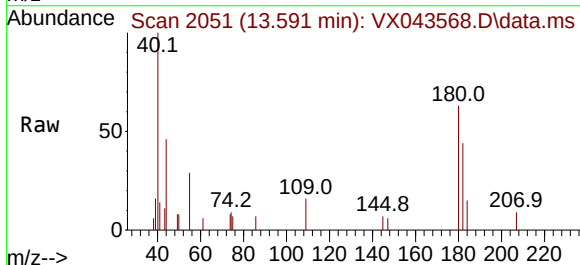



#95

Naphthalene

Concen: 0.282 ug/l

RT: 13.780 min Scan# 2081

Delta R.T. 0.006 min

Lab File: VX043568.D





Acq: 28 Oct 2024 17:14

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion:128	Resp:	2548
Ion Ratio	Lower	Upper
128	100	
127	11.9	10.2 15.4
129	10.0	8.7 13.1

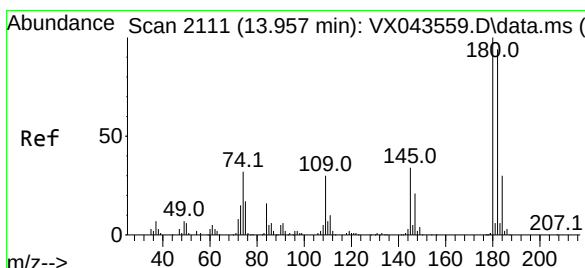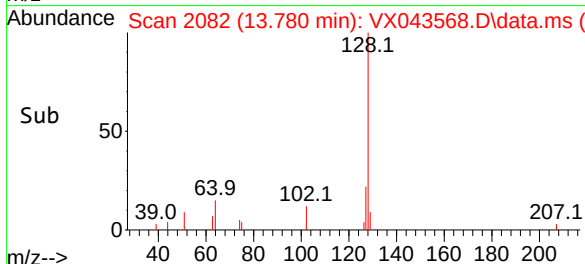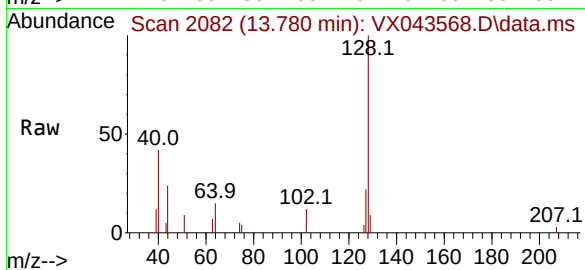

#96

1,2,3-Trichlorobenzene

Concen: 0.226 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. 0.000 min

Lab File: VX043568.D

Acq: 28 Oct 2024 17:14

Tgt Ion:180	Resp:	563
Ion Ratio	Lower	Upper
180	100	
182	109.9	47.1 141.3
145	42.1	17.4 52.3

