


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102824\
Data File : VX043555.D
Acq On : 28 Oct 2024 10:09
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
Title : SW846 8260
Last Update : Mon Oct 28 13:41:34 2024

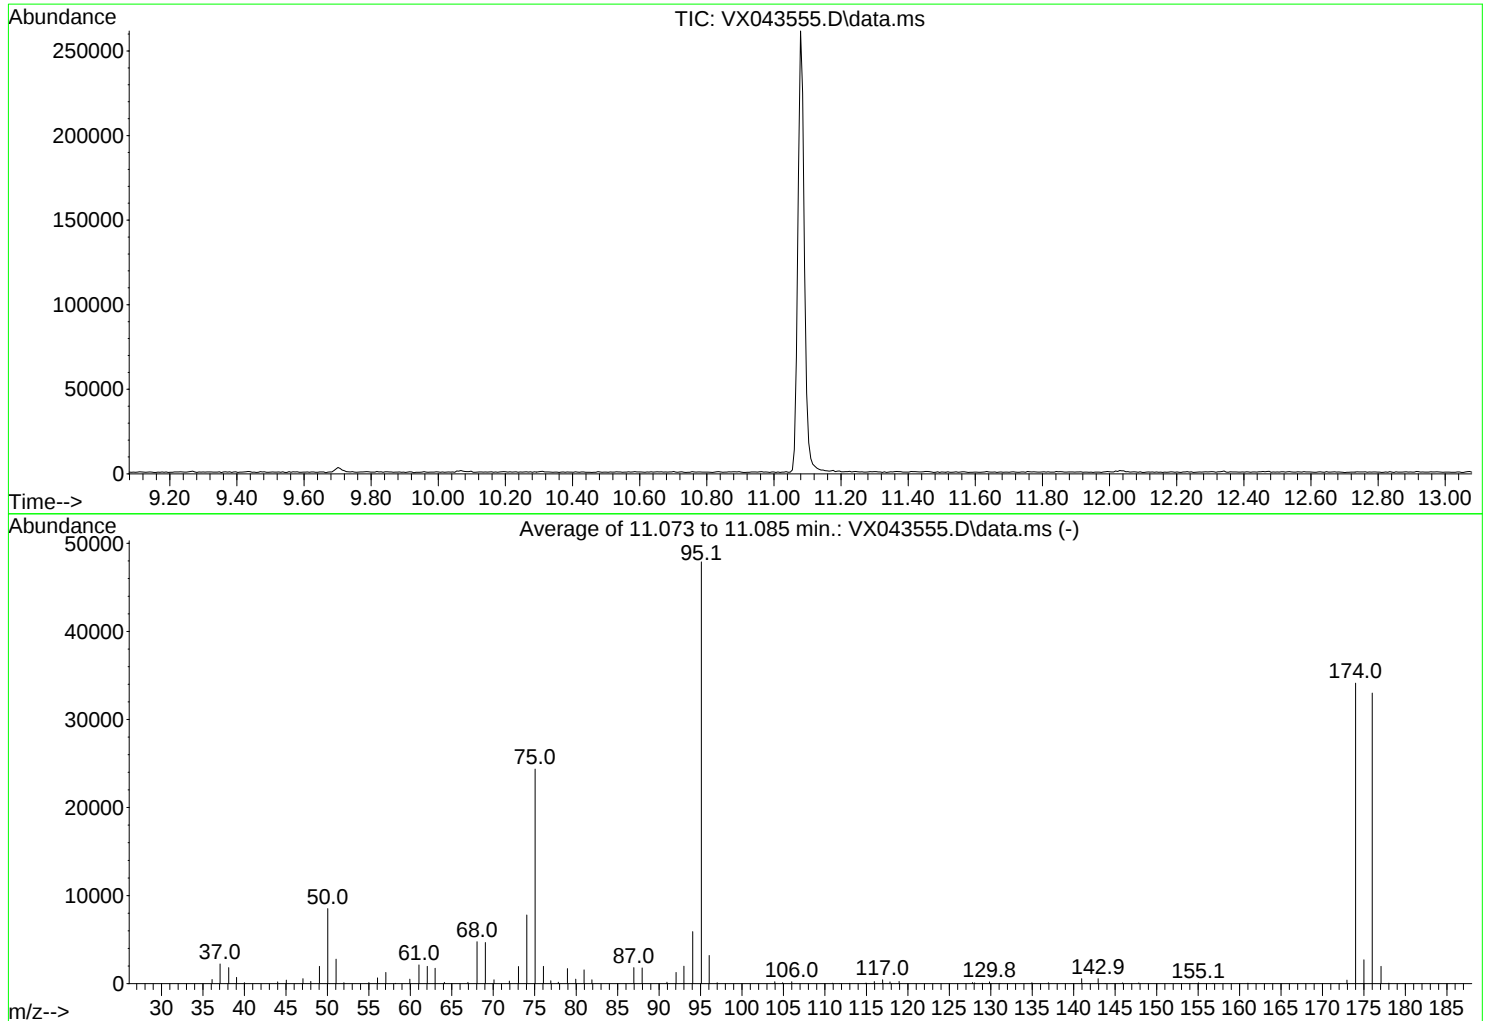

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	8521	PASS
75	95	30	60	50.9	24360	PASS
95	95	100	100	100.0	47901	PASS
96	95	5	9	6.7	3204	PASS
173	174	0.00	2	1.2	395	PASS
174	95	50	100	71.2	34123	PASS
175	174	5	9	7.9	2705	PASS
176	174	95	101	96.7	32992	PASS
177	176	5	9	6.0	1964	PASS