

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025015.D
 Acq On : 29 Oct 2021 10:40
 Operator : JC/MD
 Sample : VX1029WBL03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK621

Quant Time: Oct 30 01:07:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 30 01:06:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	174141	50.000	ug/L	# 0.00
28) Chlorobenzene-d5	10.055	117	158205	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	70164	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	44179	39.799	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	79.600%		
7) Chloroethane-d5	1.666	69	34104	44.947	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	89.900%		
11) 1,1-Dichloroethene-d2	2.306	63	88415	32.323	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	64.640%		
21) 2-Butanone-d5	4.465	46	103613	93.449	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	93.450%		
24) Chloroform-d	5.062	84	127398	43.861	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.720%		
26) 1,2-Dichloroethane-d4	5.958	65	96474	45.293	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.580%		
32) Benzene-d6	5.983	84	205045	45.663	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.320%		
36) 1,2-Dichloropropane-d6	7.312	67	70369	45.984	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.960%		
41) Toluene-d8	8.653	98	194208	45.206	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.420%		
43) trans-1,3-Dichloroprop...	8.952	79	39657	45.094	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.180%		
47) 2-Hexanone-d5	9.384	63	73875	94.816	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	94.820%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	96761	46.760	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.520%		
66) 1,2-Dichlorobenzene-d4	12.323	152	64666	47.496	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.000%		
Target Compounds						Qvalue
37) 1,2-Dichloropropane	7.312	63	8925	6.405	ug/L	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025015.D
Acq On : 29 Oct 2021 10:40
Operator : JC/MD
Sample : VX1029WBL03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK621

Quant Time: Oct 30 01:07:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 30 01:06:24 2021
Response via : Initial Calibration

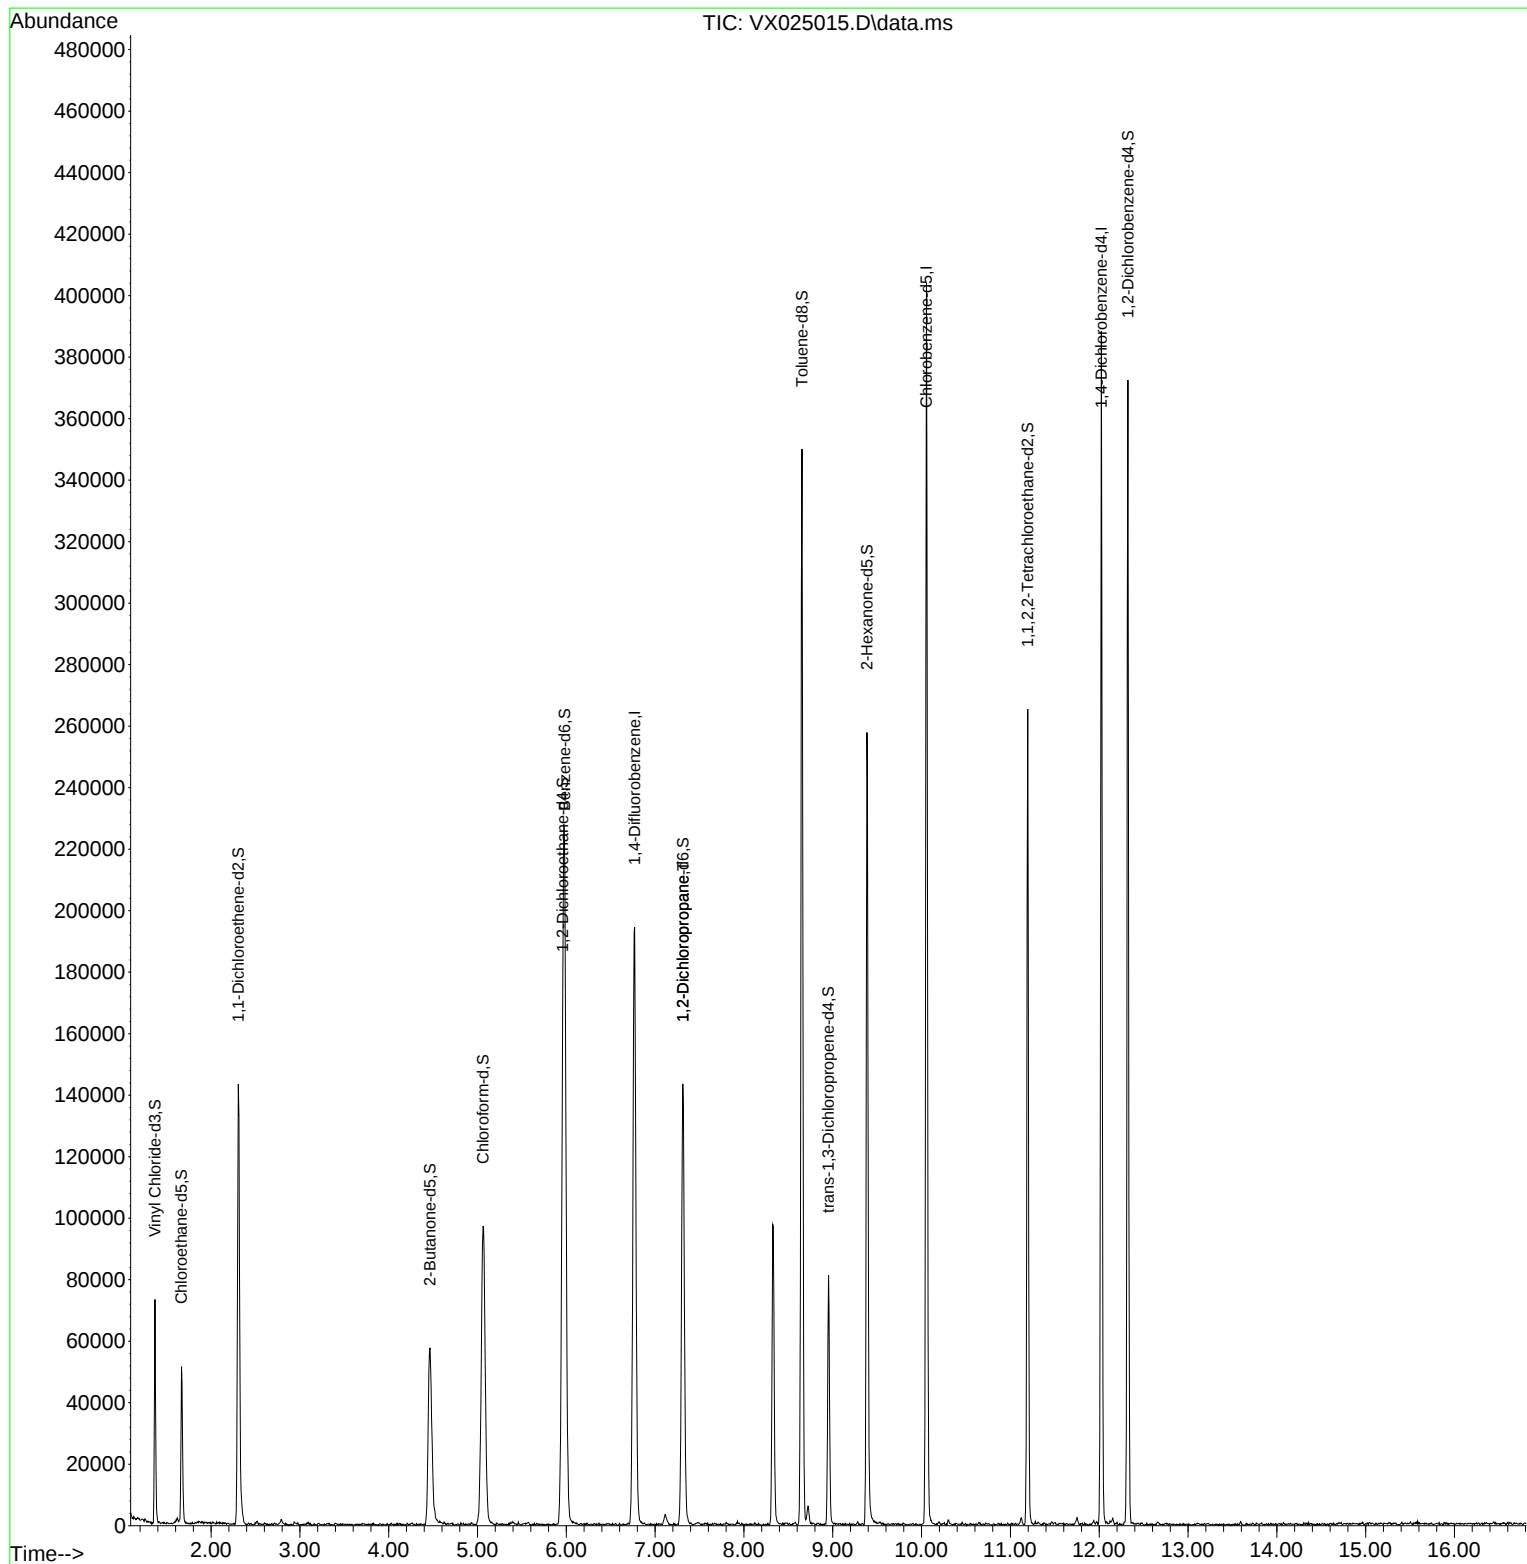

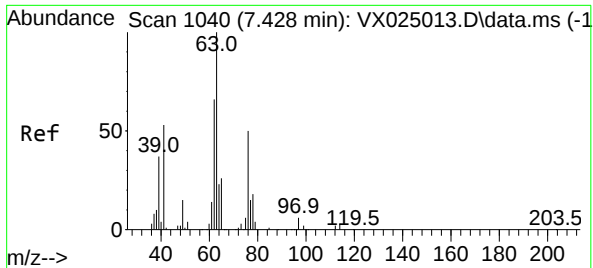

#37
 1,2-Dichloropropane
 Concen: 6.405 ug/L
 RT: 7.312 min Scan# 1021
 Delta R.T. -0.116 min
 Lab File: VX025015.D
 Acq: 29 Oct 2021 10:40

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK621

Tgt Ion: 63 Resp: 8925
 Ion Ratio Lower Upper
 63 100
 112 1.1 4.0 6.0#

