

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025018.D
 Acq On : 29 Oct 2021 11:50
 Operator : JC/MD
 Sample : VX1029MBL03
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK624

Quant Time: Oct 30 01:08:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 30 01:06:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	162548	50.000	ug/L	# 0.00
28) Chlorobenzene-d5	10.055	117	146357	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	64049	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	43970	42.436	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.880%
7) Chloroethane-d5	1.672	69	33643	47.501	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.000%
11) 1,1-Dichloroethene-d2	2.306	63	86057	33.705	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.400%
21) 2-Butanone-d5	4.464	46	103516	100.020	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.020%
24) Chloroform-d	5.068	84	127555	47.048	ug/L	0.01
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.100%
26) 1,2-Dichloroethane-d4	5.964	65	94457	47.509	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.020%
32) Benzene-d6	5.982	84	202180	48.669	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.340%
36) 1,2-Dichloropropane-d6	7.317	67	69175	48.863	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.720%
41) Toluene-d8	8.653	98	188570	47.447	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.900%
43) trans-1,3-Dichloroprop...	8.951	79	39587	48.658	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.320%
47) 2-Hexanone-d5	9.384	63	73402	101.836	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	101.840%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	97206	50.777	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.560%
66) 1,2-Dichlorobenzene-d4	12.323	152	61969	49.861	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.720%
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.312	96	718	0.710	ug/L	# 1
61) 1,2,3-Trichloropropane	12.024	75	8088	5.184	ug/L	# 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025018.D
Acq On : 29 Oct 2021 11:50
Operator : JC/MD
Sample : VX1029MBL03
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK624

Quant Time: Oct 30 01:08:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 30 01:06:24 2021
Response via : Initial Calibration

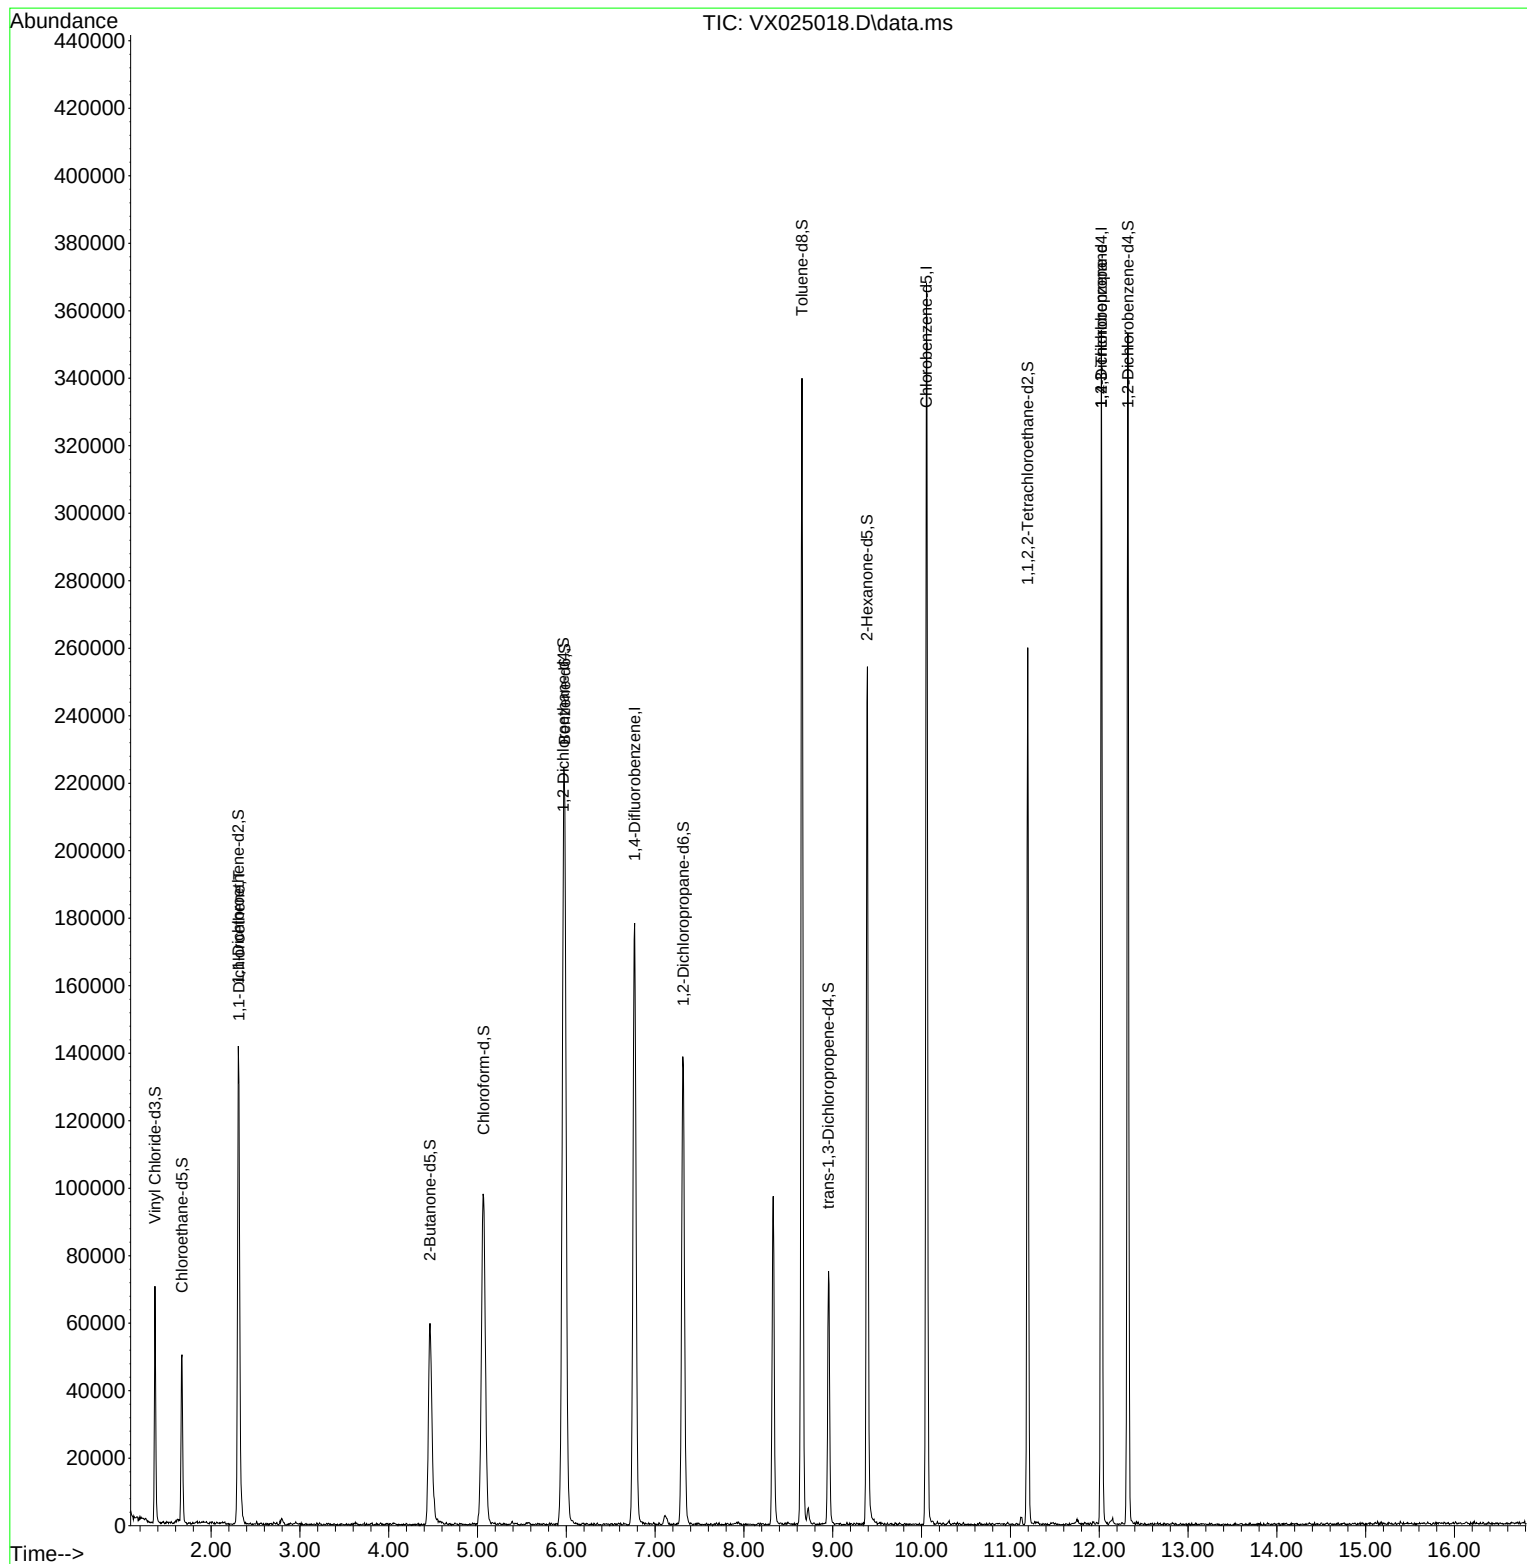

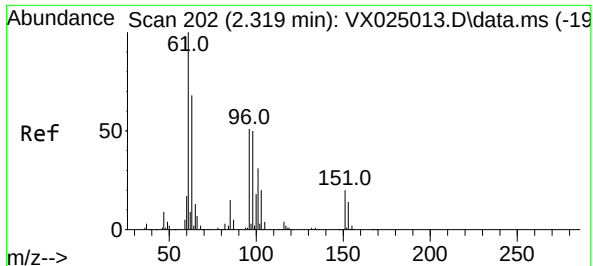

#12

1,1-Dichloroethene

Concen: 0.710 ug/L

RT: 2.312 min Scan# 201

Delta R.T. -0.007 min





Lab File: VX025018.D

Acq: 29 Oct 2021 11:50

Tgt Ion: 96 Resp: 718

Ion	Ratio	Lower	Upper
96	100		
61	1436.4	109.9	204.1#
63	10675.7	92.4	171.6#

Instrument :
MSVOA_X
ClientSampleId :
VBLK624

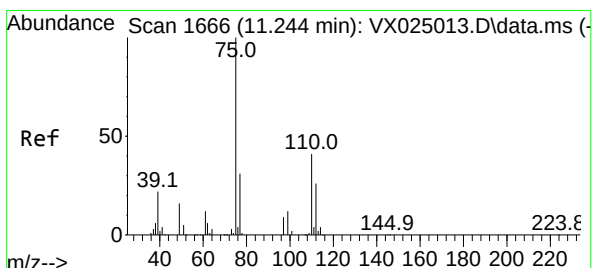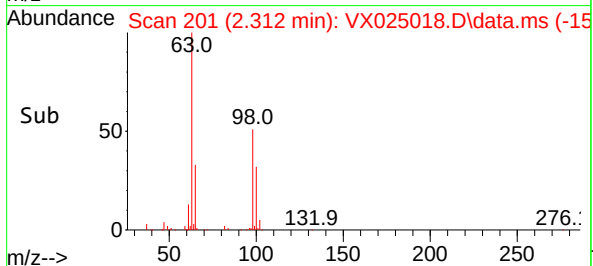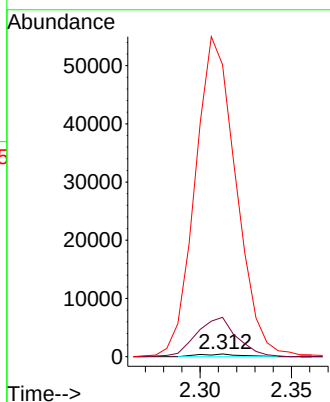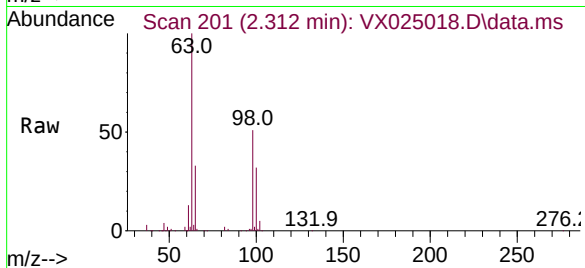

#61

1,2,3-Trichloropropane

Concen: 5.184 ug/L

RT: 12.024 min Scan# 1794

Delta R.T. 0.780 min

Lab File: VX025018.D

Acq: 29 Oct 2021 11:50

Tgt Ion: 75 Resp: 8088

Ion	Ratio	Lower	Upper
75	100		
77	39.2	26.6	39.8
110	4.0	37.2	55.8#

