

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025020.D
 Acq On : 29 Oct 2021 12:36
 Operator : JC/MD
 Sample : VX1029MBL05
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK626

Quant Time: Oct 30 01:08:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 30 01:06:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	166542	50.000	ug/L	# 0.00
28) Chlorobenzene-d5	10.055	117	147850	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	64861	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	43328	40.813	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.620%		
7) Chloroethane-d5	1.666	69	32506	44.795	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	89.600%		
11) 1,1-Dichloroethene-d2	2.307	63	85530	32.695	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.380%		
21) 2-Butanone-d5	4.465	46	102254	96.431	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.430%		
24) Chloroform-d	5.062	84	128105	46.117	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.240%		
26) 1,2-Dichloroethane-d4	5.964	65	97808	48.015	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.020%		
32) Benzene-d6	5.983	84	203183	48.417	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.840%		
36) 1,2-Dichloropropane-d6	7.312	67	71232	49.808	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	99.620%		
41) Toluene-d8	8.653	98	189823	47.280	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.560%		
43) trans-1,3-Dichloroprop...	8.952	79	38176	46.450	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.900%		
47) 2-Hexanone-d5	9.391	63	73681	101.190	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	101.190%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	95471	49.368	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.740%		
66) 1,2-Dichlorobenzene-d4	12.323	152	64191	51.002	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.000%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	8.324	75	2512	1.187	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025020.D
Acq On : 29 Oct 2021 12:36
Operator : JC/MD
Sample : VX1029MBL05
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK626

Quant Time: Oct 30 01:08:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 30 01:06:24 2021
Response via : Initial Calibration

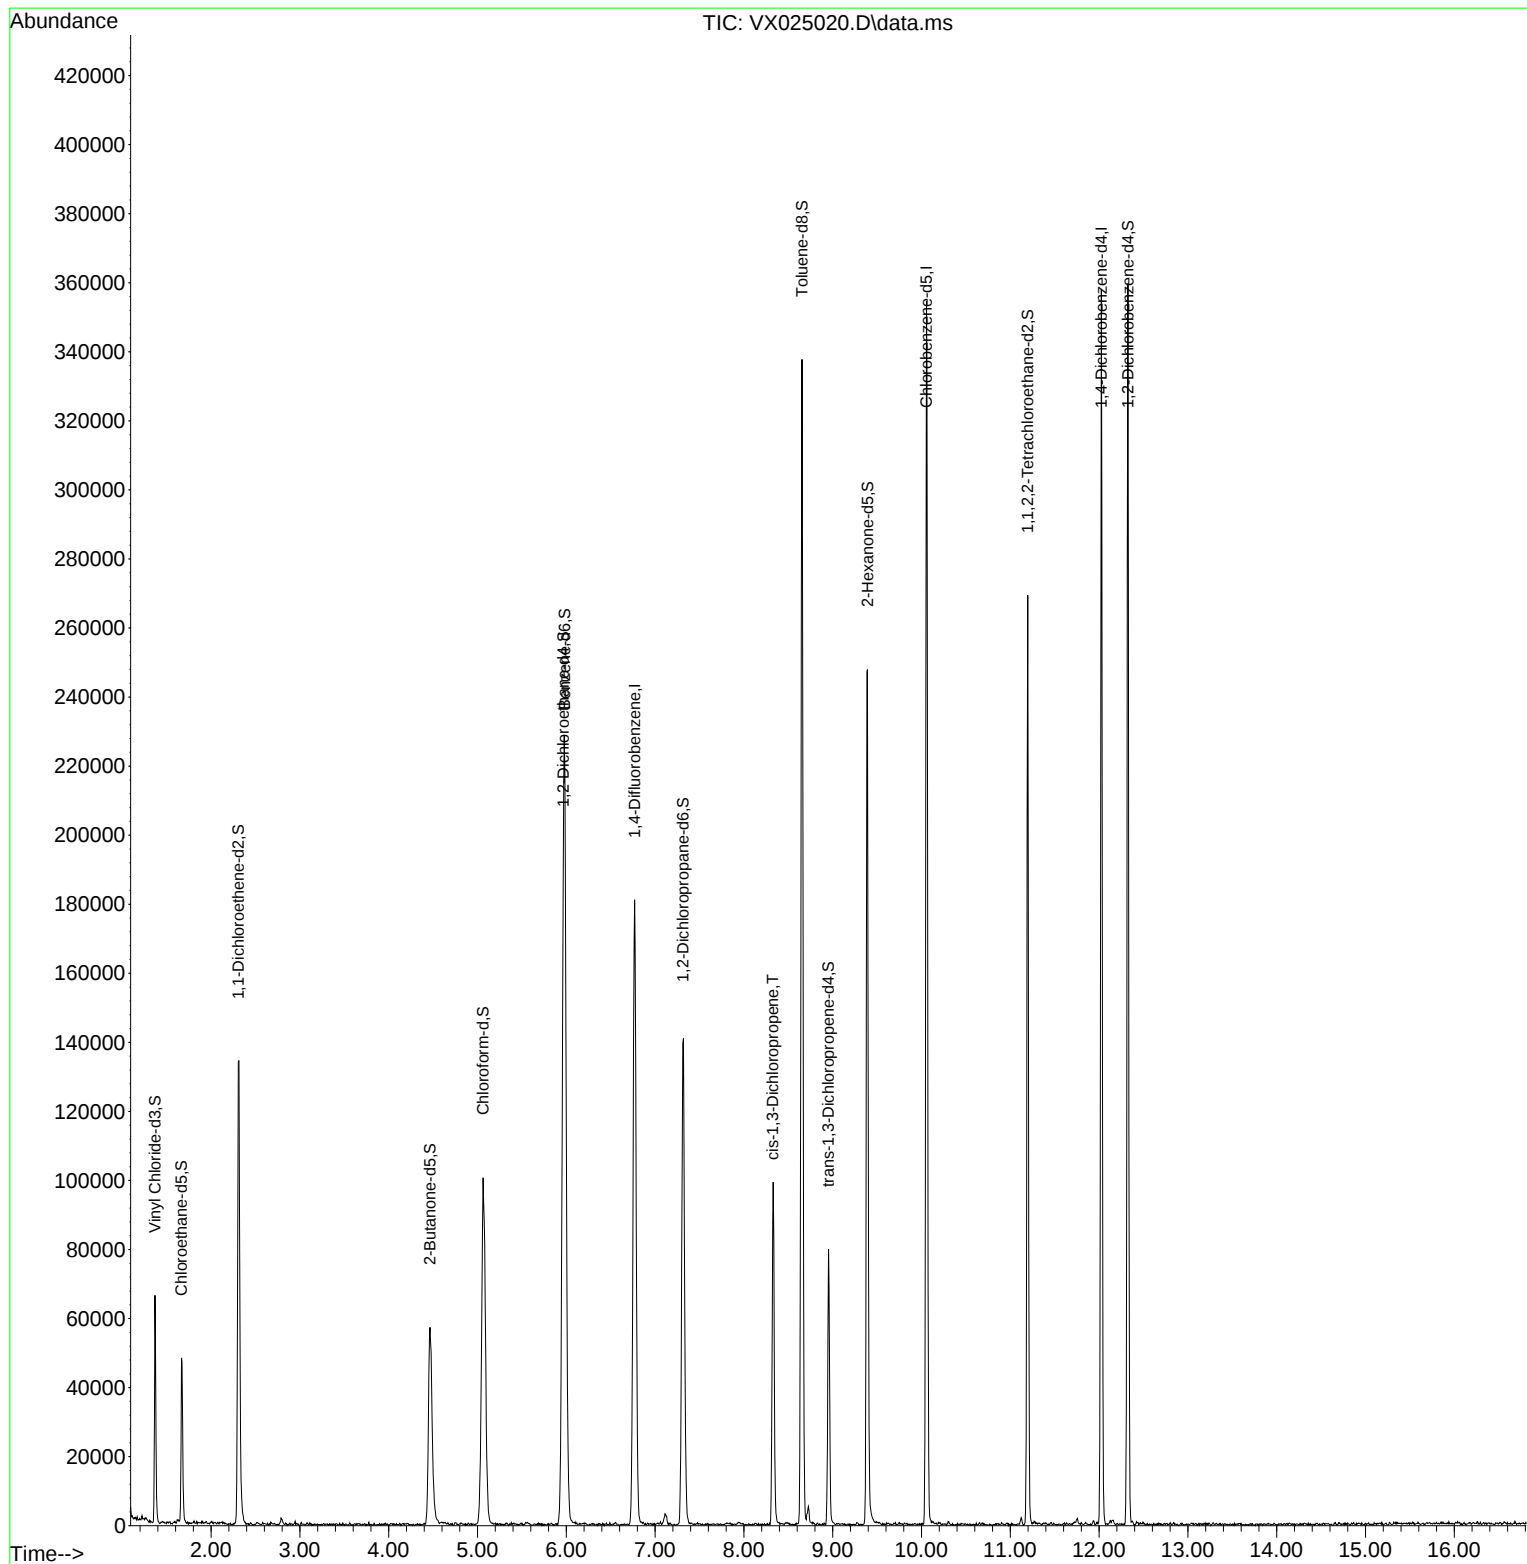

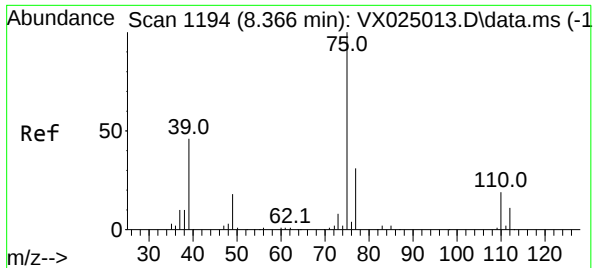

#39
 cis-1,3-Dichloropropene
 Concen: 1.187 ug/L
 RT: 8.324 min Scan# 1187
 Delta R.T. -0.043 min
 Lab File: VX025020.D
 Acq: 29 Oct 2021 12:36

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK626

Tgt Ion: 75 Resp: 2512
 Ion Ratio Lower Upper
 75 100
 77 34.1 23.1 42.9

