

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025014.D
 Acq On : 29 Oct 2021 10:17
 Operator : JC/MD
 Sample : VX1029WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK620

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

Signal : TIC: VX025014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	52	rVB	76523	75465	10.56%	1.356%
2	1.538	70	74	76	rBV2	979	949	0.13%	0.017%
3	1.666	91	95	102	rVB	53247	65807	9.21%	1.182%
4	1.794	114	116	119	rVB2	842	774	0.11%	0.014%
5	1.922	136	137	139	rVB2	953	561	0.08%	0.010%
6	2.306	192	200	212	rBV	144603	239569	33.53%	4.304%
7	2.508	229	233	234	rVV3	1264	1432	0.20%	0.026%
8	2.788	273	279	285	rBV7	2149	4198	0.59%	0.075%
9	2.947	303	305	309	rVB2	607	596	0.08%	0.011%
10	3.056	319	323	325	rBV2	495	491	0.07%	0.009%
11	3.093	327	329	332	rVB	1119	913	0.13%	0.016%
12	3.123	332	334	338	rVB	729	750	0.10%	0.013%
13	3.227	349	351	355	rBV2	458	649	0.09%	0.012%
14	3.373	373	375	378	rVB2	993	786	0.11%	0.014%
15	3.434	381	385	386	rVV	497	508	0.07%	0.009%
16	3.788	442	443	447	rVV2	408	542	0.08%	0.010%
17	3.843	450	452	455	rVB2	683	505	0.07%	0.009%
18	3.885	455	459	460	rBV2	441	516	0.07%	0.009%
19	4.276	521	523	526	rVB2	638	584	0.08%	0.010%
20	4.312	526	529	532	rBV	505	690	0.10%	0.012%
21	4.458	544	553	564	rBV2	54683	165472	23.16%	2.973%
22	4.641	581	583	586	rVB3	761	755	0.11%	0.014%
23	4.903	624	626	630	rBV3	719	667	0.09%	0.012%
24	4.946	630	633	636	rVB	583	645	0.09%	0.012%
25	5.062	636	652	670	rBV2	103406	319253	44.68%	5.736%
26	5.233	679	680	685	rBV3	643	672	0.09%	0.012%
27	5.611	739	742	746	rBV	365	563	0.08%	0.010%
28	5.733	759	762	767	rVB3	786	1071	0.15%	0.019%
29	5.970	787	801	815	rBV2	237686	714566	100.00%	12.838%
30	6.293	853	854	857	rBV2	718	580	0.08%	0.010%
31	6.519	889	891	893	rVV2	640	575	0.08%	0.010%
32	6.763	921	931	942	rBV	199998	470925	65.90%	8.461%
33	7.025	972	974	979	rVB	638	833	0.12%	0.015%
34	7.110	979	988	995	rBV6	3252	8804	1.23%	0.158%
35	7.312	1012	1021	1030	rVV2	147117	324256	45.38%	5.826%
36	7.409	1035	1037	1039	rVB2	648	499	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025014.D
 Acq On : 29 Oct 2021 10:17
 Operator : JC/MD
 Sample : VX1029WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK620

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

37	7.799	1098	1101	1103	rBV2	709	669	0.09%	0.012%
38	7.879	1113	1114	1117	rVB2	778	666	0.09%	0.012%
39	7.909	1117	1119	1120	rBV2	688	609	0.09%	0.011%
40	8.141	1155	1157	1160	rBV	366	548	0.08%	0.010%
41	8.324	1181	1187	1200	rVV	107276	175832	24.61%	3.159%
42	8.653	1233	1241	1248	rBV	336874	543656	76.08%	9.768%
43	8.726	1250	1253	1260	rVB2	6308	8673	1.21%	0.156%
44	8.952	1284	1290	1298	rBV	84757	124018	17.36%	2.228%
45	9.116	1314	1317	1319	rBV3	485	487	0.07%	0.009%
46	9.183	1326	1328	1331	rVB2	754	727	0.10%	0.013%
47	9.226	1331	1335	1337	rVB2	637	648	0.09%	0.012%
48	9.256	1337	1340	1343	rBV	844	1173	0.16%	0.021%
49	9.384	1356	1361	1374	rVV	264120	373664	52.29%	6.713%
50	9.519	1381	1383	1384	rBV	781	649	0.09%	0.012%
51	9.634	1400	1402	1404	rVB2	856	599	0.08%	0.011%
52	9.677	1404	1409	1411	rBV3	477	792	0.11%	0.014%
53	9.848	1435	1437	1440	rBV2	645	690	0.10%	0.012%
54	10.055	1465	1471	1480	rBV	393310	545262	76.31%	9.796%
55	10.195	1492	1494	1498	rVB	968	1091	0.15%	0.020%
56	10.305	1509	1512	1517	rVV2	1445	2139	0.30%	0.038%
57	10.348	1517	1519	1522	rVB	801	690	0.10%	0.012%
58	10.378	1522	1524	1526	rBV2	461	501	0.07%	0.009%
59	10.872	1602	1605	1611	rVV2	518	719	0.10%	0.013%
60	10.963	1618	1620	1625	rVB2	796	948	0.13%	0.017%
61	11.024	1628	1630	1632	rBV	656	702	0.10%	0.013%
62	11.098	1636	1642	1643	rBV	573	1102	0.15%	0.020%
63	11.122	1643	1646	1649	rVB3	2747	3233	0.45%	0.058%
64	11.195	1652	1658	1669	rBV	266028	341994	47.86%	6.144%
65	11.451	1696	1700	1702	rBV2	1187	1208	0.17%	0.022%
66	11.475	1702	1704	1709	rVV3	1140	1689	0.24%	0.030%
67	11.549	1712	1716	1719	rVV3	606	819	0.11%	0.015%
68	11.634	1723	1730	1732	rVB	730	1260	0.18%	0.023%
69	11.677	1732	1737	1740	rBV2	598	1019	0.14%	0.018%
70	11.750	1740	1749	1753	rBV4	3335	5788	0.81%	0.104%
71	11.933	1776	1779	1783	rBV4	1519	1904	0.27%	0.034%
72	12.024	1788	1794	1807	rVV	403462	506883	70.94%	9.107%
73	12.122	1807	1810	1812	rVV3	1278	1513	0.21%	0.027%
74	12.152	1812	1815	1821	rVB3	2192	3237	0.45%	0.058%
75	12.323	1837	1843	1850	rBV	389163	476755	66.72%	8.566%
76	12.433	1858	1861	1866	rVB	795	1394	0.20%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025014.D
 Acq On : 29 Oct 2021 10:17
 Operator : JC/MD
 Sample : VX1029WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK620

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

77	12.542	1876	1879	1882	rVB2	657	868	0.12%	0.016%
78	12.695	1902	1904	1907	rBV	510	559	0.08%	0.010%
79	12.896	1935	1937	1942	rBV	593	650	0.09%	0.012%
80	12.957	1943	1947	1949	rBV	671	765	0.11%	0.014%
81	13.189	1983	1985	1989	rBV	488	575	0.08%	0.010%
82	13.548	2042	2044	2046	rBV2	683	605	0.08%	0.011%
83	13.591	2048	2051	2055	rVB3	2615	3015	0.42%	0.054%
84	13.774	2074	2081	2084	rBV3	1261	2617	0.37%	0.047%
85	13.963	2109	2112	2118	rVV4	1932	2396	0.34%	0.043%
86	14.036	2120	2124	2128	rVB	713	1032	0.14%	0.019%
87	14.268	2159	2162	2164	rBV3	459	538	0.08%	0.010%
88	14.457	2190	2193	2195	rBV	432	527	0.07%	0.009%
89	14.585	2212	2214	2216	rBV3	566	507	0.07%	0.009%
90	14.755	2240	2242	2244	rBV	665	686	0.10%	0.012%
91	15.036	2287	2288	2291	rVB	826	642	0.09%	0.012%
92	15.066	2291	2293	2295	rBV	692	740	0.10%	0.013%
93	15.103	2297	2299	2301	rVB	833	621	0.09%	0.011%
94	15.133	2301	2304	2307	rBV	894	1319	0.18%	0.024%
95	15.322	2332	2335	2337	rBV	693	744	0.10%	0.013%
96	15.658	2386	2390	2392	rBV2	642	814	0.11%	0.015%
97	15.877	2424	2426	2428	rBV3	948	741	0.10%	0.013%
98	15.987	2442	2444	2449	rBV3	545	828	0.12%	0.015%
99	16.219	2479	2482	2484	rBV	680	868	0.12%	0.016%
100	16.517	2528	2531	2534	rBV3	626	878	0.12%	0.016%




Sum of corrected areas: 5565906

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025014.D
Acq On : 29 Oct 2021 10:17
Operator : JC/MD
Sample : VX1029WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK620

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

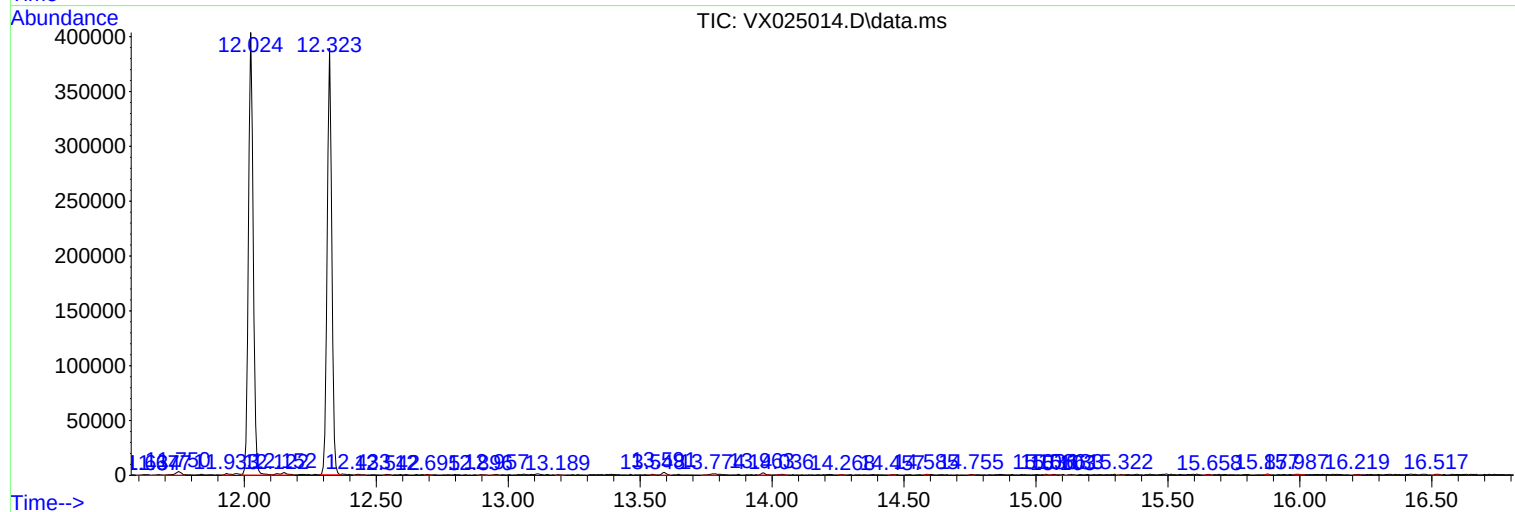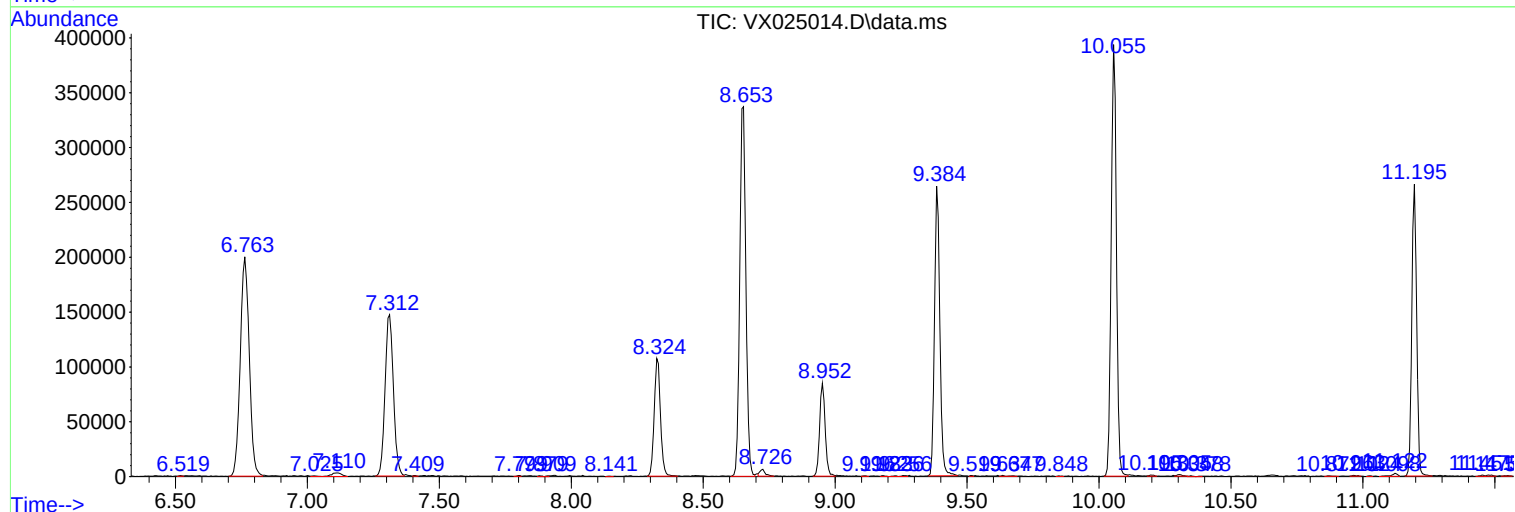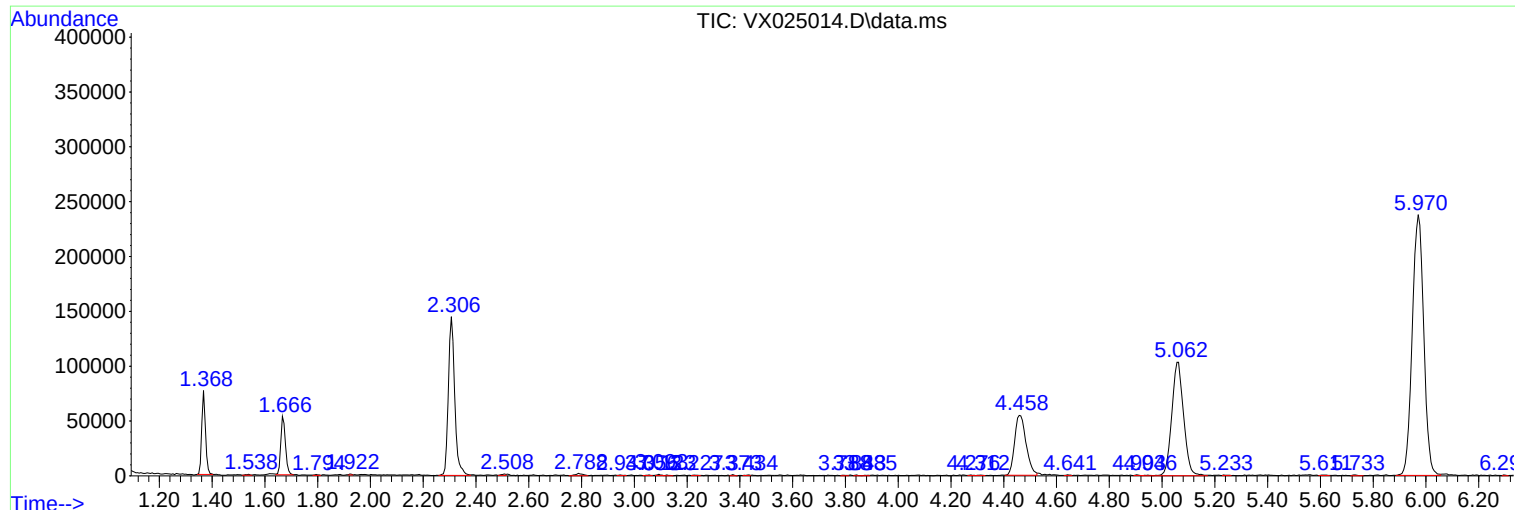

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025014.D
Acq On : 29 Oct 2021 10:17
Operator : JC/MD
Sample : VX1029WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK620

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025014.D
Acq On : 29 Oct 2021 10:17
Operator : JC/MD
Sample : VX1029WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK620

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
