

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025015.D
 Acq On : 29 Oct 2021 10:40
 Operator : JC/MD
 Sample : VX1029WBL03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK621

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

Signal : TIC: VX025015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	52	rBV	72862	71273	10.35%	1.334%
2	1.666	91	95	102	rVB	50812	64312	9.34%	1.204%
3	2.306	194	200	215	rVB	143359	236532	34.36%	4.427%
4	2.495	229	231	232	rBV	710	430	0.06%	0.008%
5	2.709	264	266	269	rBV	701	824	0.12%	0.015%
6	2.934	301	303	308	rBV2	854	1123	0.16%	0.021%
7	3.215	345	349	352	rBV	596	961	0.14%	0.018%
8	3.355	370	372	373	rBV	349	309	0.04%	0.006%
9	3.398	376	379	385	rVV3	649	1182	0.17%	0.022%
10	3.459	388	389	391	rBV2	466	264	0.04%	0.005%
11	3.483	391	393	396	rBV2	495	465	0.07%	0.009%
12	3.562	403	406	407	rBV	314	250	0.04%	0.005%
13	3.934	465	467	469	rBV	487	491	0.07%	0.009%
14	4.160	503	504	505	rBV	352	153	0.02%	0.003%
15	4.312	527	529	530	rBV	611	311	0.05%	0.006%
16	4.465	545	554	570	rBV	57544	170670	24.79%	3.194%
17	4.812	609	611	612	rBV	719	395	0.06%	0.007%
18	4.867	619	620	622	rBV	386	277	0.04%	0.005%
19	5.062	640	652	666	rBV2	97150	303921	44.15%	5.688%
20	5.214	676	677	681	rBV2	627	663	0.10%	0.012%
21	5.367	700	702	703	rBV	861	627	0.09%	0.012%
22	5.458	715	717	719	rBV	959	621	0.09%	0.012%
23	5.538	723	730	731	rBV3	630	1291	0.19%	0.024%
24	5.641	745	747	748	rBV2	649	389	0.06%	0.007%
25	5.666	750	751	753	rBV2	471	339	0.05%	0.006%
26	5.970	790	801	817	rBV2	227726	688357	100.00%	12.884%
27	6.519	889	891	893	rVB2	529	288	0.04%	0.005%
28	6.598	901	904	907	rVB	686	563	0.08%	0.011%
29	6.769	922	932	944	rBV	194213	462603	67.20%	8.658%
30	6.946	960	961	962	rBV	538	303	0.04%	0.006%
31	7.013	971	972	974	rBV	609	424	0.06%	0.008%
32	7.110	983	988	996	rBV6	3360	7504	1.09%	0.140%
33	7.208	1002	1004	1005	rBV	495	227	0.03%	0.004%
34	7.312	1013	1021	1034	rBV2	143215	316052	45.91%	5.915%
35	7.592	1066	1067	1068	rVB2	626	229	0.03%	0.004%
36	7.732	1089	1090	1094	rVB	682	560	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025015.D
 Acq On : 29 Oct 2021 10:40
 Operator : JC/MD
 Sample : VX1029WBL03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK621

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
 Title : VOC Analysis

37	7.769	1094	1096	1097	rBV	582	505	0.07%	0.009%
38	8.013	1134	1136	1138	rBV	524	611	0.09%	0.011%
39	8.147	1157	1158	1159	rBV	303	203	0.03%	0.004%
40	8.220	1167	1170	1173	rBV	520	554	0.08%	0.010%
41	8.244	1173	1174	1176	rBV	400	308	0.04%	0.006%
42	8.269	1176	1178	1181	rVB2	643	466	0.07%	0.009%
43	8.324	1181	1187	1199	rBV	97815	169810	24.67%	3.178%
44	8.580	1223	1229	1232	rVB2	897	1492	0.22%	0.028%
45	8.653	1234	1241	1248	rBV	349635	530533	77.07%	9.930%
46	8.952	1285	1290	1300	rVB	81023	116941	16.99%	2.189%
47	9.384	1355	1361	1378	rBV	257706	377662	54.86%	7.069%
48	10.055	1466	1471	1487	rVB	403615	532592	77.37%	9.968%
49	10.305	1509	1512	1519	rVB3	1745	2736	0.40%	0.051%
50	10.512	1545	1546	1548	rBV3	492	374	0.05%	0.007%
51	10.695	1573	1576	1579	rVB2	402	437	0.06%	0.008%
52	10.720	1579	1580	1583	rBV2	697	745	0.11%	0.014%
53	10.817	1592	1596	1597	rBV	502	532	0.08%	0.010%
54	10.896	1607	1609	1610	rVB	513	210	0.03%	0.004%
55	11.195	1652	1658	1666	rBV	265239	334145	48.54%	6.254%
56	11.360	1683	1685	1686	rBV	411	229	0.03%	0.004%
57	12.024	1789	1794	1802	rVB	387636	476320	69.20%	8.915%
58	12.323	1838	1843	1849	rVB	371715	449462	65.29%	8.412%
59	12.518	1874	1875	1877	rBV	302	293	0.04%	0.005%
60	12.536	1877	1878	1880	rVB	613	260	0.04%	0.005%
61	12.792	1918	1920	1924	rBV2	561	780	0.11%	0.015%
62	12.908	1938	1939	1940	rBV	472	257	0.04%	0.005%
63	12.945	1943	1945	1947	rBV	494	334	0.05%	0.006%
64	13.353	2011	2012	2015	rBV2	415	411	0.06%	0.008%
65	13.402	2019	2020	2022	rVB	441	259	0.04%	0.005%
66	13.432	2022	2025	2027	rBV	251	313	0.05%	0.006%
67	13.560	2045	2046	2049	rBV	480	313	0.05%	0.006%
68	13.658	2059	2062	2063	rBV	663	598	0.09%	0.011%
69	13.768	2079	2080	2081	rBV	554	290	0.04%	0.005%
70	14.073	2128	2130	2133	rBV2	775	747	0.11%	0.014%
71	14.304	2166	2168	2171	rBV3	818	711	0.10%	0.013%
72	14.329	2171	2172	2175	rVB3	632	564	0.08%	0.011%
73	14.359	2175	2177	2178	rBV	747	336	0.05%	0.006%
74	14.536	2204	2206	2209	rVB	612	590	0.09%	0.011%
75	14.603	2214	2217	2219	rBV2	718	1044	0.15%	0.020%
76	14.640	2222	2223	2227	rVB2	572	375	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025015.D
Acq On : 29 Oct 2021 10:40
Operator : JC/MD
Sample : VX1029WBL03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK621

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Title : VOC Analysis

77	15.115	2299	2301	2304	rBV	613	492	0.07%	0.009%
78	15.883	2425	2427	2429	rBV2	927	921	0.13%	0.017%
79	16.603	2541	2545	2546	rBV2	843	938	0.14%	0.018%


Sum of corrected areas: 5342876

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025015.D
Acq On : 29 Oct 2021 10:40
Operator : JC/MD
Sample : VX1029WBL03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

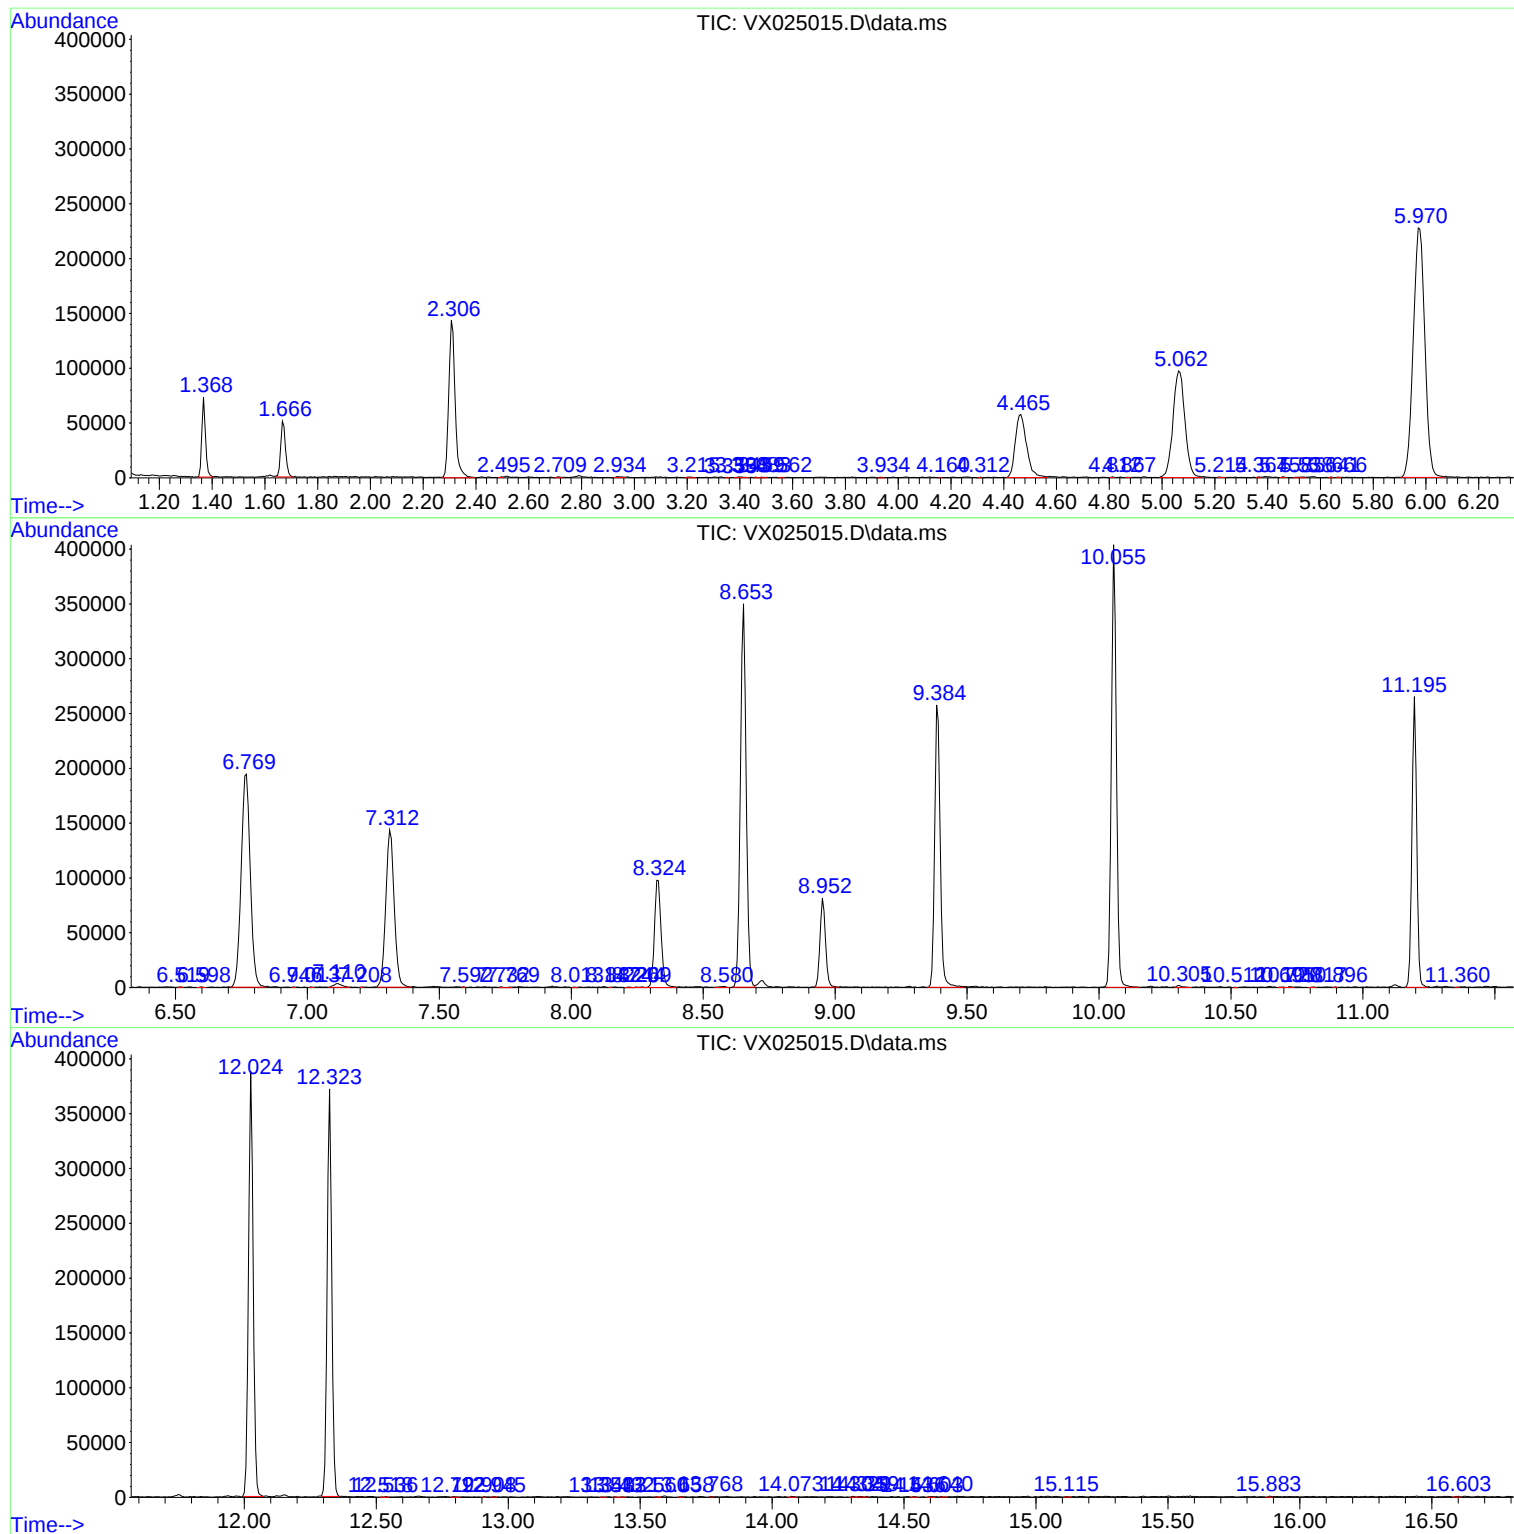

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025015.D
Acq On : 29 Oct 2021 10:40
Operator : JC/MD
Sample : VX1029WBL03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025015.D
Acq On : 29 Oct 2021 10:40
Operator : JC/MD
Sample : VX1029WBL03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
