

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025016.D
 Acq On : 29 Oct 2021 11:03
 Operator : JC/MD
 Sample : VX1029WBL04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK622

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M

Title : VOC Analysis

Signal : TIC: VX025016.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	74322	73567	10.55%	1.385%
2	1.514	68	70	71	rBV	733	472	0.07%	0.009%
3	1.599	79	84	85	rBV2	889	1371	0.20%	0.026%
4	1.666	91	95	102	rVB	52516	65356	9.37%	1.230%
5	1.782	109	114	116	rBV3	627	1175	0.17%	0.022%
6	2.306	194	200	214	rVB	143272	233429	33.48%	4.393%
7	2.514	231	234	238	rBV2	627	929	0.13%	0.017%
8	2.575	242	244	247	rBV2	570	545	0.08%	0.010%
9	2.629	251	253	255	rBV	578	592	0.08%	0.011%
10	2.709	262	266	267	rBV2	611	811	0.12%	0.015%
11	2.794	274	280	283	rBV3	2091	4316	0.62%	0.081%
12	2.904	296	298	300	rVV2	560	500	0.07%	0.009%
13	2.947	303	305	309	rVB	831	1050	0.15%	0.020%
14	3.093	327	329	333	rVV3	683	693	0.10%	0.013%
15	3.312	363	365	367	rBV	466	480	0.07%	0.009%
16	3.428	380	384	386	rBV	622	811	0.12%	0.015%
17	3.629	416	417	421	rBV	326	464	0.07%	0.009%
18	3.873	455	457	458	rBV	607	490	0.07%	0.009%
19	4.465	544	554	568	rBV	58210	169135	24.26%	3.183%
20	4.830	611	614	617	rVB	478	510	0.07%	0.010%
21	4.971	635	637	639	rVB2	894	535	0.08%	0.010%
22	5.068	639	653	668	rBV2	98967	310553	44.54%	5.845%
23	5.300	688	691	692	rBV2	595	492	0.07%	0.009%
24	5.379	699	704	706	rBV3	1181	1794	0.26%	0.034%
25	5.477	717	720	725	rBV3	812	1097	0.16%	0.021%
26	5.544	729	731	733	rBV	613	731	0.10%	0.014%
27	5.696	753	756	757	rBV2	439	473	0.07%	0.009%
28	5.794	768	772	774	rBV2	314	537	0.08%	0.010%
29	5.976	789	802	814	rBV2	231747	697249	100.00%	13.122%
30	6.269	848	850	854	rVB2	962	1028	0.15%	0.019%
31	6.367	863	866	868	rVB	776	728	0.10%	0.014%
32	6.428	874	876	880	rBV	640	1037	0.15%	0.020%
33	6.543	892	895	896	rBV2	852	703	0.10%	0.013%
34	6.635	907	910	914	rVV	603	943	0.14%	0.018%
35	6.769	922	932	945	rBV	181271	434957	62.38%	8.186%
36	7.019	971	973	976	rVB	621	606	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025016.D
 Acq On : 29 Oct 2021 11:03
 Operator : JC/MD
 Sample : VX1029WBL04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK622

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
 Title : VOC Analysis

37	7.116	983	989	995	rBV6	3217	7264	1.04%	0.137%
38	7.312	1011	1021	1032	rBV	147708	316823	45.44%	5.963%
39	7.488	1048	1050	1052	rVB	794	649	0.09%	0.012%
40	7.525	1052	1056	1057	rVB	573	584	0.08%	0.011%
41	7.543	1057	1059	1062	rVB	831	533	0.08%	0.010%
42	7.574	1062	1064	1065	rBV	873	489	0.07%	0.009%
43	7.738	1089	1091	1094	rVV	540	522	0.07%	0.010%
44	8.055	1141	1143	1145	rBV	697	636	0.09%	0.012%
45	8.171	1156	1162	1163	rBV2	763	1110	0.16%	0.021%
46	8.244	1170	1174	1175	rBV3	629	679	0.10%	0.013%
47	8.330	1180	1188	1199	rVV	103796	171640	24.62%	3.230%
48	8.433	1202	1205	1208	rBV	532	893	0.13%	0.017%
49	8.470	1209	1211	1213	rVV2	611	606	0.09%	0.011%
50	8.598	1230	1232	1234	rBV	767	721	0.10%	0.014%
51	8.653	1234	1241	1249	rBV	340224	530664	76.11%	9.987%
52	8.952	1284	1290	1302	rVB	78724	116164	16.66%	2.186%
53	9.092	1309	1313	1319	rVB3	659	1200	0.17%	0.023%
54	9.384	1354	1361	1373	rBV	256716	375756	53.89%	7.072%
55	9.695	1409	1412	1417	rVB4	659	1206	0.17%	0.023%
56	10.006	1460	1463	1465	rBV	641	739	0.11%	0.014%
57	10.055	1465	1471	1482	rBV	365159	498610	71.51%	9.384%
58	10.305	1509	1512	1515	rVB	1244	1180	0.17%	0.022%
59	10.427	1529	1532	1534	rBV	511	657	0.09%	0.012%
60	10.646	1566	1568	1570	rBV	940	892	0.13%	0.017%
61	10.787	1589	1591	1594	rVB	546	548	0.08%	0.010%
62	11.030	1630	1631	1635	rVB2	590	469	0.07%	0.009%
63	11.097	1635	1642	1643	rBV2	465	993	0.14%	0.019%
64	11.122	1643	1646	1650	rVB2	2543	3498	0.50%	0.066%
65	11.195	1652	1658	1668	rVB	261657	337749	48.44%	6.356%
66	11.366	1685	1686	1688	rBV	621	482	0.07%	0.009%
67	11.451	1698	1700	1702	rBV	384	504	0.07%	0.009%
68	11.543	1710	1715	1716	rBV	552	873	0.13%	0.016%
69	11.610	1723	1726	1729	rVB3	760	799	0.11%	0.015%
70	11.640	1729	1731	1734	rBV2	529	667	0.10%	0.013%
71	11.750	1744	1749	1753	rVV4	2440	4024	0.58%	0.076%
72	11.841	1762	1764	1768	rVV2	1112	973	0.14%	0.018%
73	11.933	1775	1779	1782	rBV2	1253	1684	0.24%	0.032%
74	12.024	1789	1794	1803	rBV	365742	445715	63.92%	8.388%
75	12.128	1807	1811	1813	rBV4	1630	2141	0.31%	0.040%
76	12.225	1824	1827	1828	rBV4	707	570	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025016.D
 Acq On : 29 Oct 2021 11:03
 Operator : JC/MD
 Sample : VX1029WBL04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK622

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

77	12.256	1828	1832	1835	rBV2	684	1004	0.14%	0.019%
78	12.323	1836	1843	1850	rBV	357513	454363	65.17%	8.551%
79	12.427	1857	1860	1862	rBV2	930	977	0.14%	0.018%
80	12.481	1865	1869	1870	rBV2	533	537	0.08%	0.010%
81	12.683	1901	1902	1906	rVB	1150	978	0.14%	0.018%
82	12.719	1906	1908	1910	rBV	560	644	0.09%	0.012%
83	13.439	2024	2026	2028	rVV2	479	451	0.06%	0.008%
84	13.469	2028	2031	2032	rVV2	617	571	0.08%	0.011%
85	13.585	2048	2050	2053	rBV	698	529	0.08%	0.010%
86	14.194	2148	2150	2154	rVB	504	482	0.07%	0.009%
87	14.231	2154	2156	2160	rVB	647	735	0.11%	0.014%
88	14.286	2160	2165	2168	rBV2	708	1123	0.16%	0.021%
89	14.414	2181	2186	2190	rBV2	627	1557	0.22%	0.029%
90	14.518	2200	2203	2206	rVB2	572	659	0.09%	0.012%
91	14.609	2215	2218	2220	rBV2	731	692	0.10%	0.013%
92	14.902	2263	2266	2269	rBV3	523	742	0.11%	0.014%
93	15.261	2323	2325	2326	rBV	859	485	0.07%	0.009%
94	15.280	2326	2328	2330	rVB2	748	579	0.08%	0.011%
95	15.798	2411	2413	2418	rBV3	488	735	0.11%	0.014%
96	15.847	2418	2421	2427	rBV4	754	1150	0.16%	0.022%
97	16.042	2450	2453	2456	rBV2	432	667	0.10%	0.013%
98	16.066	2456	2457	2460	rVB2	683	475	0.07%	0.009%
99	16.182	2474	2476	2479	rVB2	863	769	0.11%	0.014%
100	16.286	2491	2493	2496	rBV2	607	599	0.09%	0.011%




Sum of corrected areas: 5313568

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025016.D
Acq On : 29 Oct 2021 11:03
Operator : JC/MD
Sample : VX1029WBL04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK622

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

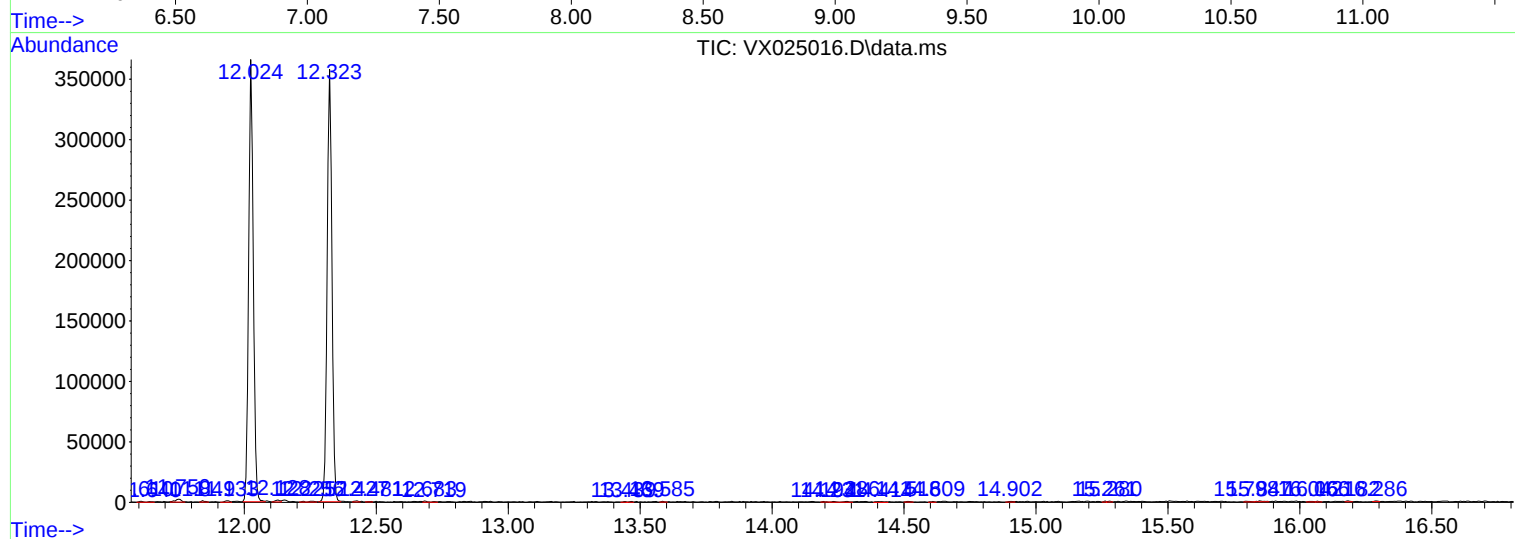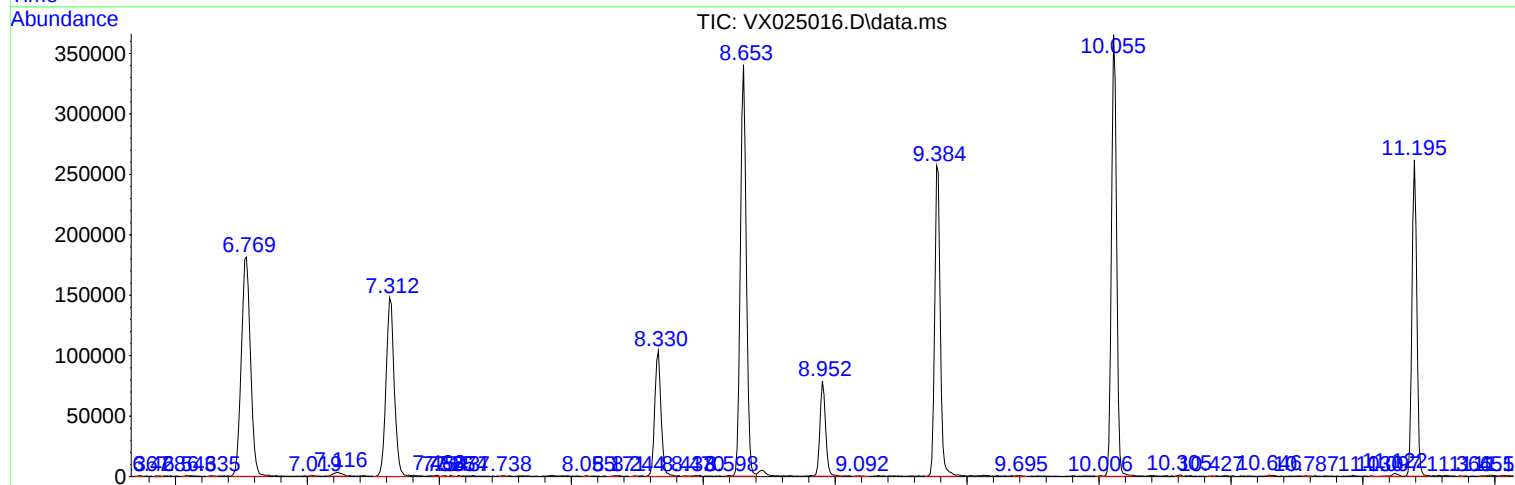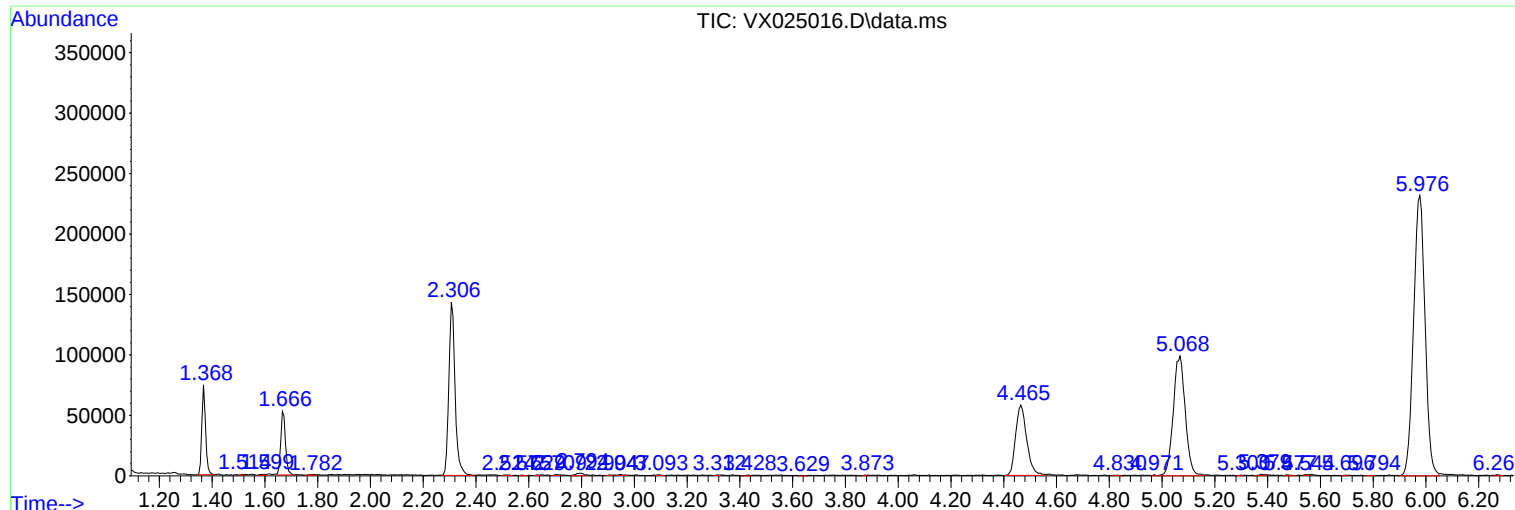

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025016.D
Acq On : 29 Oct 2021 11:03
Operator : JC/MD
Sample : VX1029WBL04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK622

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025016.D
Acq On : 29 Oct 2021 11:03
Operator : JC/MD
Sample : VX1029WBL04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK622

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
