

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025017.D
 Acq On : 29 Oct 2021 11:27
 Operator : JC/MD
 Sample : VX1029WBL05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK623

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M

Title : VOC Analysis

Signal : TIC: VX025017.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	55	rVB	71336	71925	10.66%	1.388%
2	1.666	92	95	105	rVB	49855	63299	9.38%	1.222%
3	2.306	194	200	213	rBV	138820	226515	33.56%	4.372%
4	2.556	239	241	243	rBV	466	458	0.07%	0.009%
5	2.770	274	276	277	rBV	629	417	0.06%	0.008%
6	2.928	301	302	304	rBV	508	363	0.05%	0.007%
7	3.007	312	315	318	rBV	508	687	0.10%	0.013%
8	3.178	341	343	344	rBV	361	348	0.05%	0.007%
9	3.331	366	368	371	rBV	580	628	0.09%	0.012%
10	3.526	398	400	401	rBV	426	224	0.03%	0.004%
11	3.812	445	447	450	rBV2	658	729	0.11%	0.014%
12	3.873	455	457	460	rVV	550	324	0.05%	0.006%
13	4.093	492	493	496	rBV	357	315	0.05%	0.006%
14	4.215	511	513	515	rBV	321	229	0.03%	0.004%
15	4.355	534	536	538	rBV	376	256	0.04%	0.005%
16	4.464	546	554	571	rBV	56805	165152	24.47%	3.188%
17	4.970	636	637	639	rBV	506	274	0.04%	0.005%
18	5.068	643	653	666	rVB	98472	295880	43.84%	5.711%
19	5.306	689	692	693	rBV	589	575	0.09%	0.011%
20	5.367	701	702	704	rBV	307	255	0.04%	0.005%
21	5.385	704	705	706	rBV	831	471	0.07%	0.009%
22	5.446	713	715	718	rBV	536	635	0.09%	0.012%
23	5.477	718	720	723	rVV2	469	406	0.06%	0.008%
24	5.781	769	770	772	rBV	339	321	0.05%	0.006%
25	5.873	784	785	787	rBV	391	303	0.04%	0.006%
26	5.976	791	802	816	rVV2	226799	674953	100.00%	13.029%
27	6.141	828	829	832	rBV	638	718	0.11%	0.014%
28	6.385	867	869	873	rBV2	597	488	0.07%	0.009%
29	6.562	897	898	900	rBV	290	234	0.03%	0.005%
30	6.629	908	909	912	rVB	571	535	0.08%	0.010%
31	6.665	912	915	918	rBV2	434	588	0.09%	0.011%
32	6.769	922	932	943	rBV	182518	435103	64.46%	8.399%
33	7.013	970	972	974	rBV	827	656	0.10%	0.013%
34	7.055	977	979	981	rVB	412	283	0.04%	0.005%
35	7.116	981	989	997	rBV6	3233	8035	1.19%	0.155%
36	7.312	1011	1021	1034	rBV	141137	313412	46.43%	6.050%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025017.D
 Acq On : 29 Oct 2021 11:27
 Operator : JC/MD
 Sample : VX1029WBL05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK623

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

37	7.653	1075	1077	1079	rBV2	381	412	0.06%	0.008%
38	7.677	1079	1081	1084	rVB	559	367	0.05%	0.007%
39	7.811	1101	1103	1107	rBV2	702	1000	0.15%	0.019%
40	7.842	1107	1108	1110	rVB2	658	339	0.05%	0.007%
41	7.872	1110	1113	1115	rBV	1132	947	0.14%	0.018%
42	7.933	1118	1123	1127	rBV2	1273	1928	0.29%	0.037%
43	8.208	1166	1168	1169	rBV	399	265	0.04%	0.005%
44	8.269	1177	1178	1180	rBV	283	259	0.04%	0.005%
45	8.330	1181	1188	1198	rVV	102183	165298	24.49%	3.191%
46	8.653	1234	1241	1248	rBV	334820	515920	76.44%	9.959%
47	8.769	1258	1260	1263	rBV	626	645	0.10%	0.012%
48	8.866	1274	1276	1277	rBV	372	303	0.04%	0.006%
49	8.951	1285	1290	1299	rBV	80170	115303	17.08%	2.226%
50	9.147	1320	1322	1323	rBV	471	270	0.04%	0.005%
51	9.275	1340	1343	1344	rBV2	439	394	0.06%	0.008%
52	9.390	1356	1362	1375	rBV	247776	365100	54.09%	7.047%
53	9.567	1389	1391	1394	rBV2	485	414	0.06%	0.008%
54	9.787	1424	1427	1428	rBV2	623	665	0.10%	0.013%
55	9.848	1435	1437	1438	rBV2	391	256	0.04%	0.005%
56	9.878	1440	1442	1445	rBV2	455	554	0.08%	0.011%
57	10.055	1466	1471	1479	rBV	368066	497614	73.73%	9.605%
58	10.183	1491	1492	1493	rBV	496	274	0.04%	0.005%
59	10.396	1523	1527	1533	rBV3	756	1341	0.20%	0.026%
60	10.518	1543	1547	1550	rBV	474	934	0.14%	0.018%
61	10.683	1573	1574	1575	rVB	679	248	0.04%	0.005%
62	10.695	1575	1576	1579	rBV	723	643	0.10%	0.012%
63	10.799	1592	1593	1594	rBV	466	242	0.04%	0.005%
64	10.896	1607	1609	1610	rVB	541	387	0.06%	0.007%
65	10.915	1610	1612	1614	rVB	624	403	0.06%	0.008%
66	11.073	1637	1638	1640	rBV	283	285	0.04%	0.006%
67	11.195	1653	1658	1666	rVB	266276	329387	48.80%	6.358%
68	11.384	1688	1689	1691	rBV	449	407	0.06%	0.008%
69	11.841	1762	1764	1767	rVB	596	642	0.10%	0.012%
70	12.024	1788	1794	1801	rBV	354916	453581	67.20%	8.755%
71	12.323	1838	1843	1856	rVB	348777	442855	65.61%	8.548%
72	12.487	1869	1870	1873	rVB	1064	646	0.10%	0.012%
73	12.664	1892	1899	1901	rBV3	939	1241	0.18%	0.024%
74	12.719	1905	1908	1910	rBV2	435	500	0.07%	0.010%
75	12.878	1932	1934	1935	rBV	487	392	0.06%	0.008%
76	13.170	1979	1982	1986	rVB	481	676	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025017.D
 Acq On : 29 Oct 2021 11:27
 Operator : JC/MD
 Sample : VX1029WBL05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK623

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

77	13.225	1988	1991	1994	rBV	569	665	0.10%	0.013%
78	13.256	1994	1996	1999	rVB	754	688	0.10%	0.013%
79	13.378	2014	2016	2017	rBV	344	298	0.04%	0.006%
80	13.591	2049	2051	2057	rBV2	510	843	0.12%	0.016%
81	13.676	2063	2065	2066	rBV	409	314	0.05%	0.006%
82	13.823	2088	2089	2091	rVB	736	347	0.05%	0.007%
83	13.853	2092	2094	2096	rVB	638	398	0.06%	0.008%
84	13.877	2096	2098	2099	rBV	347	235	0.03%	0.005%
85	13.932	2106	2107	2110	rVB2	366	298	0.04%	0.006%
86	13.969	2110	2113	2116	rBV2	645	720	0.11%	0.014%
87	14.018	2119	2121	2123	rBV	815	622	0.09%	0.012%
88	14.036	2123	2124	2128	rBV2	546	647	0.10%	0.012%
89	14.176	2146	2147	2150	rBV	269	267	0.04%	0.005%
90	14.201	2150	2151	2152	rBV	591	284	0.04%	0.005%
91	14.274	2162	2163	2165	rBV	677	351	0.05%	0.007%
92	14.310	2167	2169	2172	rVV2	733	673	0.10%	0.013%
93	14.365	2176	2178	2180	rBV2	376	404	0.06%	0.008%
94	14.426	2187	2188	2191	rBV	443	403	0.06%	0.008%
95	14.475	2194	2196	2199	rBV	360	450	0.07%	0.009%
96	14.505	2199	2201	2204	rVV	406	267	0.04%	0.005%
97	14.926	2269	2270	2272	rBV	821	356	0.05%	0.007%
98	15.158	2307	2308	2310	rBV	666	536	0.08%	0.010%
99	15.475	2358	2360	2363	rBV2	656	705	0.10%	0.014%
100	16.481	2523	2525	2526	rVB	898	459	0.07%	0.009%


Sum of corrected areas: 5180561

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025017.D
Acq On : 29 Oct 2021 11:27
Operator : JC/MD
Sample : VX1029WBL05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK623

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

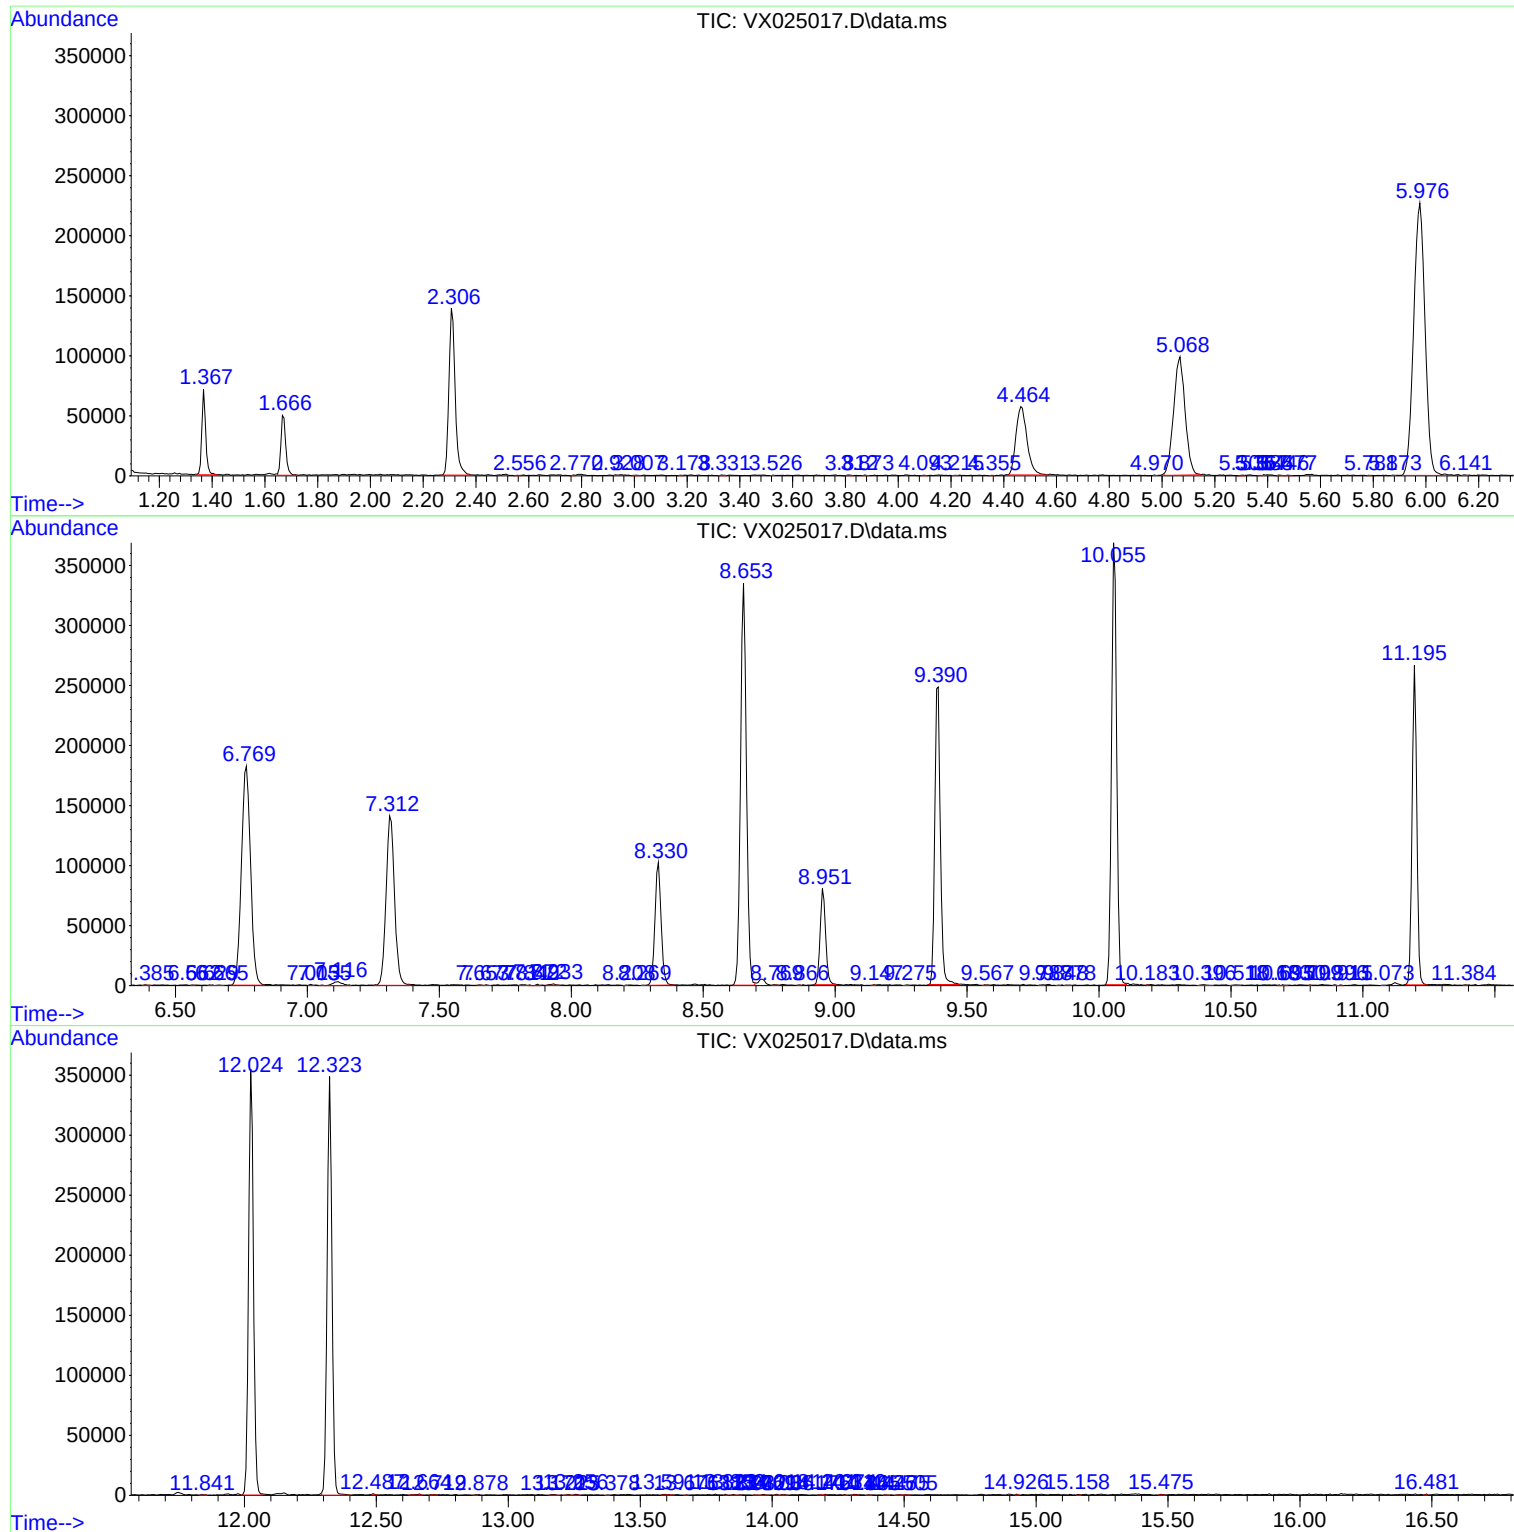

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025017.D
Acq On : 29 Oct 2021 11:27
Operator : JC/MD
Sample : VX1029WBL05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK623

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025017.D
Acq On : 29 Oct 2021 11:27
Operator : JC/MD
Sample : VX1029WBL05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK623

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
