

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025018.D
 Acq On : 29 Oct 2021 11:50
 Operator : JC/MD
 Sample : VX1029MBL03
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK624

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

Signal : TIC: VX025018.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	56	rVB	70269	72562	10.66%	1.403%
2	1.672	92	96	103	rVB	49779	64539	9.48%	1.248%
3	2.306	194	200	212	rVB	141438	229550	33.73%	4.438%
4	2.776	275	277	278	rBV	978	550	0.08%	0.011%
5	3.013	315	316	317	rBV	651	289	0.04%	0.006%
6	3.263	355	357	361	rBV	344	472	0.07%	0.009%
7	3.452	386	388	389	rBV	407	247	0.04%	0.005%
8	3.586	406	410	412	rBV	534	584	0.09%	0.011%
9	3.605	412	413	414	rBV	394	237	0.03%	0.005%
10	3.751	434	437	439	rBV	574	513	0.08%	0.010%
11	4.348	534	535	536	rBV	379	157	0.02%	0.003%
12	4.367	536	538	540	rBV	475	422	0.06%	0.008%
13	4.464	545	554	566	rBV	59571	167059	24.55%	3.230%
14	4.800	607	609	611	rBV	603	632	0.09%	0.012%
15	5.062	641	652	667	rBV	97920	304565	44.75%	5.888%
16	5.342	696	698	699	rBV	309	213	0.03%	0.004%
17	5.488	720	722	725	rBV2	442	566	0.08%	0.011%
18	5.879	785	786	788	rBV2	464	456	0.07%	0.009%
19	5.970	790	801	816	rBV2	224499	680592	100.00%	13.157%
20	6.153	830	831	832	rVB2	364	133	0.02%	0.003%
21	6.312	856	857	860	rBV	599	414	0.06%	0.008%
22	6.501	886	888	890	rBV	577	685	0.10%	0.013%
23	6.549	892	896	897	rBV2	574	613	0.09%	0.012%
24	6.568	897	899	900	rBV	337	183	0.03%	0.004%
25	6.769	921	932	944	rBV	178462	432555	63.56%	8.362%
26	7.043	976	977	981	rVB	649	523	0.08%	0.010%
27	7.189	998	1001	1002	rBV2	361	337	0.05%	0.007%
28	7.311	1013	1021	1034	rVB	138565	307002	45.11%	5.935%
29	7.433	1040	1041	1044	rBV	361	431	0.06%	0.008%
30	7.671	1076	1080	1081	rBV	624	803	0.12%	0.016%
31	7.750	1092	1093	1096	rBV	367	332	0.05%	0.006%
32	7.994	1131	1133	1134	rBV	373	229	0.03%	0.004%
33	8.183	1163	1164	1166	rBV	755	606	0.09%	0.012%
34	8.244	1172	1174	1177	rBV	412	350	0.05%	0.007%
35	8.329	1182	1188	1199	rVV	97215	164071	24.11%	3.172%
36	8.653	1234	1241	1249	rBV	339194	517761	76.08%	10.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025018.D
 Acq On : 29 Oct 2021 11:50
 Operator : JC/MD
 Sample : VX1029MBL03
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK624

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
 Title : VOC Analysis

37	8.848	1271	1273	1274	rBV	428	187	0.03%	0.004%
38	8.951	1285	1290	1301	rVB	75111	116087	17.06%	2.244%
39	9.238	1335	1337	1340	rBV2	537	535	0.08%	0.010%
40	9.390	1356	1362	1373	rBV	253957	368108	54.09%	7.116%
41	9.701	1411	1413	1415	rBV2	778	746	0.11%	0.014%
42	9.811	1429	1431	1433	rVB2	567	537	0.08%	0.010%
43	9.866	1438	1440	1444	rBV2	386	492	0.07%	0.010%
44	10.012	1461	1464	1465	rBV	436	480	0.07%	0.009%
45	10.055	1466	1471	1480	rVV	367587	492445	72.36%	9.520%
46	10.500	1541	1544	1545	rBV	271	234	0.03%	0.005%
47	10.597	1559	1560	1564	rVB	455	343	0.05%	0.007%
48	10.634	1564	1566	1567	rBV	585	459	0.07%	0.009%
49	10.652	1567	1569	1572	rVV	677	649	0.10%	0.013%
50	10.969	1617	1621	1624	rBV	870	1274	0.19%	0.025%
51	11.067	1634	1637	1639	rBV	519	555	0.08%	0.011%
52	11.116	1643	1645	1652	rVB3	2218	3233	0.48%	0.063%
53	11.195	1652	1658	1665	rBV	259910	332914	48.92%	6.436%
54	11.365	1684	1686	1689	rBV2	437	386	0.06%	0.007%
55	11.457	1698	1701	1702	rBV	734	709	0.10%	0.014%
56	11.622	1726	1728	1734	rBV2	461	688	0.10%	0.013%
57	11.664	1734	1735	1737	rBV2	604	386	0.06%	0.007%
58	11.902	1772	1774	1776	rVB2	708	669	0.10%	0.013%
59	11.926	1776	1778	1783	rBV2	1045	1572	0.23%	0.030%
60	12.024	1789	1794	1807	rVB	353958	445404	65.44%	8.611%
61	12.323	1837	1843	1855	rBV	352798	442104	64.96%	8.547%
62	12.420	1857	1859	1861	rBV	812	586	0.09%	0.011%
63	12.621	1890	1892	1893	rBV	476	285	0.04%	0.006%
64	12.859	1930	1931	1934	rVB	530	400	0.06%	0.008%
65	13.012	1954	1956	1959	rBV2	619	621	0.09%	0.012%
66	13.042	1959	1961	1962	rBV	628	416	0.06%	0.008%
67	13.243	1992	1994	1996	rBV	471	245	0.04%	0.005%
68	13.371	2014	2015	2016	rBV	253	104	0.02%	0.002%
69	13.475	2030	2032	2035	rVB	347	235	0.03%	0.005%
70	13.530	2038	2041	2042	rBV	607	485	0.07%	0.009%
71	13.688	2065	2067	2068	rBV	593	353	0.05%	0.007%
72	13.786	2082	2083	2087	rBV	548	686	0.10%	0.013%
73	13.853	2092	2094	2097	rVB2	618	419	0.06%	0.008%
74	14.011	2117	2120	2121	rBV2	356	452	0.07%	0.009%
75	14.060	2124	2128	2129	rBV	592	697	0.10%	0.013%
76	14.267	2160	2162	2165	rBV	356	517	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025018.D
 Acq On : 29 Oct 2021 11:50
 Operator : JC/MD
 Sample : VX1029MBL03
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK624

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M

Title : VOC Analysis

77	14.426	2186	2188	2190	rBV	774	548	0.08%	0.011%
78	14.798	2247	2249	2250	rBV	374	242	0.04%	0.005%
79	14.908	2265	2267	2270	rBV	434	442	0.06%	0.009%
80	14.999	2281	2282	2283	rBV	502	237	0.03%	0.005%
81	15.176	2308	2311	2313	rVB	861	625	0.09%	0.012%
82	15.194	2313	2314	2317	rBV	506	531	0.08%	0.010%
83	15.389	2345	2346	2348	rBV	800	564	0.08%	0.011%
84	16.182	2475	2476	2479	rBV2	709	575	0.08%	0.011%




Sum of corrected areas: 5172694

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025018.D
Acq On : 29 Oct 2021 11:50
Operator : JC/MD
Sample : VX1029MBL03
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
VBLK624

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

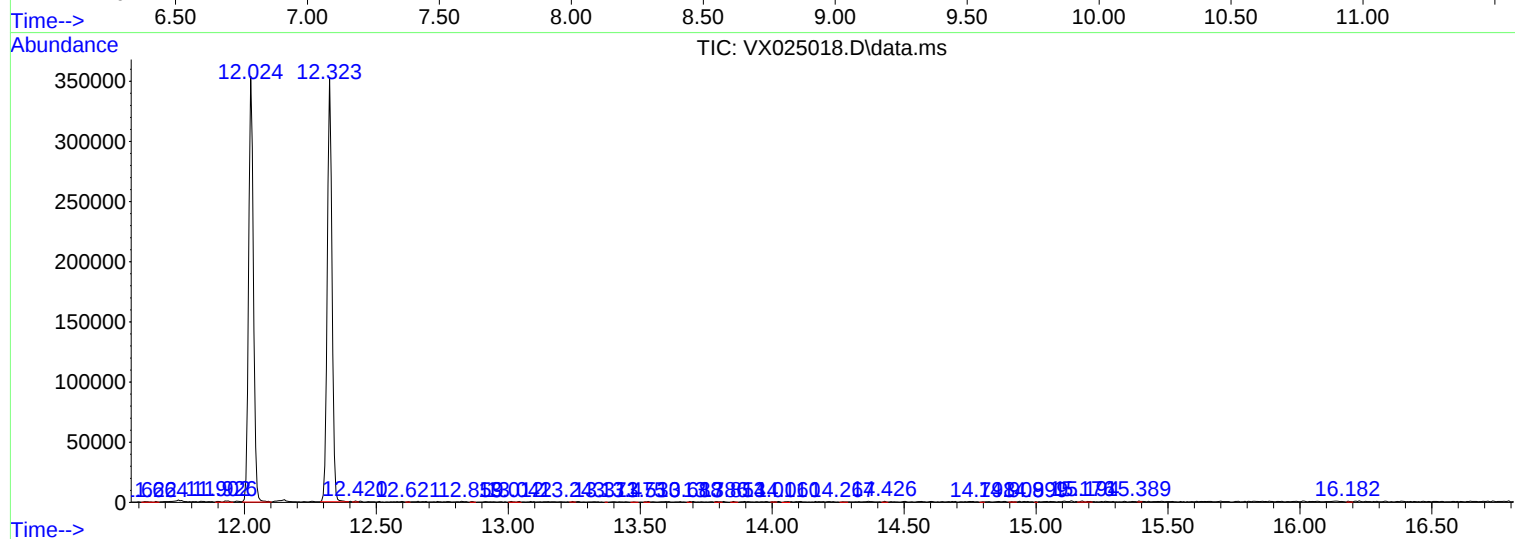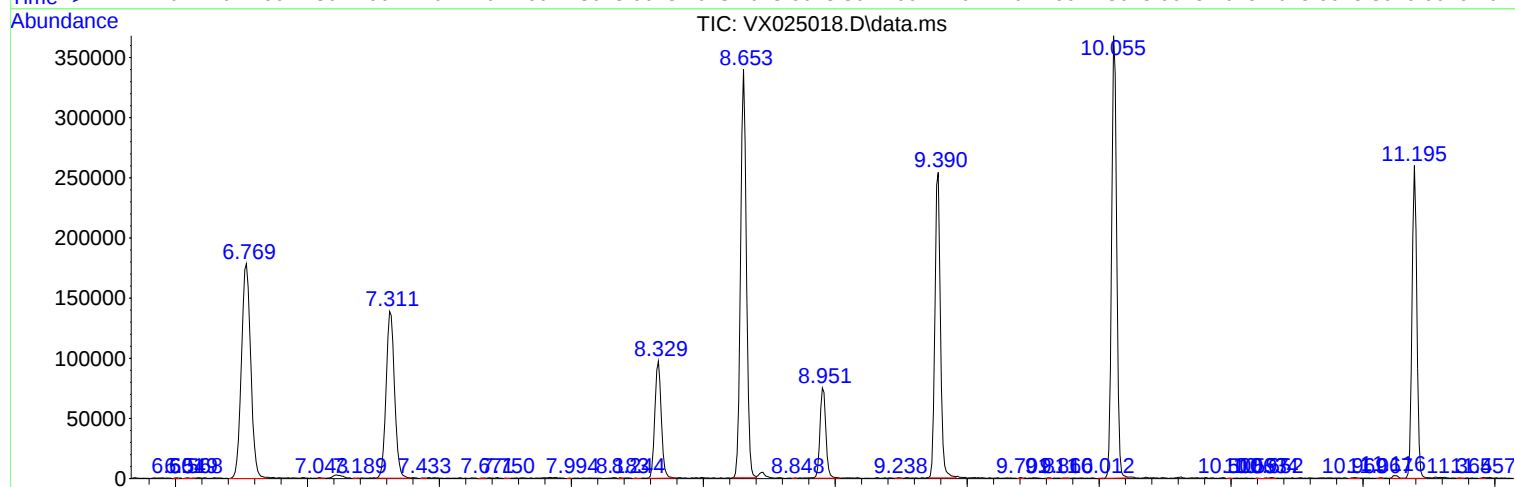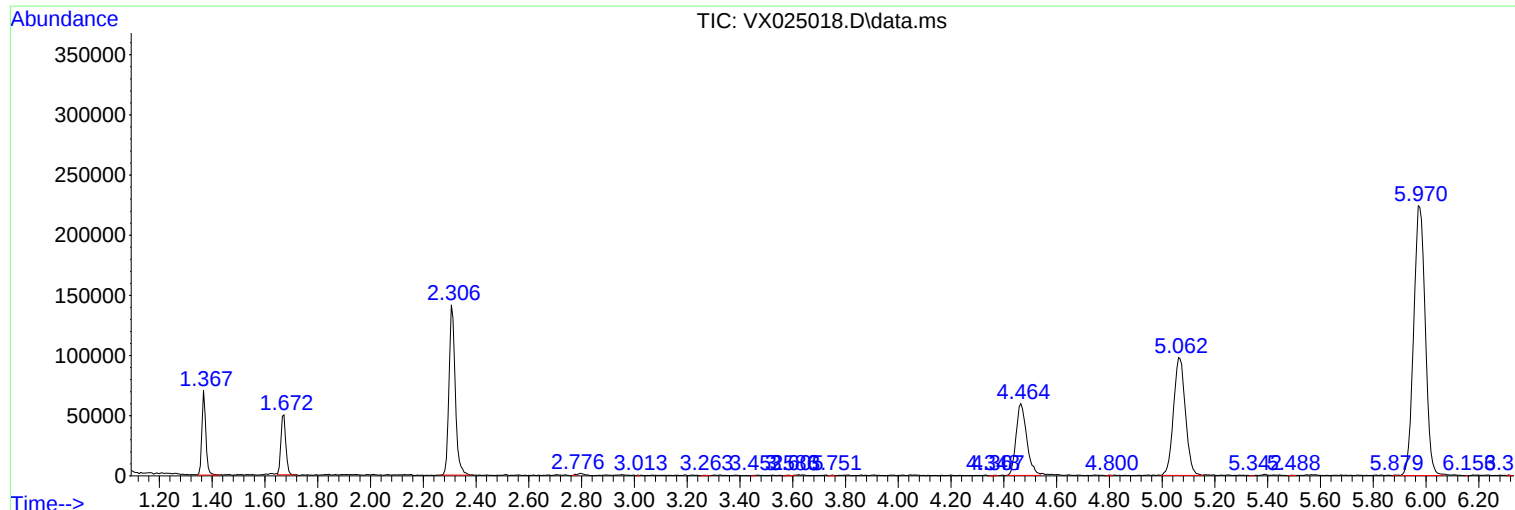

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025018.D
Acq On : 29 Oct 2021 11:50
Operator : JC/MD
Sample : VX1029MBL03
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK624

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
Data File : VX025018.D
Acq On : 29 Oct 2021 11:50
Operator : JC/MD
Sample : VX1029MBL03
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK624

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
