
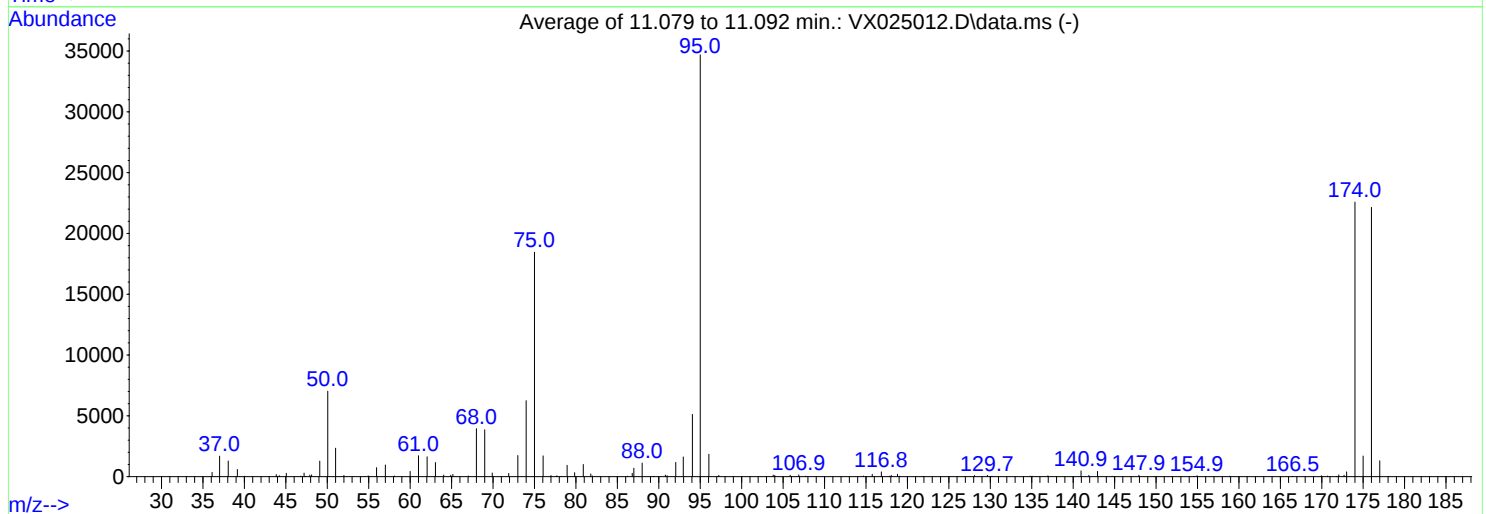


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102921\
 Data File : VX025012.D
 Acq On : 29 Oct 2021 09:06
 Operator : JC/MD
 Sample : BFB608
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB608

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
 Title : VOC Analysis
 Last Update : Tue Nov 02 03:29:47 2021

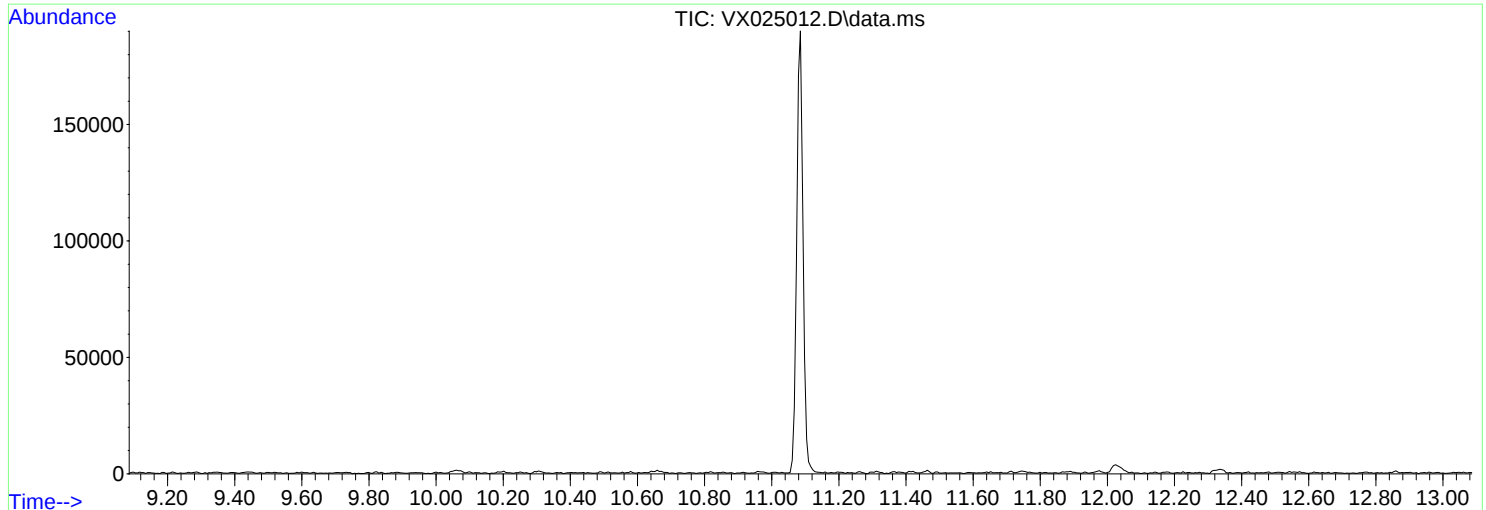

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	7027	PASS
75	95	30	80	53.2	18465	PASS
95	95	100	100	100.0	34683	PASS
96	95	5	9	5.3	1847	PASS
173	174	0.00	2	1.7	391	PASS
174	95	50	120	65.1	22576	PASS
175	174	5	9	7.5	1697	PASS
176	174	95	101	98.1	22149	PASS
177	176	5	9	5.9	1305	PASS

m/z	Abundance
40.10	72.0
44.10	255.0
44.80	69.0
78.00	60.0

Instrument :
MSVOA_X
ClientSampleId :
BFB608

m/z	Abundance
36.10	391.0
37.00	2167.0
38.10	1686.0
39.20	766.0
40.10	57.0
42.90	63.0
43.80	238.0
44.20	230.0
45.10	317.0
47.20	430.0
47.90	395.0
49.10	1405.0
50.10	8249.0
51.00	2719.0
52.00	143.0
54.90	102.0
56.00	879.0
57.00	1212.0
59.90	550.0
61.00	2016.0
62.00	1883.0
63.10	1156.0
64.10	211.0
64.90	357.0
68.00	4530.0
69.00	4140.0
69.90	240.0
72.00	348.0
73.00	1840.0
74.00	6722.0
75.00	20848.0
76.10	1936.0
77.00	207.0
77.70	145.0
78.00	143.0
78.90	894.0
79.90	381.0
80.90	1021.0
81.80	317.0
86.80	838.0
88.10	1495.0
90.80	102.0
92.00	1363.0
92.90	1694.0
94.10	5584.0
95.00	36584.0
96.00	2194.0
97.20	157.0
103.80	231.0
105.90	117.0
107.00	221.0
115.70	265.0
116.80	295.0
117.80	124.0
118.80	186.0
121.90	70.0
128.10	94.0
129.60	109.0
130.00	78.0
135.10	83.0
137.00	96.0
141.00	510.0
142.00	84.0
142.90	413.0
147.90	192.0
149.80	59.0
154.90	68.0
170.00	82.0
171.80	92.0
173.00	440.0
174.00	21728.0
175.00	2078.0
176.00	20808.0
177.00	1326.0

Instrument :
MSVOA_X
ClientSampleId :
BFB608

m/z	Abundance
36.10	248.0
37.00	1691.0
38.00	1289.0
39.10	756.0
40.00	133.0
43.90	262.0
45.00	295.0
47.20	442.0
48.10	306.0
49.10	1543.0
50.00	8360.0
51.00	2583.0
52.00	182.0
55.00	93.0
55.90	834.0
57.00	1090.0
58.10	93.0
60.00	417.0
61.00	1891.0
62.10	1732.0
63.00	1555.0
64.00	137.0
65.20	299.0
67.10	90.0
68.00	4849.0
69.00	4613.0
70.00	479.0
71.90	274.0
73.00	2137.0
74.00	7442.0
75.00	21360.0
76.00	1689.0
77.00	82.0
77.70	102.0
78.20	94.0
79.00	1255.0
79.80	258.0
80.00	193.0
81.00	1161.0
81.80	336.0
87.00	1055.0
87.90	1199.0
89.40	81.0
90.80	301.0
92.10	1128.0
93.00	2023.0
94.00	5770.0
95.00	41544.0
96.10	2098.0
97.30	155.0
103.80	169.0
105.80	136.0
106.80	94.0
107.70	59.0
114.70	76.0
115.80	233.0
116.80	542.0
118.00	222.0
118.90	304.0
128.10	184.0
129.70	153.0
134.80	124.0
140.90	633.0
141.80	135.0
143.00	462.0
144.70	106.0
148.00	173.0
151.90	62.0
154.90	111.0
158.90	64.0
169.90	73.0
170.70	71.0
172.10	230.0
172.70	359.0
173.00	449.0
174.00	27520.0
175.00	1956.0
176.00	25960.0
177.00	1479.0

Instrument :
MSVOA_X
ClientSampleId :
BFB608

m/z	Abundance
36.10	420.0
37.10	1204.0
38.10	881.0
39.10	241.0
39.90	130.0
44.00	220.0
45.00	220.0
46.80	138.0
47.40	91.0
48.10	138.0
49.10	891.0
50.10	4471.0
51.00	1744.0
56.00	501.0
57.00	565.0
58.10	64.0
60.10	342.0
61.00	1263.0
62.00	1267.0
63.10	764.0
64.00	54.0
65.10	243.0
67.00	58.0
68.00	2475.0
69.00	2826.0
69.80	180.0
71.80	181.0
73.00	1245.0
74.00	4594.0
75.00	13187.0
76.10	1498.0
78.90	657.0
79.70	173.0
80.80	835.0
82.00	174.0
86.20	126.0
87.00	1031.0
88.00	677.0
91.00	246.0
92.00	1012.0
93.00	1127.0
94.10	3986.0
95.10	25920.0
96.00	1249.0
104.00	302.0
105.80	93.0
106.80	121.0
107.70	51.0
114.70	81.0
115.70	107.0
116.90	341.0
118.10	80.0
118.70	115.0
119.10	123.0
129.70	53.0
130.20	104.0
135.00	58.0
136.90	91.0
140.90	291.0
141.90	96.0
143.00	445.0
154.60	56.0
155.00	75.0
158.90	77.0
166.50	89.0
169.90	72.0
170.70	85.0
172.00	222.0
173.00	284.0
174.00	18480.0
175.00	1056.0
176.00	19680.0
177.00	1110.0
178.10	81.0

Instrument :
MSVOA_X
ClientSampleId :
BFB608