

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102924\
 Data File : VX043589.D
 Acq On : 29 Oct 2024 12:10
 Operator : JC/MD
 Sample : P4596-07 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TOTE-WATER-COMP

Quant Time: Oct 30 01:29:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 28 13:41:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	156223	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	287122	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	260137	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	120317	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	108083	43.389	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	86.780%
35) Dibromofluoromethane	5.379	113	90176	46.316	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.640%
50) Toluene-d8	8.647	98	341763	50.709	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.420%
62) 4-Bromofluorobenzene	11.079	95	125609	50.296	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	100.600%
Target Compounds						
					Qvalue	
5) Bromomethane	1.599	94	469	0.580	ug/l #	2
11) Tert butyl alcohol	2.941	59	16238	34.924	ug/l #	100
13) Acrolein	2.240	56	101	0.278	ug/l #	77
16) Acetone	2.386	43	21152	21.383	ug/l	96
17) Carbon Disulfide	2.502	76	975	0.279	ug/l	96
18) Methyl Acetate	2.703	43	654	0.226	ug/l #	51
20) Methylene Chloride	2.782	84	490	0.230	ug/l #	92
25) 2-Butanone	4.587	43	1540	1.067	ug/l	96
31) Cyclohexane	5.538	56	3232	1.229	ug/l #	11
36) 1,1-Dichloropropene	5.544	75	12085	5.235	ug/l #	45
38) Carbon Tetrachloride	5.544	117	15871	6.222	ug/l #	15
40) Benzene	6.044	78	3548	0.461	ug/l	91
51) 4-Methyl-2-Pentanone	8.580	43	1345	0.476	ug/l #	83
52) Toluene	8.720	92	14381	3.079	ug/l	99
67) Ethyl Benzene	10.195	91	19304	2.115	ug/l	99
68) m/p-Xylenes	10.299	106	28436	8.148	ug/l	97
69) o-Xylene	10.640	106	22706	6.475	ug/l	98
70) Styrene	10.640	104	1513	0.260	ug/l #	1
73) Isopropylbenzene	10.964	105	6664	0.782	ug/l	97
76) 1,2,3-Trichloropropane	11.079	75	62647	24.352	ug/l #	33
78) n-propylbenzene	11.305	91	13813	1.486	ug/l	98
79) 2-Chlorotoluene	11.378	91	9158	1.486	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	24578	3.459	ug/l	96
81) trans-1,4-Dichloro-2-b...	11.079	75	62647	66.994	ug/l #	7
82) 4-Chlorotoluene	11.451	91	2913	0.421	ug/l #	51
83) tert-Butylbenzene	11.750	119	13135	1.817	ug/l #	58
84) 1,2,4-Trimethylbenzene	11.750	105	107004	14.775	ug/l	98
85) sec-Butylbenzene	11.890	105	6514	0.769	ug/l	95
86) p-Isopropyltoluene	12.006	119	4724	0.656	ug/l	94
89) n-Butylbenzene	12.329	91	9857	1.680	ug/l #	28
90) Hexachloroethane	12.530	117	2065	1.766	ug/l #	17
95) Naphthalene	13.774	128	46188	4.930	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102924\
Data File : VX043589.D
Acq On : 29 Oct 2024 12:10
Operator : JC/MD
Sample : P4596-07 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOTE-WATER-COMP

Quant Time: Oct 30 01:29:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
Quant Title : SW846 8260
QLast Update : Mon Oct 28 13:41:34 2024
Response via : Initial Calibration




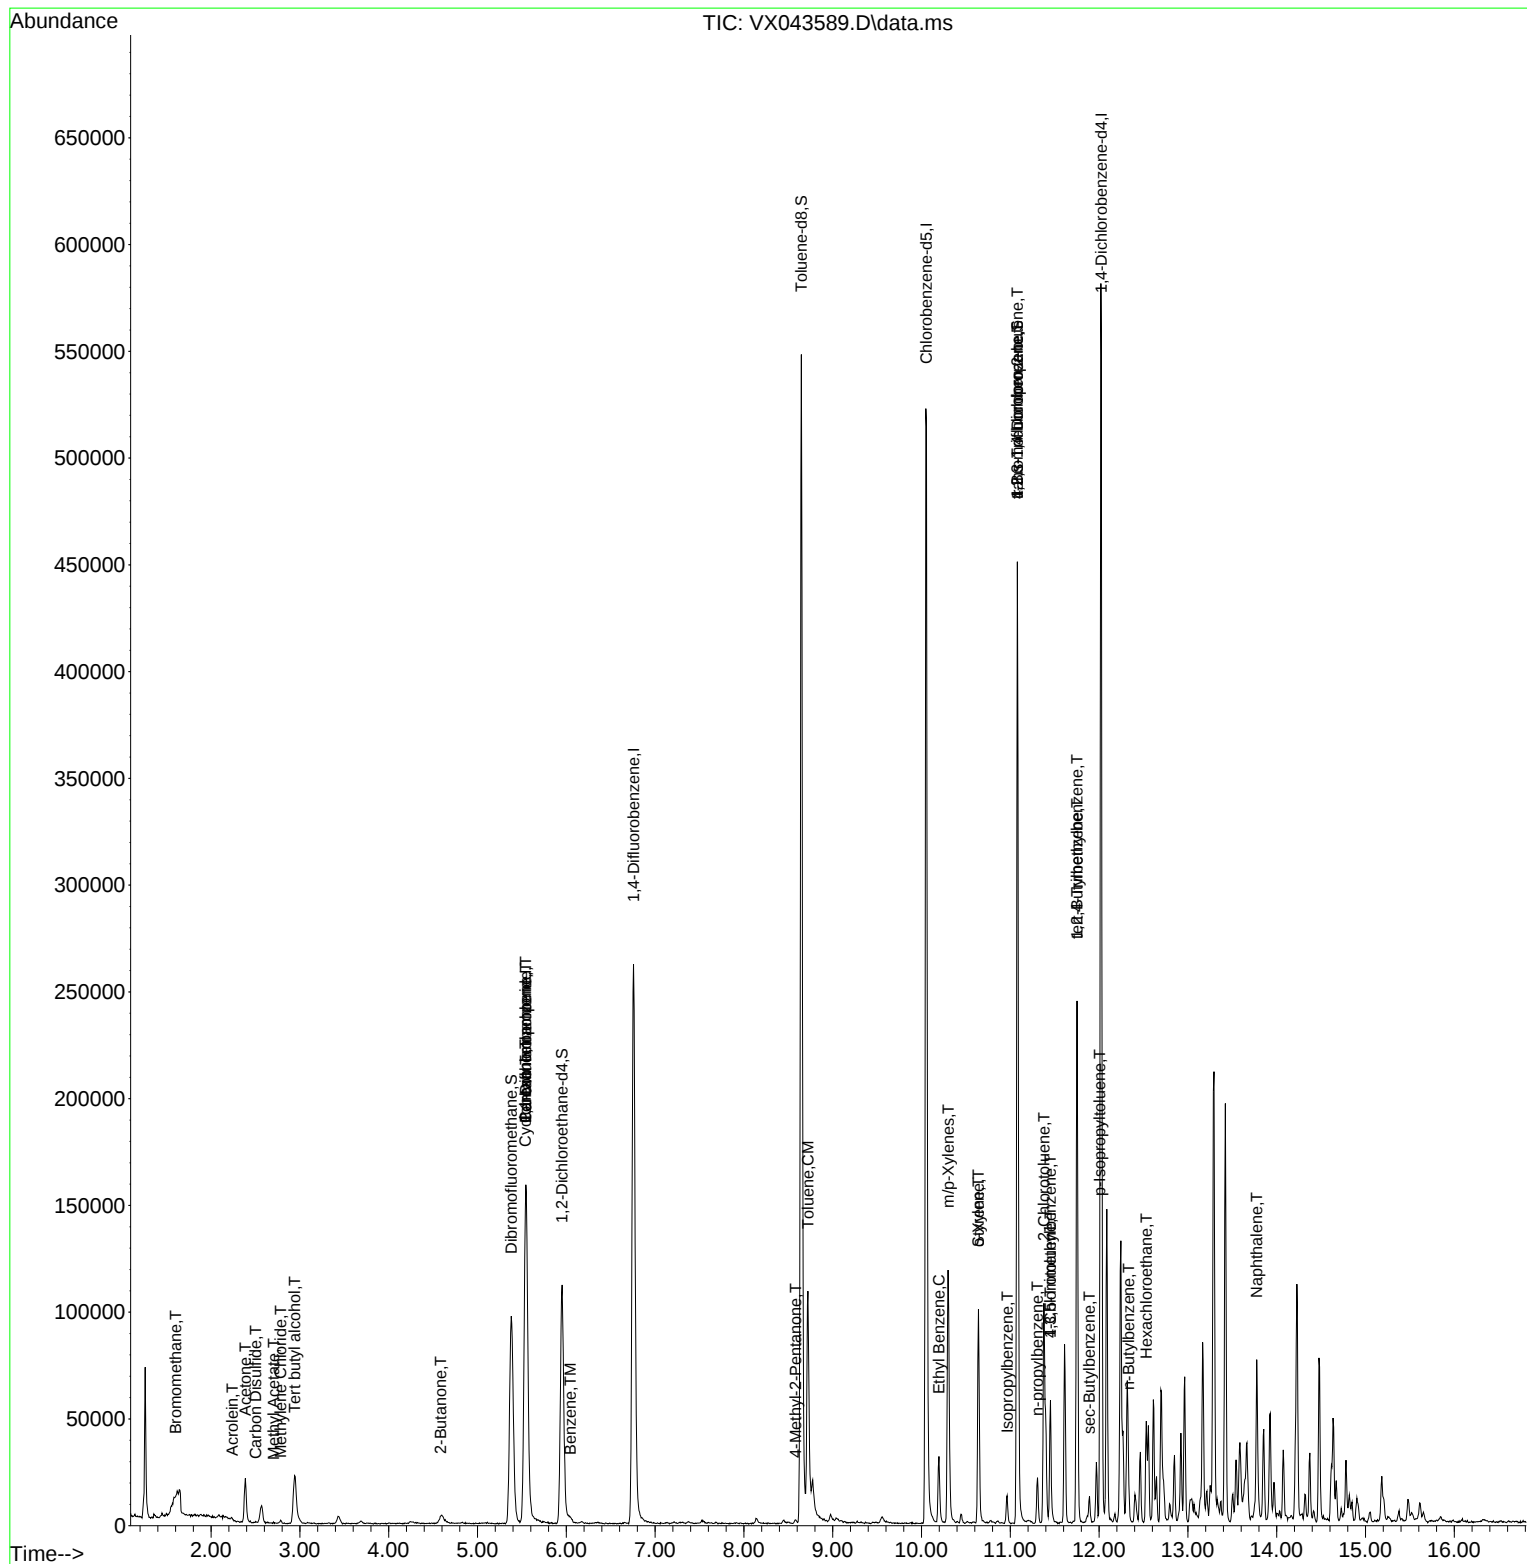




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10




Instrument :
MSVOA_X
ClientSampleId :
TOTE-WATER-COMP


Tgt Ion:168 Resp: 156223
Ion Ratio Lower Upper
168 100
99 60.6 52.6 78.8

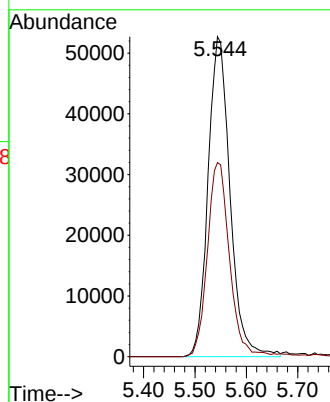

#5
Bromomethane
Concen: 0.580 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.006 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10

Tgt Ion: 94 Resp: 469
Ion Ratio Lower Upper
94 100
96 0.0 75.9 113.9#

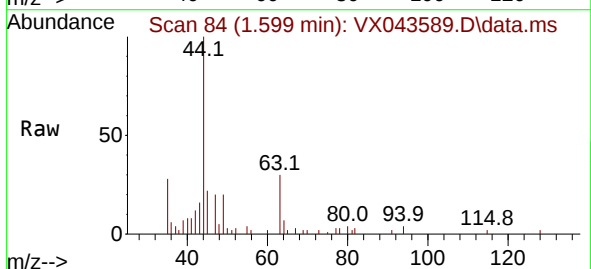



#11

Tert butyl alcohol

Concen: 34.924 ug/l

RT: 2.941 min Scan# 30

Delta R.T. -0.109 min

Lab File: VX043589.D

Acq: 29 Oct 2024 12:10

Instrument :

MSVOA_X

ClientSampleId :





TOTE-WATER-COMP

Tgt Ion: 59 Resp: 16238

Ion Ratio Lower Upper

59 100

57 0.7 0.0 0.0#

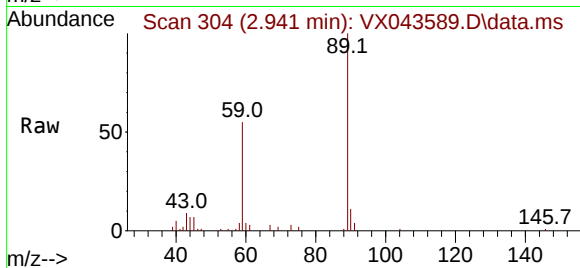

#13

Acrolein

Concen: 0.278 ug/l

RT: 2.240 min Scan# 189

Delta R.T. 0.000 min

Lab File: VX043589.D




Acq: 29 Oct 2024 12:10


Tgt Ion: 56 Resp: 101

Ion Ratio Lower Upper

56 100

55 50.5 55.3 82.9#

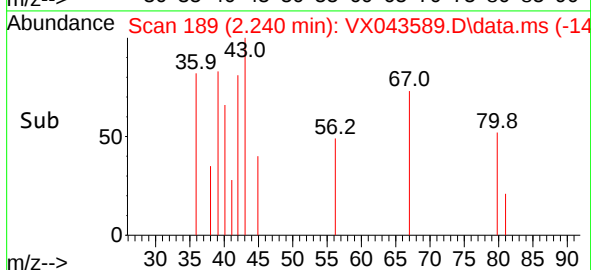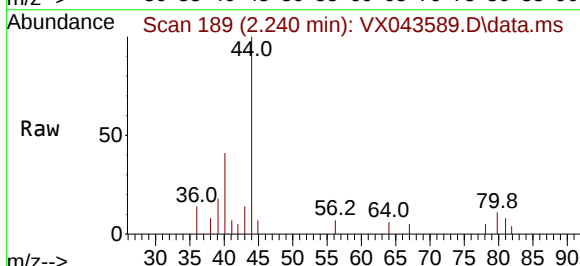



#16

Acetone

Concen: 21.383 ug/l

RT: 2.386 min Scan# 21

Delta R.T. -0.012 min

Lab File: VX043589.D

Acq: 29 Oct 2024 12:10

Instrument :

MSVOA_X

ClientSampleId :





TOTE-WATER-COMP

Tgt Ion: 43 Resp: 21152

Ion Ratio Lower Upper

43 100

58 33.6 25.1 37.7

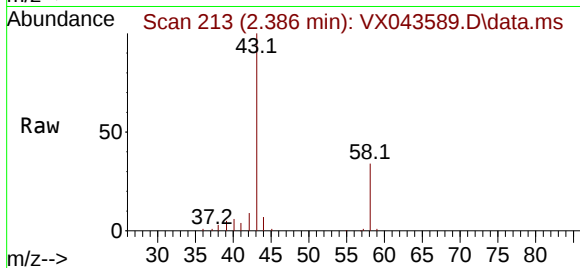

#17

Carbon Disulfide

Concen: 0.279 ug/l

RT: 2.502 min Scan# 232

Delta R.T. 0.006 min

Lab File: VX043589.D




Acq: 29 Oct 2024 12:10


Tgt Ion: 76 Resp: 975

Ion Ratio Lower Upper

76 100

78 10.3 7.1 10.7




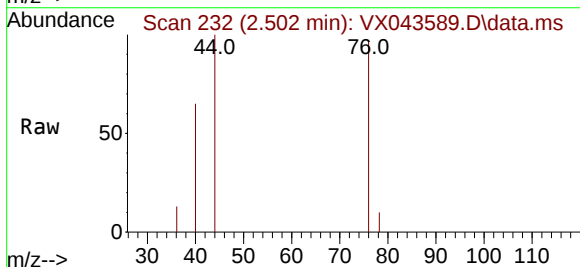




#18
Methyl Acetate
Concen: 0.226 ug/l
RT: 2.703 min Scan# 265
Delta R.T. -0.006 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10




Instrument :
MSVOA_X
ClientSampleId :
TOTE-WATER-COMP


Tgt Ion: 43 Resp: 654
Ion Ratio Lower Upper
43 100
74 0.0 19.1 28.7#



#20
Methylene Chloride
Concen: 0.230 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.000 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10

Tgt Ion: 84 Resp: 490
Ion Ratio Lower Upper
84 100
49 124.2 97.0 145.6
51 36.2 29.8 44.8
86 49.2 53.1 79.7#









#25
2-Butanone
Concen: 1.067 ug/l
RT: 4.587 min Scan# 51
Delta R.T. 0.019 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10




Instrument :
MSVOA_X
ClientSampleId :
TOTE-WATER-COMP


Tgt Ion: 43 Resp: 1540
Ion Ratio Lower Upper
43 100
72 28.7 21.1 31.7



#31
Cyclohexane
Concen: 1.229 ug/l
RT: 5.538 min Scan# 730
Delta R.T. 0.079 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10

Tgt Ion: 56 Resp: 3232
Ion Ratio Lower Upper
56 100
69 178.2 24.9 37.3#
84 118.2 73.3 109.9#

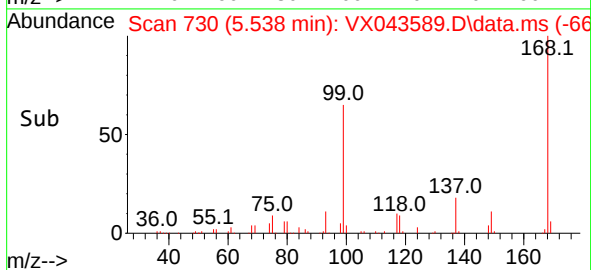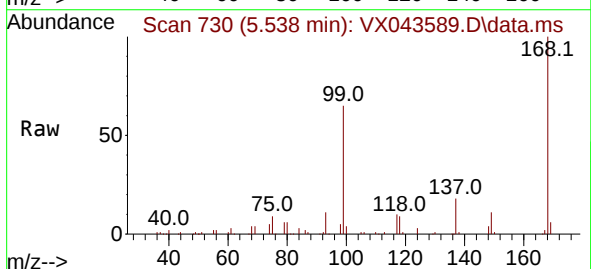



#33

1,2-Dichloroethane-d4

Concen: 43.389 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.000 min

Lab File: VX043589.D

Acq: 29 Oct 2024 12:10

Instrument :

MSVOA_X

ClientSampleId :





TOTE-WATER-COMP

Tgt Ion: 65 Resp: 108083

Ion Ratio Lower Upper

65 100

67 51.2 0.0 103.4

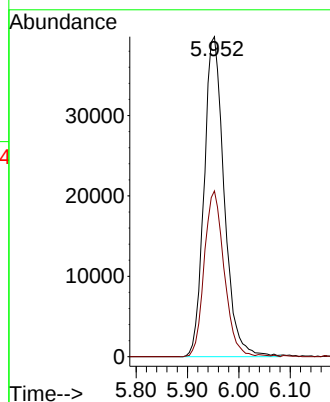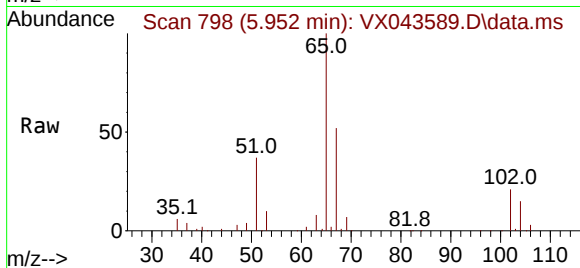

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. 0.000 min

Lab File: VX043589.D

Acq: 29 Oct 2024 12:10




Tgt Ion: 114 Resp: 287122


Ion Ratio Lower Upper

114 100

63 20.4 0.0 41.2

88 16.7 0.0 34.0


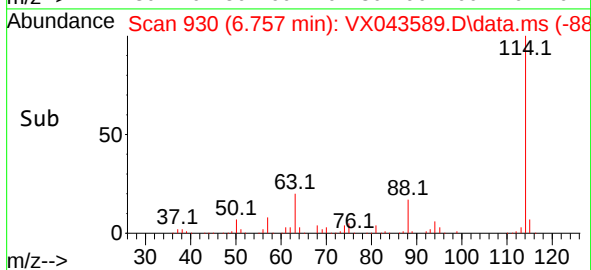

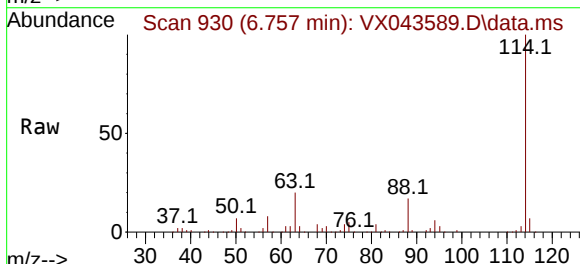




#35
Dibromofluoromethane
Concen: 46.316 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10




Instrument :
MSVOA_X
ClientSampleId :
TOTE-WATER-COMP


Tgt Ion:113 Resp: 90176
Ion Ratio Lower Upper
113 100
111 100.5 81.4 122.0
192 18.1 14.1 21.1

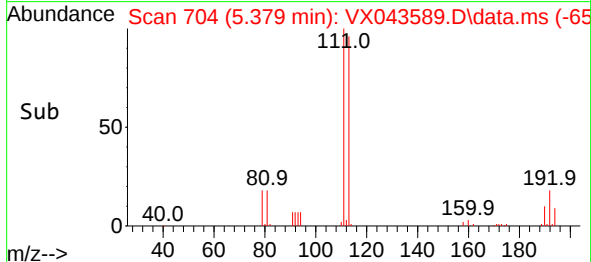

#36
1,1-Dichloropropene
Concen: 5.235 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.140 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10


Tgt Ion: 75 Resp: 12085
Ion Ratio Lower Upper
75 100
110 4.1 17.9 53.7#
77 0.0 25.0 37.4#

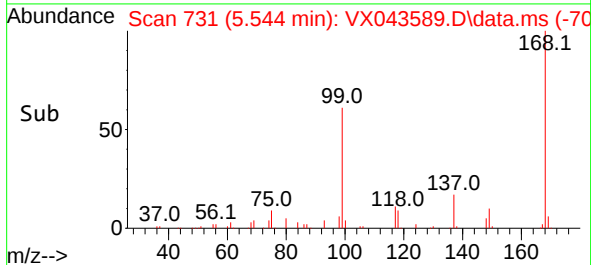






#38
Carbon Tetrachloride
Concen: 6.222 ug/l
RT: 5.544 min Scan# 711
Delta R.T. -0.128 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10

Instrument :
MSVOA_X
ClientSampleId :
TOTE-WATER-COMP



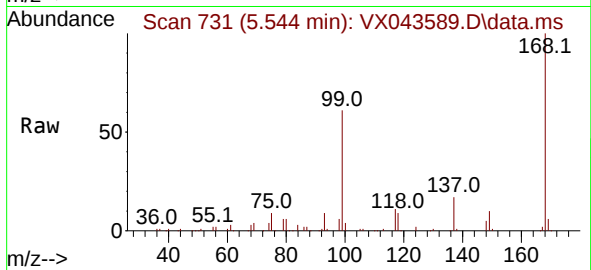



Tgt Ion:117 Resp: 15871
Ion Ratio Lower Upper
117 100
119 4.0 77.0 115.6#
121 0.0 24.7 37.1#



#40
Benzene
Concen: 0.461 ug/l
RT: 6.044 min Scan# 813
Delta R.T. 0.012 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10

Tgt Ion: 78 Resp: 3548
Ion Ratio Lower Upper
78 100
77 18.8 18.4 27.6









#50
Toluene-d8
Concen: 50.709 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10




Instrument :
MSVOA_X
ClientSampleId :
TOTE-WATER-COMP


Tgt Ion: 98 Resp: 341763
Ion Ratio Lower Upper
98 100
100 66.5 53.4 80.2



#51
4-Methyl-2-Pentanone
Concen: 0.476 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. 0.000 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10

Tgt Ion: 43 Resp: 1345
Ion Ratio Lower Upper
43 100
58 29.4 31.7 47.5#









#52
Toluene
Concen: 3.079 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10




Instrument :
MSVOA_X
ClientSampleId :
TOTE-WATER-COMP


Tgt Ion: 92 Resp: 14381
Ion Ratio Lower Upper
92 100
91 170.4 135.7 203.5



#62
4-Bromofluorobenzene
Concen: 50.296 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10

Tgt Ion: 95 Resp: 125609
Ion Ratio Lower Upper
95 100
174 77.6 0.0 146.6
176 73.5 0.0 139.6


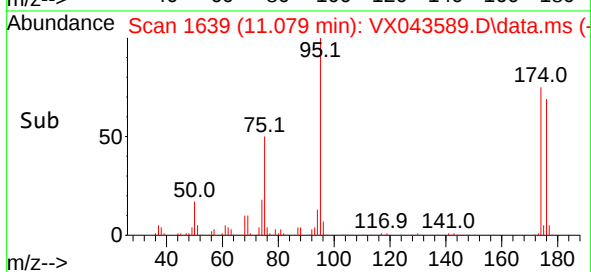

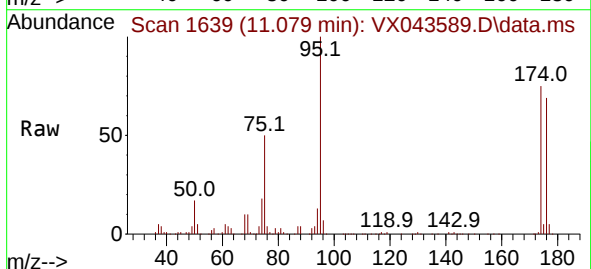




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10




Instrument :
MSVOA_X
ClientSampleId :
TOTE-WATER-COMP


Tgt Ion:117 Resp: 260137
Ion Ratio Lower Upper
117 100
82 53.0 42.1 63.1
119 31.0 25.4 38.2

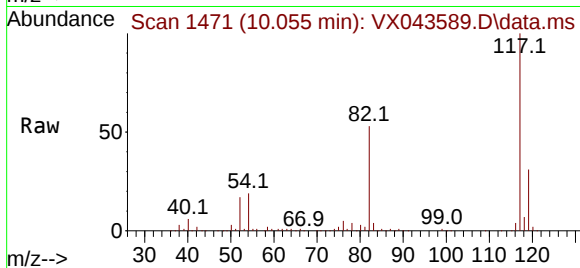

#67
Ethyl Benzene
Concen: 2.115 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10

Tgt Ion: 91 Resp: 19304
Ion Ratio Lower Upper
91 100
106 32.3 25.4 38.2


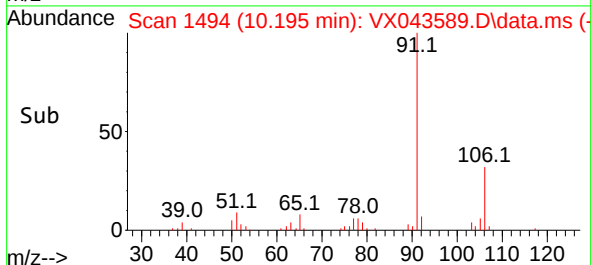
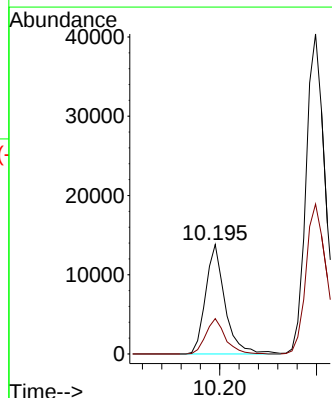
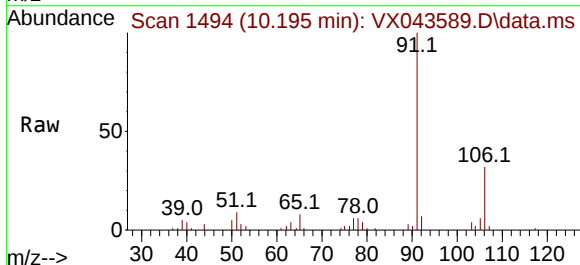




#68
m/p-Xylenes
Concen: 8.148 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10




Instrument :
MSVOA_X
ClientSampleId :
TOTE-WATER-COMP


Tgt Ion:106 Resp: 28436
Ion Ratio Lower Upper
106 100
91 200.8 164.7 247.1

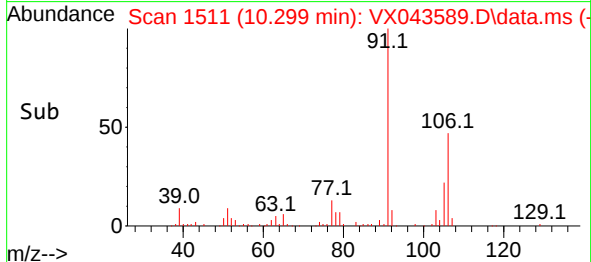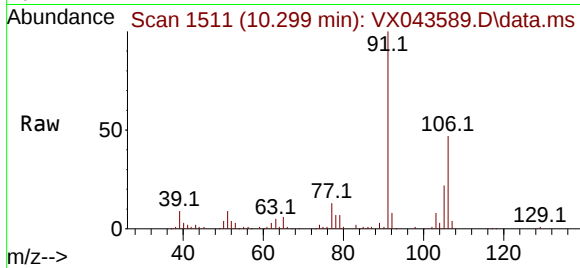

#69
o-Xylene
Concen: 6.475 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10

Tgt Ion:106 Resp: 22706
Ion Ratio Lower Upper
106 100
91 213.0 107.9 323.7

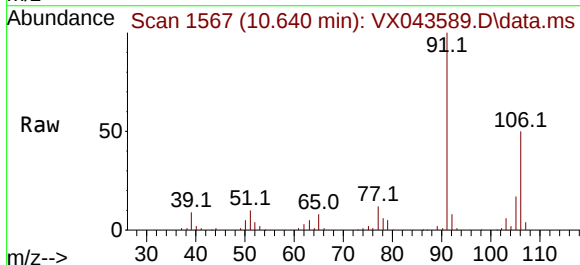



#70

Styrene

Concen: 0.260 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. -0.012 min

Lab File: VX043589.D

Acq: 29 Oct 2024 12:10

Instrument :

MSVOA_X

ClientSampleId :

TOTE-WATER-COMP





Tgt Ion:104 Resp: 1513

Ion Ratio Lower Upper

104 100

78 243.8 40.0 60.0#

103 213.6 43.4 65.0#

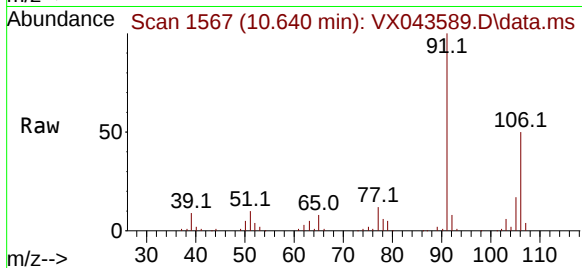

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX043589.D

Acq: 29 Oct 2024 12:10




Tgt Ion:152 Resp: 120317


Ion Ratio Lower Upper

152 100

115 64.1 42.9 128.7

150 162.5 0.0 343.6

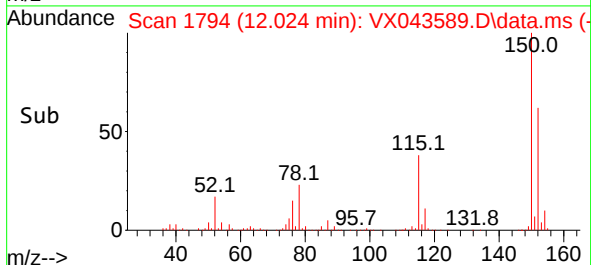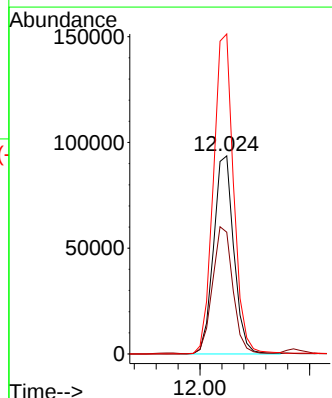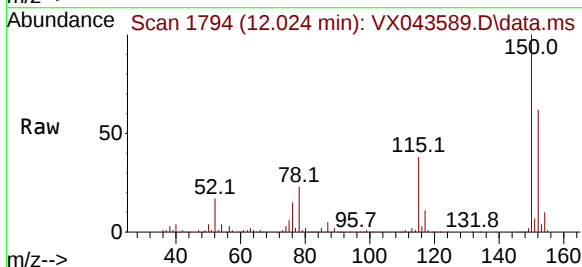



#73

Isopropylbenzene

Concen: 0.782 ug/l

RT: 10.964 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX043589.D

Acq: 29 Oct 2024 12:10

Instrument :

MSVOA_X

ClientSampleId :





TOTE-WATER-COMP

Tgt Ion:105 Resp: 6664

Ion Ratio Lower Upper

105 100

120 28.2 13.2 39.6

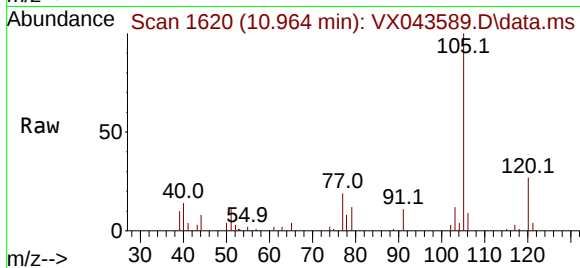

#76

1,2,3-Trichloropropane

Concen: 24.352 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX043589.D




Acq: 29 Oct 2024 12:10


Tgt Ion: 75 Resp: 62647

Ion Ratio Lower Upper

75 100

77 1.2 22.4 67.2#

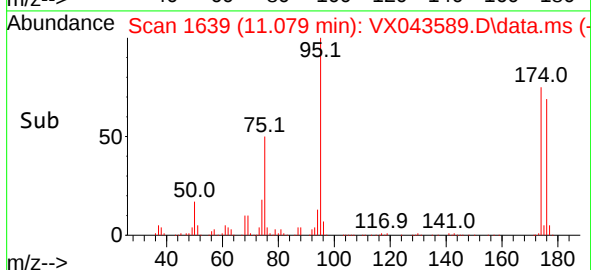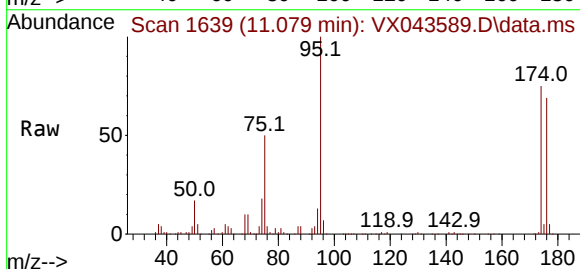



#78

n-propylbenzene

Concen: 1.486 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX043589.D

Acq: 29 Oct 2024 12:10

Instrument :

MSVOA_X

ClientSampleId :





TOTE-WATER-COMP

Tgt Ion: 91 Resp: 13813

Ion Ratio Lower Upper

91 100

120 24.2 11.6 34.7

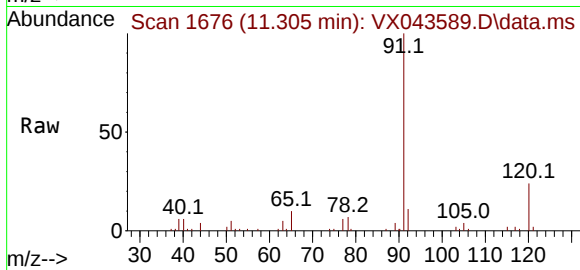

#79

2-Chlorotoluene

Concen: 1.486 ug/l

RT: 11.378 min Scan# 1688

Delta R.T. 0.012 min

Lab File: VX043589.D




Acq: 29 Oct 2024 12:10


Tgt Ion: 91 Resp: 9158

Ion Ratio Lower Upper

91 100

126 0.6 16.7 50.0#

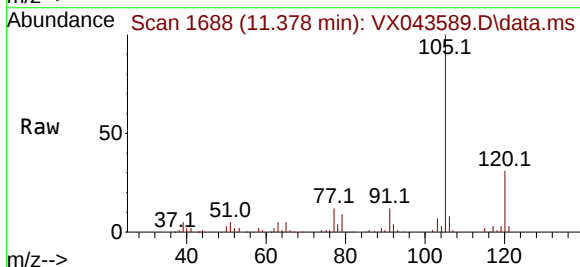

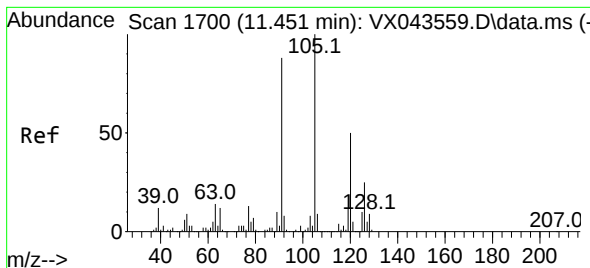

#80

1,3,5-Trimethylbenzene

Concen: 3.459 ug/l

RT: 11.451 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX043589.D

Acq: 29 Oct 2024 12:10

Instrument :

MSVOA_X

ClientSampleId :





TOTE-WATER-COMP

Tgt Ion:105 Resp: 24578

Ion Ratio Lower Upper

105 100

120 50.5 23.8 71.5

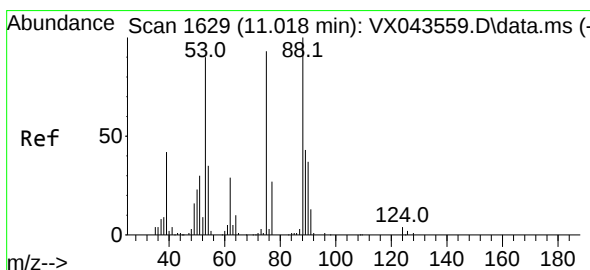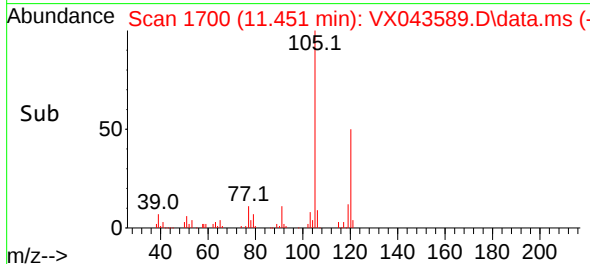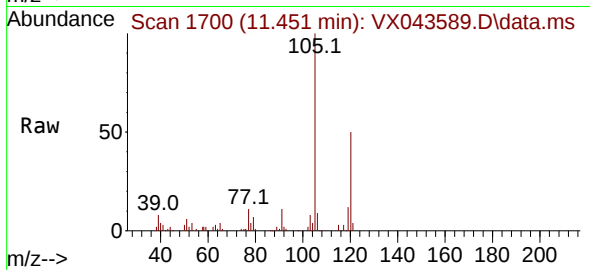

#81

trans-1,4-Dichloro-2-butene

Concen: 66.994 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX043589.D

Acq: 29 Oct 2024 12:10




Tgt Ion: 75 Resp: 62647


Ion Ratio Lower Upper

75 100

53 0.0 84.6 126.8#

89 0.0 38.6 58.0#

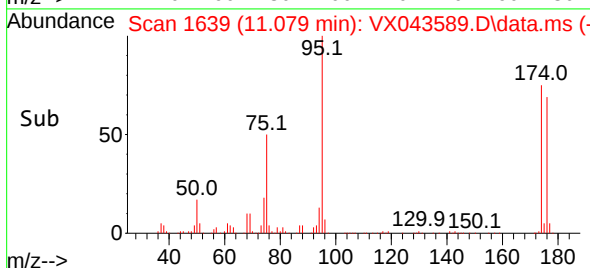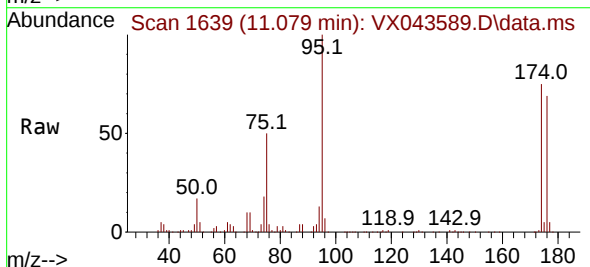



#82

4-Chlorotoluene

Concen: 0.421 ug/l

RT: 11.451 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX043589.D

Acq: 29 Oct 2024 12:10

Instrument :

MSVOA_X

ClientSampleId :





TOTE-WATER-COMP

Tgt Ion: 91 Resp: 2913

Ion Ratio Lower Upper

91 100

126 2.7 14.2 42.8#



#83

tert-Butylbenzene

Concen: 1.817 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.037 min

Lab File: VX043589.D

Acq: 29 Oct 2024 12:10




Tgt Ion: 119 Resp: 13135


Ion Ratio Lower Upper

119 100

91 89.1 29.5 88.5#

134 0.0 11.8 35.3#


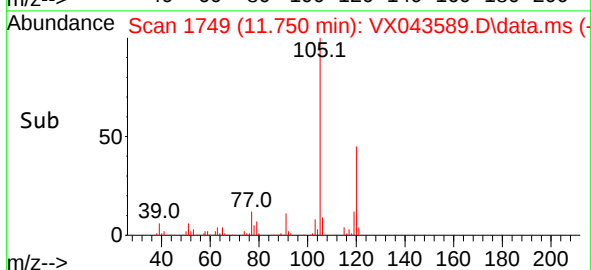






#84
1,2,4-Trimethylbenzene
Concen: 14.775 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10




Instrument :
MSVOA_X
ClientSampleId :
TOTE-WATER-COMP


Tgt Ion:105 Resp: 107004
Ion Ratio Lower Upper
105 100
120 45.3 22.1 66.1

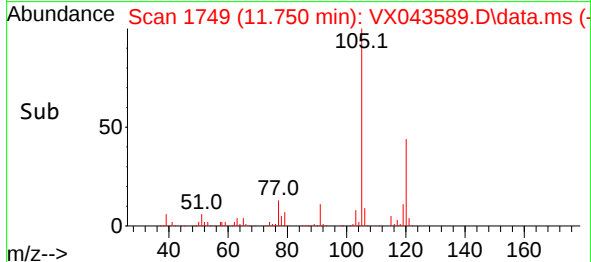

#85
sec-Butylbenzene
Concen: 0.769 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. 0.000 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10

Tgt Ion:105 Resp: 6514
Ion Ratio Lower Upper
105 100
134 22.2 9.8 29.5


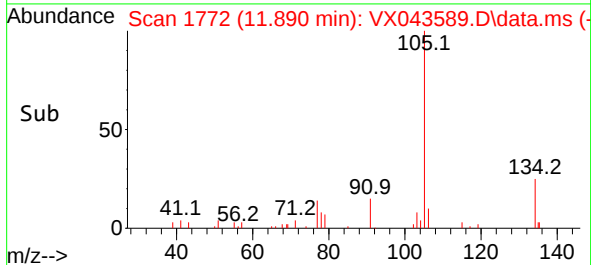






#86
p-Isopropyltoluene
Concen: 0.656 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. 0.000 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10




Instrument :
MSVOA_X
ClientSampleId :
TOTE-WATER-COMP


Tgt Ion:119 Resp: 4724
Ion Ratio Lower Upper
119 100
134 30.5 13.1 39.1
91 26.0 12.4 37.0

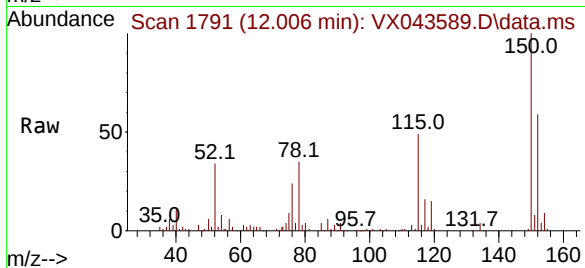

#89
n-Butylbenzene
Concen: 1.680 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. 0.000 min
Lab File: VX043589.D
Acq: 29 Oct 2024 12:10

Tgt Ion: 91 Resp: 9857
Ion Ratio Lower Upper
91 100
92 32.1 27.1 81.2
134 106.9 12.9 38.6#

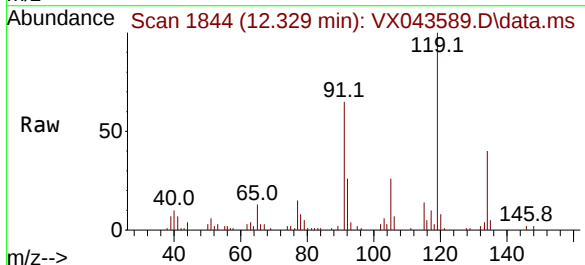



#90

Hexachloroethane

Concen: 1.766 ug/l

RT: 12.530 min Scan# 117

Delta R.T. -0.006 min

Lab File: VX043589.D

Acq: 29 Oct 2024 12:10

Instrument :

MSVOA_X

ClientSampleId :





TOTE-WATER-COMP

Tgt Ion:117 Resp: 2065

Ion Ratio Lower Upper

117 100

201 0.0 32.9 98.7#

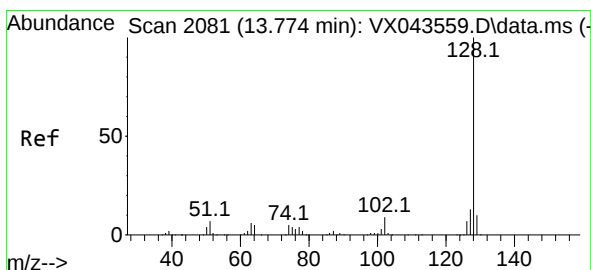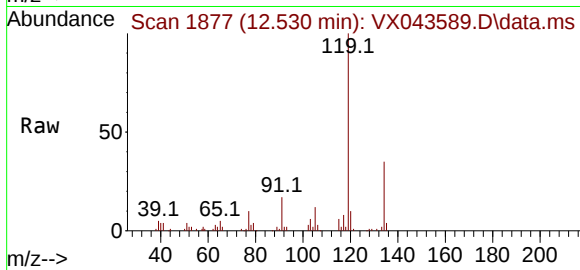

#95

Naphthalene

Concen: 4.930 ug/l

RT: 13.774 min Scan# 2081

Delta R.T. 0.000 min

Lab File: VX043589.D

Acq: 29 Oct 2024 12:10

Tgt Ion:128 Resp: 46188

Ion Ratio Lower Upper

128 100

127 12.6 10.2 15.4

129 11.6 8.7 13.1

