

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102924\
 Data File : VX043590.D
 Acq On : 29 Oct 2024 12:33
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK

Quant Time: Oct 30 01:30:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 28 13:41:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	139591	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	257439	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	221732	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	101113	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	95576	42.940	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	85.880%
35) Dibromofluoromethane	5.385	113	78818	45.150	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	90.300%
50) Toluene-d8	8.647	98	300341	49.701	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.400%
62) 4-Bromofluorobenzene	11.079	95	107919	48.195	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	96.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102924\
Data File : VX043590.D
Acq On : 29 Oct 2024 12:33
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK

Quant Time: Oct 30 01:30:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
Quant Title : SW846 8260
QLast Update : Mon Oct 28 13:41:34 2024
Response via : Initial Calibration




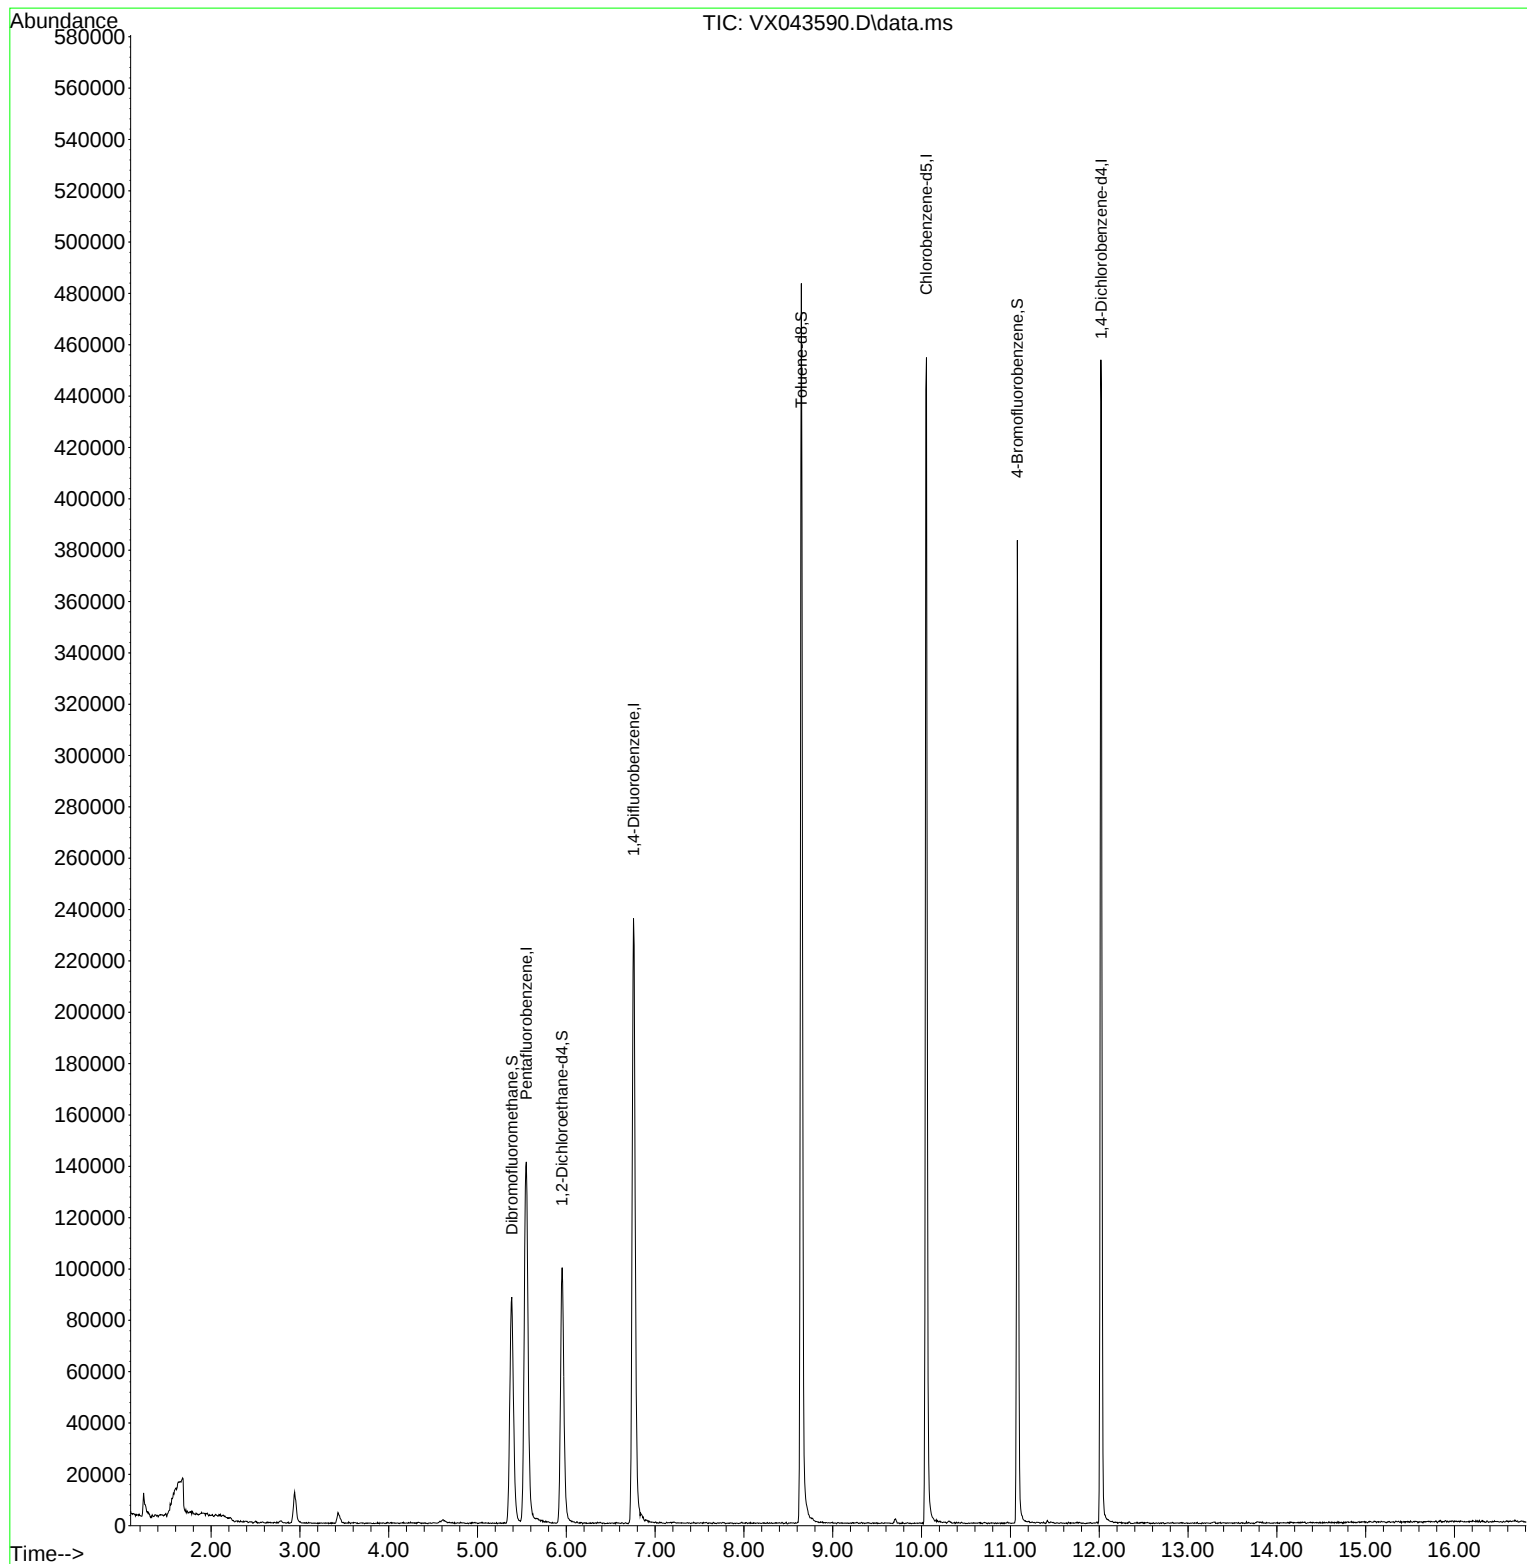


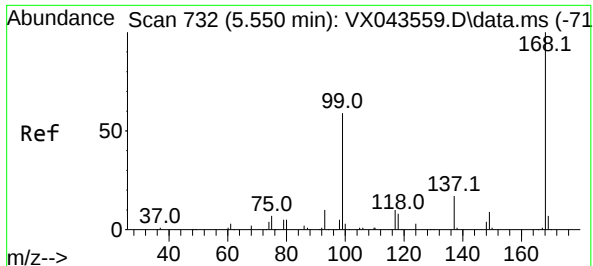

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.000 min
Lab File: VX043590.D
Acq: 29 Oct 2024 12:33




Instrument :
MSVOA_X
ClientSampleId :
VIBLK


Tgt Ion:168 Resp: 139591
Ion Ratio Lower Upper
168 100
99 62.7 52.6 78.8

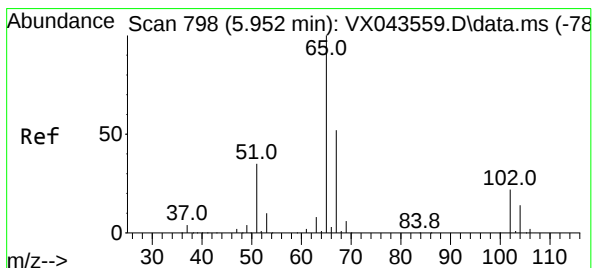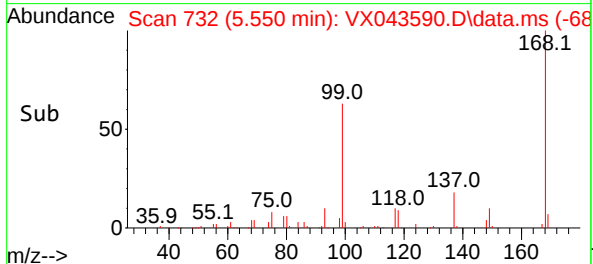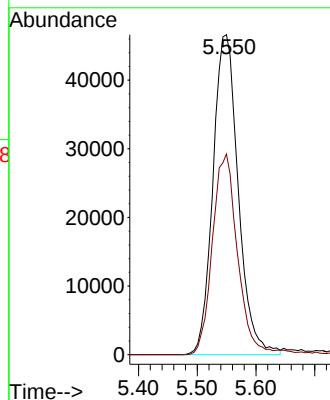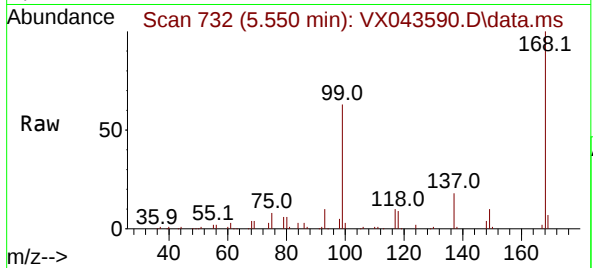

#33
1,2-Dichloroethane-d4
Concen: 42.940 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX043590.D
Acq: 29 Oct 2024 12:33

Tgt Ion: 65 Resp: 95576
Ion Ratio Lower Upper
65 100
67 53.1 0.0 103.4


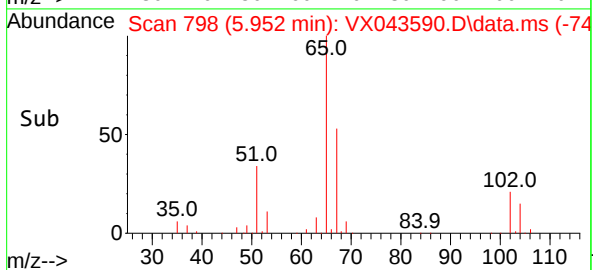
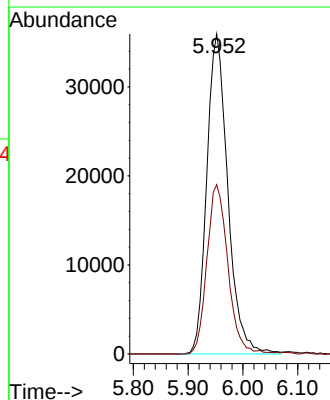
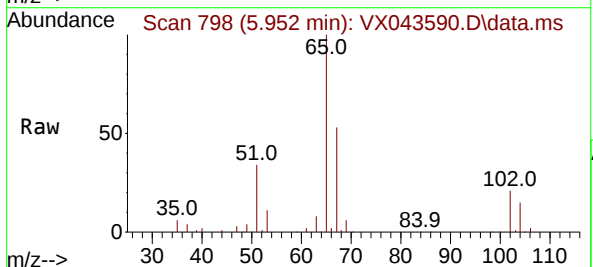


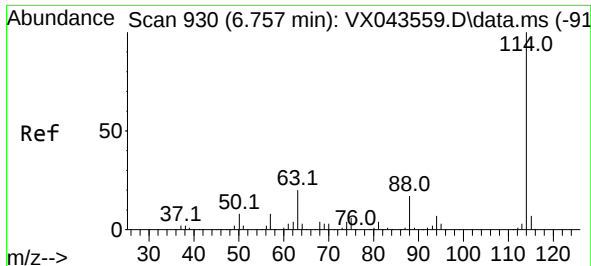

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX043590.D
Acq: 29 Oct 2024 12:33




Instrument :
MSVOA_X
ClientSampleId :
VIBLK


Tgt Ion:114 Resp: 257439
Ion Ratio Lower Upper
114 100
63 19.1 0.0 41.2
88 15.6 0.0 34.0

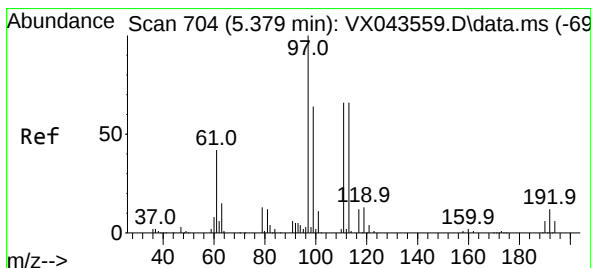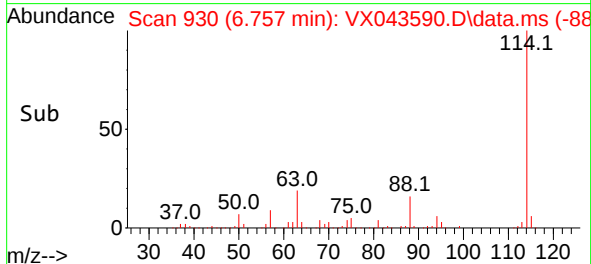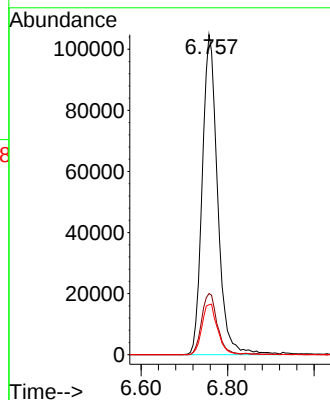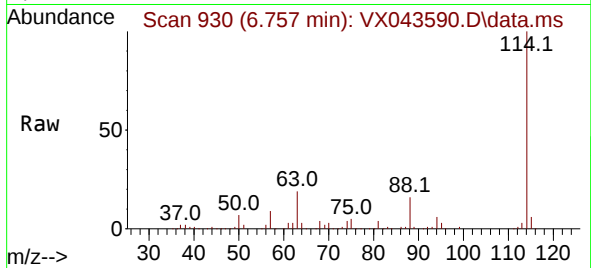

#35
Dibromofluoromethane
Concen: 45.150 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX043590.D
Acq: 29 Oct 2024 12:33

Tgt Ion:113 Resp: 78818
Ion Ratio Lower Upper
113 100
111 102.6 81.4 122.0
192 17.5 14.1 21.1


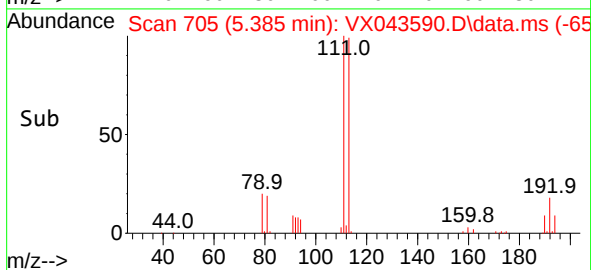
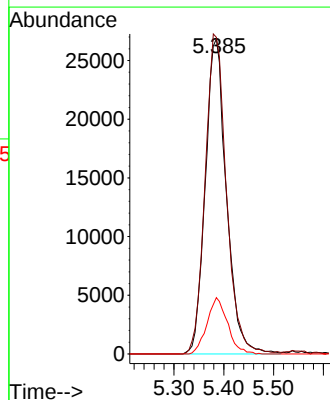
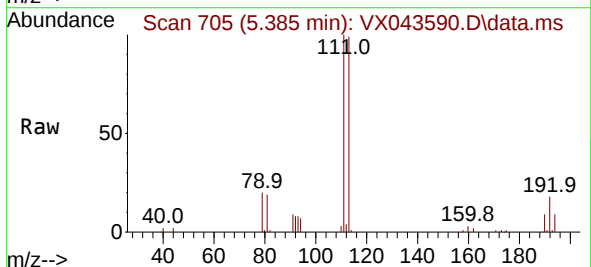


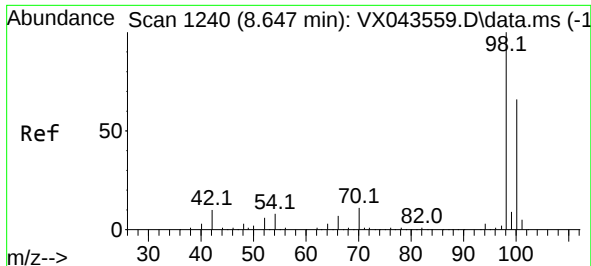

#50
Toluene-d8
Concen: 49.701 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX043590.D
Acq: 29 Oct 2024 12:33




Instrument :
MSVOA_X
ClientSampleId :
VIBLK


Tgt Ion: 98 Resp: 300341
Ion Ratio Lower Upper
98 100
100 67.0 53.4 80.2

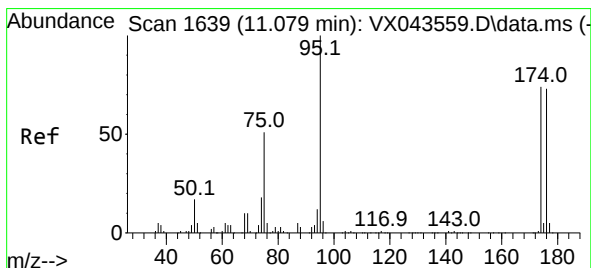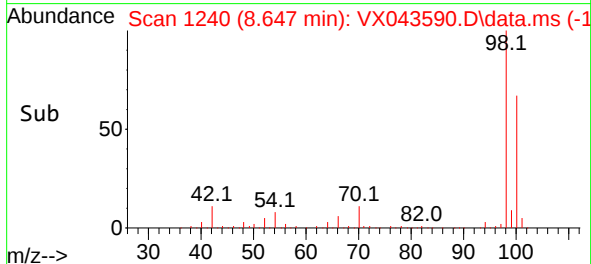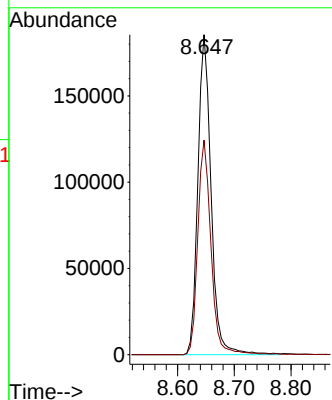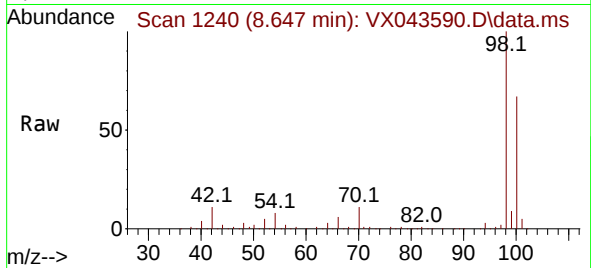

#62
4-Bromofluorobenzene
Concen: 48.195 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX043590.D
Acq: 29 Oct 2024 12:33

Tgt Ion: 95 Resp: 107919
Ion Ratio Lower Upper
95 100
174 72.6 0.0 146.6
176 71.3 0.0 139.6


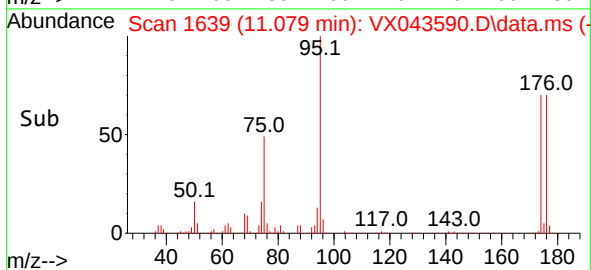
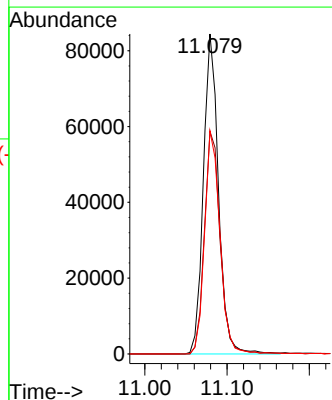
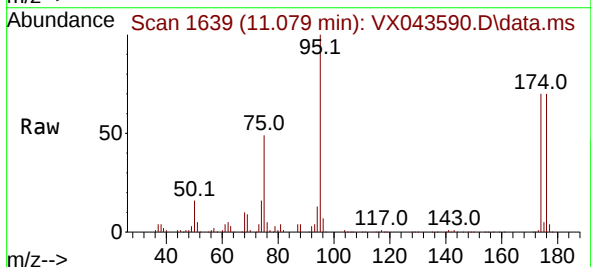


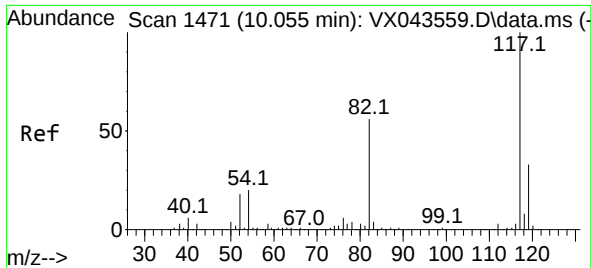

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX043590.D
Acq: 29 Oct 2024 12:33

Instrument :
MSVOA_X
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 221732
Ion Ratio Lower Upper
117 100
82 53.0 42.1 63.1
119 33.1 25.4 38.2

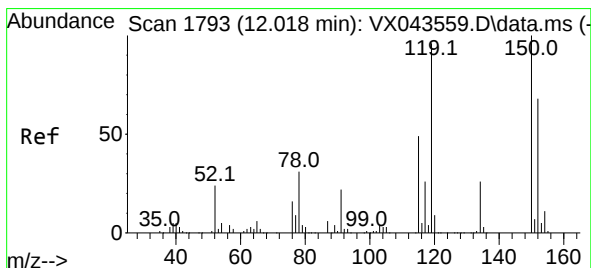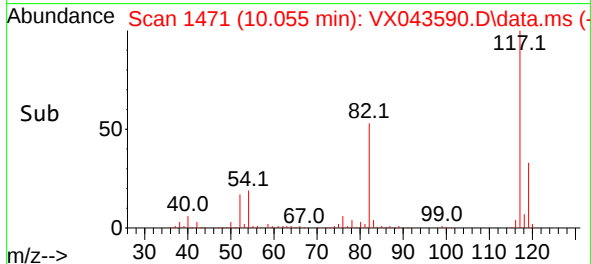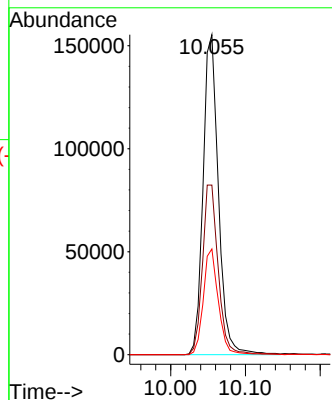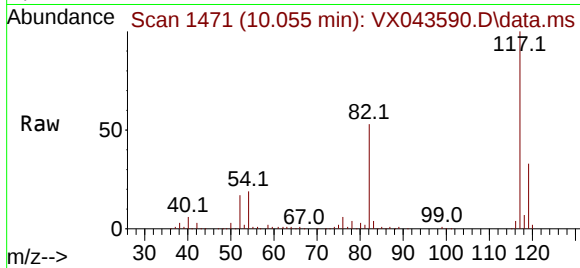

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX043590.D
Acq: 29 Oct 2024 12:33

Tgt Ion:152 Resp: 101113
Ion Ratio Lower Upper
152 100
115 59.5 42.9 128.7
150 154.2 0.0 343.6

