
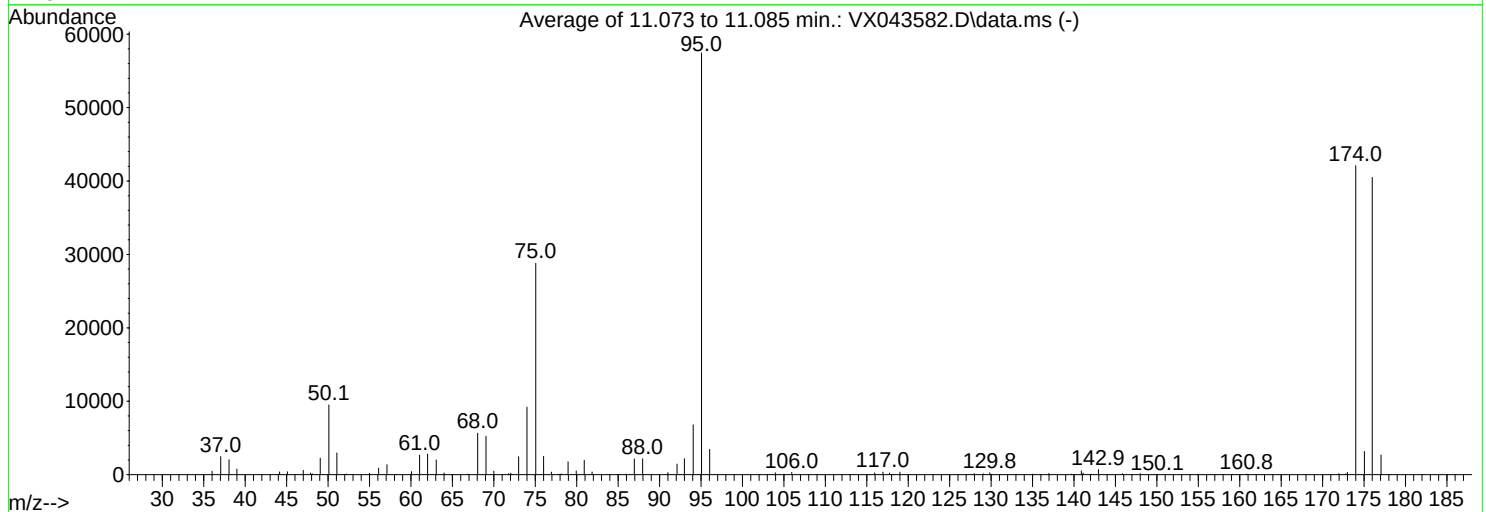


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102924\
Data File : VX043582.D
Acq On : 29 Oct 2024 08:30
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
Title : SW846 8260
Last Update : Mon Oct 28 13:41:34 2024

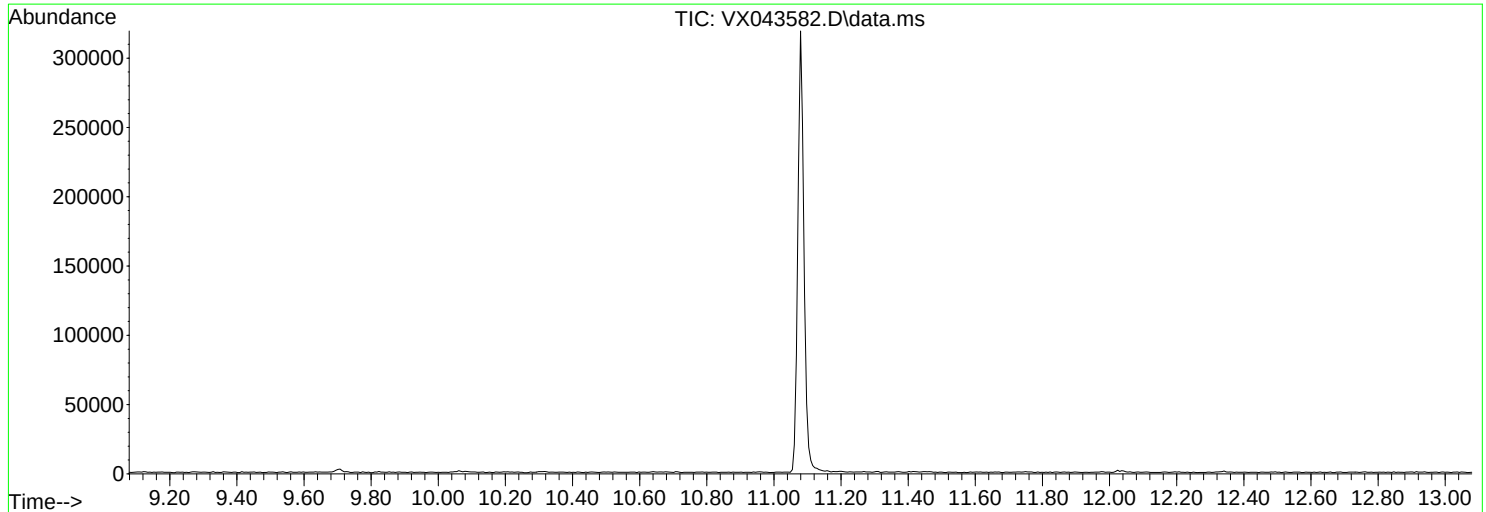

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.5	9509	PASS
75	95	30	60	50.1	28803	PASS
95	95	100	100	100.0	57464	PASS
96	95	5	9	6.0	3434	PASS
173	174	0.00	2	0.7	307	PASS
174	95	50	100	73.3	42096	PASS
175	174	5	9	7.5	3171	PASS
176	174	95	101	96.2	40501	PASS
177	176	5	9	6.6	2676	PASS