



Chloroethane

Response Ratio

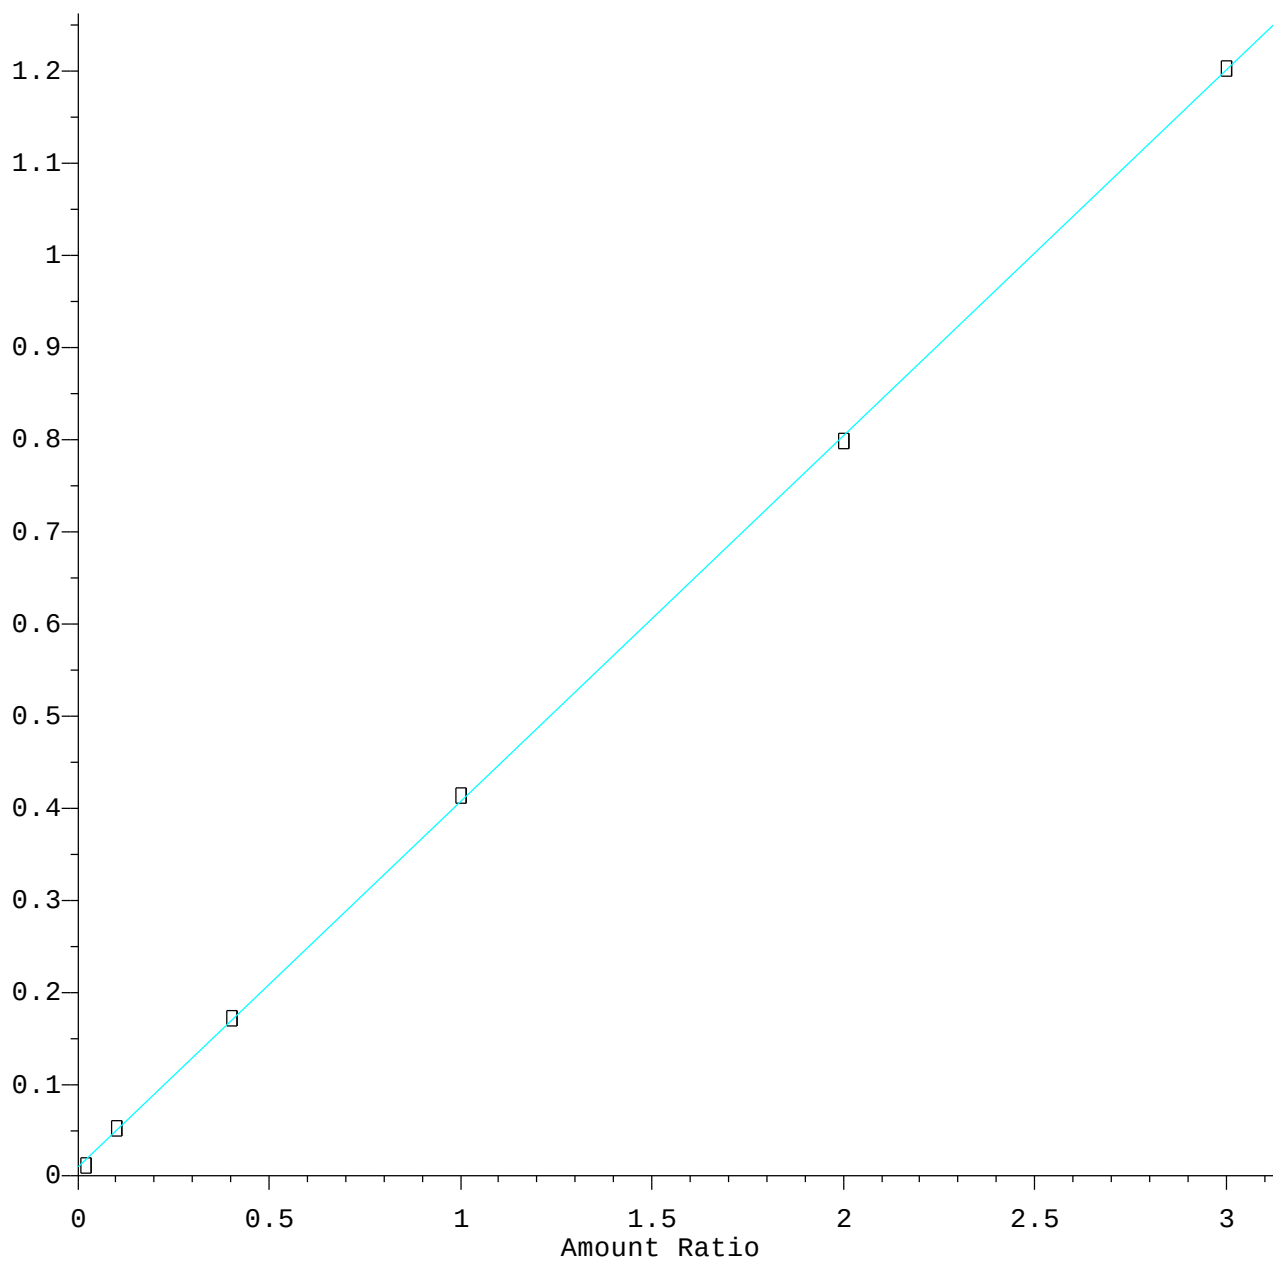


Resp Ratio = $3.97 \times 10^{-1} \times \text{Amt} + 9.69 \times 10^{-3}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Calibration Table Last Updated: Sat Nov 02 07:06:38 2019

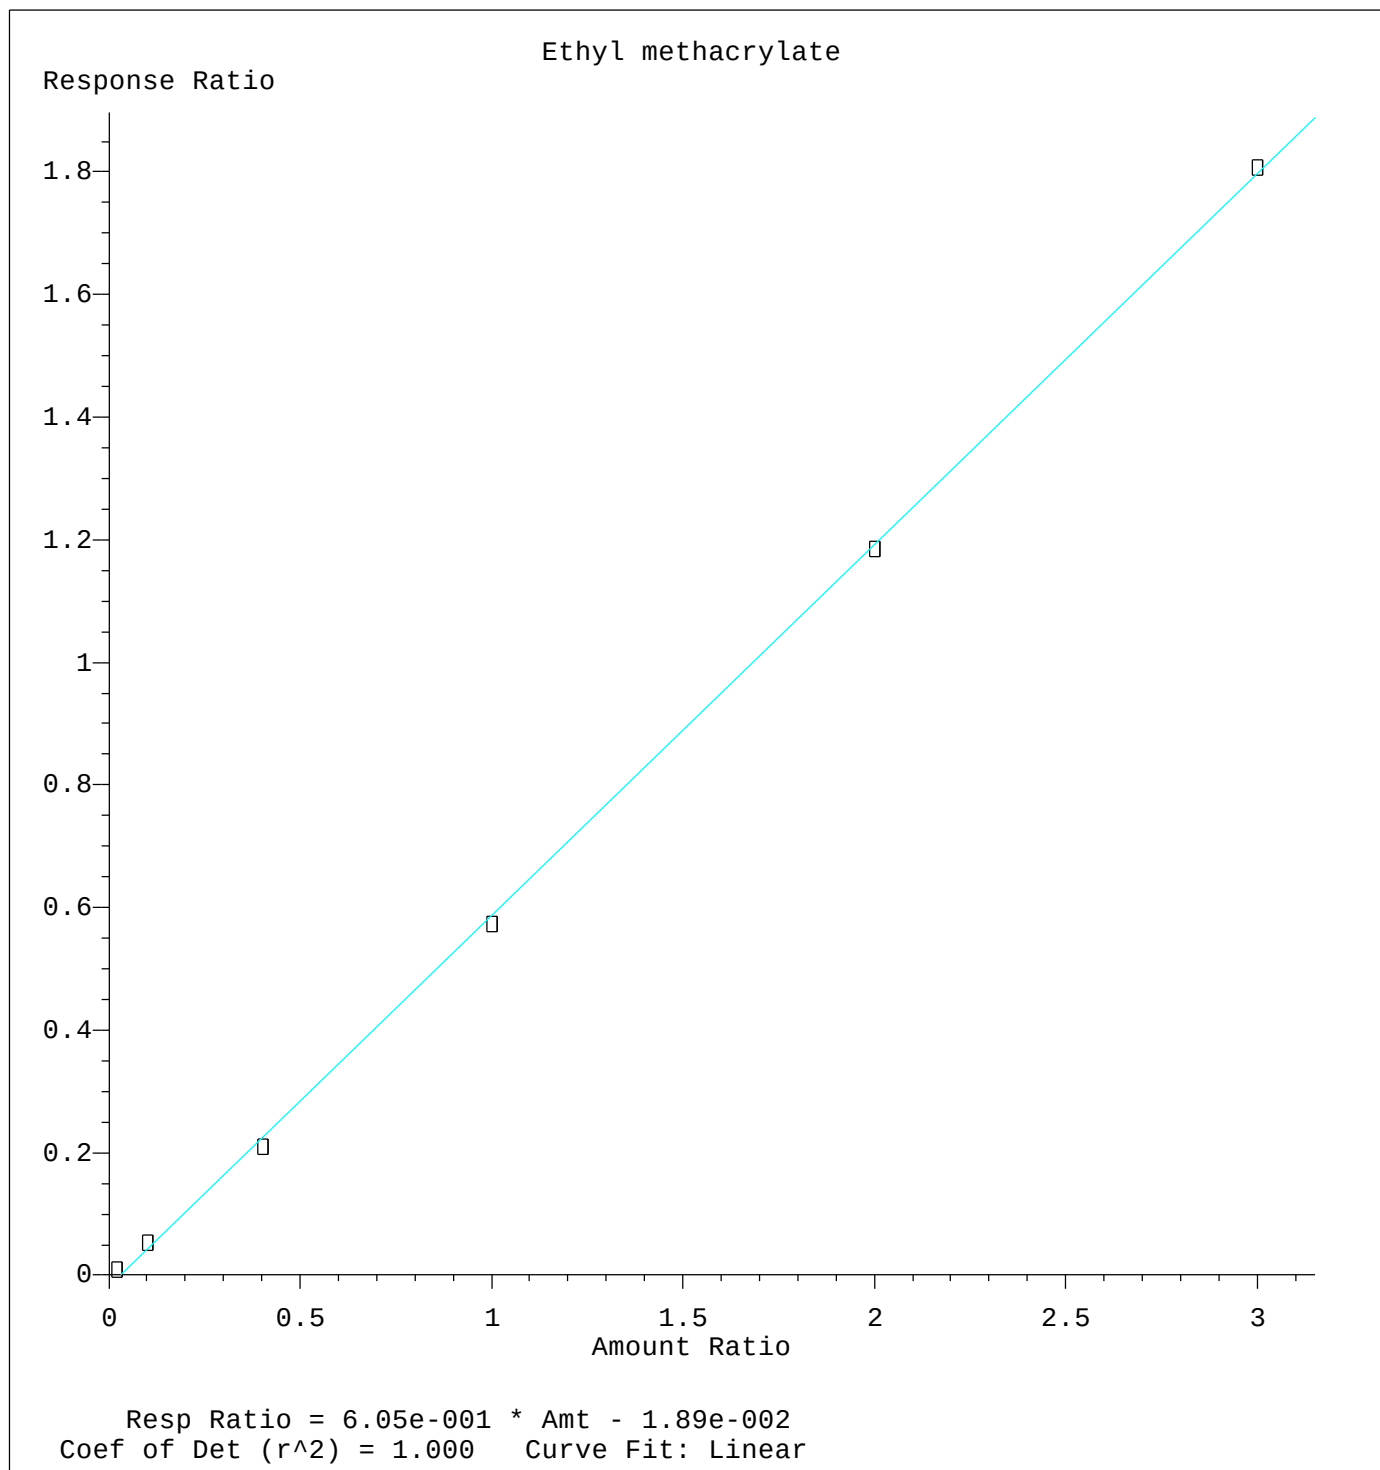

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Calibration Table Last Updated: Sat Nov 02 07:06:38 2019

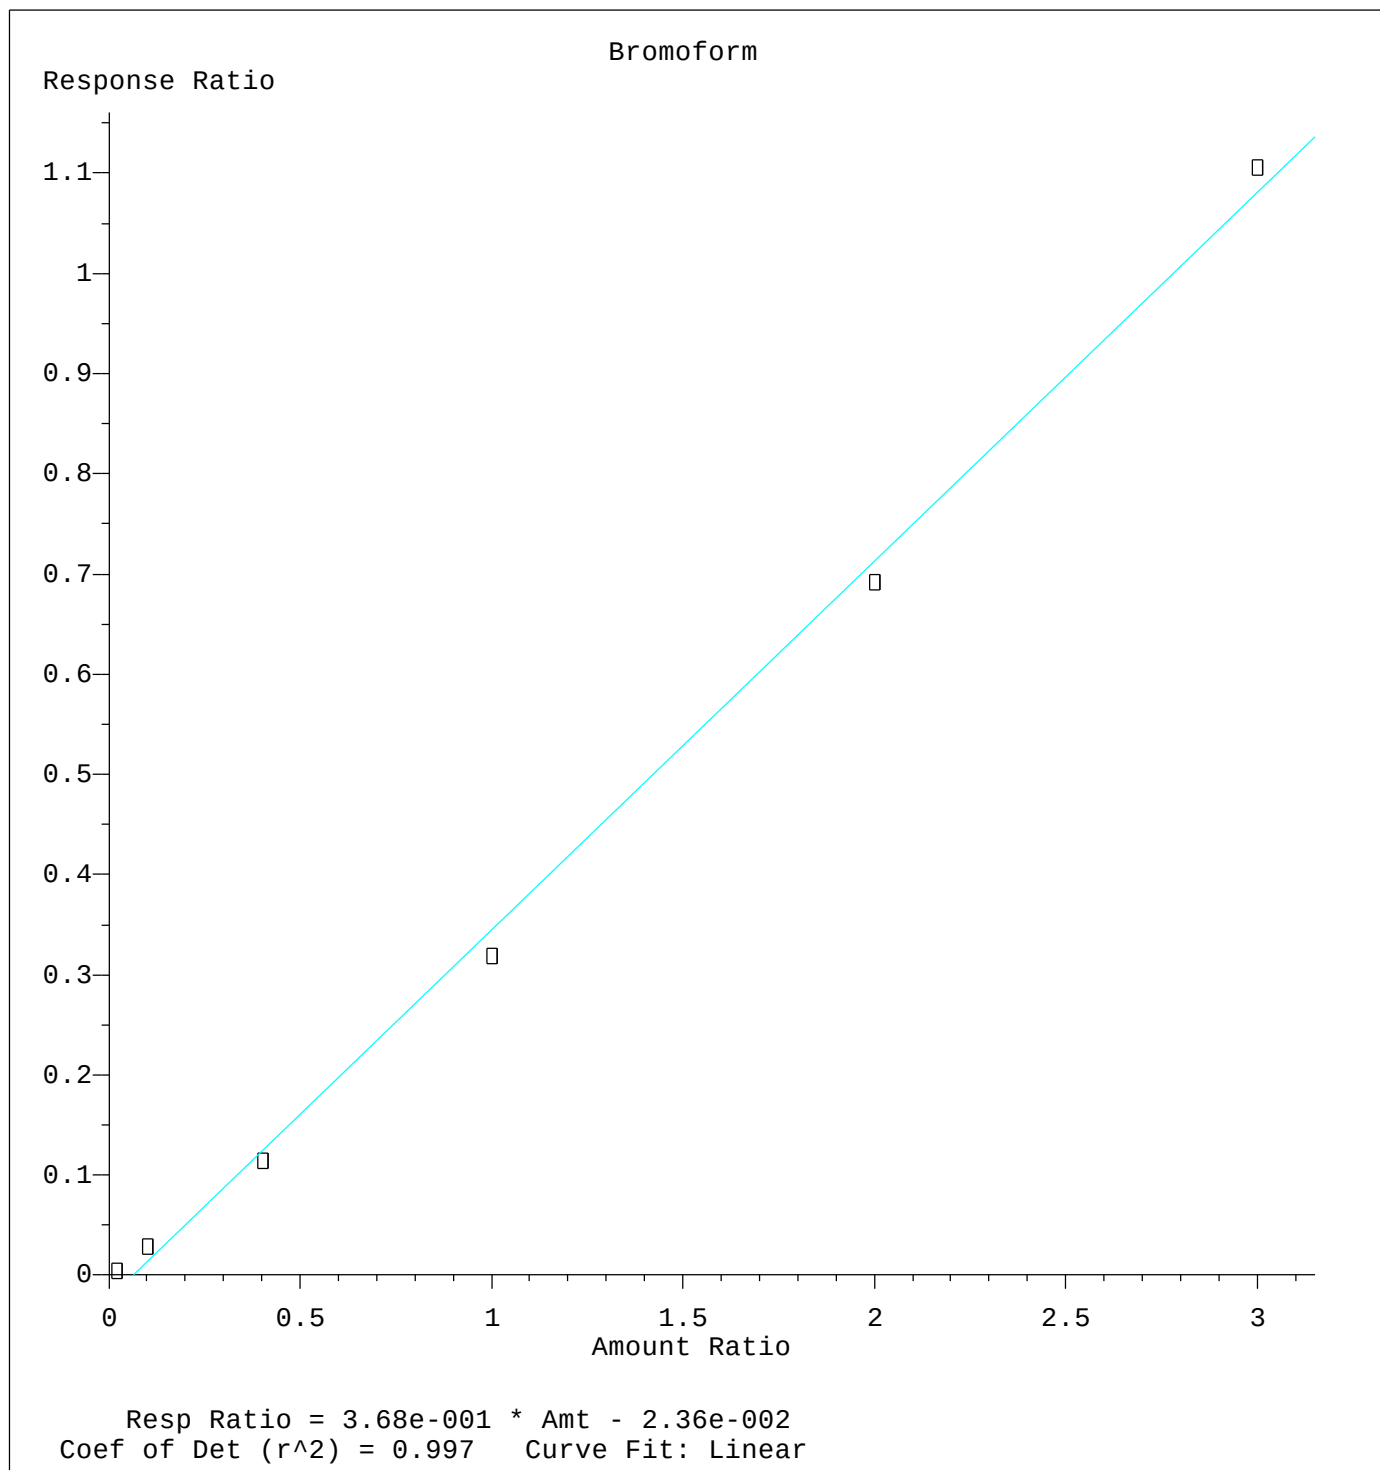

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Calibration Table Last Updated: Sat Nov 02 07:06:38 2019