

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX103124\
Data File : VX043650.D
Acq On : 31 Oct 2024 14:50
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
Title : SW846 8260

Signal : TIC: VX043650.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	68	84	85	rBV9	10236	32806	5.50%	1.038%
2	4.593	564	575	586	rBV2	4994	18395	3.08%	0.582%
3	5.385	694	705	720	rBV2	65564	196926	33.00%	6.230%
4	5.550	720	732	746	rBV	107142	313428	52.52%	9.916%
5	5.952	787	798	812	rBV2	75349	203901	34.16%	6.451%
6	6.757	919	930	944	rBV	178938	438137	73.41%	13.862%
7	8.647	1234	1240	1264	rBV	359127	596820	100.00%	18.882%
8	10.055	1465	1471	1488	rBV	352421	517810	86.76%	16.382%
9	11.079	1634	1639	1653	rBV	290789	383589	64.27%	12.136%
10	12.018	1788	1793	1803	rBV	347926	458993	76.91%	14.521%




Sum of corrected areas: 3160805

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX103124\
Data File : VX043650.D
Acq On : 31 Oct 2024 14:50
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

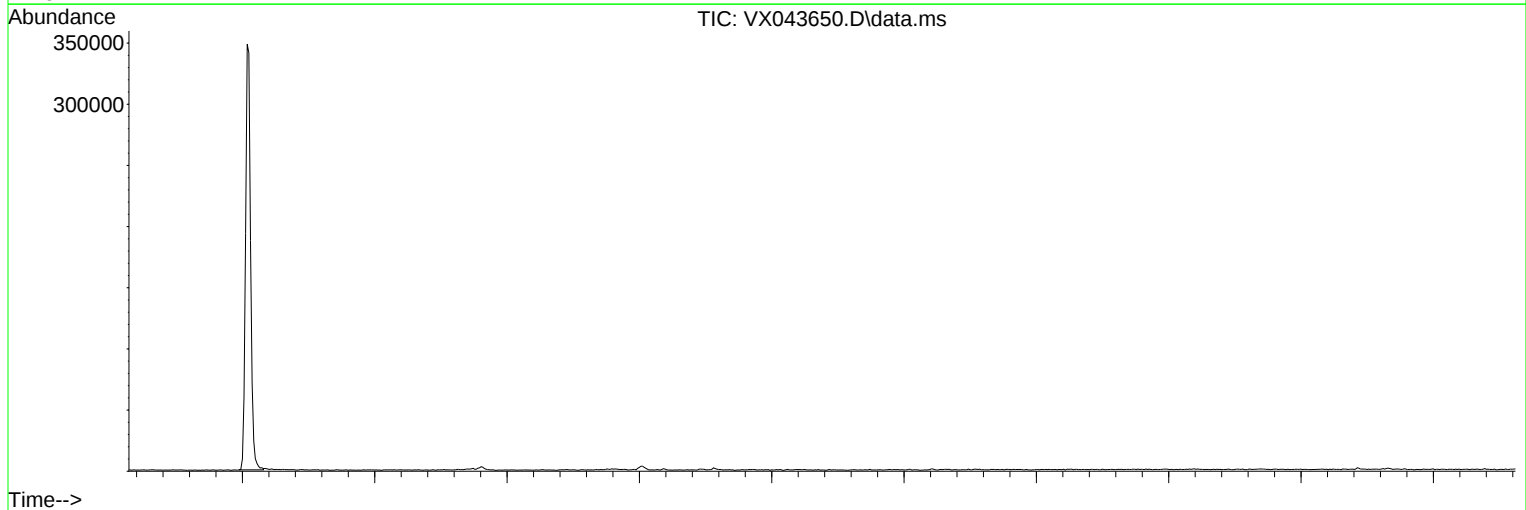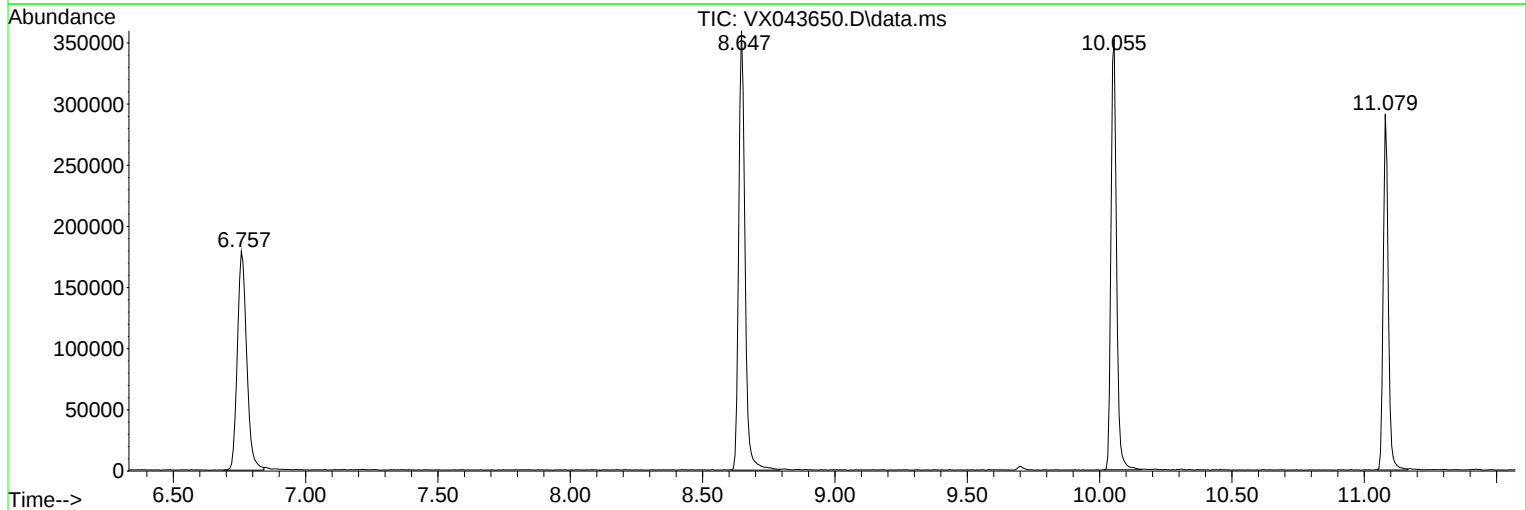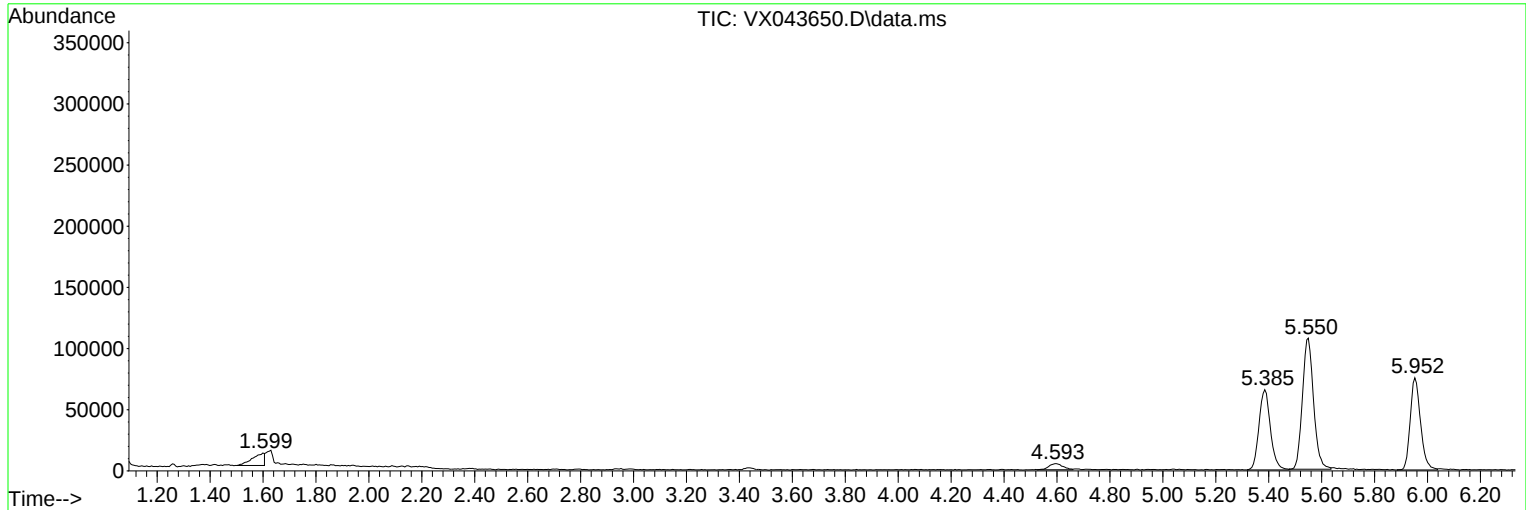

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX103124\
Data File : VX043650.D
Acq On : 31 Oct 2024 14:50
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
Quant Title : SW846 8260










TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.599 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.599	5.23 ug/l	32806	Pentafluorobenzene	5.550

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	bis(chloromethyl) carbonate	158	C3H4Cl2O3	1000404-37-0	10
2	Carbonochloridic acid, chloromet...	128	C2H2Cl2O2	022128-62-7	9
3	Dimethyl Sulfoxide	78	C2H6OS	000067-68-5	9
4	(S)-(+)-2-Chloro-1-propanol	94	C3H7ClO	019210-21-0	5
5	Boron trifluoride	68	BF3	007637-07-2	4

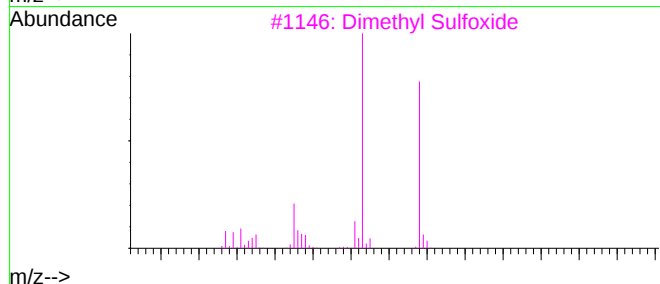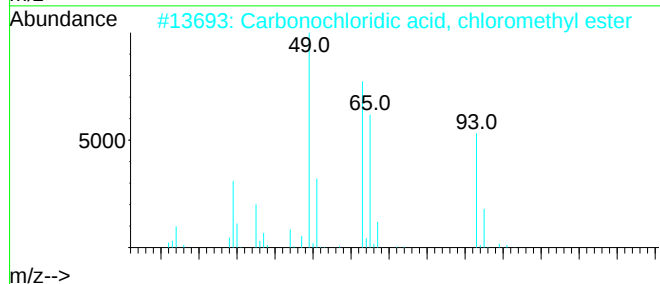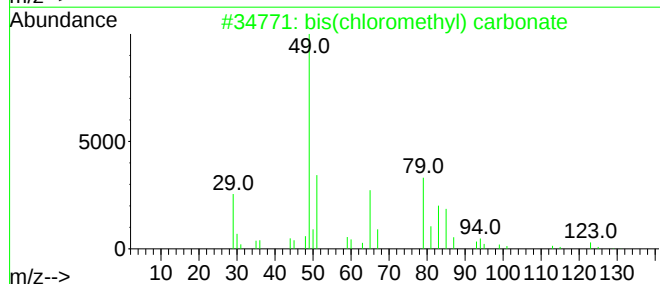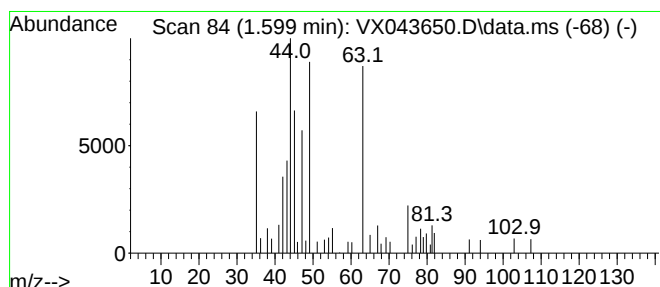

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX103124\
Data File : VX043650.D
Acq On : 31 Oct 2024 14:50
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.599	1.599	5.2	ug/l	32806	1	5.550	313428	50.0