

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110124\
 Data File : VX043662.D
 Acq On : 01 Nov 2024 14:20
 Operator : JC/MD
 Sample : P4676-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Storage-Blank-WATER-REF-5

Quant Time: Nov 04 06:12:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 28 13:41:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	139714	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	251731	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	212258	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	86030	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	92244	41.406	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	82.820%
35) Dibromofluoromethane	5.379	113	79001	46.281	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.560%
50) Toluene-d8	8.647	98	295353	49.984	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.960%
62) 4-Bromofluorobenzene	11.079	95	95866	43.783	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	87.560%


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110124\
Data File : VX043662.D
Acq On : 01 Nov 2024 14:20
Operator : JC/MD
Sample : P4676-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-5


Quant Time: Nov 04 06:12:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
Quant Title : SW846 8260
QLast Update : Mon Oct 28 13:41:34 2024
Response via : Initial Calibration

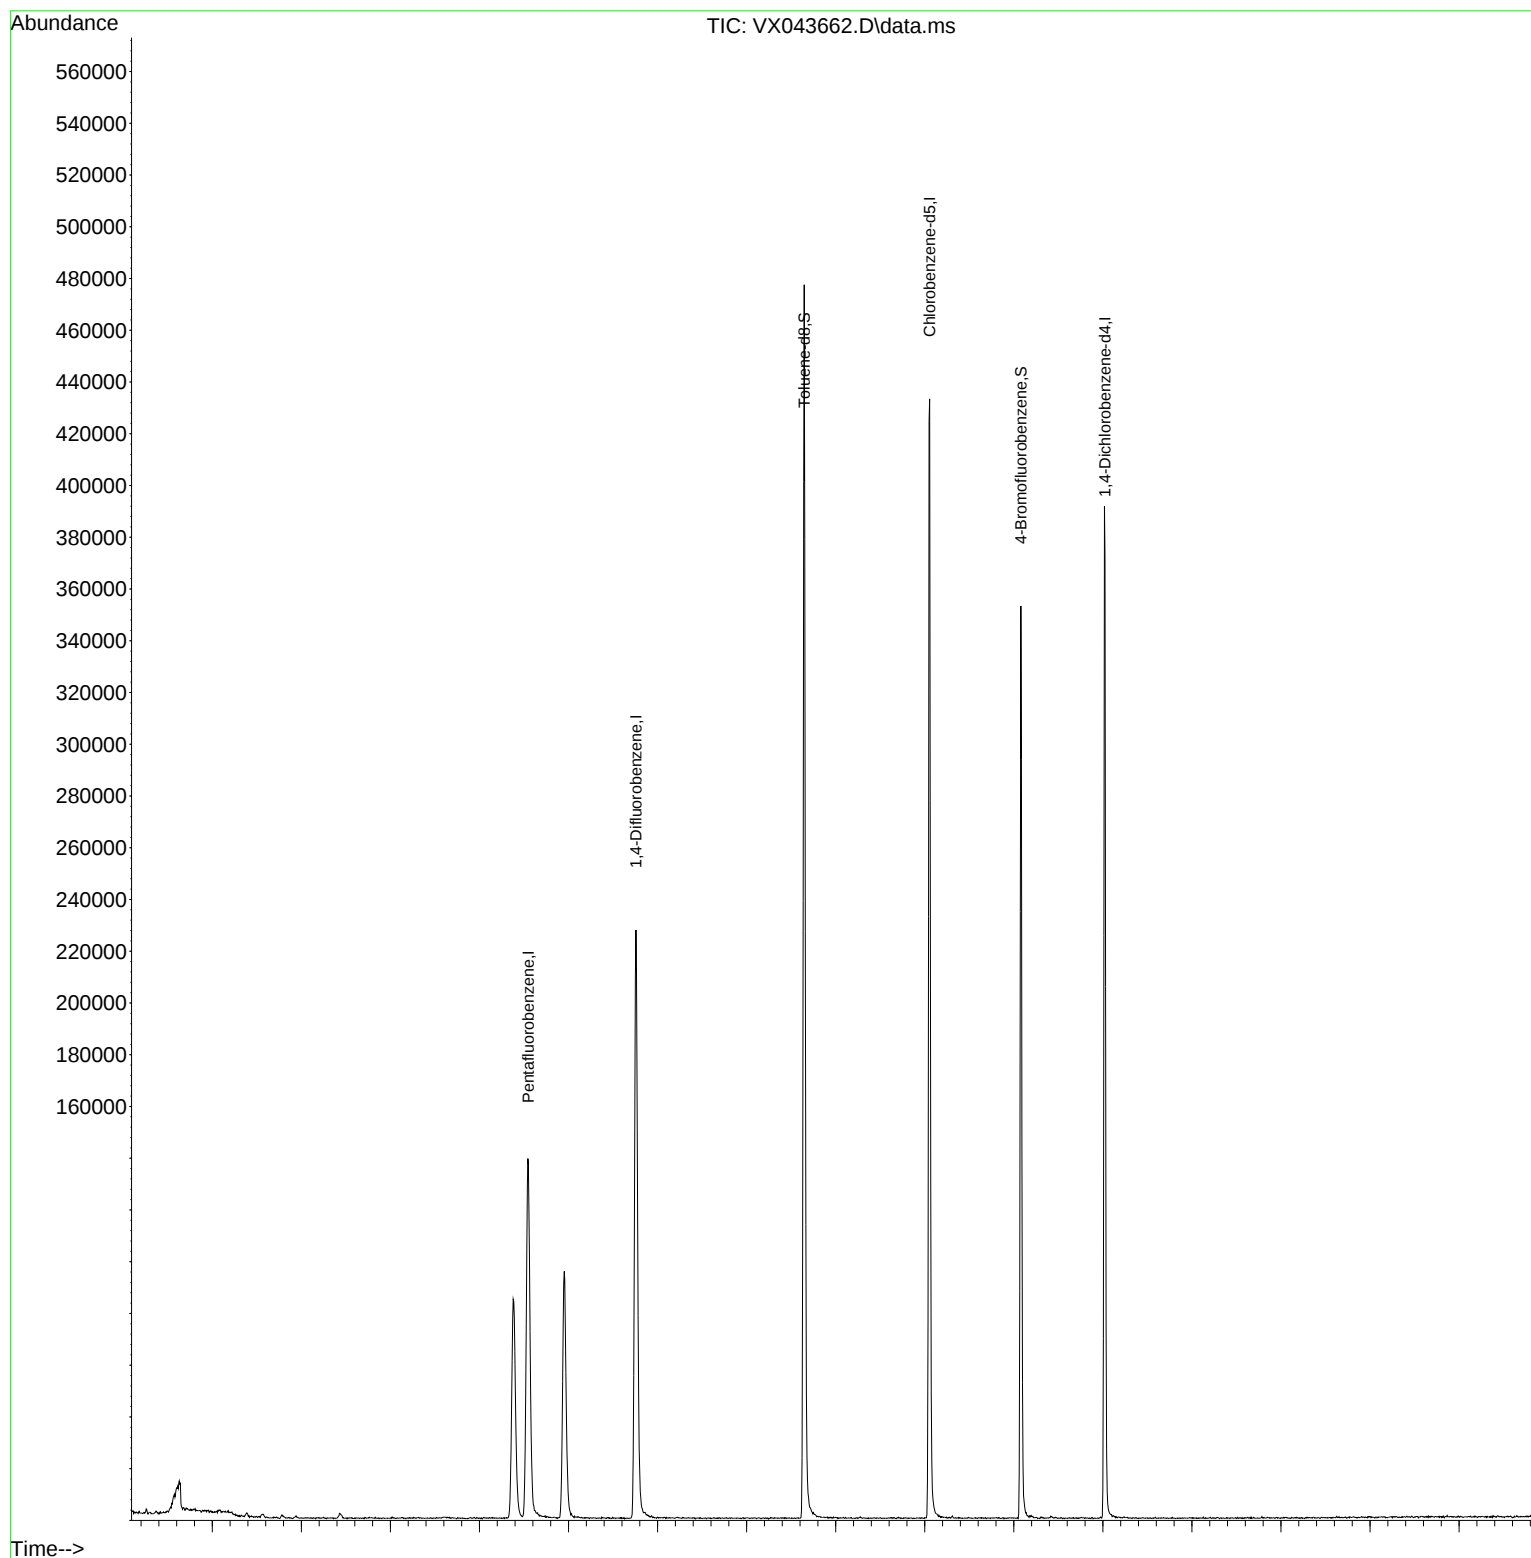



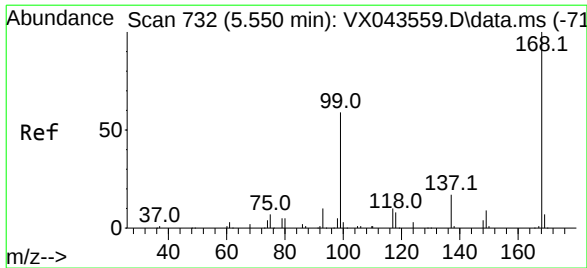


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.000 min
Lab File: VX043662.D
Acq: 01 Nov 2024 14:20

Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-5



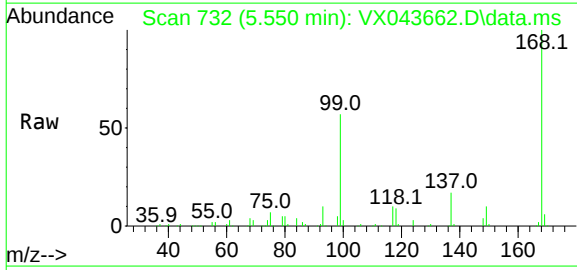



Tgt Ion: 168 Resp: 139714
Ion Ratio Lower Upper
168 100
99 56.9 52.6 78.8

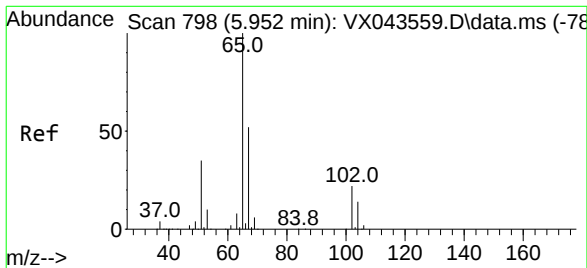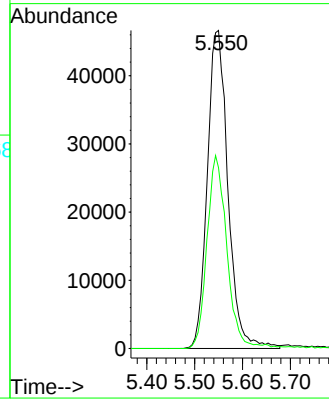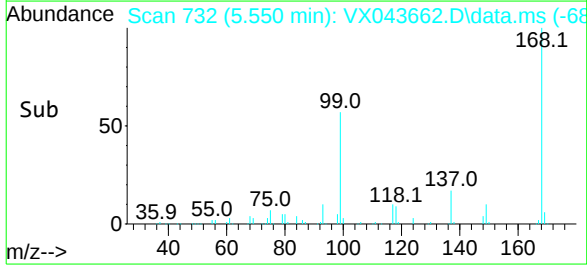

#33
1,2-Dichloroethane-d4
Concen: 41.406 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX043662.D
Acq: 01 Nov 2024 14:20

Tgt Ion: 65 Resp: 92244
Ion Ratio Lower Upper
65 100
67 53.8 0.0 103.4


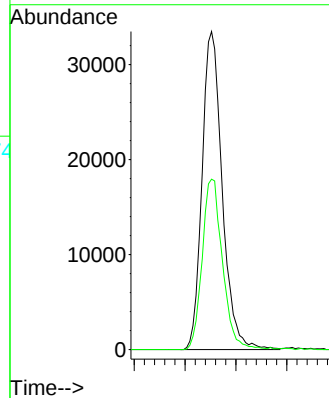
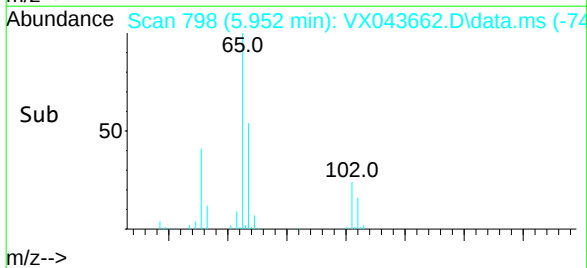
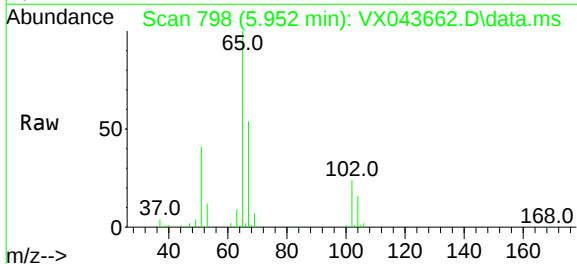


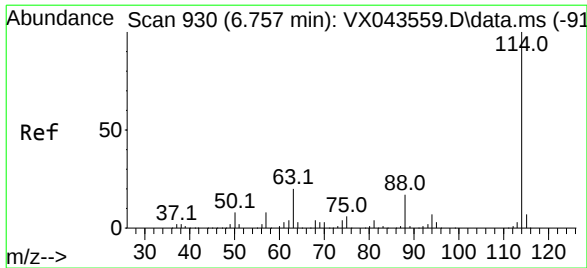

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. 0.000 min
Lab File: VX043662.D
Acq: 01 Nov 2024 14:20




Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-5


Tgt Ion:	114	Resp:	251731
Ion	Ratio	Lower	Upper
114	100		
63	18.0	0.0	41.2
88	16.3	0.0	34.0

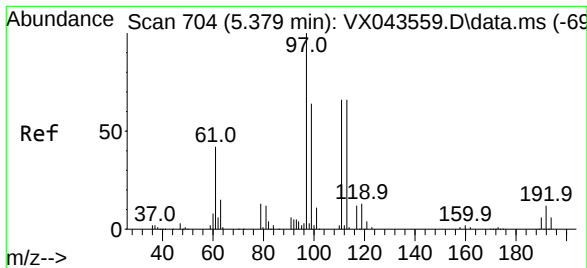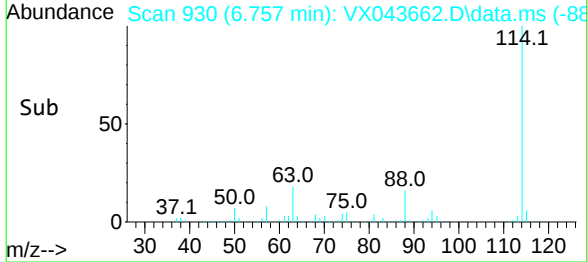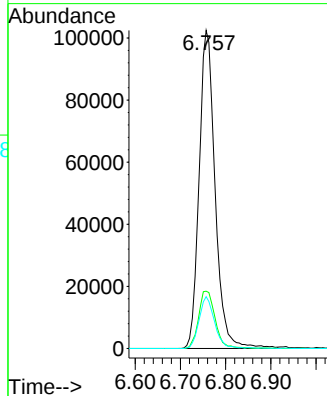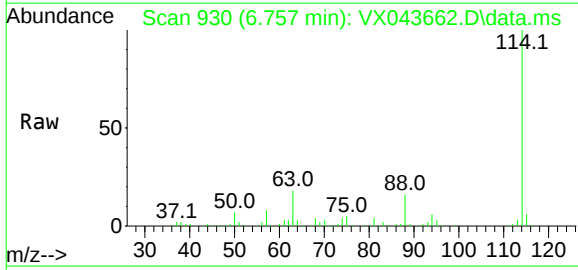

#35
Dibromofluoromethane
Concen: 46.281 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX043662.D
Acq: 01 Nov 2024 14:20

Tgt Ion:	113	Resp:	79001
Ion	Ratio	Lower	Upper
113	100		
111	100.7	81.4	122.0
192	18.5	14.1	21.1

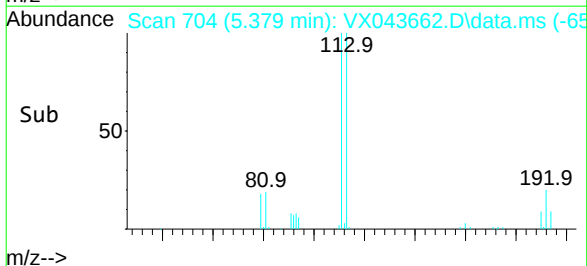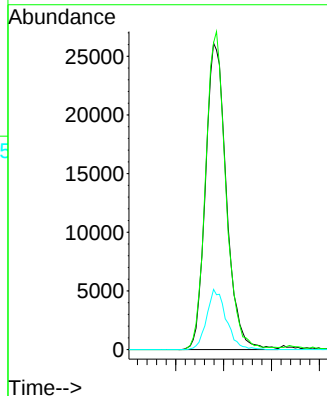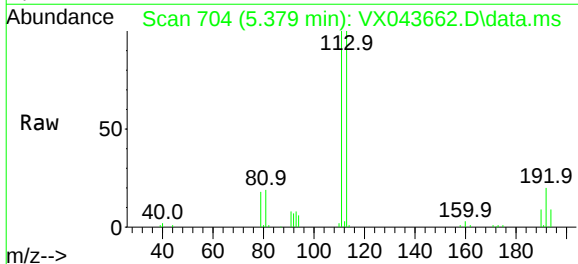

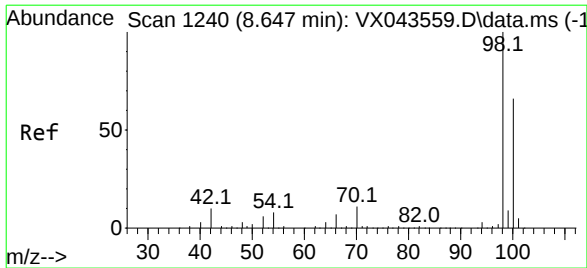

#50

Toluene-d8

Concen: 49.984 ug/l

RT: 8.647 min Scan# 12

Delta R.T. 0.000 min

Lab File: VX043662.D

Acq: 01 Nov 2024 14:20

Instrument :

MSVOA_X

ClientSampleId :





Storage-Blank-WATER-REF-5

Tgt Ion: 98 Resp: 295353

Ion Ratio Lower Upper

98 100

100 67.8 53.4 80.2

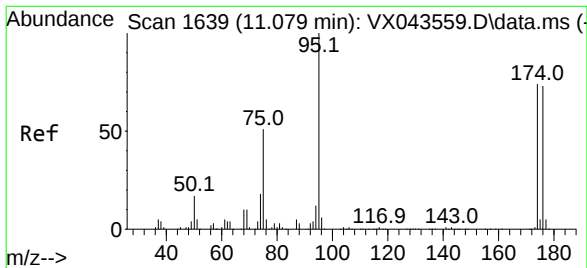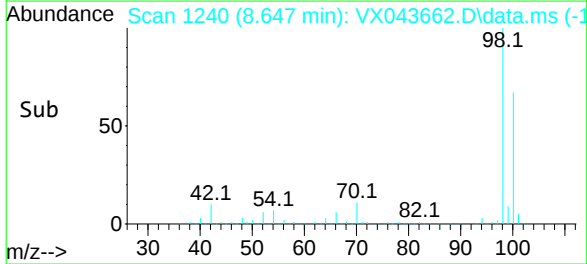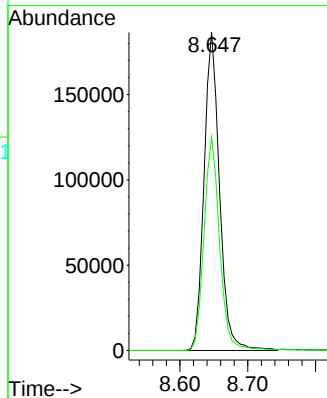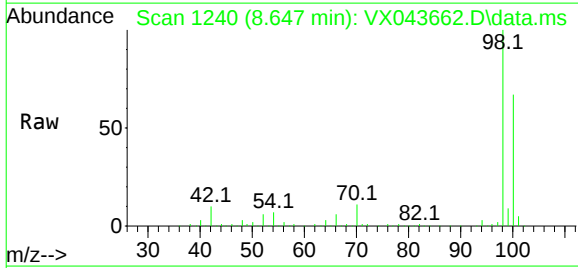

#62

4-Bromofluorobenzene

Concen: 43.783 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX043662.D

Acq: 01 Nov 2024 14:20




Tgt Ion: 95 Resp: 95866


Ion Ratio Lower Upper

95 100

174 78.4 0.0 146.6

176 75.7 0.0 139.6

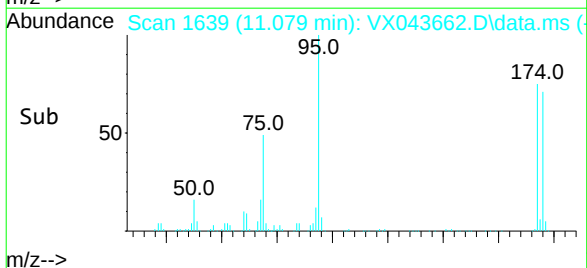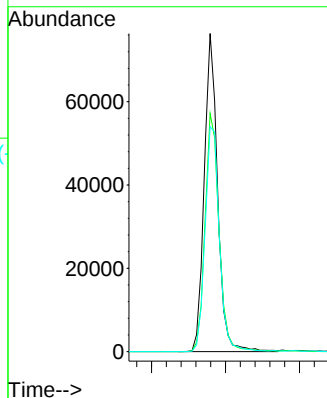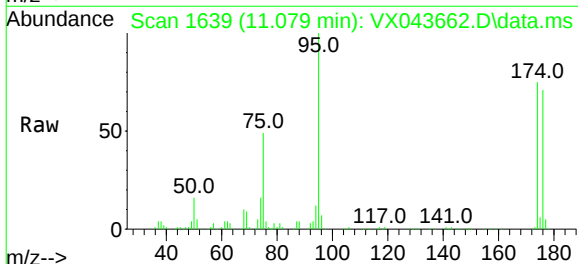

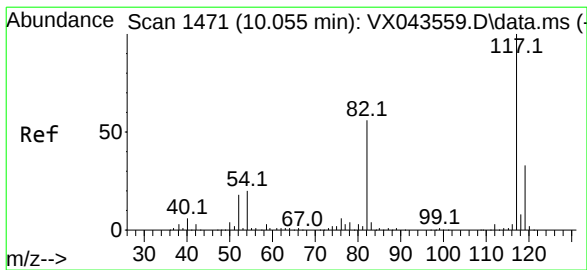

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX043662.D

Acq: 01 Nov 2024 14:20

Instrument :

MSVOA_X

ClientSampleId :

Storage-Blank-WATER-REF-5





Tgt Ion:117 Resp: 212258

Ion Ratio Lower Upper

117 100

82 52.4 42.1 63.1

119 33.0 25.4 38.2

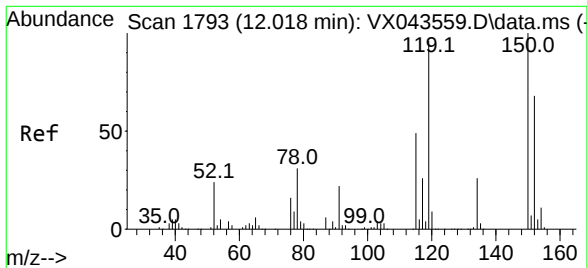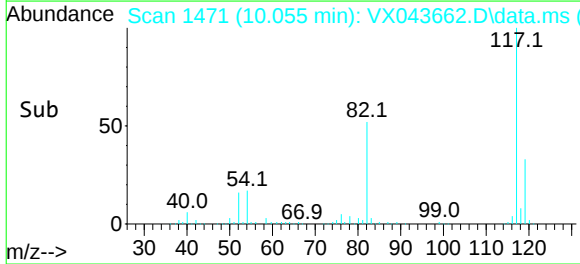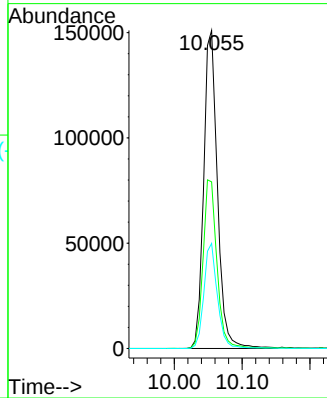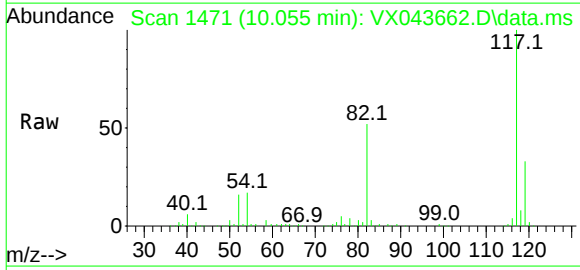

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX043662.D

Acq: 01 Nov 2024 14:20

Tgt Ion:152 Resp: 86030

Ion Ratio Lower Upper

152 100

115 59.8 42.9 128.7

150 161.3 0.0 343.6

