

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110422\
 Data File : VX032584.D
 Acq On : 04 Nov 2022 18:11
 Operator : JC/MD
 Sample : N5486-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 05 00:39:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 08:28:06 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	111523	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	185229	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	162953	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	73847	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	76510	49.374	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	98.740%		
35) Dibromofluoromethane	5.385	113	59789	45.252	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	90.500%		
50) Toluene-d8	8.653	98	221717	48.259	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	96.520%		
62) 4-Bromofluorobenzene	11.079	95	82161	45.781	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	91.560%		
Target Compounds						Qvalue
11) Tert butyl alcohol	2.971	59	3113	13.802	ug/l #	72
12) 1,1-Dichloroethene	2.319	96	307	0.274	ug/l	93
14) Allyl chloride	2.776	41	1561	0.876	ug/l #	68
15) Acrylonitrile	3.111	53	2259	3.691	ug/l #	25
16) Acetone	2.380	43	1001	1.777	ug/l #	83
18) Methyl Acetate	2.788	43	3732	2.038	ug/l #	51
19) Methyl tert-butyl Ether	3.111	73	167841	42.698	ug/l	95
22) Diisopropyl ether	3.764	45	7624	1.977	ug/l #	81
23) Vinyl Acetate	3.757	43	4053	1.301	ug/l #	72
24) 1,1-Dichloroethane	3.611	63	2872	1.295	ug/l	94
27) cis-1,2-Dichloroethene	4.489	96	16018	11.383	ug/l	91
31) Cyclohexane	5.477	56	1676	0.892	ug/l #	89
36) 1,1-Dichloropropene	5.556	75	8814	4.790	ug/l #	49
38) Carbon Tetrachloride	5.556	117	11391	5.582	ug/l #	15
39) Methylcyclohexane	7.385	83	1499	0.689	ug/l #	82
40) Benzene	6.037	78	209366	40.211	ug/l	98
42) 1,2-Dichloroethane	6.037	62	2375	1.116	ug/l #	77
43) Isopropyl Acetate	6.336	43	1214	0.413	ug/l #	25
44) Trichloroethene	7.135	130	4242	2.894	ug/l	88
51) 4-Methyl-2-Pentanone	8.647	43	1156	0.624	ug/l #	1
60) Dibromochloromethane	9.275	129	1093	0.699	ug/l #	11
64) Tetrachloroethene	9.275	164	1140	0.956	ug/l	93
67) Ethyl Benzene	10.195	91	6972	1.068	ug/l	96
68) m/p-Xylenes	10.305	106	1161	0.458	ug/l	97
73) Isopropylbenzene	10.963	105	2305	0.394	ug/l	98
76) 1,2,3-Trichloropropane	11.079	75	45792	27.872	ug/l #	37
78) n-propylbenzene	11.305	91	1427	0.212	ug/l	97
79) 2-Chlorotoluene	11.305	91	1427	0.353	ug/l #	41
81) trans-1,4-Dichloro-2-b...	11.079	75	45792	88.691	ug/l #	6
82) 4-Chlorotoluene	11.305	91	1427	0.302	ug/l #	45
84) 1,2,4-Trimethylbenzene	11.750	105	1052	0.211	ug/l	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_X
ClientSampleId :


Instrument :
MSVOA_X
ClientSampleId :

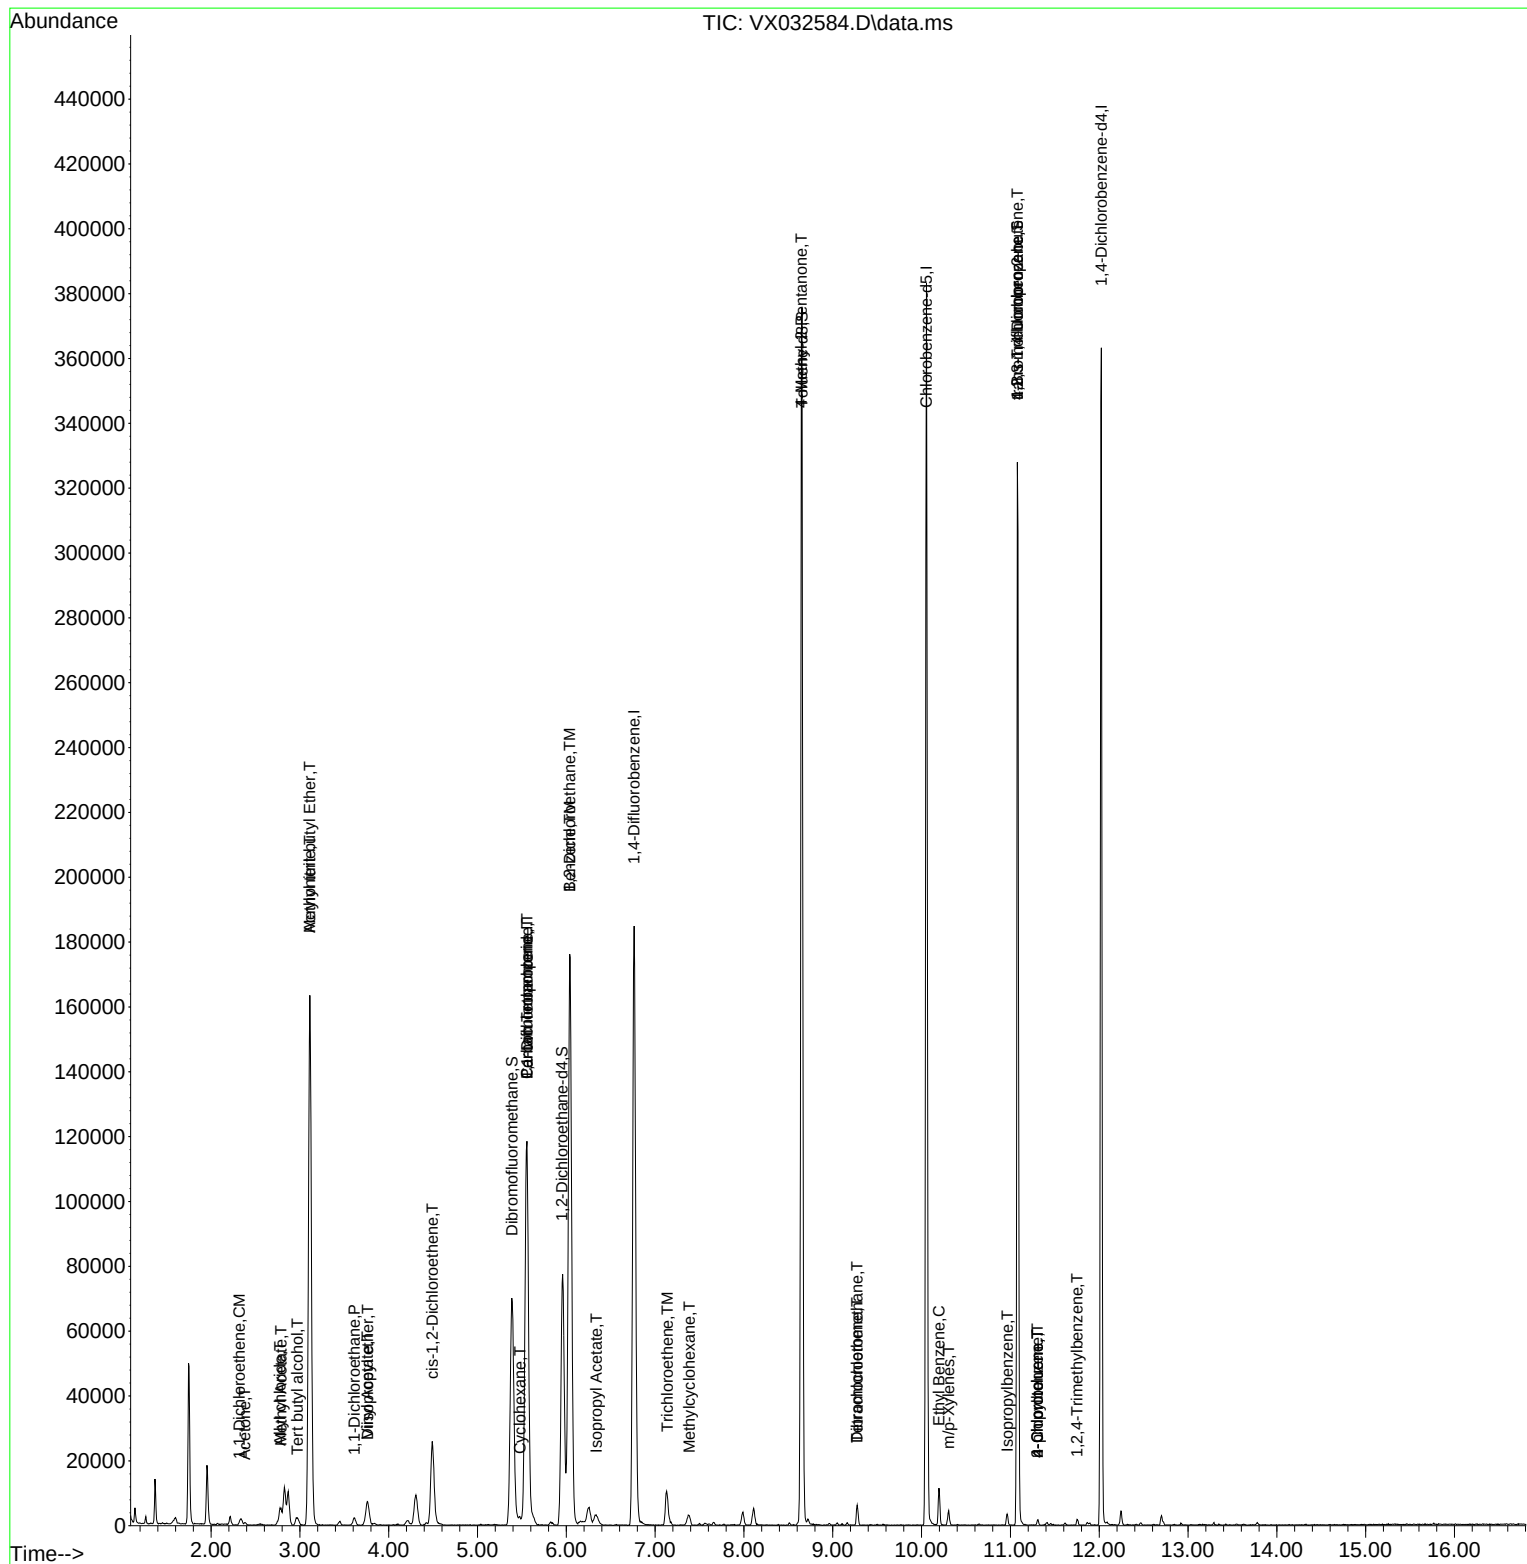



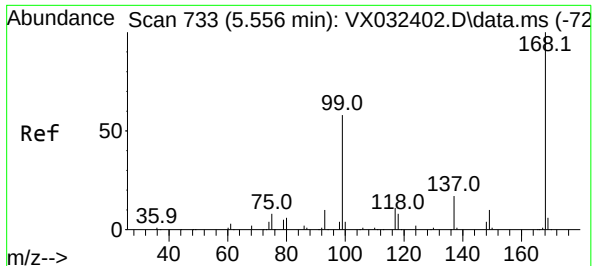


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:168 Resp: 111523
Ion Ratio Lower Upper
168 100
99 56.9 46.1 69.1

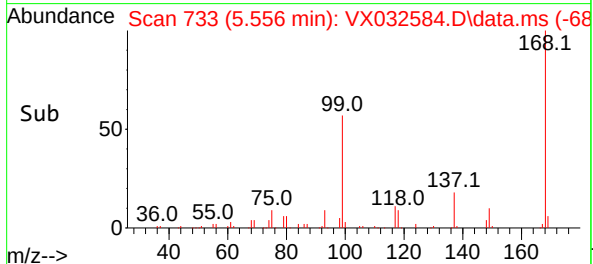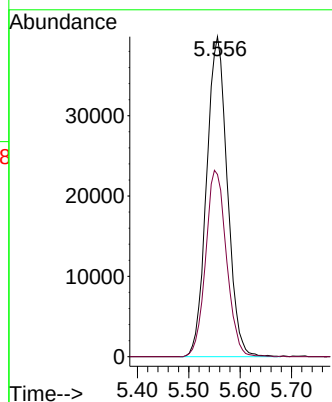

#11
Tert butyl alcohol
Concen: 13.802 ug/l
RT: 2.971 min Scan# 309
Delta R.T. 0.006 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11


Tgt Ion: 59 Resp: 3113
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

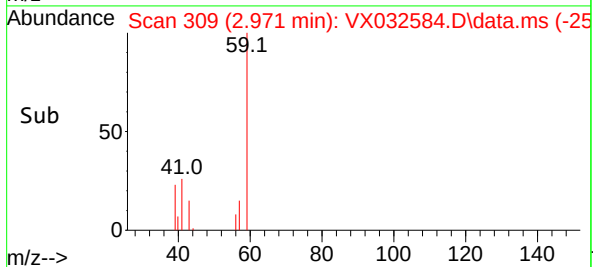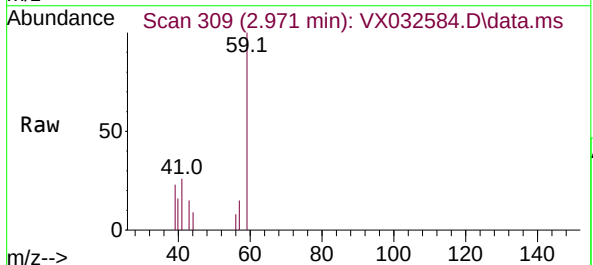






#12
1,1-Dichloroethene
Concen: 0.274 ug/l
RT: 2.319 min Scan# 20
Delta R.T. 0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Instrument :
MSVOA_X
ClientSampleId :



Tgt Ion: 96 Resp: 307




Ion	Ratio	Lower	Upper
96	100		
61	162.6	125.1	187.7
98	52.6	50.6	76.0




#14
Allyl chloride
Concen: 0.876 ug/l
RT: 2.776 min Scan# 277
Delta R.T. 0.110 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Tgt Ion: 41 Resp: 1561

Ion	Ratio	Lower	Upper
41	100		
39	61.8	61.4	92.2
76	0.0	29.2	43.8


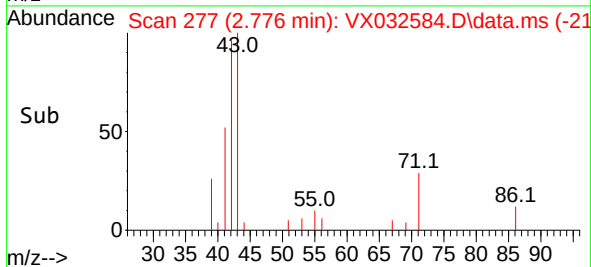

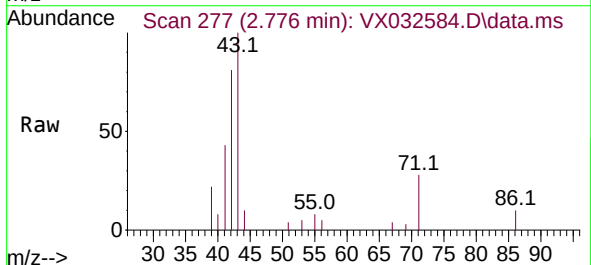




#15
Acrylonitrile
Concen: 3.691 ug/l
RT: 3.111 min Scan# 31
Delta R.T. 0.049 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 53 Resp: 2259
Ion Ratio Lower Upper
53 100
52 14.2 67.4 101.0#
51 80.3 30.3 45.5#

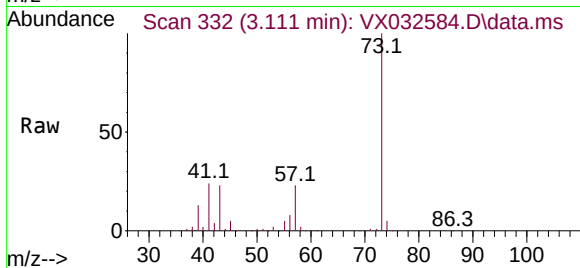

#16
Acetone
Concen: 1.777 ug/l
RT: 2.380 min Scan# 212
Delta R.T. 0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Tgt Ion: 43 Resp: 1001
Ion Ratio Lower Upper
43 100
58 20.5 23.8 35.8#


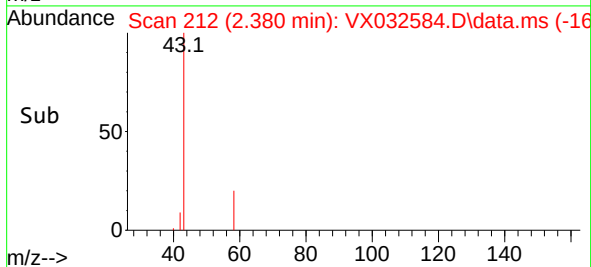
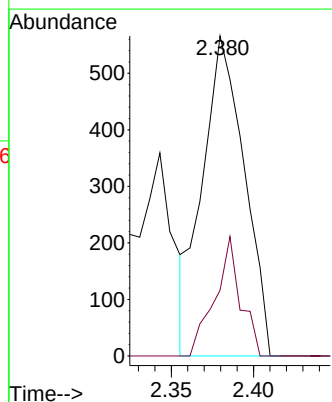
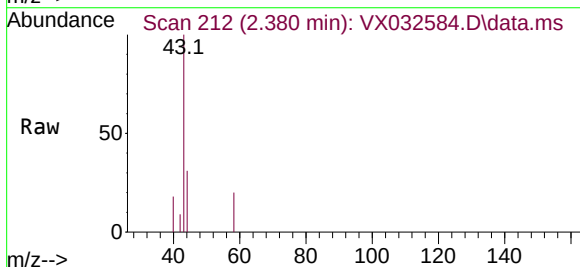




#18
Methyl Acetate
Concen: 2.038 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.085 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 3732
Ion Ratio Lower Upper
43 100
74 0.0 19.4 29.0#

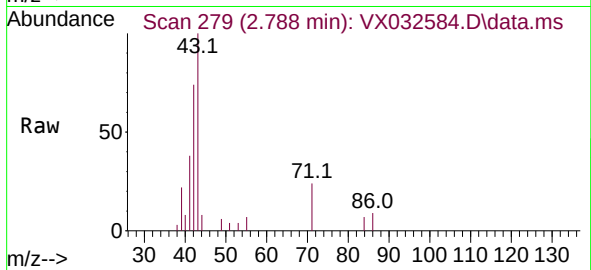

#19
Methyl tert-butyl Ether
Concen: 42.698 ug/l
RT: 3.111 min Scan# 332
Delta R.T. 0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Tgt Ion: 73 Resp: 167841
Ion Ratio Lower Upper
73 100
57 23.3 16.6 25.0




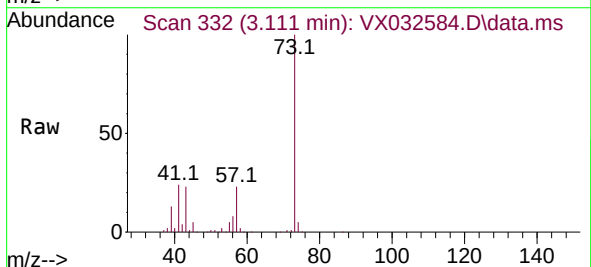




#22
Diisopropyl ether
Concen: 1.977 ug/l
RT: 3.764 min Scan# 41
Delta R.T. 0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:	45	Resp:	7624
Ion	Ratio	Lower	Upper
45	100		
43	46.5	56.4	84.6#
87	32.2	24.4	36.6
59	11.5	9.5	14.3

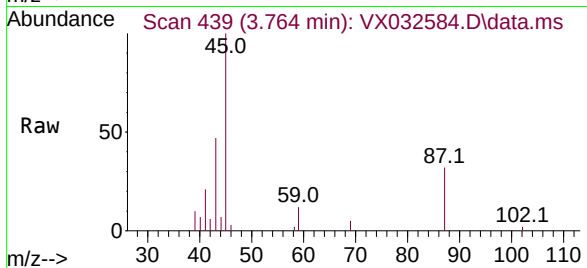

#23
Vinyl Acetate
Concen: 1.301 ug/l
RT: 3.757 min Scan# 438
Delta R.T. 0.037 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Tgt Ion:	43	Resp:	4053
Ion	Ratio	Lower	Upper
43	100		
86	0.0	8.6	12.8#


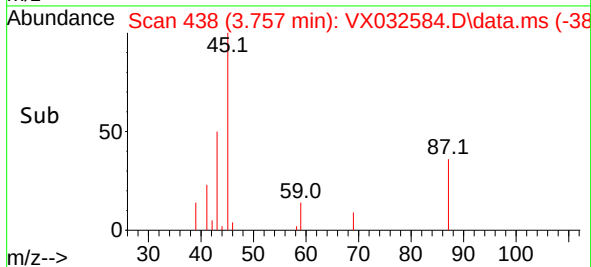

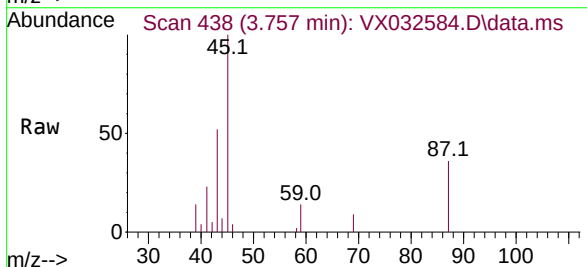




#24
 1,1-Dichloroethane
 Concen: 1.295 ug/l
 RT: 3.611 min Scan# 414
 Delta R.T. 0.000 min
 Lab File: VX032584.D
 Acq: 04 Nov 2022 18:11




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 63 Resp: 2872
 Ion Ratio Lower Upper
 63 100
 98 4.0 3.5 10.4
 100 4.0 2.3 6.8

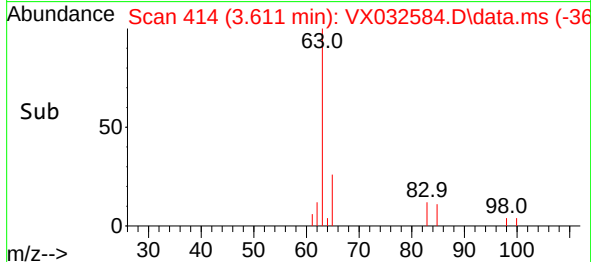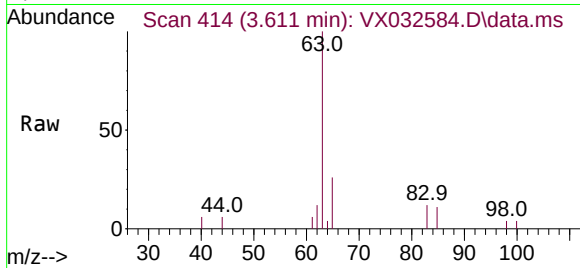

#27
 cis-1,2-Dichloroethene
 Concen: 11.383 ug/l
 RT: 4.489 min Scan# 558
 Delta R.T. 0.000 min
 Lab File: VX032584.D
 Acq: 04 Nov 2022 18:11


Tgt Ion: 96 Resp: 16018
 Ion Ratio Lower Upper
 96 100
 61 126.7 0.0 286.0
 98 65.3 0.0 129.6

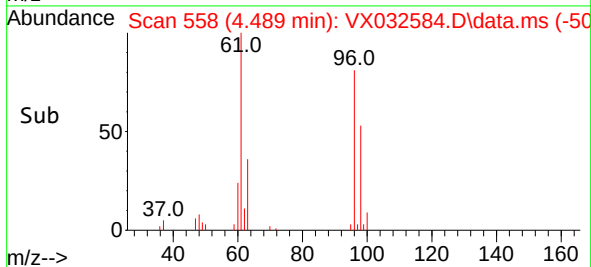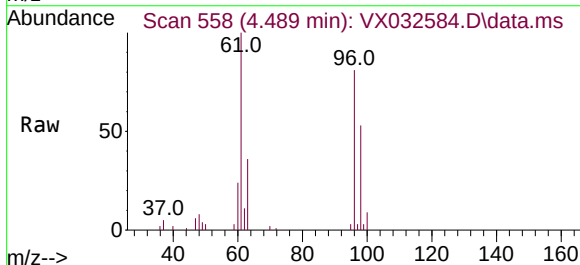






#31
Cyclohexane
Concen: 0.892 ug/l
RT: 5.477 min Scan# 719
Delta R.T. 0.006 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Instrument :
MSVOA_X
ClientSampleId :



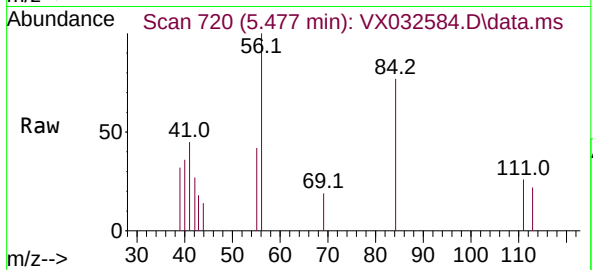



Tgt Ion: 56 Resp: 1676
Ion Ratio Lower Upper
56 100
69 19.3 24.1 36.1#
84 76.6 66.9 100.3

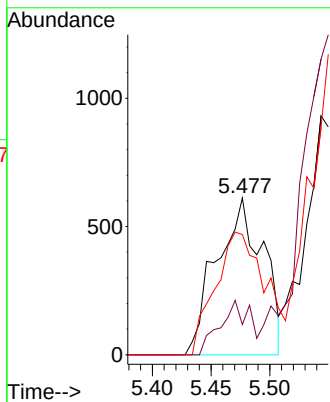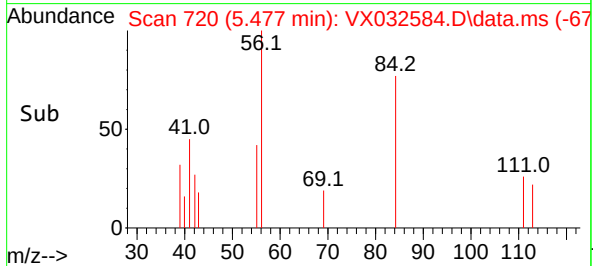

#33
1,2-Dichloroethane-d4
Concen: 49.374 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Tgt Ion: 65 Resp: 76510
Ion Ratio Lower Upper
65 100
67 49.6 0.0 101.8



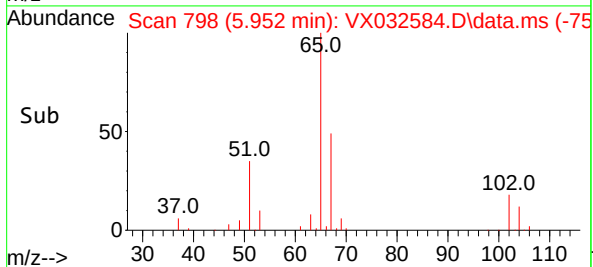
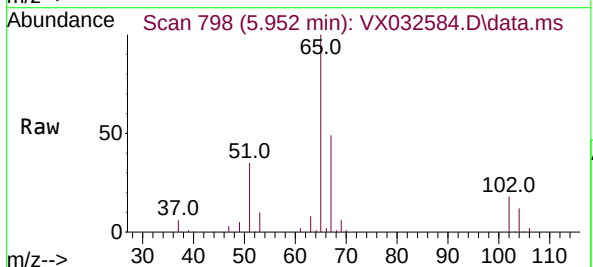




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 185229
Ion Ratio Lower Upper
114 100
63 19.8 0.0 41.6
88 16.0 0.0 33.4

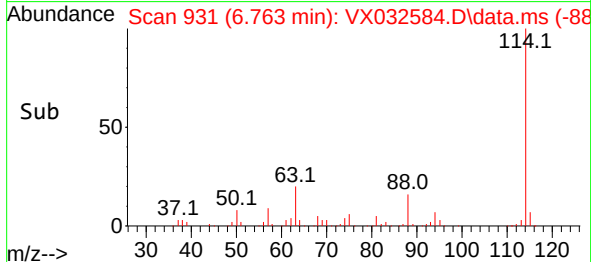

#35
Dibromofluoromethane
Concen: 45.252 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Tgt Ion:113 Resp: 59789
Ion Ratio Lower Upper
113 100
111 104.2 82.4 123.6
192 19.4 15.4 23.2

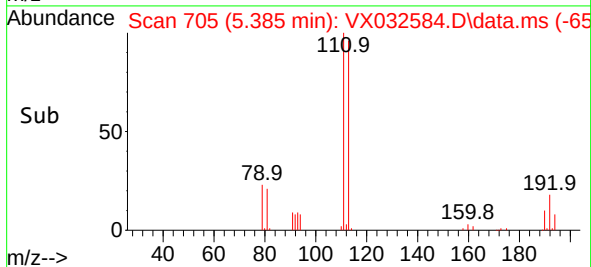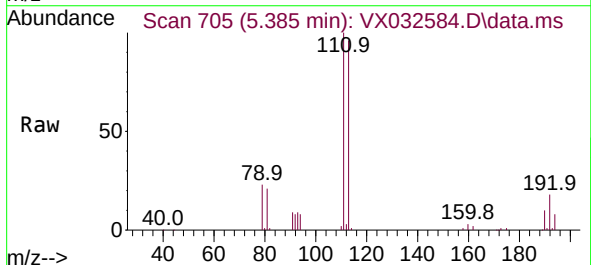



#36

1,1-Dichloropropene

Concen: 4.790 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min


Lab File: VX032584.D

Acq: 04 Nov 2022 18:11

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 75 Resp: 8814

Ion Ratio Lower Upper

75 100

110 8.5 18.4 55.2#

77 0.0 24.5 36.7#

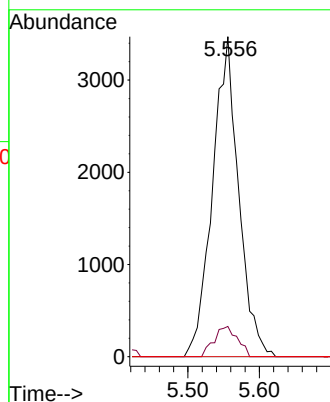

#38

Carbon Tetrachloride

Concen: 5.582 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.128 min

Lab File: VX032584.D

Acq: 04 Nov 2022 18:11




Tgt Ion: 117 Resp: 11391


Ion Ratio Lower Upper

117 100

119 3.9 77.2 115.8#

121 0.0 25.8 38.6#

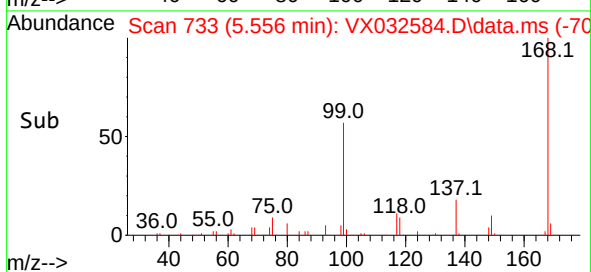

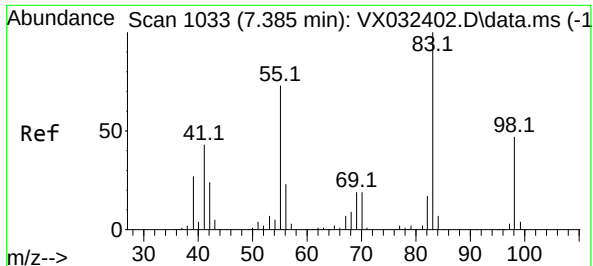

#39

Methylcyclohexane

Concen: 0.689 ug/l

RT: 7.385 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX032584.D

Acq: 04 Nov 2022 18:11

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 83 Resp: 1499

Ion Ratio Lower Upper

83 100

55 85.6 58.4 87.6

98 62.2 37.2 55.8#

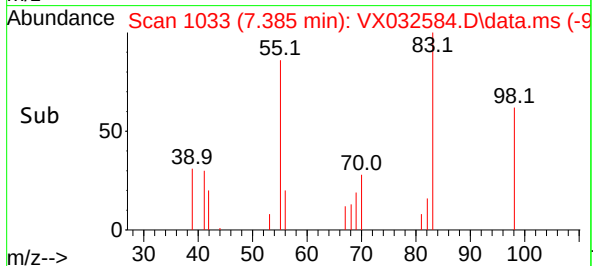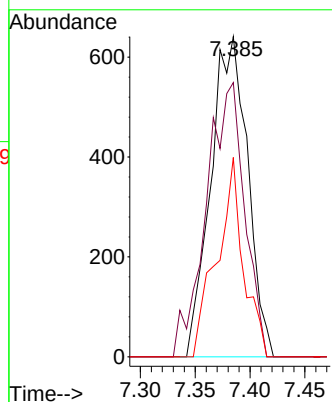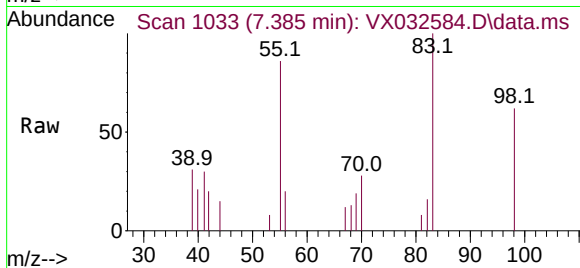

#40

Benzene

Concen: 40.211 ug/l

RT: 6.037 min Scan# 812

Delta R.T. 0.000 min

Lab File: VX032584.D




Acq: 04 Nov 2022 18:11


Tgt Ion: 78 Resp: 209366

Ion Ratio Lower Upper

78 100

77 22.5 19.0 28.4

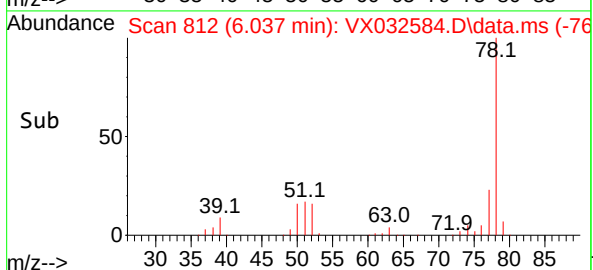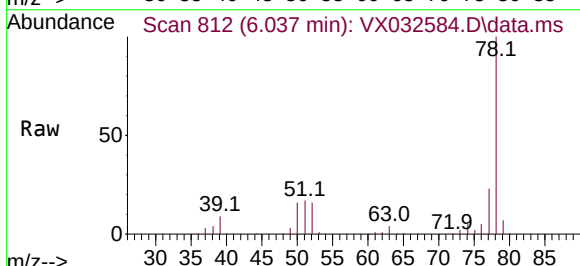



#42

1,2-Dichloroethane

Concen: 1.116 ug/l

RT: 6.037 min Scan# 81

Delta R.T. -0.049 min

Lab File: VX032584.D

Acq: 04 Nov 2022 18:11

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 62 Resp: 2375

Ion Ratio Lower Upper

62 100

98 0.0 0.0 16.0

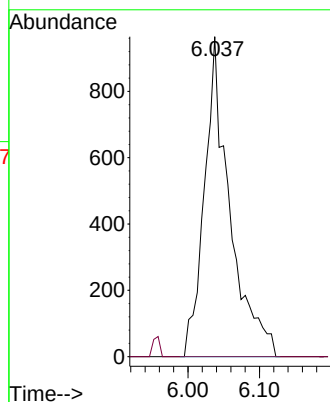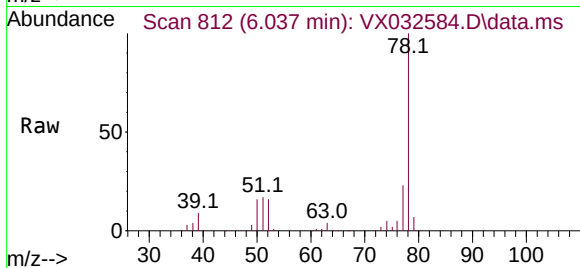

#43

Isopropyl Acetate

Concen: 0.413 ug/l

RT: 6.336 min Scan# 861

Delta R.T. -0.006 min

Lab File: VX032584.D

Acq: 04 Nov 2022 18:11




Tgt Ion: 43 Resp: 1214


Ion Ratio Lower Upper

43 100

61 0.0 15.4 23.0#

87 62.1 10.8 16.2#


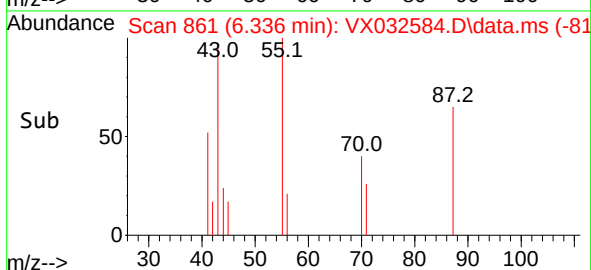

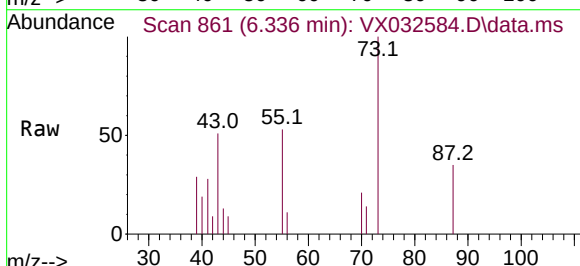


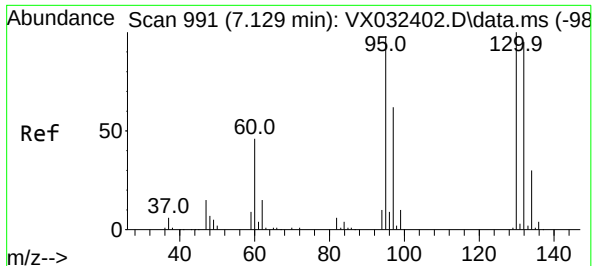

#44
Trichloroethene
Concen: 2.894 ug/l
RT: 7.135 min Scan# 991
Delta R.T. 0.006 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:130 Resp: 4242
Ion Ratio Lower Upper
130 100
95 85.4 0.0 195.2

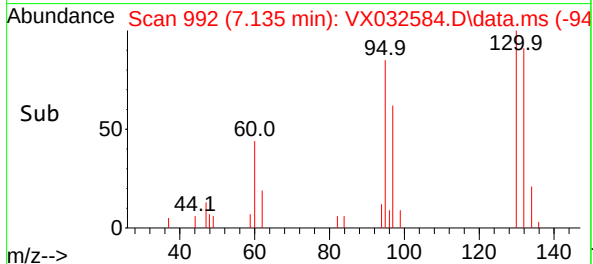

#50
Toluene-d8
Concen: 48.259 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Tgt Ion: 98 Resp: 221717
Ion Ratio Lower Upper
98 100
100 64.0 50.9 76.3


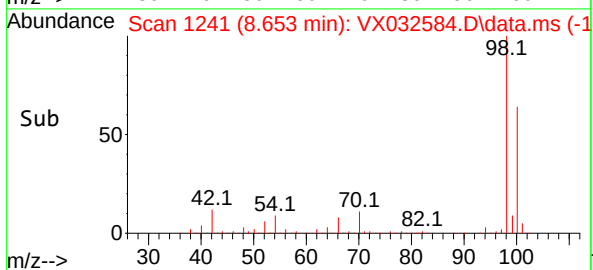

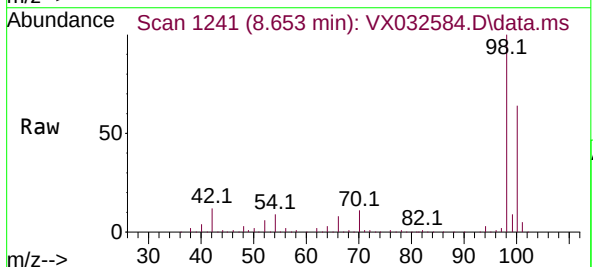




#51
4-Methyl-2-Pentanone
Concen: 0.624 ug/l
RT: 8.647 min Scan# 1156
Delta R.T. 0.073 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 1156
Ion Ratio Lower Upper
43 100
58 156.6 30.9 46.3#

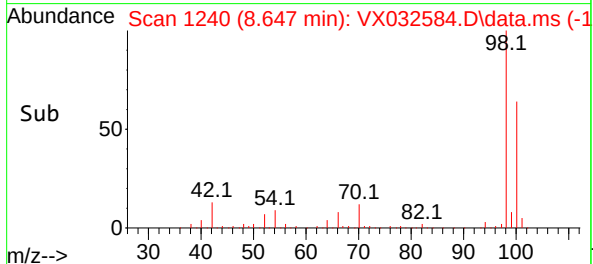

#60
Dibromochloromethane
Concen: 0.699 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.250 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Tgt Ion: 129 Resp: 1093
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#



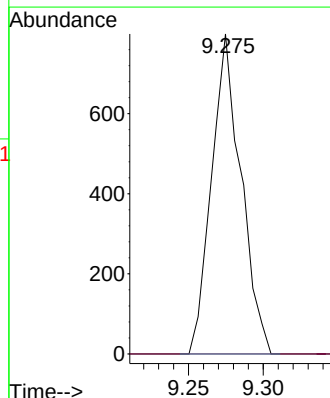
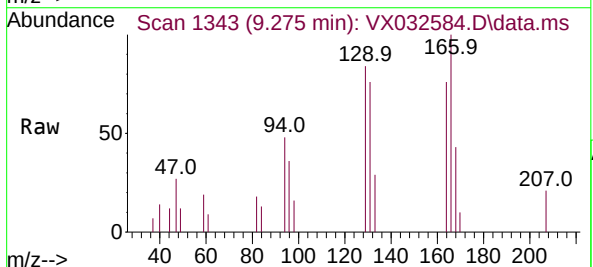




#62
4-Bromofluorobenzene
Concen: 45.781 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 82161
Ion Ratio Lower Upper
95 100
174 82.3 0.0 164.0
176 79.9 0.0 154.4

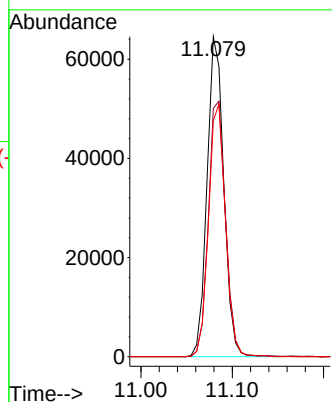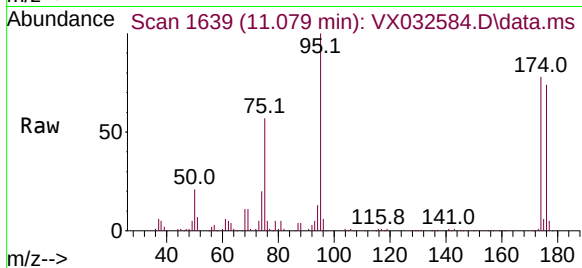

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11


Tgt Ion: 117 Resp: 162953
Ion Ratio Lower Upper
117 100
82 56.3 44.3 66.5
119 33.3 25.7 38.5

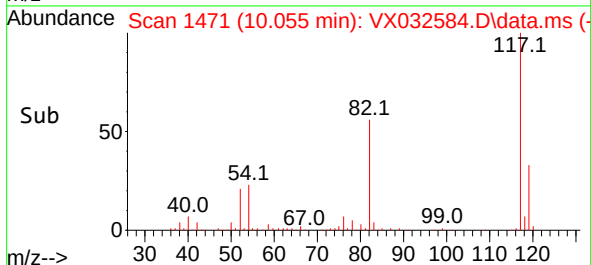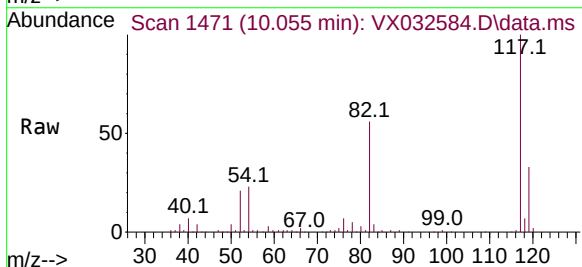






#64
Tetrachloroethene
Concen: 0.956 ug/l
RT: 9.275 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Instrument :
MSVOA_X
ClientSampleId :



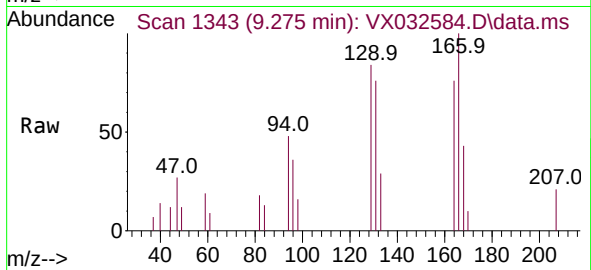



Tgt Ion:164 Resp: 1140
Ion Ratio Lower Upper
164 100
166 131.2 105.4 158.2
129 110.4 78.2 117.2
131 100.0 72.5 108.7



#67
Ethyl Benzene
Concen: 1.068 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Tgt Ion: 91 Resp: 6972
Ion Ratio Lower Upper
91 100
106 28.8 25.0 37.6


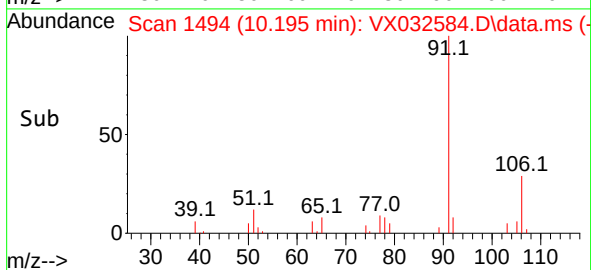

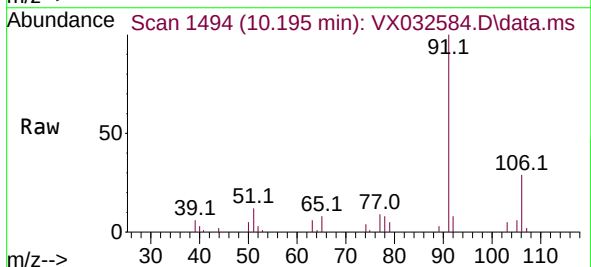




#68
m/p-Xylenes
Concen: 0.458 ug/l
RT: 10.305 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 1161
Ion Ratio Lower Upper
106 100
91 200.3 164.5 246.7

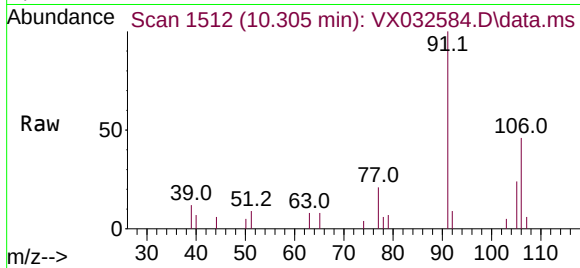

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Tgt Ion:152 Resp: 73847
Ion Ratio Lower Upper
152 100
115 61.1 44.0 132.0
150 156.9 0.0 351.8



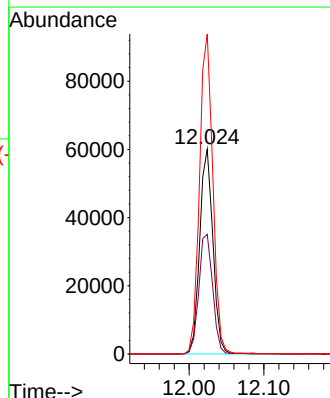
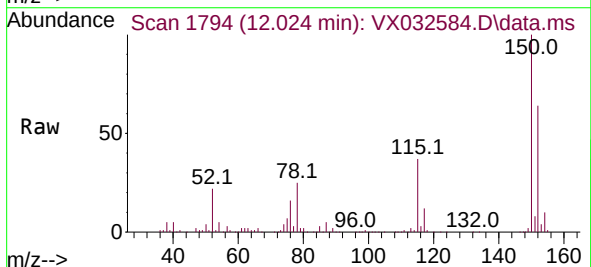




#73
Isopropylbenzene
Concen: 0.394 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 2305
Ion Ratio Lower Upper
105 100
120 25.1 13.1 39.3

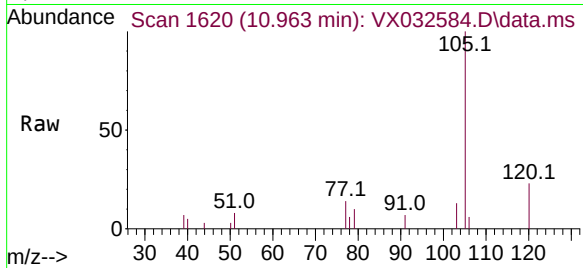

#76
1,2,3-Trichloropropane
Concen: 27.872 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Tgt Ion: 75 Resp: 45792
Ion Ratio Lower Upper
75 100
77 0.9 20.0 60.0#


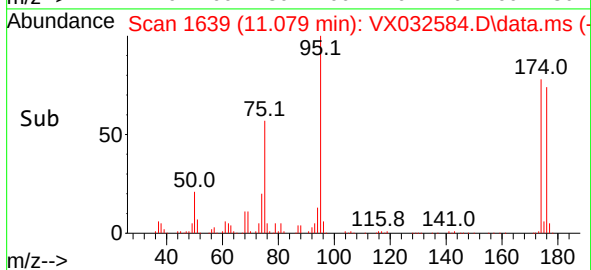

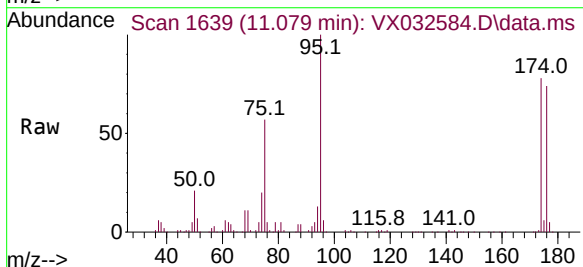


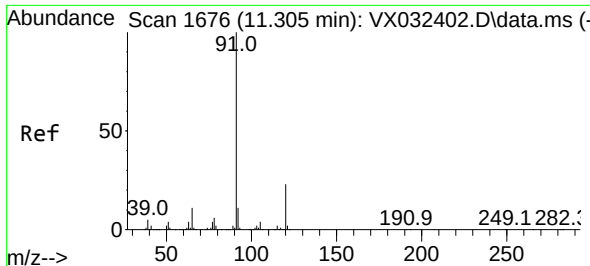

#78
n-propylbenzene
Concen: 0.212 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 1427
Ion Ratio Lower Upper
91 100
120 21.7 11.6 34.8

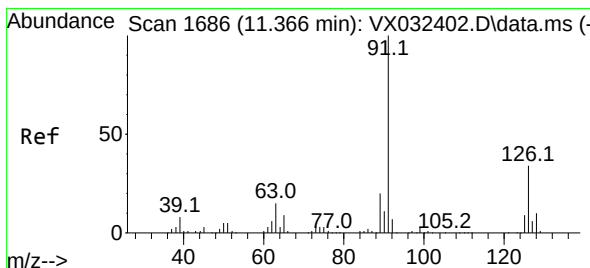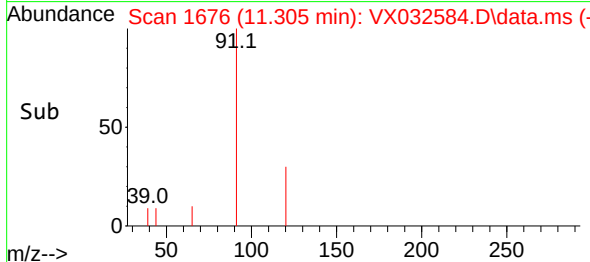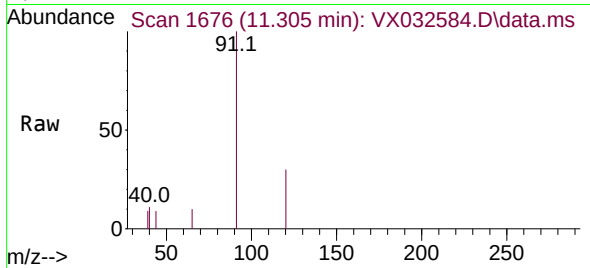

#79
2-Chlorotoluene
Concen: 0.353 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.061 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11

Tgt Ion: 91 Resp: 1427
Ion Ratio Lower Upper
91 100
126 0.0 17.1 51.2#


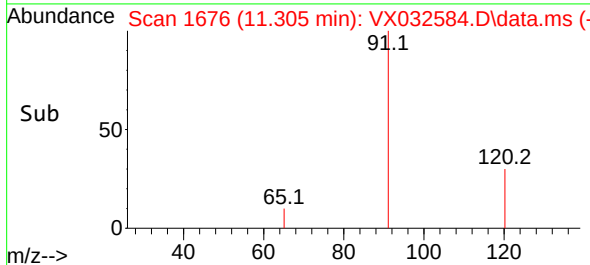

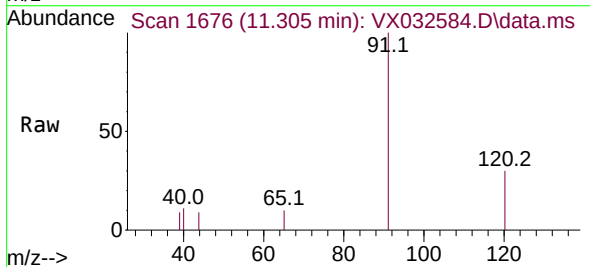




#81
trans-1,4-Dichloro-2-butene
Concen: 88.691 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 45792
Ion Ratio Lower Upper
75 100
53 0.0 86.9 130.3#
89 0.0 38.3 57.5#

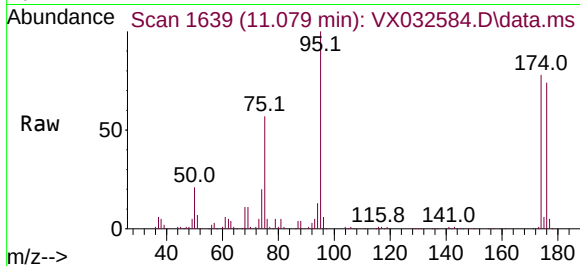

#82
4-Chlorotoluene
Concen: 0.302 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.152 min
Lab File: VX032584.D
Acq: 04 Nov 2022 18:11


Tgt Ion: 91 Resp: 1427
Ion Ratio Lower Upper
91 100
126 0.0 14.8 44.4#

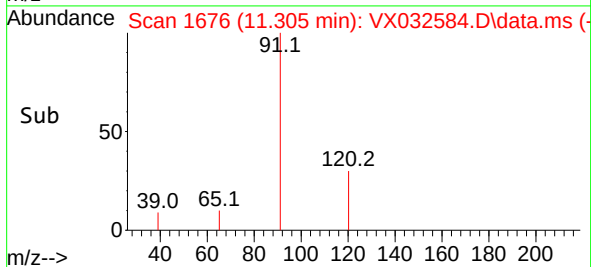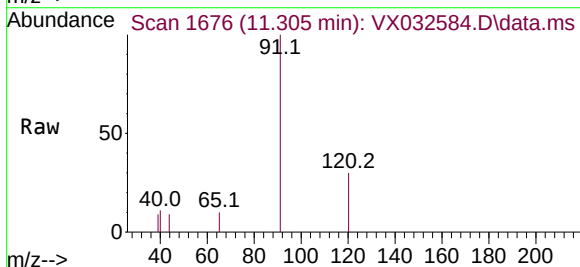



#84
 1,2,4-Trimethylbenzene
 Concen: 0.211 ug/l
 RT: 11.750 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX032584.D
 Acq: 04 Nov 2022 18:11

Instrument :
 MSVOA_X
 ClientSampleId :

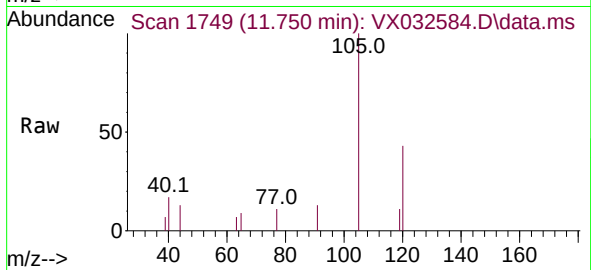

Tgt Ion:105 Resp: 1052
 Ion Ratio Lower Upper
 105 100
 120 50.9 21.9 65.5

