

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110422\
 Data File : VX032595.D
 Acq On : 05 Nov 2022 01:17
 Operator : JC/MD
 Sample : N5483-03 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 07 05:05:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 08:28:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	119249	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	195812	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	171832	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	82911	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	82065	49.528	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	99.060%		
35) Dibromofluoromethane	5.385	113	63511	45.471	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	90.940%		
50) Toluene-d8	8.647	98	233804	48.140	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	96.280%		
62) 4-Bromofluorobenzene	11.079	95	91153	48.047	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	96.100%		
Target Compounds						
					Qvalue	
5) Bromomethane	1.618	94	225	0.220	ug/l	81
10) Methyl Iodide	2.459	142	131	2.005	ug/l #	37
11) Tert butyl alcohol	2.947	59	525	2.177	ug/l #	72
13) Acrolein	2.233	56	87	0.361	ug/l #	14
15) Acrylonitrile	3.087	53	180	0.275	ug/l #	29
16) Acetone	2.386	43	516	0.857	ug/l #	45
17) Carbon Disulfide	2.508	76	731	0.257	ug/l #	74
18) Methyl Acetate	2.782	43	2584	1.319	ug/l #	51
20) Methylene Chloride	2.794	84	1963	1.422	ug/l #	90
31) Cyclohexane	5.477	56	4362	2.171	ug/l	97
36) 1,1-Dichloropropene	5.550	75	9321	4.792	ug/l #	49
38) Carbon Tetrachloride	5.556	117	12437	5.765	ug/l #	14
39) Methylcyclohexane	7.385	83	3030	1.317	ug/l #	84
40) Benzene	6.044	78	3319	0.603	ug/l	95
52) Toluene	8.720	92	50181	13.974	ug/l	96
67) Ethyl Benzene	10.195	91	127780	18.564	ug/l	98
68) m/p-Xylenes	10.299	106	175899	65.812	ug/l	100
69) o-Xylene	10.640	106	69385	26.700	ug/l	99
70) Styrene	10.647	104	4604	1.066	ug/l #	1
73) Isopropylbenzene	10.964	105	8667	1.319	ug/l	98
76) 1,2,3-Trichloropropane	11.079	75	49641	26.912	ug/l #	35
78) n-propylbenzene	11.305	91	24412	3.225	ug/l	97
79) 2-Chlorotoluene	11.378	91	18001	3.971	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	45789	8.155	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	49641	85.635	ug/l #	6
82) 4-Chlorotoluene	11.451	91	5710	1.076	ug/l #	49
83) tert-Butylbenzene	11.750	119	18077	3.225	ug/l #	50
84) 1,2,4-Trimethylbenzene	11.750	105	154039	27.582	ug/l	99
85) sec-Butylbenzene	11.750	105	154039	22.836	ug/l #	57
86) p-Isopropyltoluene	11.969	119	2058	0.360	ug/l	98
89) n-Butylbenzene	12.329	91	4026	0.809	ug/l #	26
90) Hexachloroethane	12.530	117	1354	1.448	ug/l #	12
93) 1,2,4-Trichlorobenzene	13.591	180	411	0.210	ug/l	82
94) Hexachlorobutadiene	13.719	225	304	0.373	ug/l	90
95) Naphthalene	13.774	128	38643	5.937	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110422\
Data File : VX032595.D
Acq On : 05 Nov 2022 01:17
Operator : JC/MD
Sample : N5483-03 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 07 05:05:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 08:28:06 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110422\
Data File : VX032595.D
Acq On : 05 Nov 2022 01:17
Operator : JC/MD
Sample : N5483-03 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Nov 07 05:05:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 08:28:06 2022
Response via : Initial Calibration

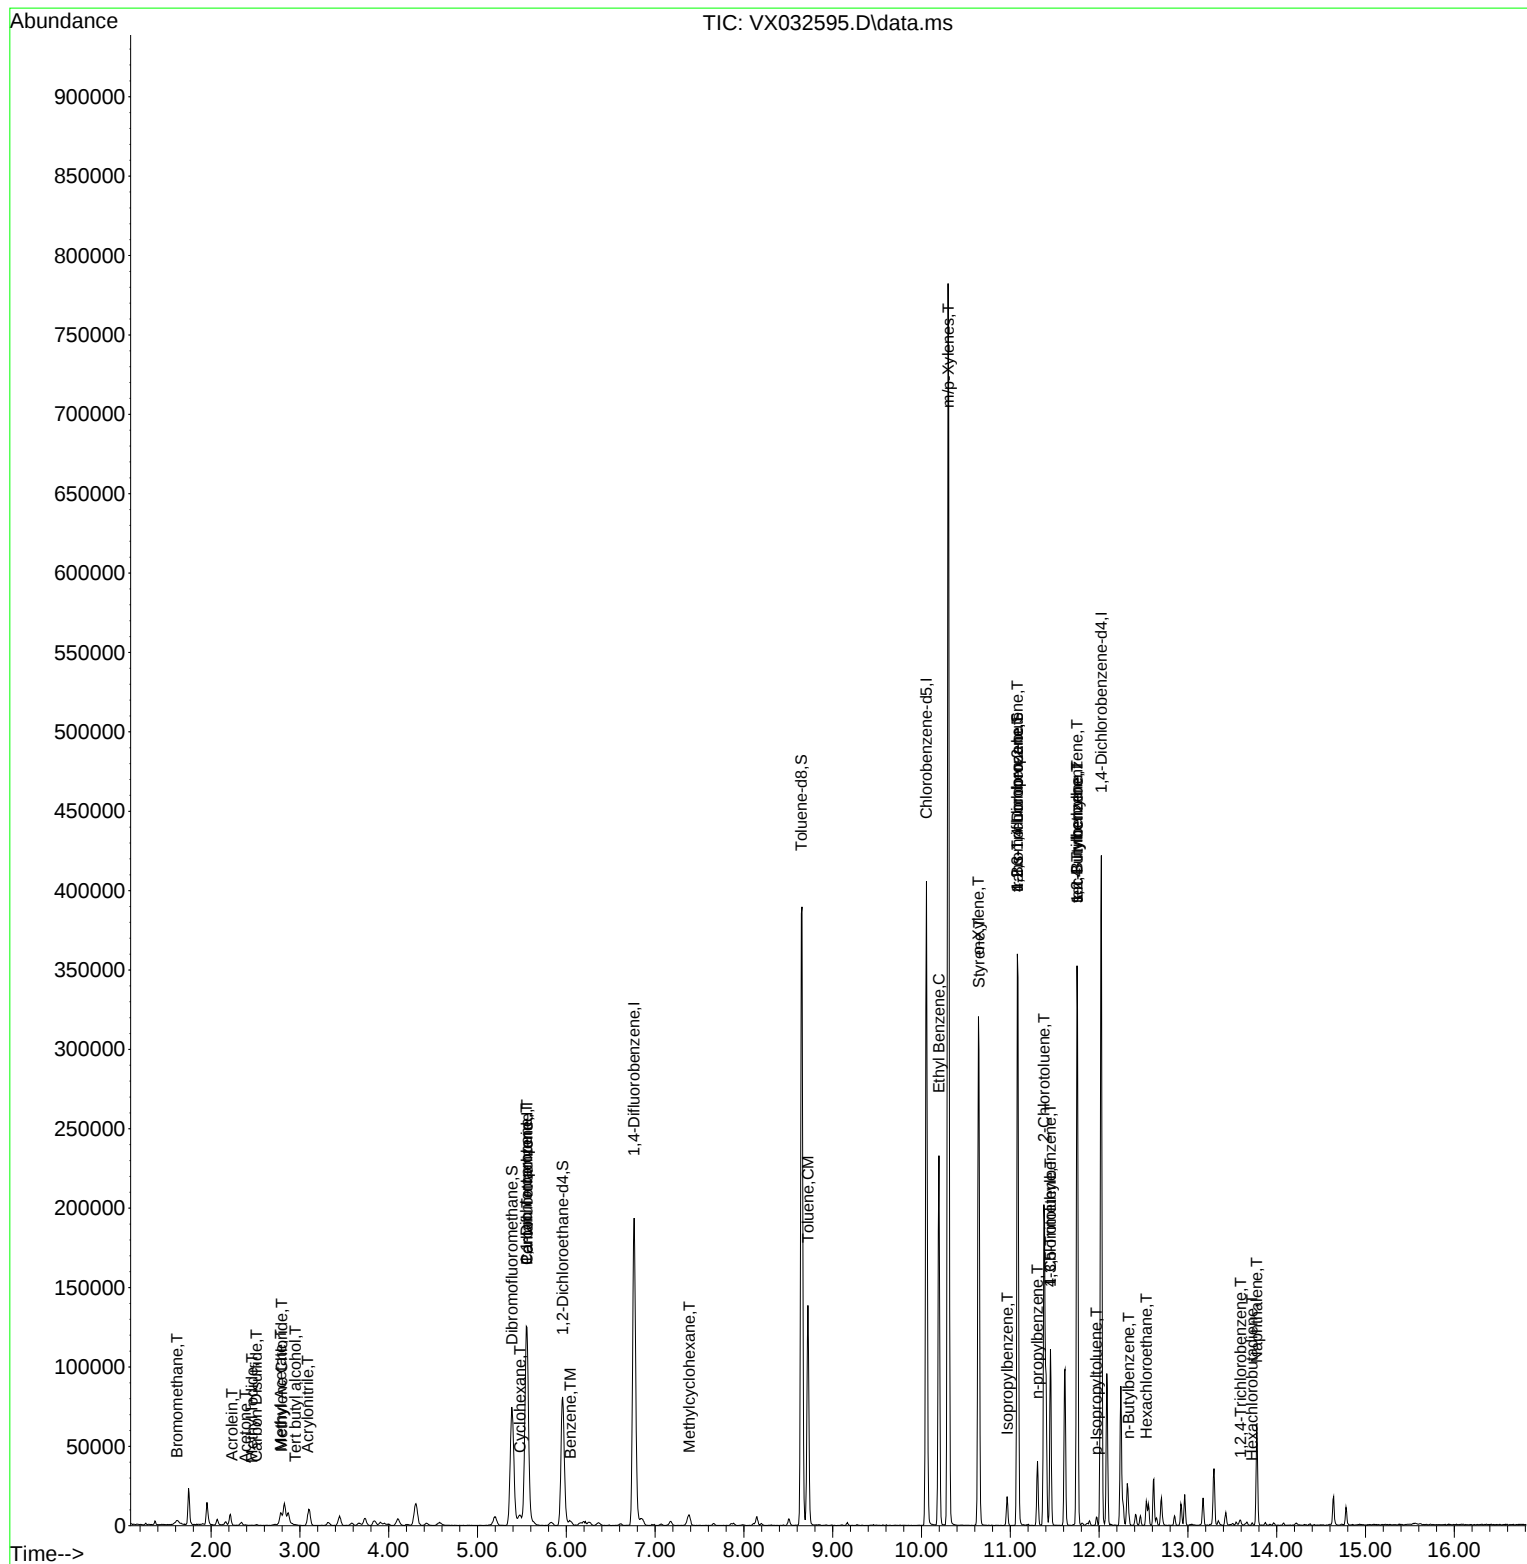






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:168 Resp: 119249
Ion Ratio Lower Upper
168 100
99 58.1 46.1 69.1



#5
Bromomethane
Concen: 0.220 ug/l
RT: 1.618 min Scan# 87
Delta R.T. 0.012 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17


Tgt Ion: 94 Resp: 225
Ion Ratio Lower Upper
94 100
96 115.3 77.6 116.4

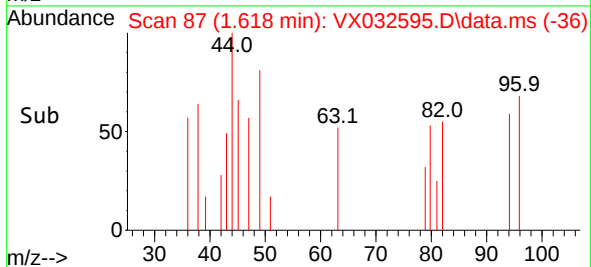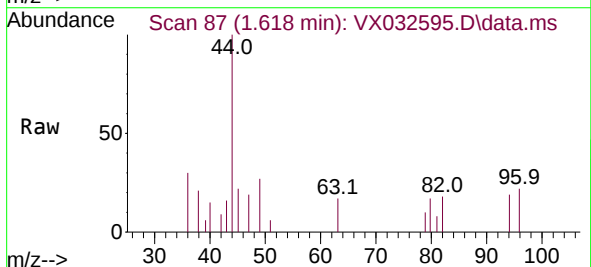



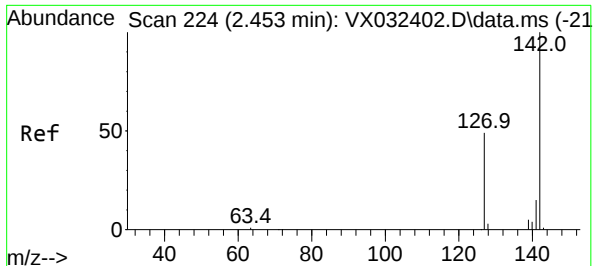


#10
Methyl Iodide
Concen: 2.005 ug/l
RT: 2.459 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:142 Resp: 131
Ion Ratio Lower Upper
142 100
127 0.0 38.6 57.8#
141 0.0 11.4 17.2#

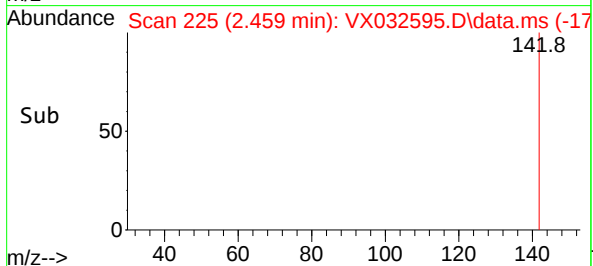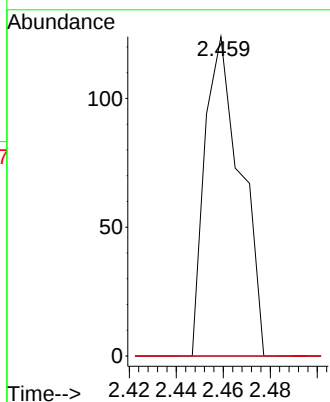

#11
Tert butyl alcohol
Concen: 2.177 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.018 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17


Tgt Ion: 59 Resp: 525
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

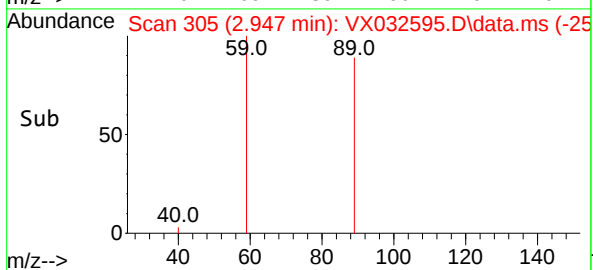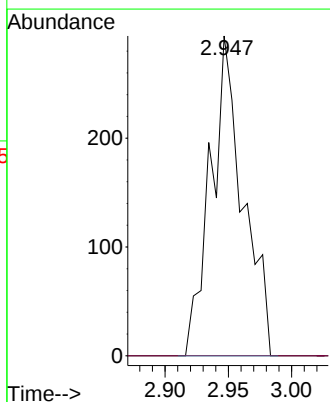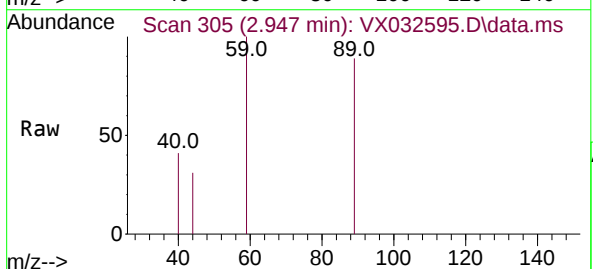



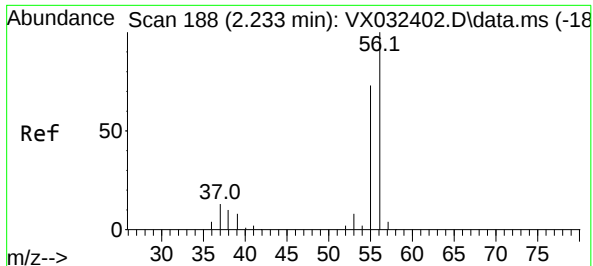


#13
Acrolein
Concen: 0.361 ug/l
RT: 2.233 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion: 56 Resp: 87
Ion Ratio Lower Upper
56 100
55 0.0 56.9 85.3#

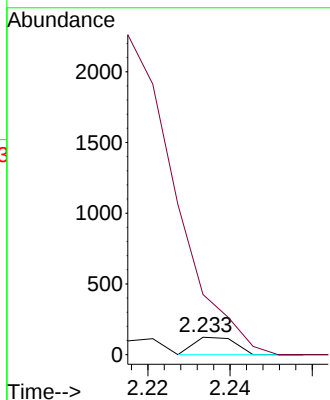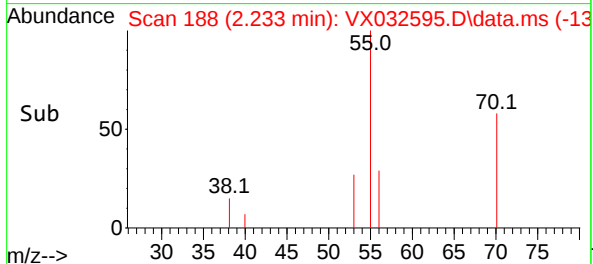


#15
Acrylonitrile
Concen: 0.275 ug/l
RT: 3.087 min Scan# 328
Delta R.T. 0.025 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17

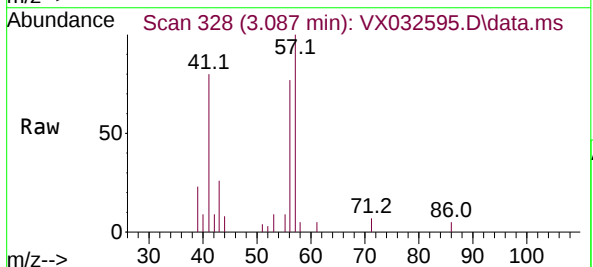

Tgt Ion: 53 Resp: 180
Ion Ratio Lower Upper
53 100
52 21.7 67.4 101.0#
51 83.9 30.3 45.5#



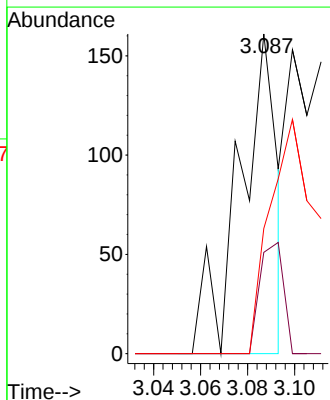
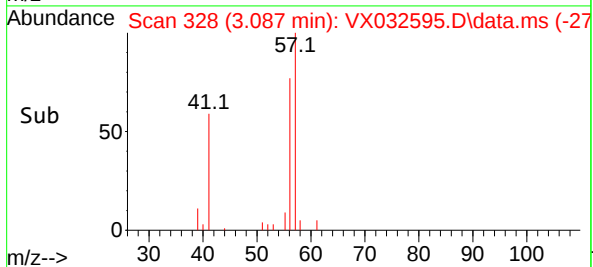


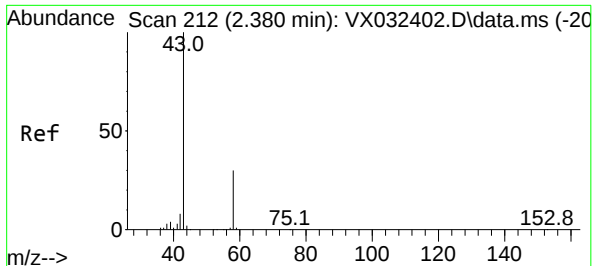

#16
Acetone
Concen: 0.857 ug/l
RT: 2.386 min Scan# 212
Delta R.T. 0.006 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 516
Ion Ratio Lower Upper
43 100
58 0.0 23.8 35.8#

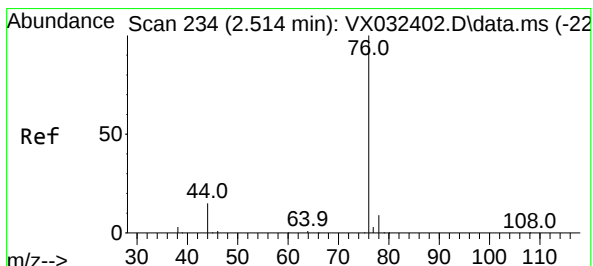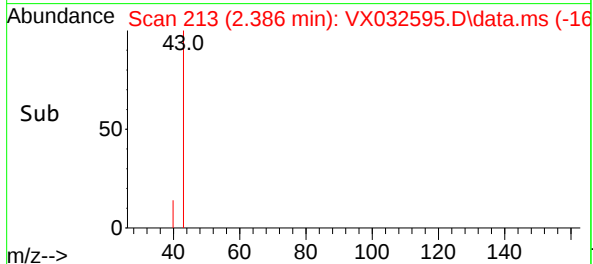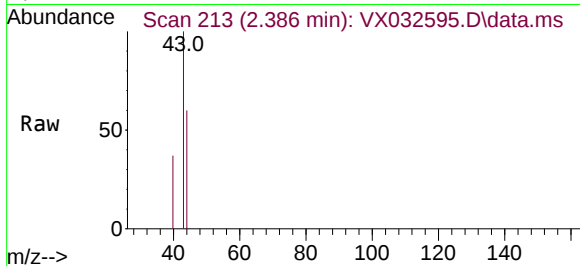

#17
Carbon Disulfide
Concen: 0.257 ug/l
RT: 2.508 min Scan# 233
Delta R.T. -0.006 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17

Tgt Ion: 76 Resp: 731
Ion Ratio Lower Upper
76 100
78 0.0 7.5 11.3#

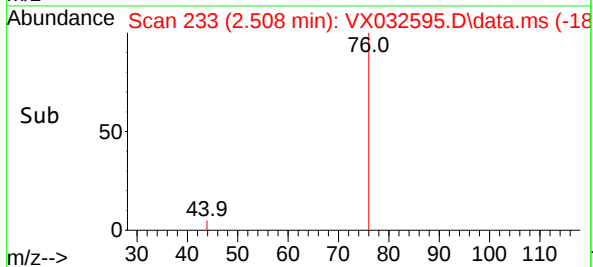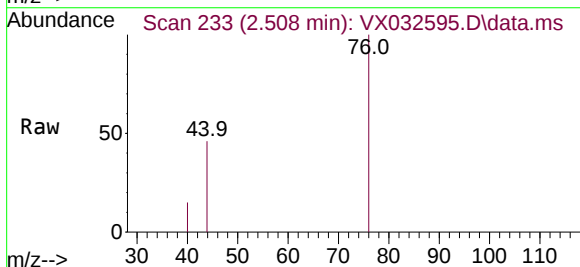

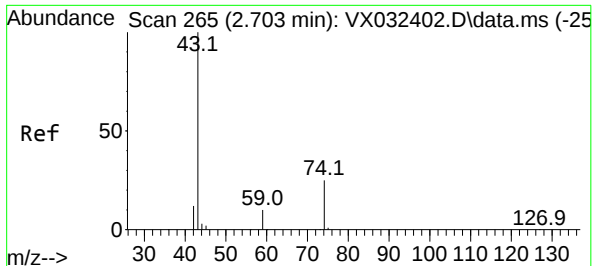

#18

Methyl Acetate

Concen: 1.319 ug/l

RT: 2.782 min Scan# 21

Delta R.T. 0.079 min

Lab File: VX032595.D

Acq: 05 Nov 2022 01:17

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 2584

Ion Ratio Lower Upper

43 100

74 0.0 19.4 29.0#

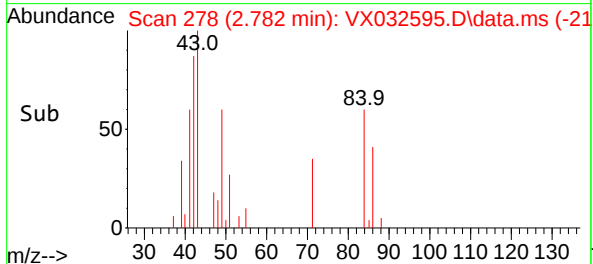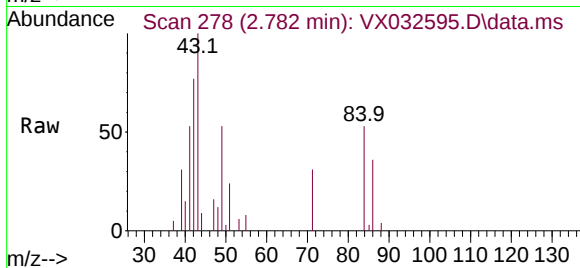

#20

Methylene Chloride

Concen: 1.422 ug/l

RT: 2.794 min Scan# 280

Delta R.T. 0.006 min

Lab File: VX032595.D

Acq: 05 Nov 2022 01:17

Tgt Ion: 84 Resp: 1963




Ion Ratio Lower Upper


84 100

49 133.0 101.0 151.6

51 33.3 31.1 46.7


86 51.5 52.3 78.5#

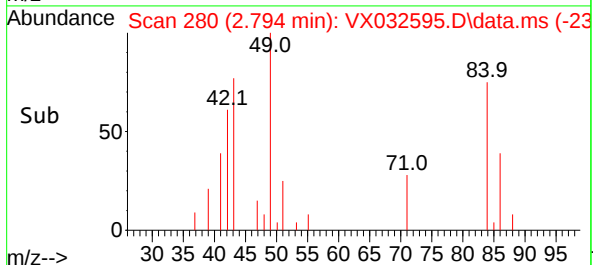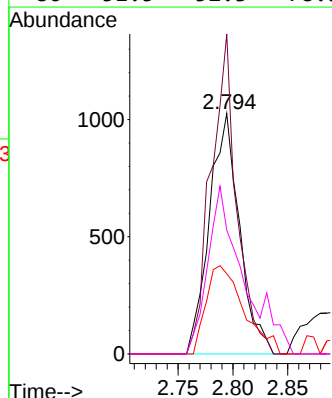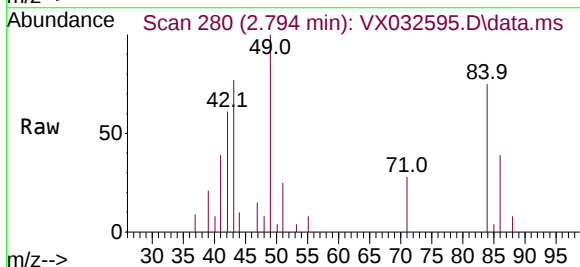






#31
Cyclohexane
Concen: 2.171 ug/l
RT: 5.477 min Scan# 719
Delta R.T. 0.006 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 4362
Ion Ratio Lower Upper
56 100
69 32.0 24.1 36.1
84 86.6 66.9 100.3

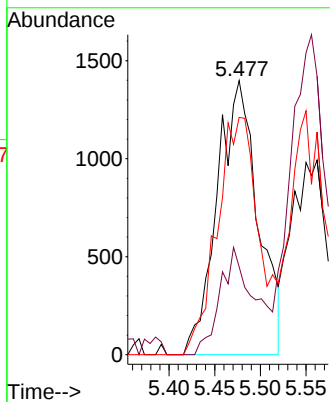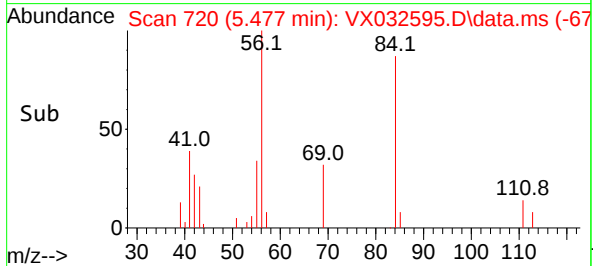

#33
1,2-Dichloroethane-d4
Concen: 49.528 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17

Tgt Ion: 65 Resp: 82065
Ion Ratio Lower Upper
65 100
67 49.2 0.0 101.8


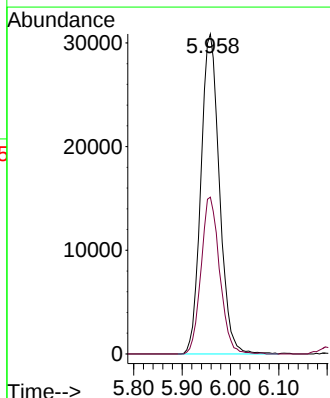

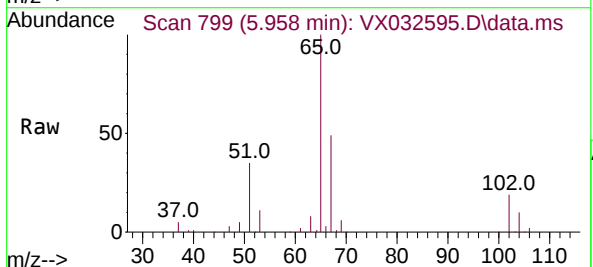




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 195812
Ion Ratio Lower Upper
114 100
63 20.2 0.0 41.6
88 16.1 0.0 33.4



#35
Dibromofluoromethane
Concen: 45.471 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17


Tgt Ion:113 Resp: 63511
Ion Ratio Lower Upper
113 100
111 101.8 82.4 123.6
192 19.4 15.4 23.2

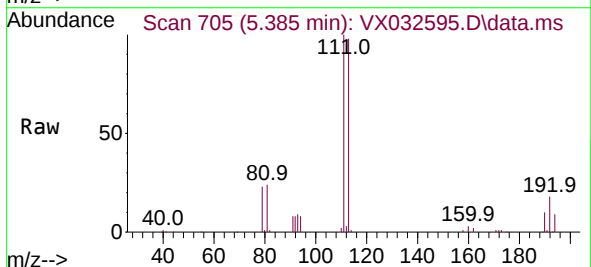






#36
1,1-Dichloropropene
Concen: 4.792 ug/l
RT: 5.550 min Scan# 711
Delta R.T. -0.146 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion: 75 Resp: 9321
Ion Ratio Lower Upper
75 100
110 8.6 18.4 55.2#
77 0.0 24.5 36.7#

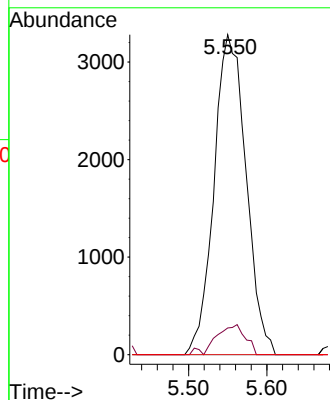


#38
Carbon Tetrachloride
Concen: 5.765 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.128 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17

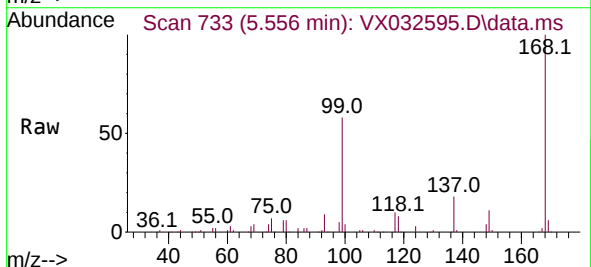

Tgt Ion: 117 Resp: 12437
Ion Ratio Lower Upper
117 100
119 3.6 77.2 115.8#
121 0.0 25.8 38.6#



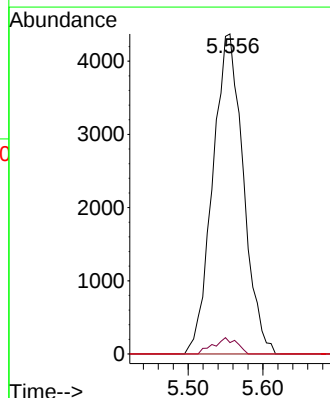
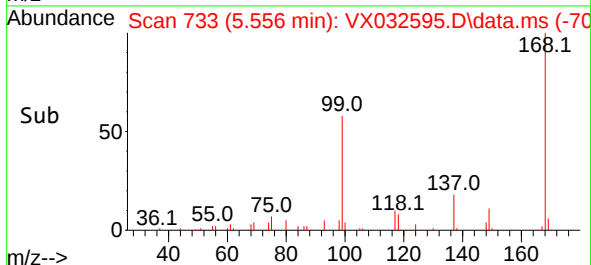




#39
Methylcyclohexane
Concen: 1.317 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. 0.000 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 83 Resp: 3030
Ion Ratio Lower Upper
83 100
55 55.1 58.4 87.6#
98 51.4 37.2 55.8

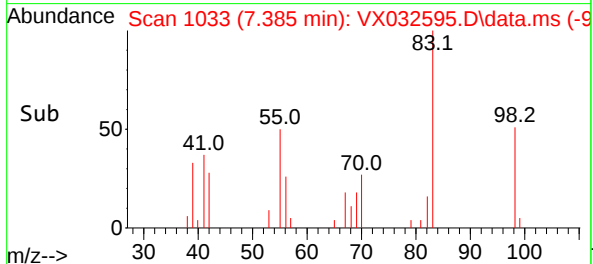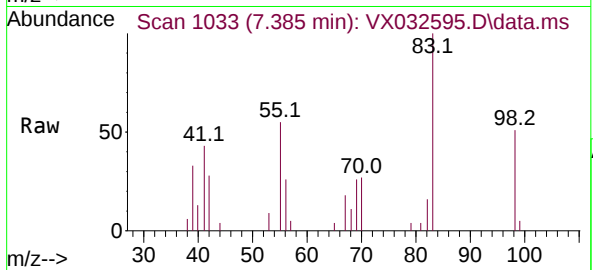

#40
Benzene
Concen: 0.603 ug/l
RT: 6.044 min Scan# 813
Delta R.T. 0.006 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17

Tgt Ion: 78 Resp: 3319
Ion Ratio Lower Upper
78 100
77 21.3 19.0 28.4


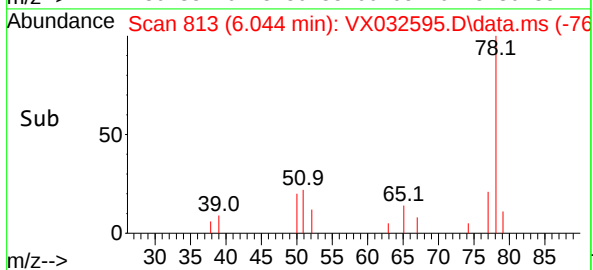

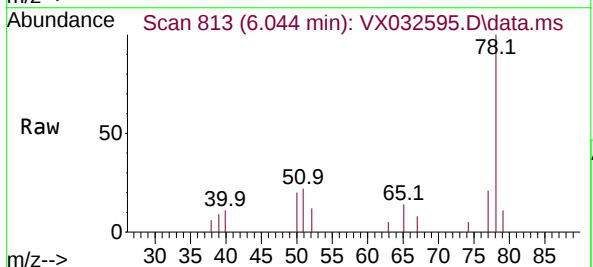


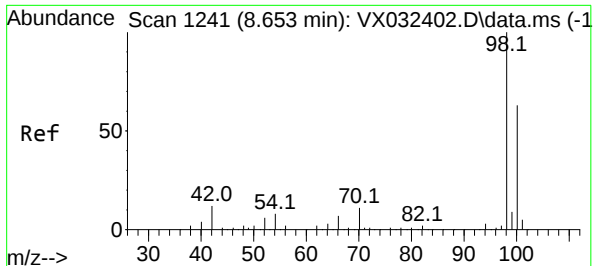

#50
Toluene-d8
Concen: 48.140 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 233804
Ion Ratio Lower Upper
98 100
100 63.8 50.9 76.3

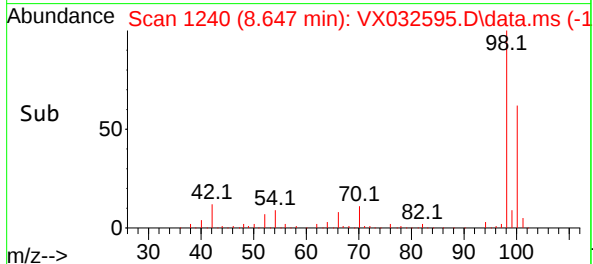

#52
Toluene
Concen: 13.974 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.000 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17

Tgt Ion: 92 Resp: 50181
Ion Ratio Lower Upper
92 100
91 177.9 138.3 207.5




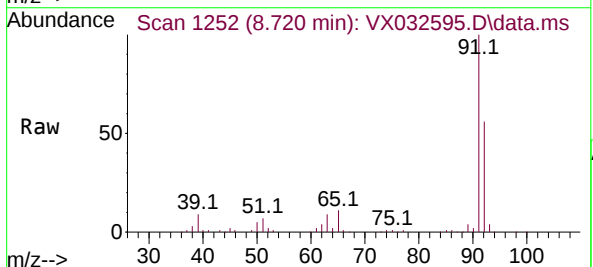




#62
4-Bromofluorobenzene
Concen: 48.047 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 91153
Ion Ratio Lower Upper
95 100
174 82.4 0.0 164.0
176 79.9 0.0 154.4

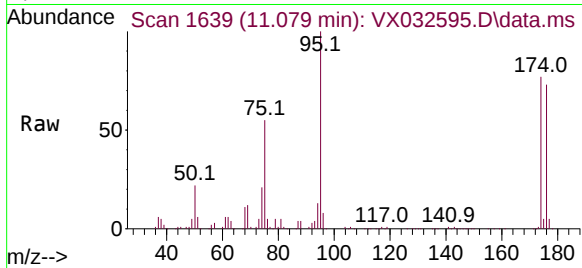

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17

Tgt Ion: 117 Resp: 171832
Ion Ratio Lower Upper
117 100
82 56.5 44.3 66.5
119 32.5 25.7 38.5




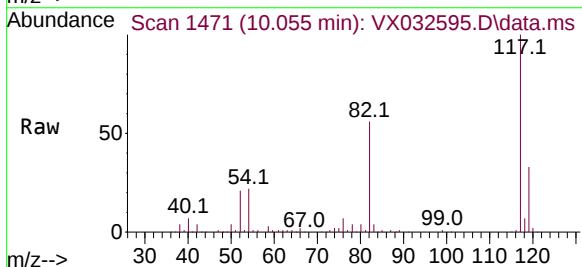




#67
Ethyl Benzene
Concen: 18.564 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 127780
Ion Ratio Lower Upper
91 100
106 30.1 25.0 37.6



#68
m/p-Xylenes
Concen: 65.812 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.006 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17

Tgt Ion:106 Resp: 175899
Ion Ratio Lower Upper
106 100
91 205.7 164.5 246.7




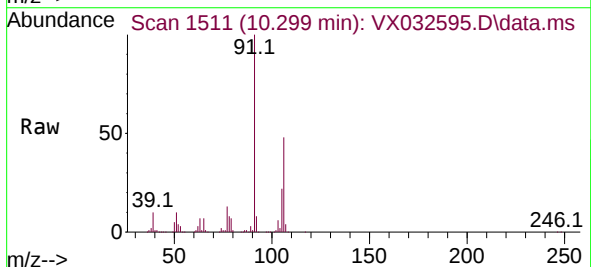




#69
o-Xylene
Concen: 26.700 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 69385
Ion Ratio Lower Upper
106 100
91 220.5 109.2 327.6

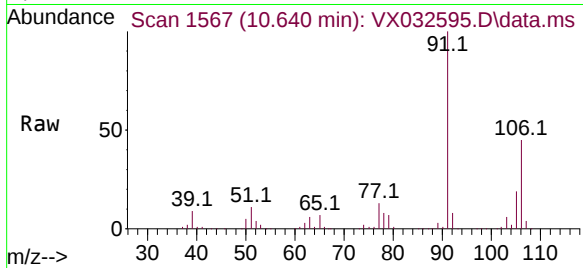

#70
Styrene
Concen: 1.066 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. -0.012 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17

Tgt Ion:104 Resp: 4604
Ion Ratio Lower Upper
104 100
78 258.0 41.8 62.8#
103 220.8 44.5 66.7#




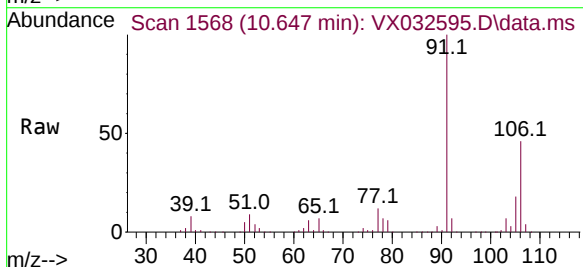




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:152 Resp: 82911
Ion Ratio Lower Upper
152 100
115 61.0 44.0 132.0
150 158.4 0.0 351.8

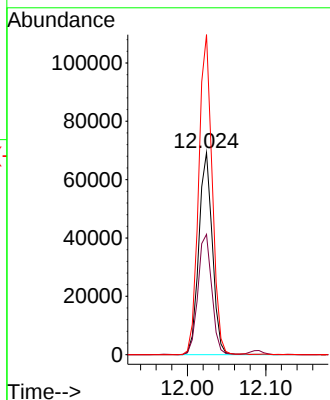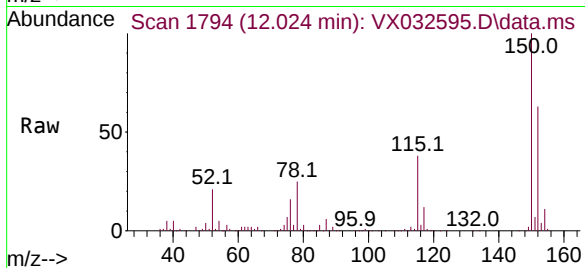

#73
Isopropylbenzene
Concen: 1.319 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17

Tgt Ion:105 Resp: 8667
Ion Ratio Lower Upper
105 100
120 27.1 13.1 39.3

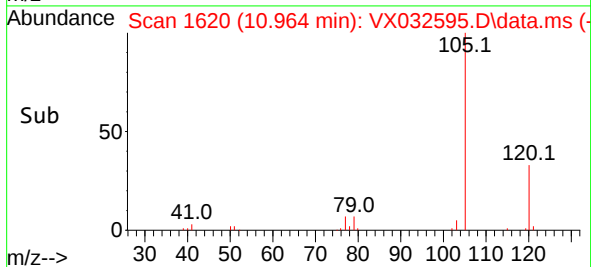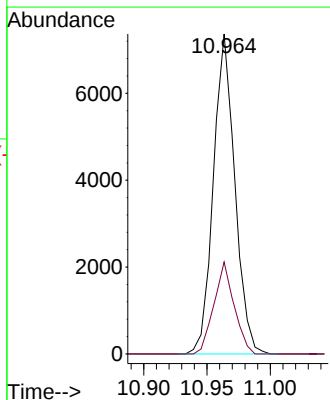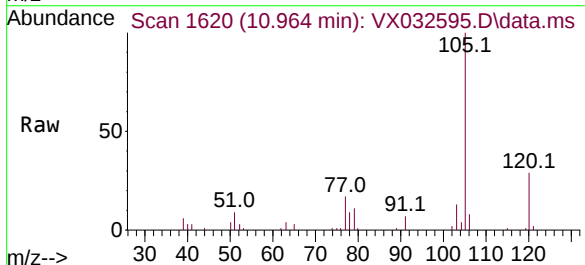



#76

1,2,3-Trichloropropane

Concen: 26.912 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.164 min

Lab File: VX032595.D

Acq: 05 Nov 2022 01:17

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 49641

Ion Ratio Lower Upper

75 100

77 0.0 20.0 60.0#



#78

n-propylbenzene

Concen: 3.225 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX032595.D




Acq: 05 Nov 2022 01:17


Tgt Ion: 91 Resp: 24412

Ion Ratio Lower Upper

91 100

120 21.5 11.6 34.8

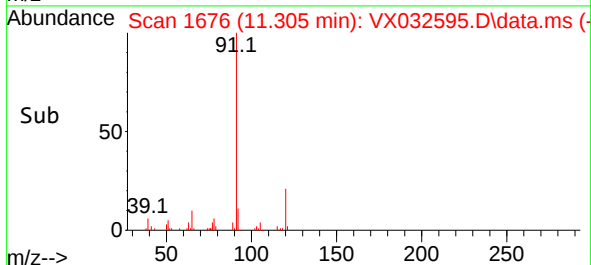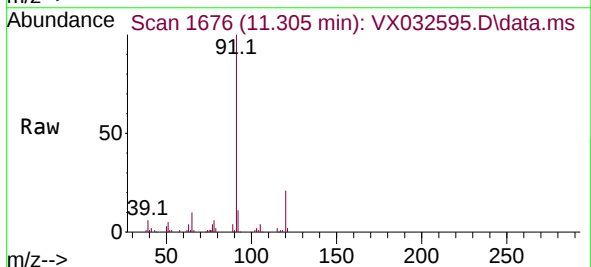



#79

2-Chlorotoluene

Concen: 3.971 ug/l

RT: 11.378 min Scan# 1

Delta R.T. 0.012 min

Lab File: VX032595.D

Acq: 05 Nov 2022 01:17

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 18001

Ion Ratio Lower Upper

91 100

126 0.8 17.1 51.2#

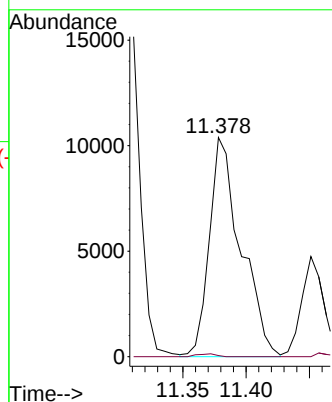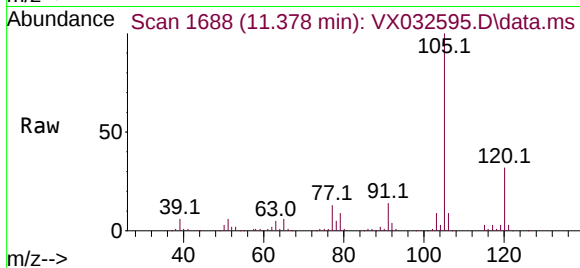

#80

1,3,5-Trimethylbenzene

Concen: 8.155 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX032595.D




Acq: 05 Nov 2022 01:17


Tgt Ion:105 Resp: 45789

Ion Ratio Lower Upper

105 100

120 48.1 23.6 71.0




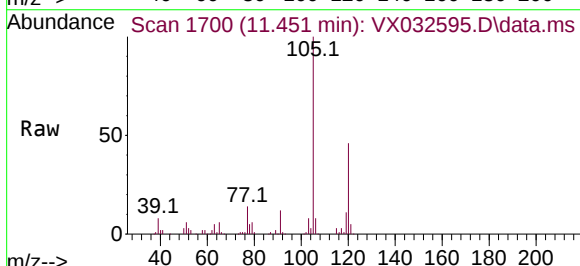




#81
trans-1,4-Dichloro-2-butene
Concen: 85.635 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 49641
Ion Ratio Lower Upper
75 100
53 0.0 86.9 130.3#
89 0.0 38.3 57.5#

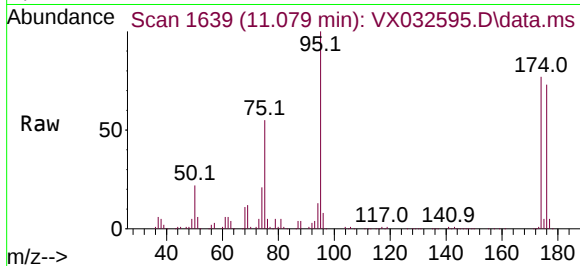

#82
4-Chlorotoluene
Concen: 1.076 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX032595.D
Acq: 05 Nov 2022 01:17

Tgt Ion: 91 Resp: 5710
Ion Ratio Lower Upper
91 100
126 2.2 14.8 44.4#

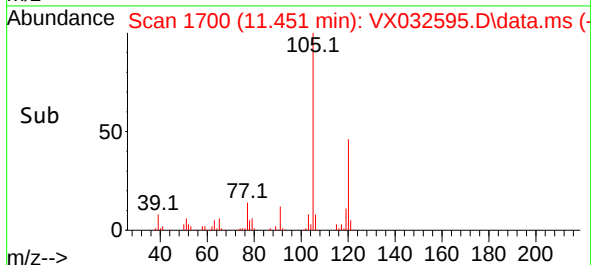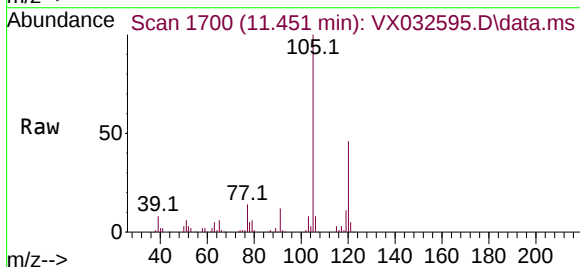



#83

tert-Butylbenzene

Concen: 3.225 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.037 min

Lab File: VX032595.D

Acq: 05 Nov 2022 01:17

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:119 Resp: 18077

Ion Ratio Lower Upper

119 100

91 97.8 29.4 88.2#

134 0.0 11.0 33.0#

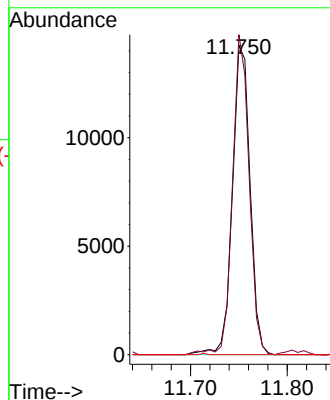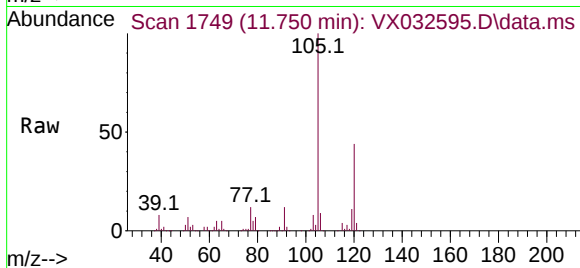

#84

1,2,4-Trimethylbenzene

Concen: 27.582 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX032595.D




Acq: 05 Nov 2022 01:17


Tgt Ion:105 Resp: 154039

Ion Ratio Lower Upper

105 100

120 44.1 21.9 65.5



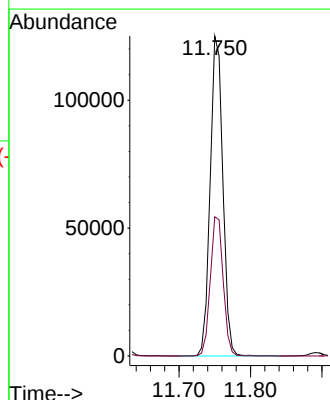
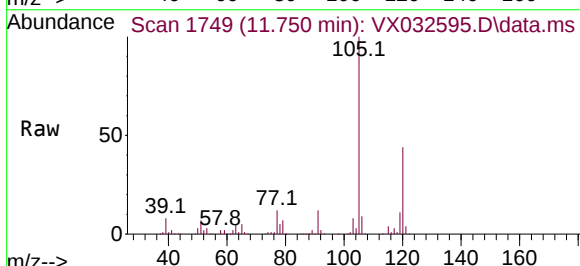




#85
 sec-Butylbenzene
 Concen: 22.836 ug/l
 RT: 11.750 min Scan# 1178
 Delta R.T. -0.140 min
 Lab File: VX032595.D
 Acq: 05 Nov 2022 01:17




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:105 Resp: 154039
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.9 29.7#

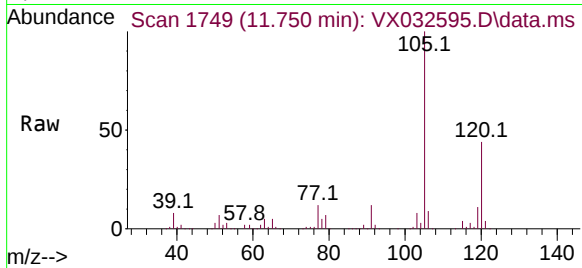

#86
 p-Isopropyltoluene
 Concen: 0.360 ug/l
 RT: 11.969 min Scan# 1785
 Delta R.T. -0.043 min
 Lab File: VX032595.D
 Acq: 05 Nov 2022 01:17

Tgt Ion:119 Resp: 2058
 Ion Ratio Lower Upper
 119 100
 134 25.3 12.9 38.7
 91 26.6 12.5 37.5

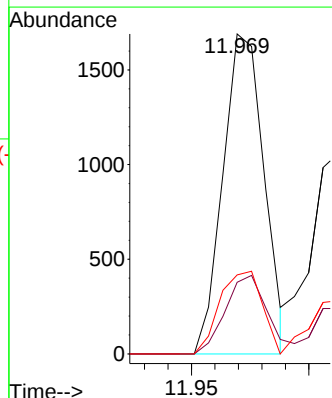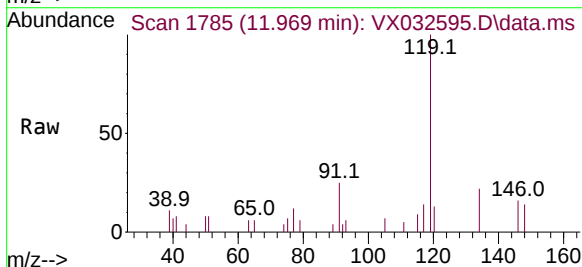



#89

n-Butylbenzene

Concen: 0.809 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.006 min

Lab File: VX032595.D

Acq: 05 Nov 2022 01:17

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 91 Resp: 4026

Ion Ratio Lower Upper

91 100

92 29.5 26.2 78.6

134 106.1 12.9 38.6#

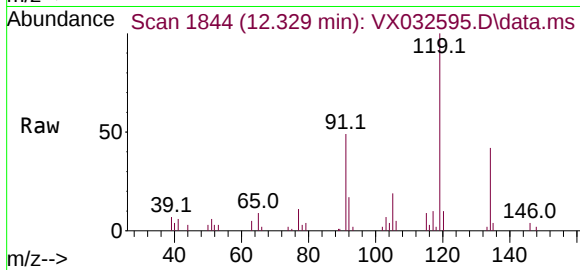

#90

Hexachloroethane

Concen: 1.448 ug/l

RT: 12.530 min Scan# 1877

Delta R.T. -0.012 min

Lab File: VX032595.D




Acq: 05 Nov 2022 01:17


Tgt Ion: 117 Resp: 1354

Ion Ratio Lower Upper

117 100


201 0.0 37.6 112.9#

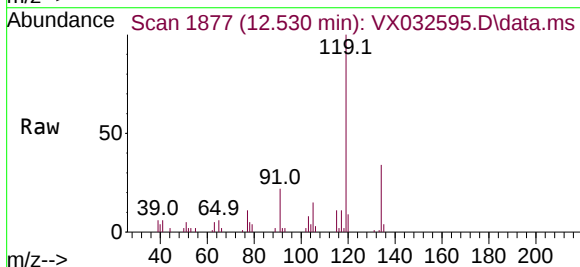






#93
 1,2,4-Trichlorobenzene
 Concen: 0.210 ug/l
 RT: 13.591 min Scan# 2051
 Delta R.T. 0.000 min
 Lab File: VX032595.D
 Acq: 05 Nov 2022 01:17

Instrument :
 MSVOA_X
 ClientSampleId :

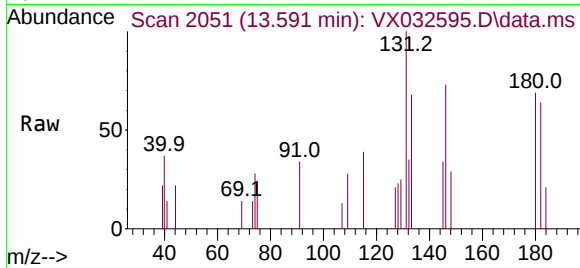

Tgt Ion:180 Resp: 411




Ion	Ratio	Lower	Upper
180	100		
182	78.1	48.4	145.0
145	40.1	16.2	48.5

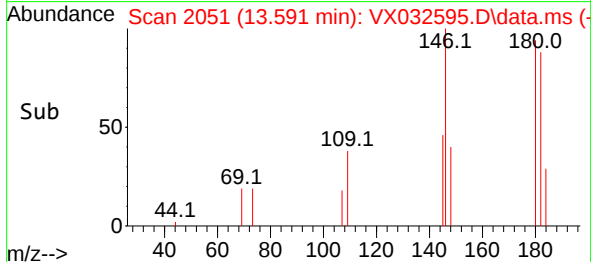


#94
 Hexachlorobutadiene
 Concen: 0.373 ug/l
 RT: 13.719 min Scan# 2072
 Delta R.T. -0.006 min
 Lab File: VX032595.D
 Acq: 05 Nov 2022 01:17

Tgt Ion:225 Resp: 304

Ion	Ratio	Lower	Upper
225	100		
223	61.8	31.9	95.9
227	49.7	31.9	95.5

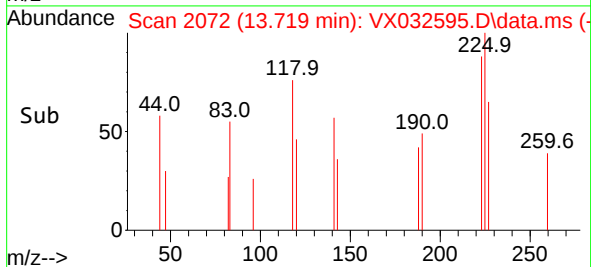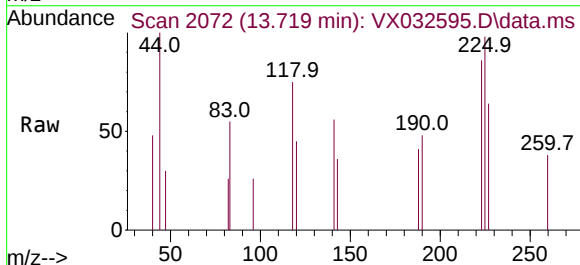



#95

Naphthalene

Concen: 5.937 ug/l

RT: 13.774 min Scan# 20

Delta R.T. -0.006 min


Lab File: VX032595.D

Acq: 05 Nov 2022 01:17

Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion:128 Resp: 38643

Ion Ratio Lower Upper

128 100

127 13.2 10.2 15.4

129 10.7 8.9 13.3

