

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX110422\  
Data File : VX032577.D  
Acq On : 04 Nov 2022 15:28  
Operator : JC/MD  
Sample : N5474-02  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
5592-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X102622W.M

Title : SW846 8260

Signal : TIC: VX032577.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.391       | 694           | 706         | 721          | rBV2     | 72875          | 214130        | 34.20%          | 6.286%        |
| 2         | 5.556       | 721           | 733         | 748          | rVV      | 125933         | 354608        | 56.64%          | 10.410%       |
| 3         | 5.958       | 789           | 799         | 812          | rBV      | 81466          | 215221        | 34.38%          | 6.318%        |
| 4         | 6.763       | 915           | 931         | 945          | rBV      | 197297         | 469522        | 74.99%          | 13.783%       |
| 5         | 8.653       | 1234          | 1241        | 1254         | rBV      | 392553         | 626078        | 100.00%         | 18.379%       |
| 6         | 10.055      | 1465          | 1471        | 1485         | rBV      | 412373         | 543137        | 86.75%          | 15.944%       |
| 7         | 11.079      | 1634          | 1639        | 1653         | rBV      | 358312         | 465049        | 74.28%          | 13.652%       |
| 8         | 12.024      | 1788          | 1794        | 1804         | rBV      | 412957         | 518749        | 82.86%          | 15.228%       |




Sum of corrected areas: 3406494

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX110422\  
Data File : VX032577.D  
Acq On : 04 Nov 2022 15:28  
Operator : JC/MD  
Sample : N5474-02  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
5592-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X102622W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

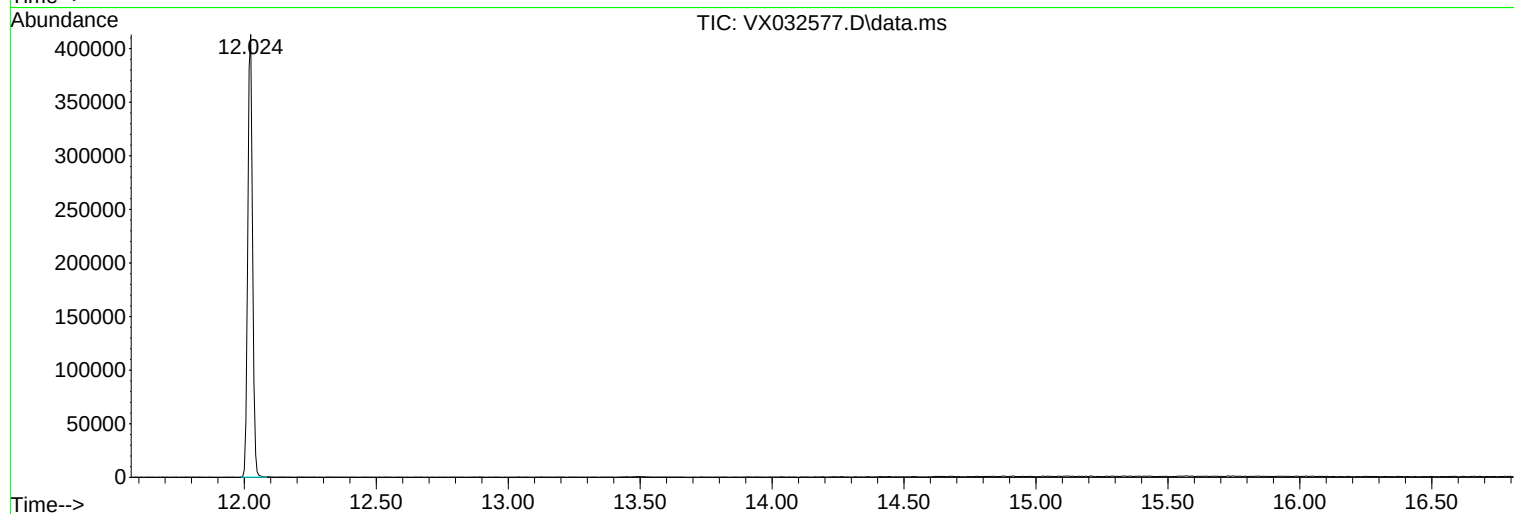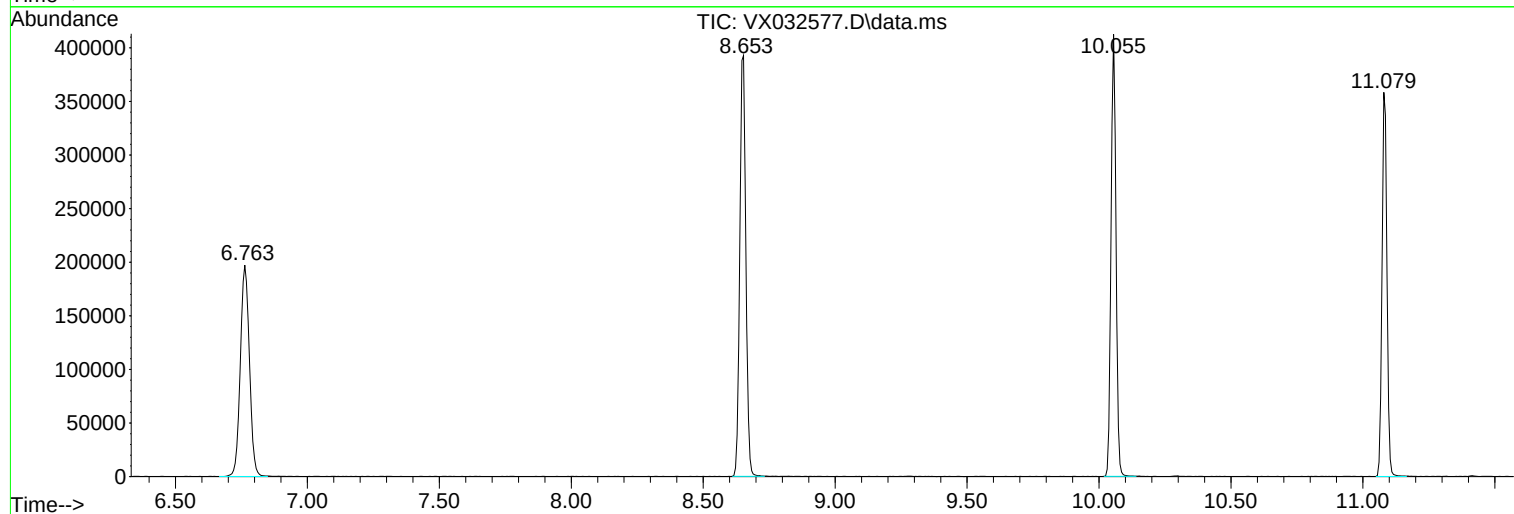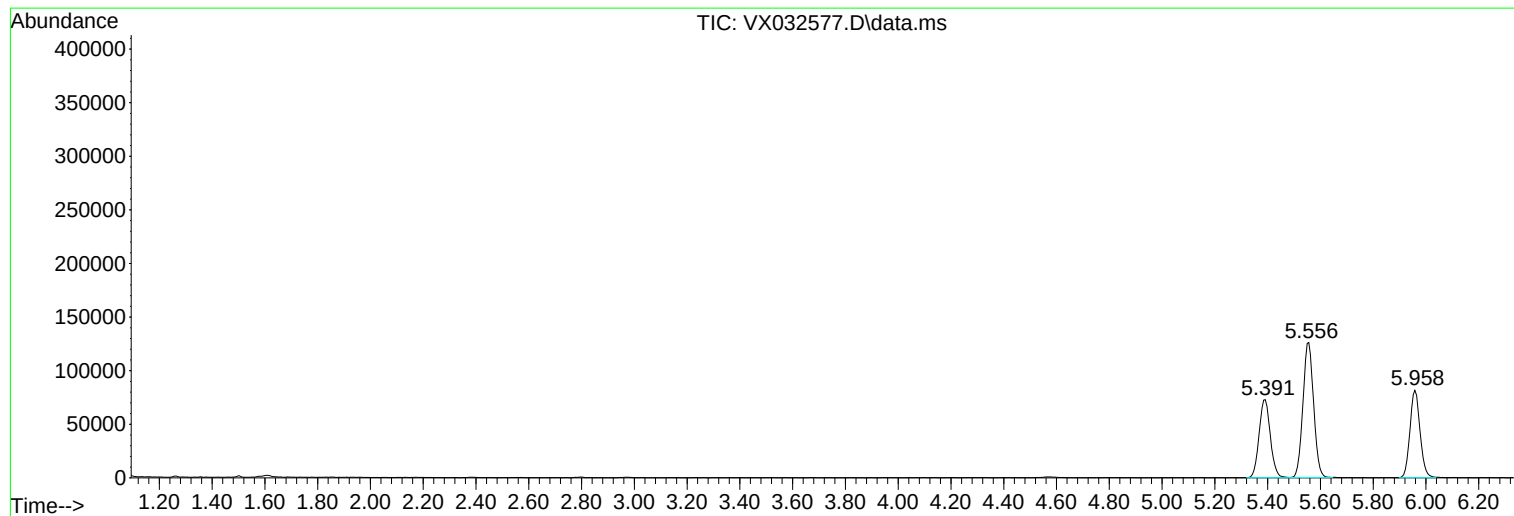

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX110422\  
Data File : VX032577.D  
Acq On : 04 Nov 2022 15:28  
Operator : JC/MD  
Sample : N5474-02  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
5592-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X102622W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX110422\  
Data File : VX032577.D  
Acq On : 04 Nov 2022 15:28  
Operator : JC/MD  
Sample : N5474-02  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
5592-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X102622W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|