

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX110422\  
Data File : VX032578.D  
Acq On : 04 Nov 2022 15:52  
Operator : JC/MD  
Sample : N5476-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RED-006-5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X102622W.M

Title : SW846 8260

Signal : TIC: VX032578.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.385       | 693           | 705         | 721          | rBV      | 73421          | 213498        | 34.42%          | 6.355%        |
| 2         | 5.556       | 721           | 733         | 749          | rVV      | 123879         | 350523        | 56.51%          | 10.434%       |
| 3         | 5.958       | 788           | 799         | 816          | rBV      | 79718          | 213368        | 34.40%          | 6.351%        |
| 4         | 6.763       | 921           | 931         | 946          | rBV      | 191225         | 456476        | 73.59%          | 13.587%       |
| 5         | 8.647       | 1234          | 1240        | 1251         | rBV      | 383965         | 620285        | 100.00%         | 18.463%       |
| 6         | 10.055      | 1465          | 1471        | 1485         | rBV      | 400007         | 536173        | 86.44%          | 15.960%       |
| 7         | 11.079      | 1634          | 1639        | 1648         | rBV      | 348037         | 457144        | 73.70%          | 13.607%       |
| 8         | 12.024      | 1788          | 1794        | 1805         | rBV      | 410264         | 512064        | 82.55%          | 15.242%       |




Sum of corrected areas: 3359531

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX110422\  
Data File : VX032578.D  
Acq On : 04 Nov 2022 15:52  
Operator : JC/MD  
Sample : N5476-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RED-006-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X102622W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

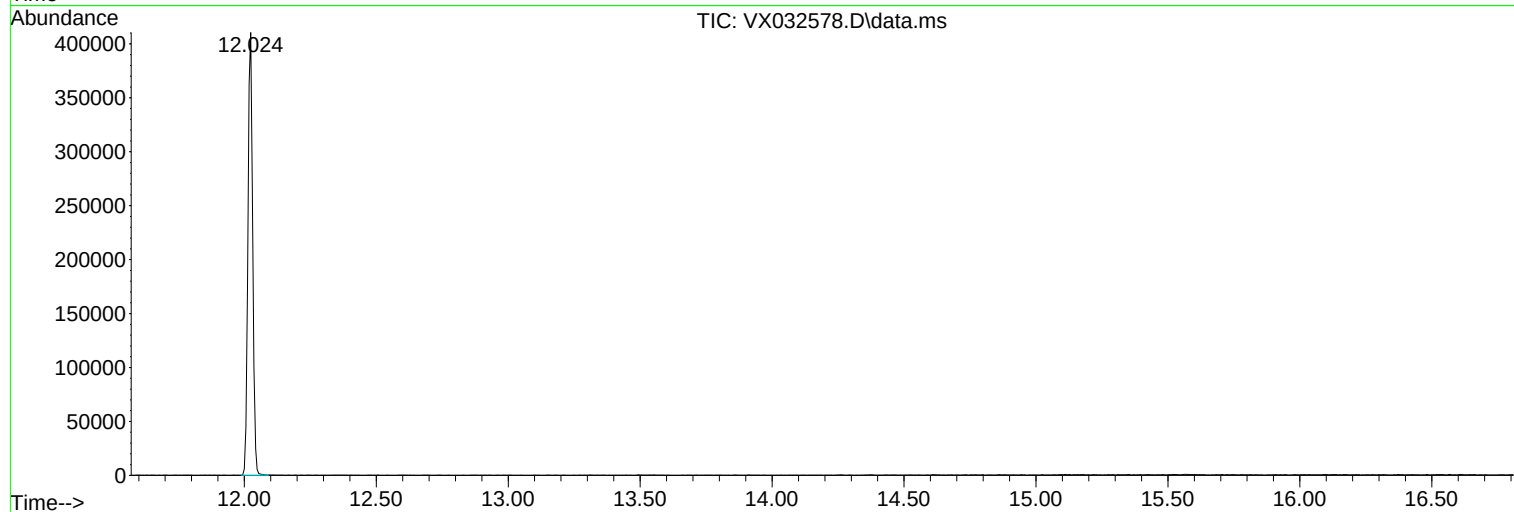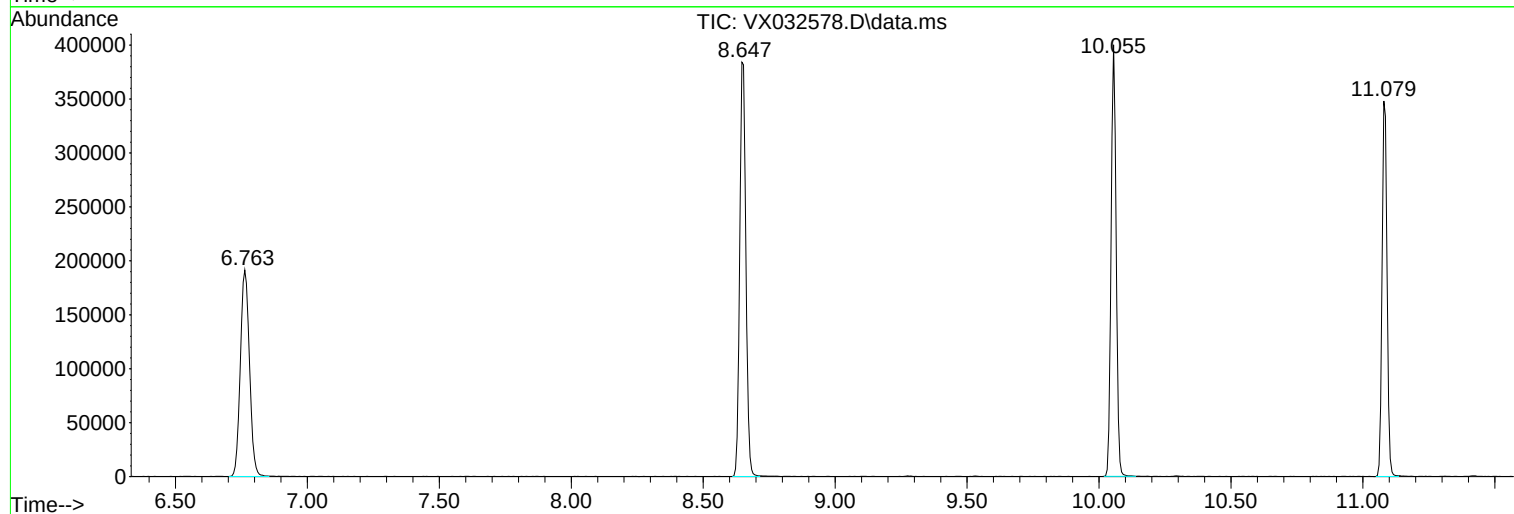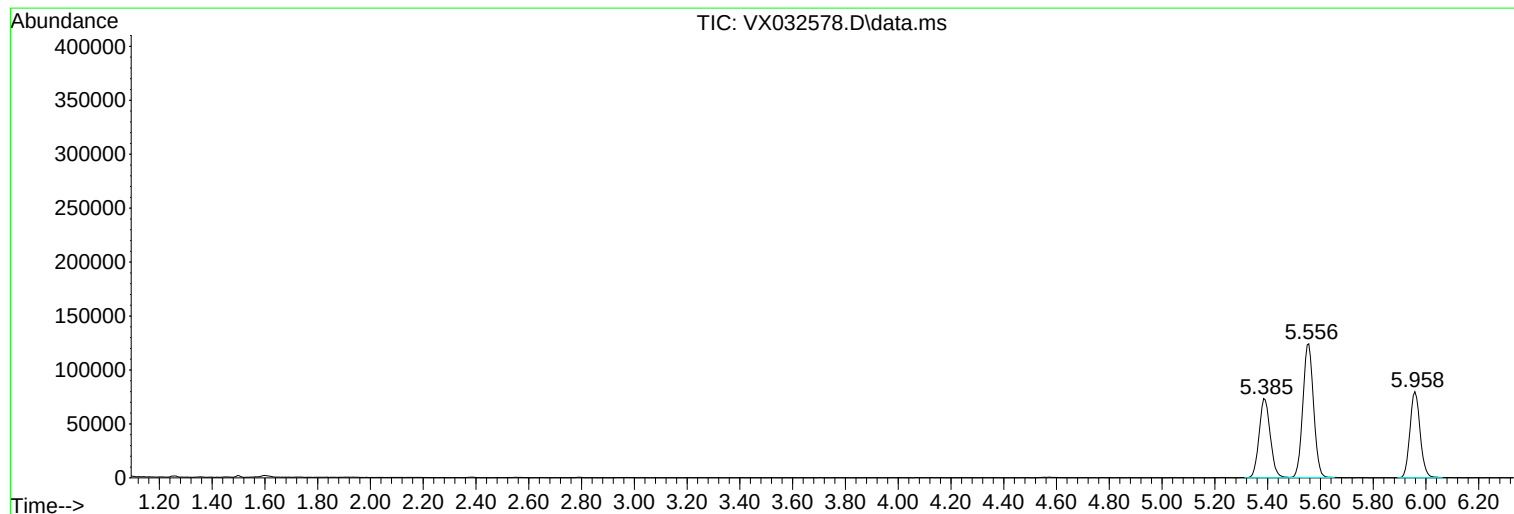

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX110422\  
Data File : VX032578.D  
Acq On : 04 Nov 2022 15:52  
Operator : JC/MD  
Sample : N5476-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RED-006-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X102622W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX110422\  
Data File : VX032578.D  
Acq On : 04 Nov 2022 15:52  
Operator : JC/MD  
Sample : N5476-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RED-006-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X102622W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|