


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110422\
Data File : VX032590.D
Acq On : 04 Nov 2022 22:35
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Title : SW846 8260
Last Update : Thu Oct 27 08:28:06 2022

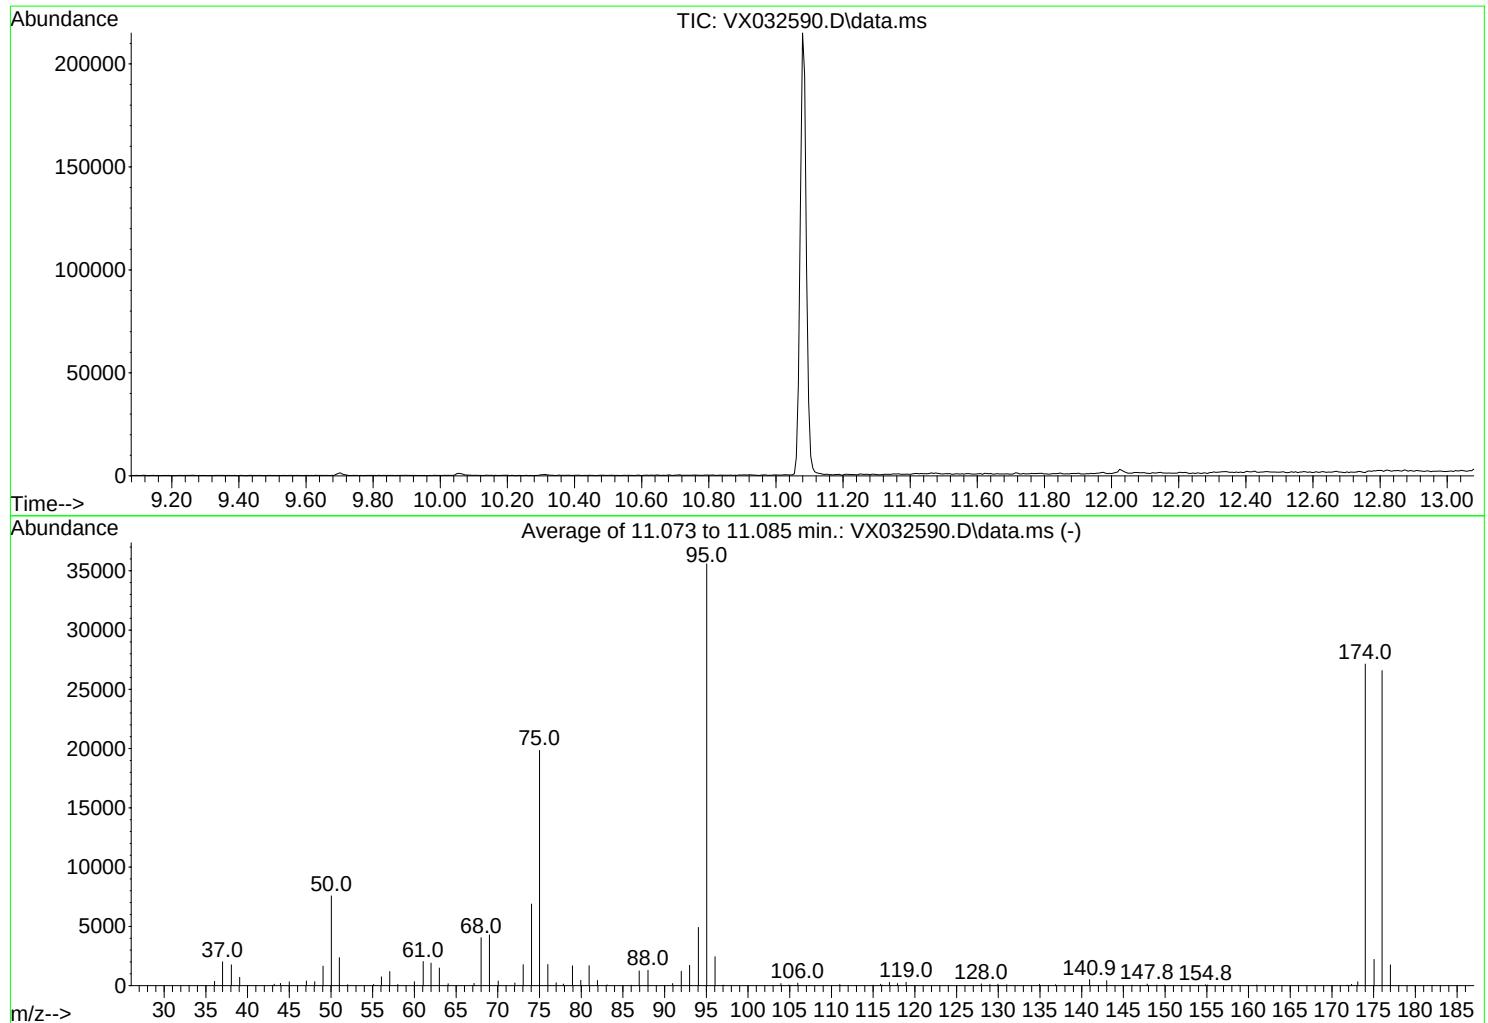

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	7571	PASS
75	95	30	60	55.8	19845	PASS
95	95	100	100	100.0	35587	PASS
96	95	5	9	6.9	2440	PASS
173	174	0.00	2	1.2	322	PASS
174	95	50	100	76.3	27141	PASS
175	174	5	9	8.2	2212	PASS
176	174	95	101	97.9	26579	PASS
177	176	5	9	6.6	1760	PASS