

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043683.D
 Acq On : 04 Nov 2024 15:32
 Operator : JC/MD
 Sample : PB164621TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 05 03:46:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 05 03:44:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	359659	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	311849	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	136989	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	65776	34.329	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	68.660%
7) Chloroethane-d5	1.642	69	32630	39.619	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.240%
11) 1,1-Dichloroethene-d2	2.294	65	31934	36.104	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.200%
21) 2-Butanone-d5	4.465	46	136218	108.581	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	108.580%
24) Chloroform-d	5.050	84	180247	43.638	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.280%
26) 1,2-Dichloroethane-d4	5.952	65	121643	46.358	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.720%
32) Benzene-d6	5.964	84	346796	43.013	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.020%
36) 1,2-Dichloropropane-d6	7.305	67	115002	46.884	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.760%
41) Toluene-d8	8.647	98	306927	41.906	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.820%
43) trans-1,3-Dichloroprop...	8.952	79	51005	43.480	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.960%
47) 2-Hexanone-d5	9.384	63	103970	107.102	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	107.100%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	162433	51.611	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.220%
66) 1,2-Dichlorobenzene-d4	12.317	152	116454	49.064	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.120%
Target Compounds						
37) 1,2-Dichloropropane	7.312	63	13001	5.491	ug/L	Qvalue # 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043683.D
Acq On : 04 Nov 2024 15:32
Operator : JC/MD
Sample : PB164621TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 05 03:46:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 05 03:44:12 2024
Response via : Initial Calibration

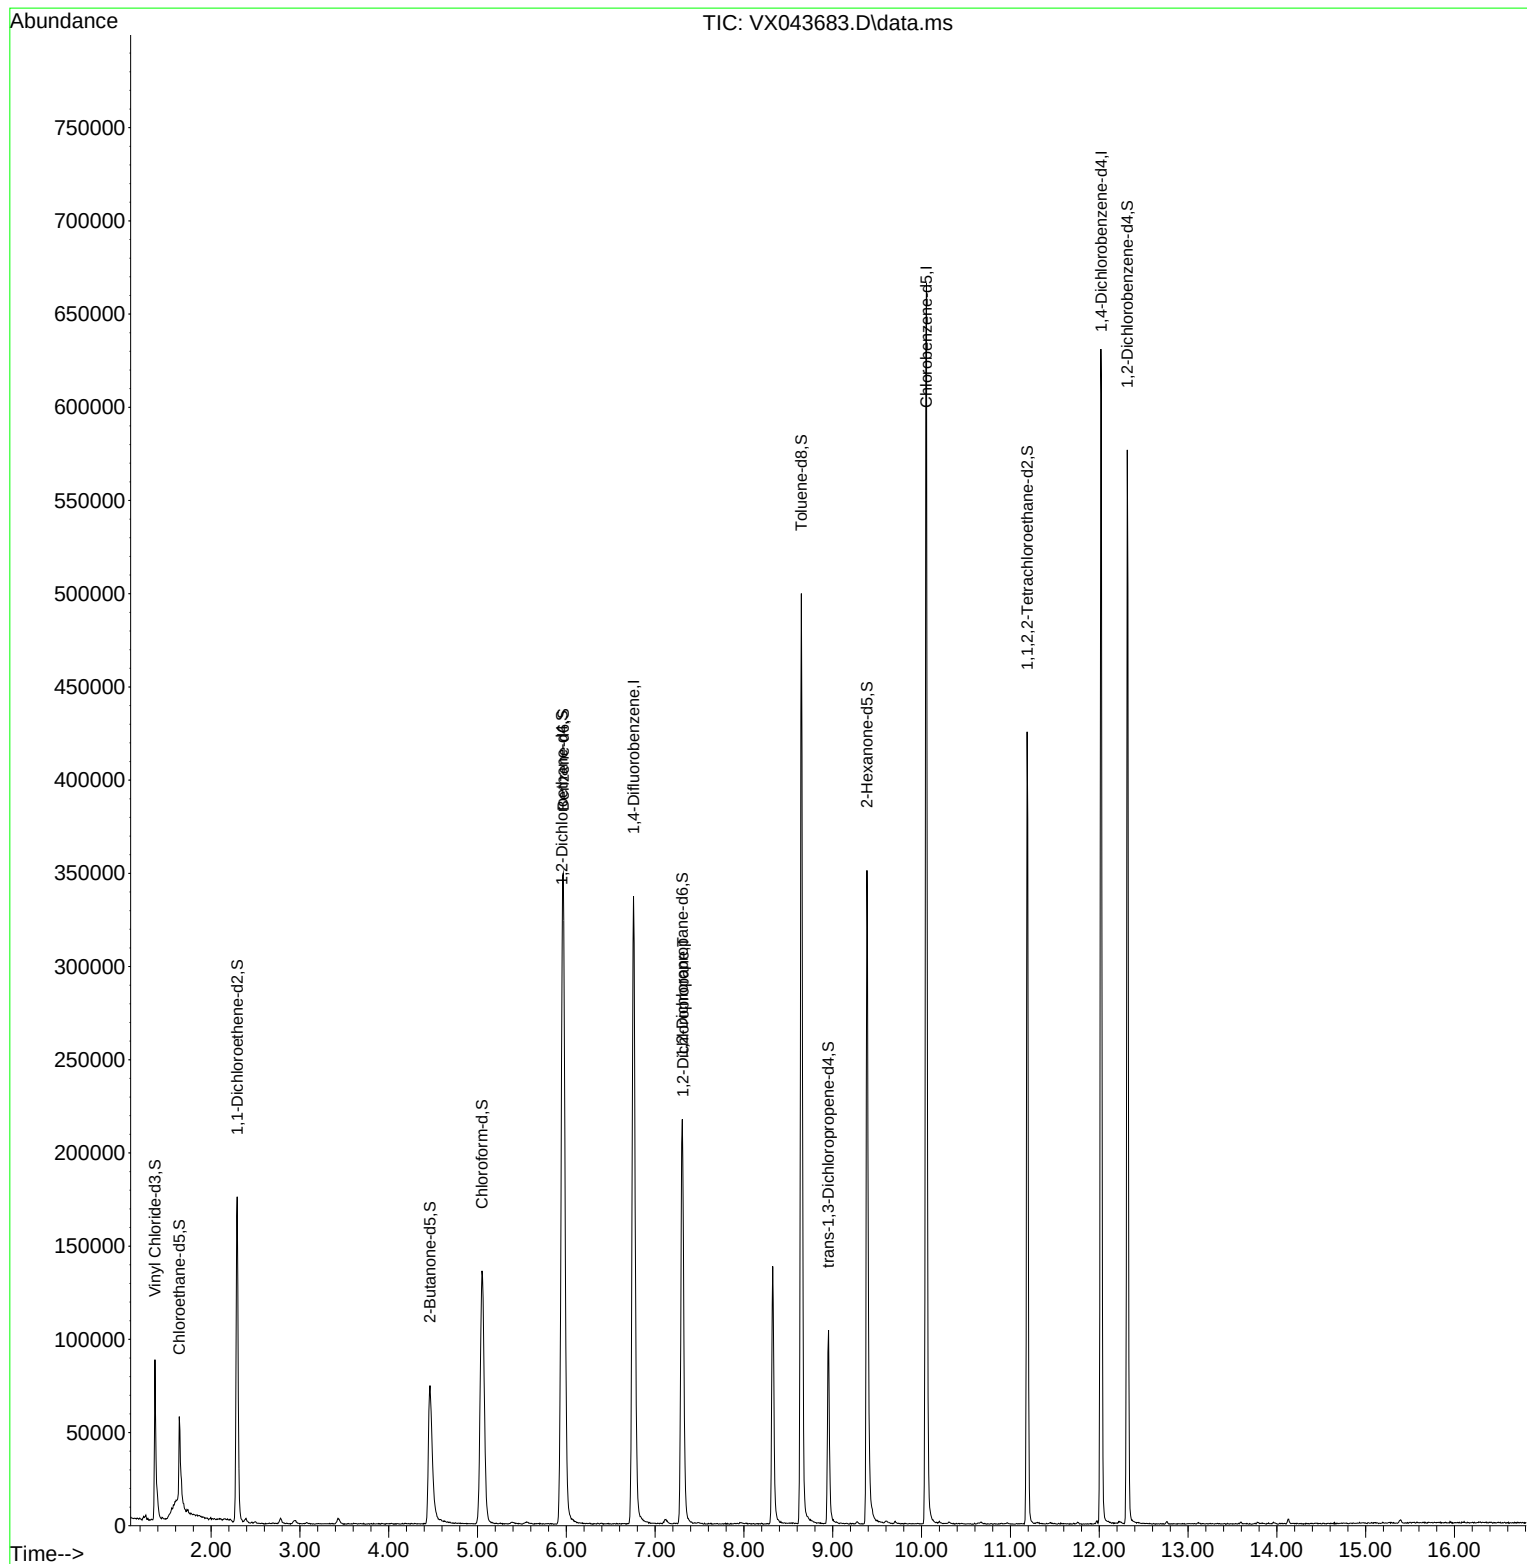

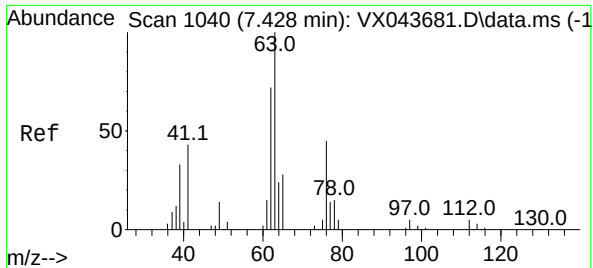

#37
 1,2-Dichloropropane
 Concen: 5.491 ug/L
 RT: 7.312 min Scan# 10
 Delta R.T. -0.116 min
 Lab File: VX043683.D
 Acq: 04 Nov 2024 15:32

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 63 Resp: 13001
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.8 5.8#

