

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043690.D
 Acq On : 04 Nov 2024 18:14
 Operator : JC/MD
 Sample : P4621-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 05 03:47:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 05 03:44:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	357106	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	322653	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	145231	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	86037	45.225	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	90.440%	
7) Chloroethane-d5	1.642	69	44535	54.461	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	108.920%	
11) 1,1-Dichloroethene-d2	2.294	65	41165	46.873	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	93.740%	
21) 2-Butanone-d5	4.465	46	184284	147.945	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	147.950%#	
24) Chloroform-d	5.050	84	227949	55.581	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	111.160%	
26) 1,2-Dichloroethane-d4	5.952	65	156569	60.095	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	120.180%	
32) Benzene-d6	5.964	84	457532	54.848	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	109.700%	
36) 1,2-Dichloropropane-d6	7.306	67	151440	59.671	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	119.340%	
41) Toluene-d8	8.647	98	406008	53.578	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	107.160%	
43) trans-1,3-Dichloroprop...	8.952	79	68259	56.240	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	112.480%	
47) 2-Hexanone-d5	9.384	63	132572	131.993	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	131.990%#	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	221864	68.134	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	136.260%#	
66) 1,2-Dichlorobenzene-d4	12.317	152	169749	67.460	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	134.920%#	
Target Compounds						Qvalue
13) Acetone	2.386	43	314370	271.356	ug/L	98
48) 2-Hexanone	9.384	43	16041	6.436	ug/L #	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043690.D
Acq On : 04 Nov 2024 18:14
Operator : JC/MD
Sample : P4621-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Nov 05 03:47:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 05 03:44:12 2024
Response via : Initial Calibration

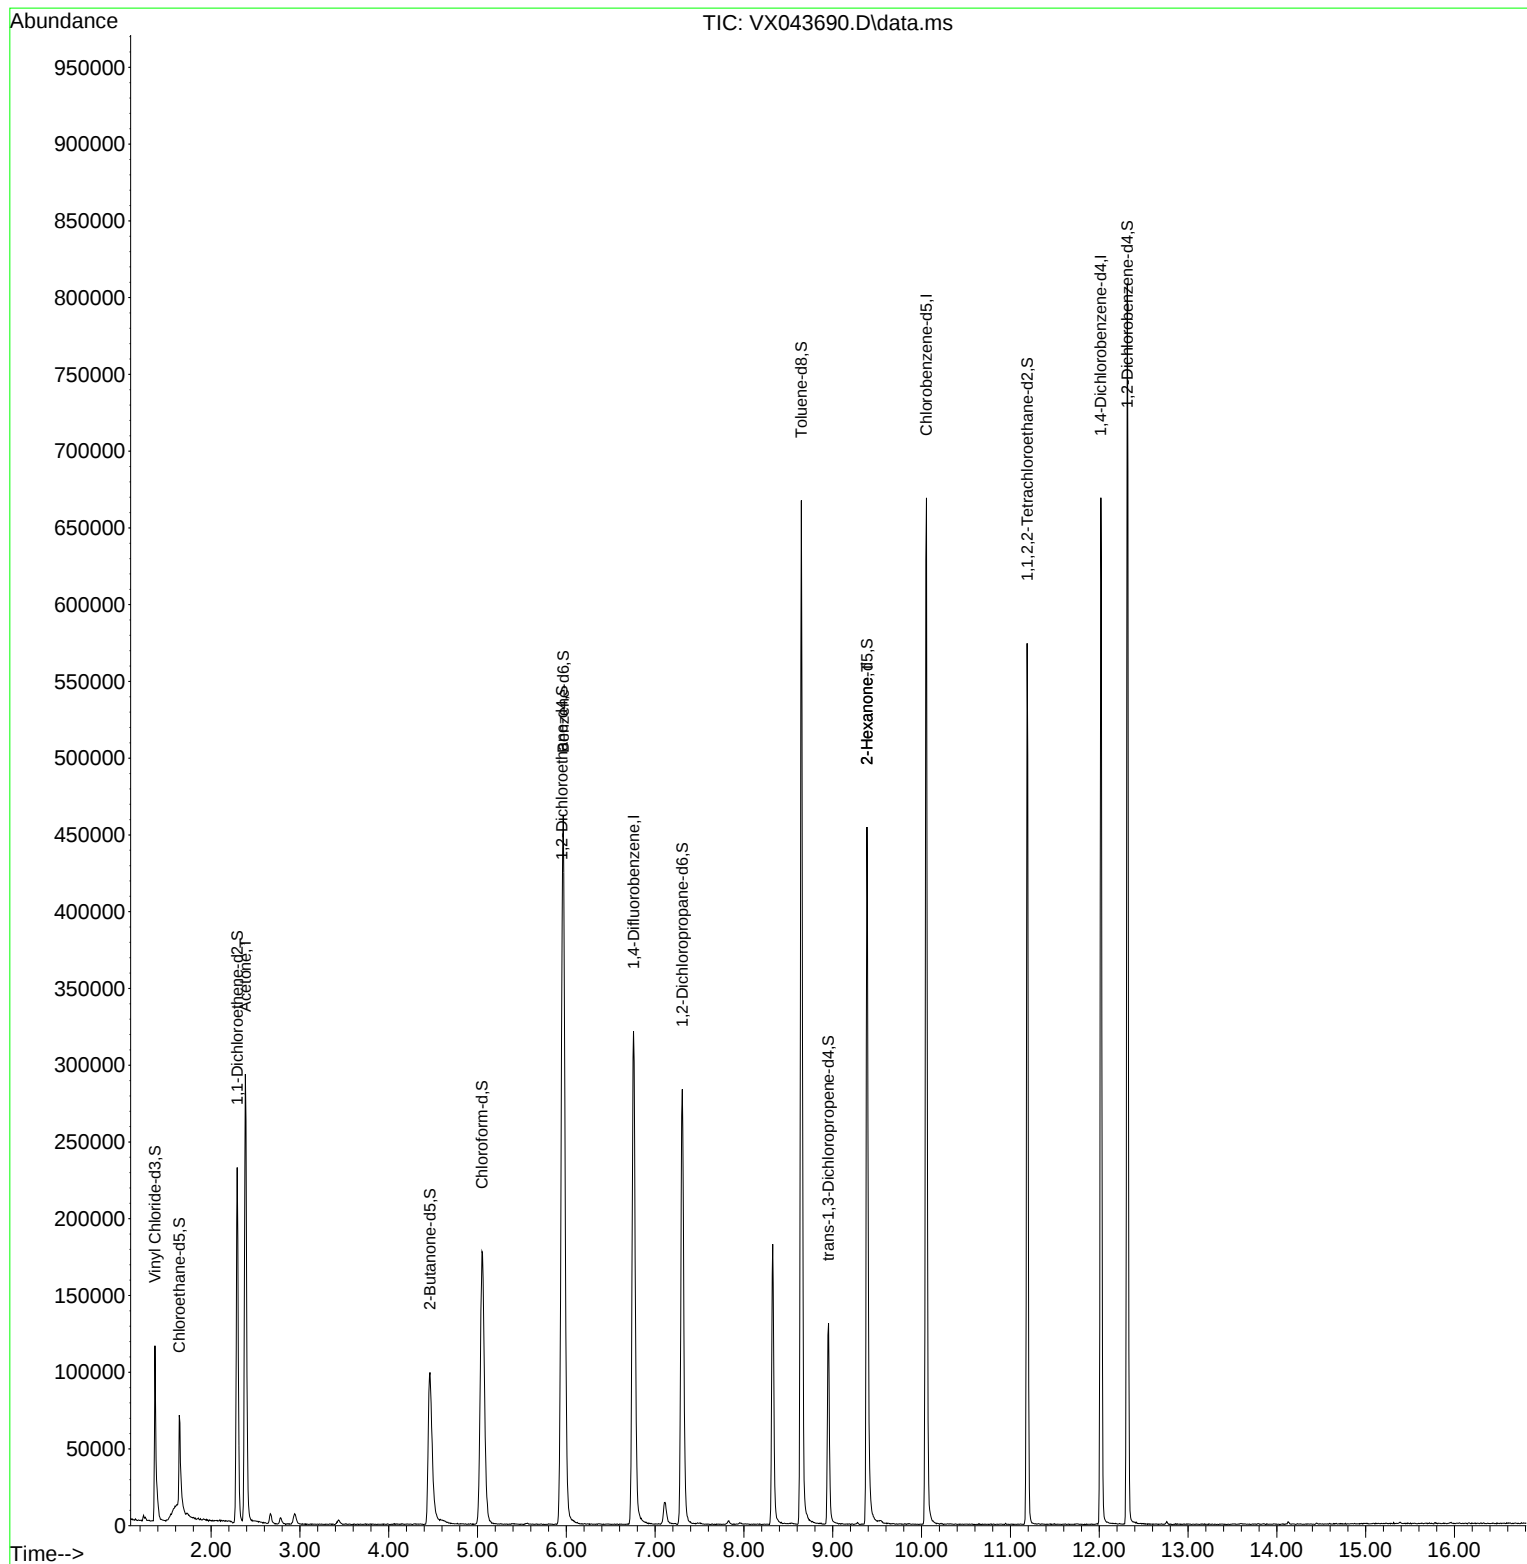



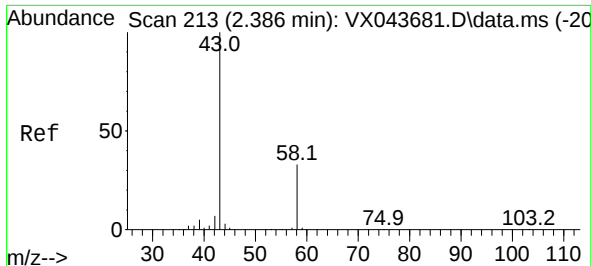


#13
Acetone
Concen: 271.356 ug/L
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX043690.D
Acq: 04 Nov 2024 18:14

Instrument :
MSVOA_X
ClientSampleId :

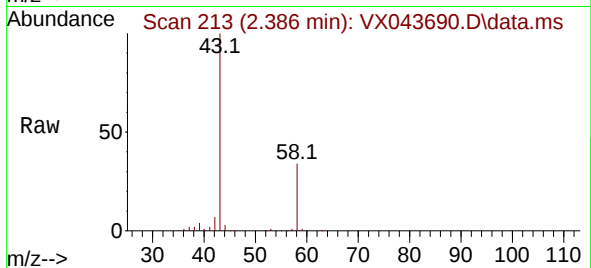

Tgt Ion: 43 Resp: 314370
Ion Ratio Lower Upper
43 100
58 32.8 0.0 63.6

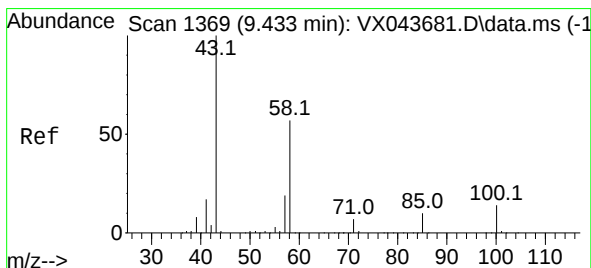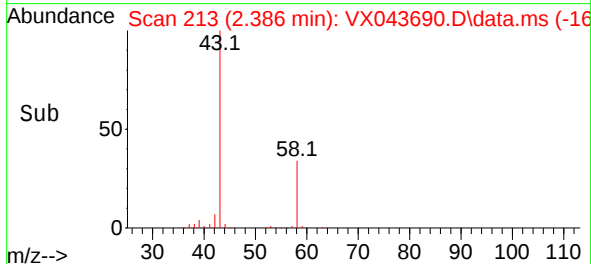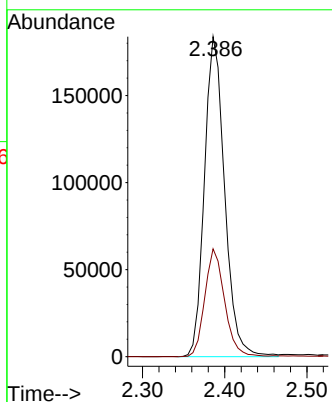

#48
2-Hexanone
Concen: 6.436 ug/L
RT: 9.384 min Scan# 1361
Delta R.T. -0.049 min
Lab File: VX043690.D
Acq: 04 Nov 2024 18:14

Tgt Ion: 43 Resp: 16041
Ion Ratio Lower Upper
43 100
58 34.1 44.6 67.0#
57 25.2 15.7 23.5#
100 0.0 11.0 16.4#

