

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043689.D
 Acq On : 04 Nov 2024 17:51
 Operator : JC/MD
 Sample : P4621-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N2

Quant Time: Nov 05 03:47:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 05 03:44:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	126608	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	113958	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	49367	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	88573	131.319	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	= 262.640%#	
7) Chloroethane-d5	1.642	69	45159	155.763	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	= 311.520%#	
11) 1,1-Dichloroethene-d2	2.294	65	41012	131.716	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 263.440%#	
21) 2-Butanone-d5	4.465	46	202149	457.742	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	= 457.740%#	
24) Chloroform-d	5.056	84	240487	165.393	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 330.780%#	
26) 1,2-Dichloroethane-d4	5.952	65	165371	179.031	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 358.060%#	
32) Benzene-d6	5.964	84	478771	162.500	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 325.000%#	
36) 1,2-Dichloropropane-d6	7.306	67	161232	179.873	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	= 359.740%#	
41) Toluene-d8	8.647	98	413585	154.529	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 309.060%#	
43) trans-1,3-Dichloroprop...	8.952	79	71737	167.347	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 334.700%#	
47) 2-Hexanone-d5	9.384	63	154439	435.359	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	= 435.360%#	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	228035	198.276	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	= 396.560%#	
66) 1,2-Dichlorobenzene-d4	12.317	152	168824	197.376	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 394.760%#	
Target Compounds						Qvalue
13) Acetone	2.386	43	15647	38.095	ug/L	100
16) Methylene chloride	2.788	84	1873	2.295	ug/L #	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043689.D
Acq On : 04 Nov 2024 17:51
Operator : JC/MD
Sample : P4621-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N2

Quant Time: Nov 05 03:47:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 05 03:44:12 2024
Response via : Initial Calibration

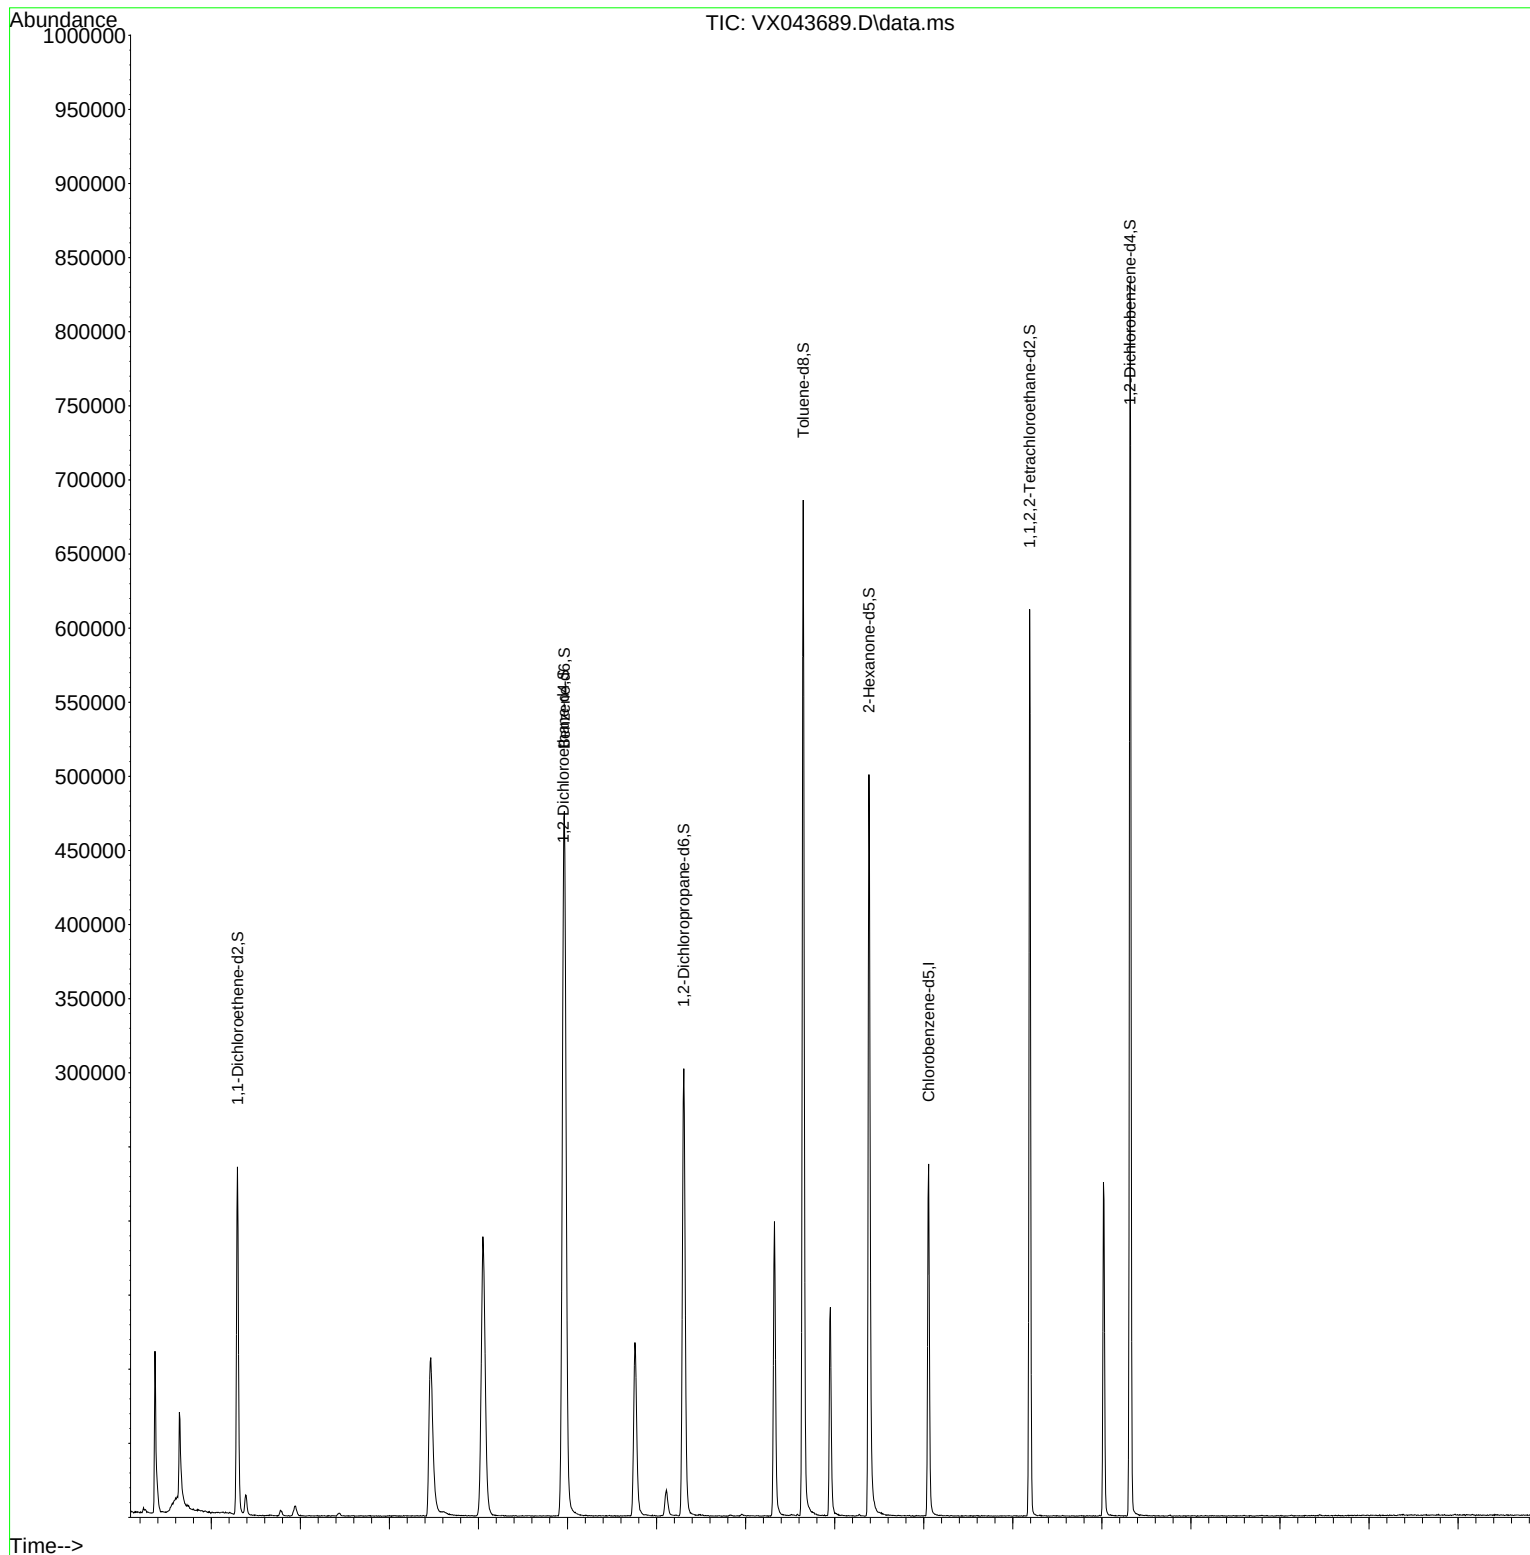

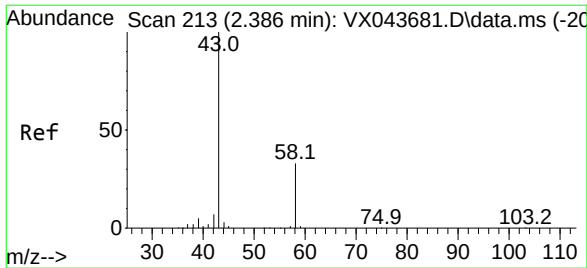

#13

Acetone

Concen: 38.095 ug/L

RT: 2.386 min Scan# 213

Delta R.T. -0.000 min

Lab File: VX043689.D

Acq: 04 Nov 2024 17:51

Instrument :

MSVOA_X

ClientSampleId :





BH6N2

Tgt Ion: 43 Resp: 15647

Ion Ratio Lower Upper

43 100

58 31.7 0.0 63.6

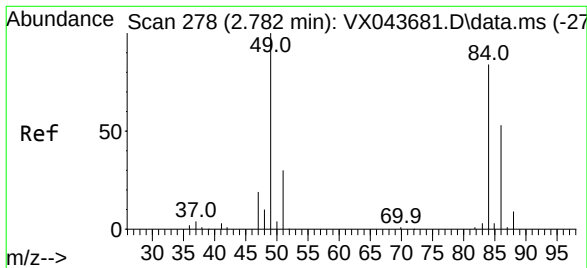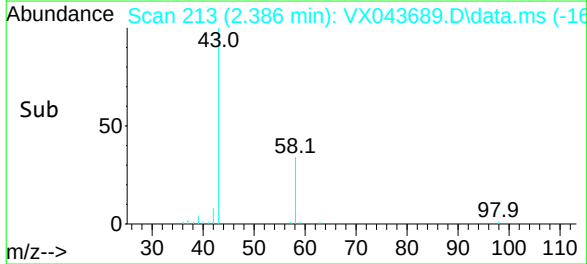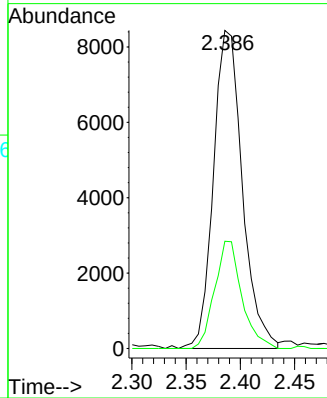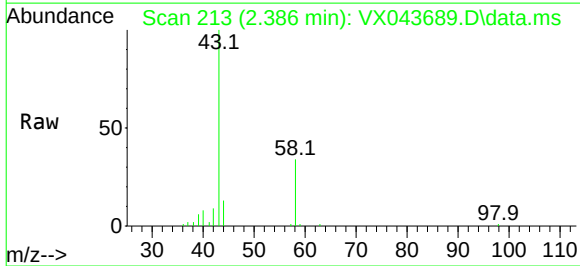

#16

Methylene chloride

Concen: 2.295 ug/L

RT: 2.788 min Scan# 279

Delta R.T. 0.006 min

Lab File: VX043689.D

Acq: 04 Nov 2024 17:51

Tgt Ion: 84 Resp: 1873

Ion Ratio Lower Upper

84 100

86 40.5 44.7 83.1#

49 59.9 83.2 154.4#

