

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043682.D
 Acq On : 04 Nov 2024 15:09
 Operator : JC/MD
 Sample : VX1104WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK716

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043682.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rBV	103788	131811	13.14%	1.673%
2	1.642	88	91	104	rVB	51970	89857	8.96%	1.141%
3	2.294	192	198	211	rVB	209768	330662	32.97%	4.197%
4	2.495	228	231	237	rVB5	1523	2234	0.22%	0.028%
5	2.593	245	247	249	rBV	520	444	0.04%	0.006%
6	2.691	261	263	264	rBV2	450	317	0.03%	0.004%
7	2.776	273	277	281	rBV6	1462	2774	0.28%	0.035%
8	2.861	290	291	293	rBV2	427	346	0.03%	0.004%
9	2.941	298	304	311	rVB	3984	8770	0.87%	0.111%
10	3.026	317	318	322	rVB	512	379	0.04%	0.005%
11	3.087	324	328	332	rVV3	931	1195	0.12%	0.015%
12	3.355	371	372	376	rBV2	427	384	0.04%	0.005%
13	3.434	378	385	392	rVV4	3269	7988	0.80%	0.101%
14	3.550	402	404	407	rVB	613	661	0.07%	0.008%
15	3.581	407	409	410	rBV2	416	392	0.04%	0.005%
16	3.666	419	423	424	rBV	307	383	0.04%	0.005%
17	3.751	435	437	438	rVB2	528	297	0.03%	0.004%
18	3.794	443	444	446	rVB	469	305	0.03%	0.004%
19	3.989	472	476	478	rBV3	417	568	0.06%	0.007%
20	4.154	502	503	506	rBV2	409	428	0.04%	0.005%
21	4.379	539	540	542	rVB	556	322	0.03%	0.004%
22	4.404	542	544	546	rBV	258	286	0.03%	0.004%
23	4.465	546	554	571	rBV	59895	190113	18.95%	2.413%
24	4.897	622	625	630	rBV3	533	626	0.06%	0.008%
25	5.050	636	650	669	rBV	125591	399732	39.85%	5.074%
26	5.312	691	693	696	rVB2	424	458	0.05%	0.006%
27	5.343	696	698	700	rBV2	278	351	0.03%	0.004%
28	5.538	725	730	731	rBV2	833	1156	0.12%	0.015%
29	5.635	744	746	750	rVB2	321	333	0.03%	0.004%
30	5.684	750	754	755	rBV2	267	320	0.03%	0.004%
31	5.751	764	765	769	rBV2	369	507	0.05%	0.006%
32	5.836	776	779	781	rBV3	388	410	0.04%	0.005%
33	5.855	781	782	786	rBV	468	524	0.05%	0.007%
34	5.964	789	800	820	rVV2	338540	1003032	100.00%	12.731%
35	6.355	862	864	865	rBV2	609	643	0.06%	0.008%
36	6.403	871	872	875	rVB3	544	411	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043682.D
 Acq On : 04 Nov 2024 15:09
 Operator : JC/MD
 Sample : VX1104WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK716

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	6.544	892	895	896	rBV2	421	362	0.04%	0.005%
38	6.574	896	900	902	rBV	229	408	0.04%	0.005%
39	6.653	911	913	915	rBV2	406	466	0.05%	0.006%
40	6.757	921	930	948	rBV	322215	781210	77.88%	9.916%
41	7.184	998	1000	1002	rBV2	383	473	0.05%	0.006%
42	7.208	1002	1004	1005	rBV	376	289	0.03%	0.004%
43	7.306	1011	1020	1037	rBV	199157	449386	44.80%	5.704%
44	7.446	1041	1043	1046	rBV2	648	506	0.05%	0.006%
45	7.659	1075	1078	1080	rBV3	404	476	0.05%	0.006%
46	7.775	1096	1097	1099	rBV	654	333	0.03%	0.004%
47	8.007	1133	1135	1137	rBV	417	324	0.03%	0.004%
48	8.116	1151	1153	1155	rBV	458	398	0.04%	0.005%
49	8.324	1181	1187	1199	rBV	134630	225905	22.52%	2.867%
50	8.488	1213	1214	1216	rBV	651	438	0.04%	0.006%
51	8.555	1223	1225	1226	rBV2	567	446	0.04%	0.006%
52	8.647	1234	1240	1252	rBV	495038	804774	80.23%	10.215%
53	8.952	1283	1290	1302	rBV	94259	147366	14.69%	1.870%
54	9.208	1331	1332	1336	rVB	482	502	0.05%	0.006%
55	9.275	1340	1343	1347	rVB3	1417	2001	0.20%	0.025%
56	9.336	1352	1353	1356	rBV2	376	437	0.04%	0.006%
57	9.384	1356	1361	1382	rBV	291907	468123	46.67%	5.942%
58	9.701	1409	1413	1418	rVB3	1189	2303	0.23%	0.029%
59	9.756	1418	1422	1425	rVB3	550	870	0.09%	0.011%
60	9.884	1441	1443	1447	rBV3	384	571	0.06%	0.007%
61	10.049	1465	1470	1486	rBV	600967	886757	88.41%	11.255%
62	10.646	1562	1568	1569	rBV2	832	1039	0.10%	0.013%
63	10.787	1589	1591	1594	rVV2	486	636	0.06%	0.008%
64	10.817	1594	1596	1599	rVV3	497	512	0.05%	0.006%
65	10.860	1601	1603	1604	rVV	419	327	0.03%	0.004%
66	10.903	1607	1610	1613	rVV3	288	391	0.04%	0.005%
67	10.957	1616	1619	1624	rVV4	908	1470	0.15%	0.019%
68	11.098	1641	1642	1644	rVB2	432	289	0.03%	0.004%
69	11.140	1648	1649	1652	rBV	417	451	0.04%	0.006%
70	11.189	1652	1657	1668	rBV	354721	460509	45.91%	5.845%
71	11.451	1695	1700	1704	rBV3	1464	2201	0.22%	0.028%
72	11.518	1710	1711	1714	rBV2	386	374	0.04%	0.005%
73	11.549	1714	1716	1718	rVB3	503	365	0.04%	0.005%
74	11.677	1735	1737	1738	rBV2	437	350	0.03%	0.004%
75	11.719	1738	1744	1746	rVB2	393	634	0.06%	0.008%
76	11.756	1746	1750	1753	rBV5	1259	2034	0.20%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043682.D
 Acq On : 04 Nov 2024 15:09
 Operator : JC/MD
 Sample : VX1104WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK716

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	11.841	1762	1764	1767	rVB	465	418	0.04%	0.005%
78	11.896	1771	1773	1776	rBV2	328	410	0.04%	0.005%
79	11.969	1782	1785	1788	rBV2	2126	2528	0.25%	0.032%
80	12.018	1788	1793	1804	rVV	608037	780214	77.79%	9.903%
81	12.317	1837	1842	1851	rBV	516442	653840	65.19%	8.299%
82	12.756	1912	1914	1915	rBV2	534	493	0.05%	0.006%
83	13.000	1950	1954	1957	rVB2	476	767	0.08%	0.010%
84	13.024	1957	1958	1960	rBV	577	397	0.04%	0.005%
85	13.122	1970	1974	1976	rBV2	1404	1477	0.15%	0.019%
86	13.341	2007	2010	2011	rBV3	336	379	0.04%	0.005%
87	13.518	2037	2039	2040	rVB2	460	325	0.03%	0.004%
88	13.573	2046	2048	2049	rBV	407	363	0.04%	0.005%
89	13.597	2049	2052	2056	rVV2	1329	1820	0.18%	0.023%
90	13.786	2080	2083	2087	rVB2	1121	1635	0.16%	0.021%
91	13.963	2109	2112	2116	rBV3	1364	1888	0.19%	0.024%
92	14.085	2131	2132	2134	rBV	398	278	0.03%	0.004%
93	14.128	2136	2139	2143	rVB3	1112	1394	0.14%	0.018%
94	14.225	2153	2155	2159	rBV3	442	516	0.05%	0.007%
95	14.749	2240	2241	2245	rVB2	585	517	0.05%	0.007%
96	14.829	2250	2254	2255	rBV2	810	736	0.07%	0.009%
97	14.926	2268	2270	2272	rVB2	685	606	0.06%	0.008%
98	15.072	2293	2294	2296	rBV	592	503	0.05%	0.006%
99	16.219	2481	2482	2483	rBV	544	294	0.03%	0.004%
100	16.511	2528	2530	2532	rVB2	841	552	0.06%	0.007%

Sum of corrected areas: 7878475




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043682.D
Acq On : 04 Nov 2024 15:09
Operator : JC/MD
Sample : VX1104WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK716

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

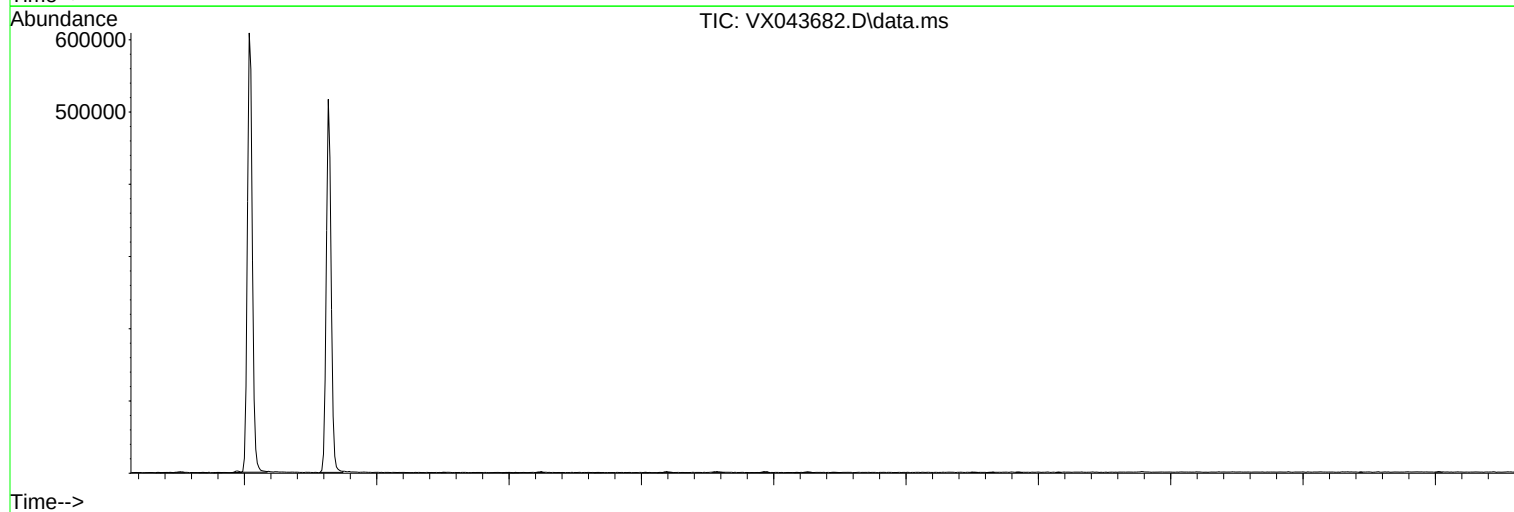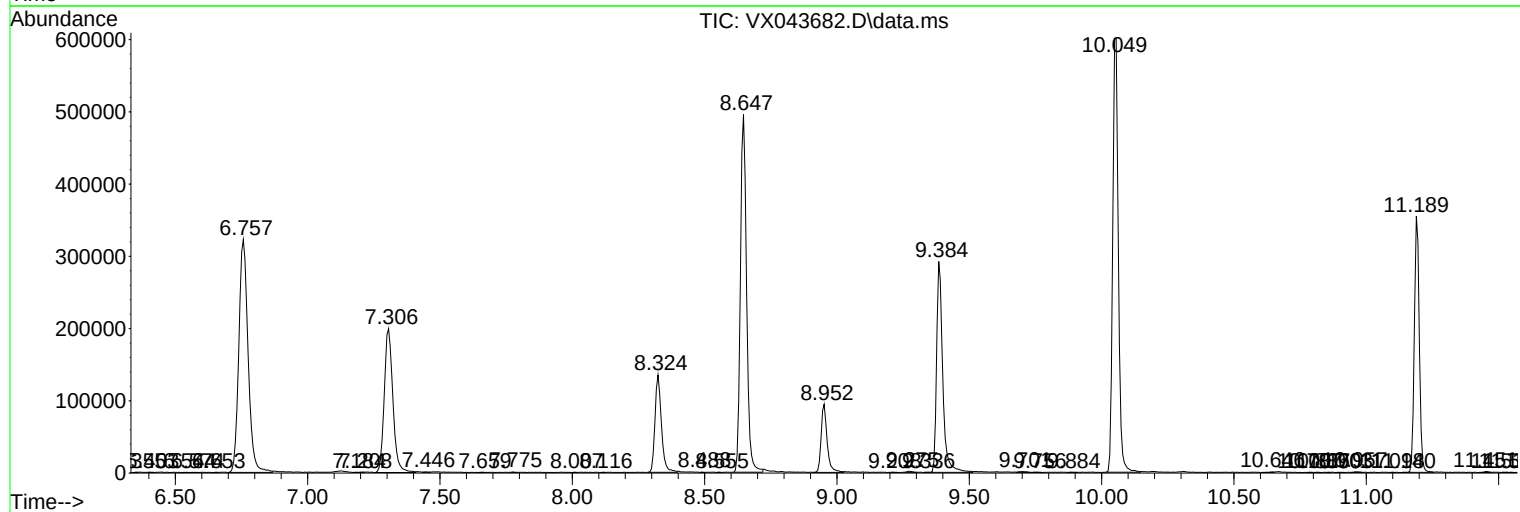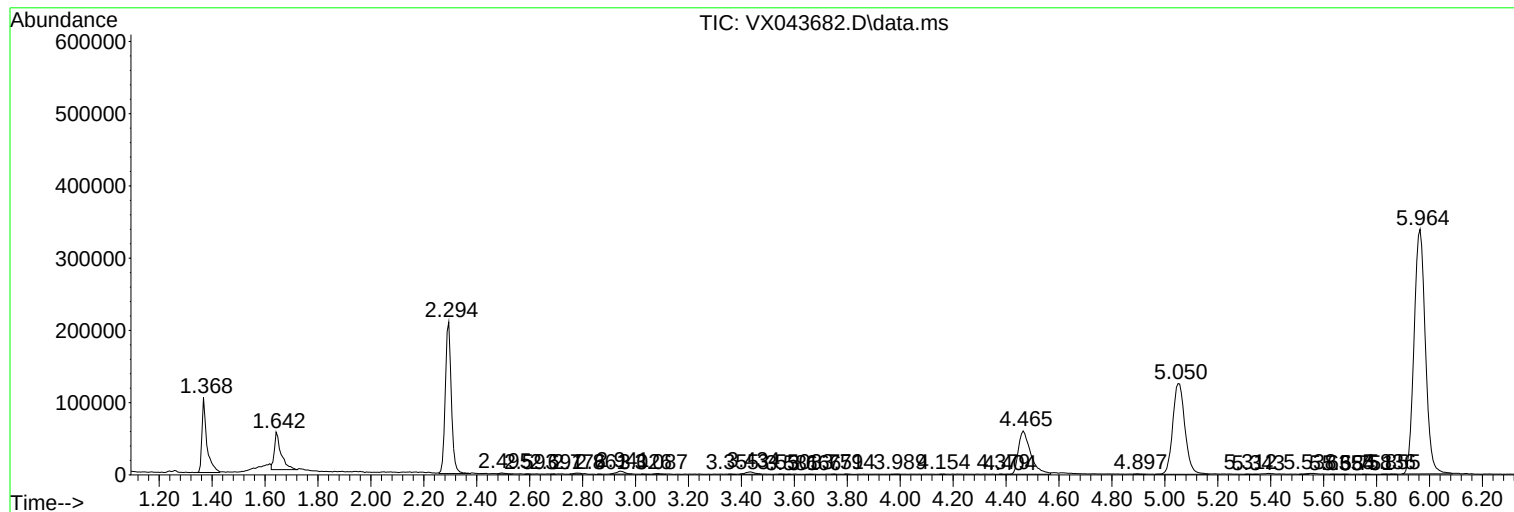

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043682.D
Acq On : 04 Nov 2024 15:09
Operator : JC/MD
Sample : VX1104WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK716

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043682.D
Acq On : 04 Nov 2024 15:09
Operator : JC/MD
Sample : VX1104WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK716

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
