

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043683.D
 Acq On : 04 Nov 2024 15:32
 Operator : JC/MD
 Sample : PB164621TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VLEB621

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043683.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	58	rVB	85424	106083	10.15%	1.269%
2	1.642	88	91	104	rVB	50989	81778	7.83%	0.978%
3	2.294	192	198	208	rVB	174384	276556	26.47%	3.308%
4	2.654	255	257	260	rVV3	418	373	0.04%	0.004%
5	2.782	273	278	283	rBV3	2882	5130	0.49%	0.061%
6	2.898	296	297	299	rBV2	384	377	0.04%	0.005%
7	2.940	299	304	313	rVB4	1884	5319	0.51%	0.064%
8	3.075	322	326	330	rBV5	746	1182	0.11%	0.014%
9	3.428	378	384	394	rVB4	3247	8004	0.77%	0.096%
10	3.544	399	403	405	rBV2	354	427	0.04%	0.005%
11	3.770	438	440	442	rVB2	352	320	0.03%	0.004%
12	3.806	442	446	449	rBV3	429	570	0.05%	0.007%
13	3.922	463	465	470	rBV3	505	746	0.07%	0.009%
14	3.977	472	474	476	rBV	417	431	0.04%	0.005%
15	4.080	487	491	492	rBV2	326	308	0.03%	0.004%
16	4.099	492	494	498	rVV2	291	413	0.04%	0.005%
17	4.184	504	508	510	rBV3	528	558	0.05%	0.007%
18	4.294	524	526	530	rVB2	411	417	0.04%	0.005%
19	4.397	542	543	546	rBV2	385	319	0.03%	0.004%
20	4.465	546	554	571	rBV	74201	233773	22.37%	2.796%
21	5.050	638	650	667	rBV	135747	428411	41.00%	5.124%
22	5.208	674	676	680	rVB2	470	398	0.04%	0.005%
23	5.355	698	700	701	rBV	351	322	0.03%	0.004%
24	5.391	701	706	710	rVV4	827	1919	0.18%	0.023%
25	5.550	724	732	733	rBV2	1263	2374	0.23%	0.028%
26	5.964	788	800	815	rBV2	349315	1044912	100.00%	12.498%
27	6.220	841	842	846	rBV3	300	331	0.03%	0.004%
28	6.354	862	864	867	rVV3	493	507	0.05%	0.006%
29	6.397	867	871	875	rVB4	606	1105	0.11%	0.013%
30	6.434	875	877	879	rBV	354	414	0.04%	0.005%
31	6.690	916	919	920	rBV	469	497	0.05%	0.006%
32	6.757	921	930	948	rBV	336587	816387	78.13%	9.765%
33	6.940	958	960	962	rVB2	626	381	0.04%	0.005%
34	7.123	983	990	998	rBV7	2331	6077	0.58%	0.073%
35	7.220	1002	1006	1007	rBV2	350	335	0.03%	0.004%
36	7.305	1011	1020	1036	rBV	216951	487804	46.68%	5.835%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043683.D
 Acq On : 04 Nov 2024 15:32
 Operator : JC/MD
 Sample : PB164621TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VLEB621

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.921	1119	1121	1124	rBV3	289	321	0.03%	0.004%
38	7.952	1124	1126	1127	rBV	626	452	0.04%	0.005%
39	8.061	1141	1144	1146	rBV3	354	450	0.04%	0.005%
40	8.196	1164	1166	1169	rVB3	650	633	0.06%	0.008%
41	8.324	1180	1187	1201	rBV	138257	241311	23.09%	2.886%
42	8.647	1234	1240	1256	rBV	498906	803502	76.90%	9.611%
43	8.952	1284	1290	1303	rBV	103696	158329	15.15%	1.894%
44	9.080	1310	1311	1317	rBV3	340	470	0.04%	0.006%
45	9.220	1332	1334	1336	rBV2	359	321	0.03%	0.004%
46	9.275	1339	1343	1349	rVB3	1249	1970	0.19%	0.024%
47	9.384	1356	1361	1378	rBV	350445	548266	52.47%	6.558%
48	9.701	1410	1413	1418	rVB3	1214	1291	0.12%	0.015%
49	9.775	1423	1425	1429	rVB3	382	449	0.04%	0.005%
50	9.860	1437	1439	1442	rBV	281	308	0.03%	0.004%
51	10.055	1465	1471	1488	rVV	665358	937536	89.72%	11.214%
52	10.311	1510	1513	1517	rVV4	816	1114	0.11%	0.013%
53	10.598	1557	1560	1562	rBV	647	508	0.05%	0.006%
54	10.640	1562	1567	1568	rBV2	618	827	0.08%	0.010%
55	10.780	1588	1590	1593	rVB2	463	462	0.04%	0.006%
56	10.896	1605	1609	1612	rBV2	333	536	0.05%	0.006%
57	11.018	1627	1629	1633	rBV2	242	356	0.03%	0.004%
58	11.189	1652	1657	1670	rBV	424986	555810	53.19%	6.648%
59	11.347	1680	1683	1686	rVB2	318	434	0.04%	0.005%
60	11.543	1712	1715	1718	rVB2	375	339	0.03%	0.004%
61	11.713	1740	1743	1745	rVV	629	602	0.06%	0.007%
62	11.756	1745	1750	1754	rVV3	1083	1803	0.17%	0.022%
63	11.786	1754	1755	1758	rVB2	343	361	0.03%	0.004%
64	11.823	1758	1761	1762	rBV	327	328	0.03%	0.004%
65	11.975	1783	1786	1788	rBV2	1520	1542	0.15%	0.018%
66	12.018	1788	1793	1805	rBV	629935	827554	79.20%	9.899%
67	12.231	1824	1828	1834	rBV7	1113	1991	0.19%	0.024%
68	12.317	1837	1842	1857	rVV	575624	728678	69.74%	8.716%
69	12.615	1887	1891	1894	rVB2	362	412	0.04%	0.005%
70	12.762	1911	1915	1919	rVB3	1438	1999	0.19%	0.024%
71	13.073	1964	1966	1969	rVB2	302	309	0.03%	0.004%
72	13.115	1969	1973	1976	rBV4	799	1165	0.11%	0.014%
73	13.317	2003	2006	2007	rBV2	310	340	0.03%	0.004%
74	13.353	2010	2012	2015	rVB3	358	316	0.03%	0.004%
75	13.408	2019	2021	2024	rVB2	466	506	0.05%	0.006%
76	13.445	2024	2027	2028	rBV2	529	506	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043683.D
 Acq On : 04 Nov 2024 15:32
 Operator : JC/MD
 Sample : PB164621TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VLEB621

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	13.597	2049	2052	2054	rVB2	995	1064	0.10%	0.013%
78	13.695	2066	2068	2071	rVB	432	318	0.03%	0.004%
79	13.780	2080	2082	2086	rBV2	896	1194	0.11%	0.014%
80	13.835	2089	2091	2092	rBV	469	318	0.03%	0.004%
81	13.890	2099	2100	2102	rBV	479	372	0.04%	0.004%
82	13.908	2102	2103	2106	rVV	667	460	0.04%	0.006%
83	13.963	2109	2112	2120	rVB4	1074	2097	0.20%	0.025%
84	14.036	2120	2124	2125	rBV	555	537	0.05%	0.006%
85	14.085	2130	2132	2135	rVB	456	463	0.04%	0.006%
86	14.134	2135	2140	2145	rBV	2664	4430	0.42%	0.053%
87	14.225	2154	2155	2159	rBV	388	370	0.04%	0.004%
88	14.316	2167	2170	2171	rBV	386	346	0.03%	0.004%
89	14.329	2171	2172	2174	rBV2	499	328	0.03%	0.004%
90	14.444	2186	2191	2193	rVB2	420	749	0.07%	0.009%
91	14.652	2224	2225	2227	rBV	758	317	0.03%	0.004%
92	14.859	2257	2259	2261	rBV3	404	317	0.03%	0.004%
93	15.024	2285	2286	2290	rBV2	522	719	0.07%	0.009%
94	15.194	2312	2314	2316	rVB2	546	374	0.04%	0.004%
95	15.395	2342	2347	2353	rVB5	1742	2987	0.29%	0.036%
96	15.584	2374	2378	2381	rBV5	500	660	0.06%	0.008%
97	15.950	2437	2438	2442	rVB3	1016	950	0.09%	0.011%
98	16.084	2459	2460	2462	rBV	651	449	0.04%	0.005%
99	16.444	2517	2519	2521	rBV3	576	518	0.05%	0.006%
100	16.590	2541	2543	2545	rBV2	440	360	0.03%	0.004%

Sum of corrected areas: 8360362




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043683.D
Acq On : 04 Nov 2024 15:32
Operator : JC/MD
Sample : PB164621TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VLEB621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

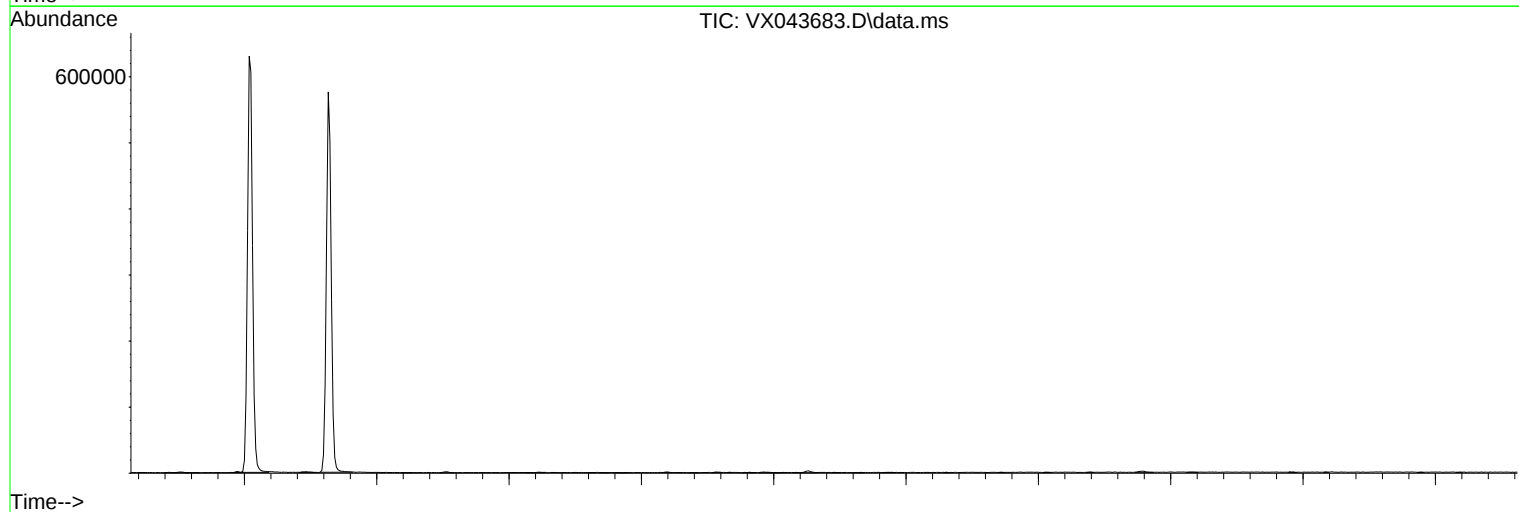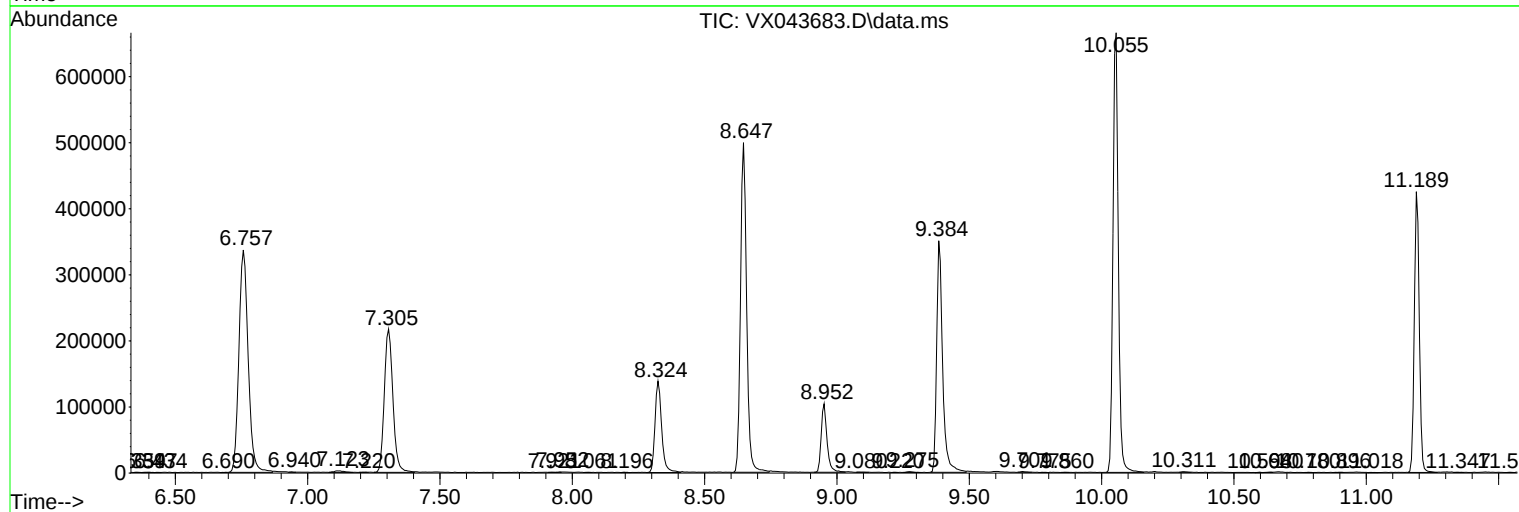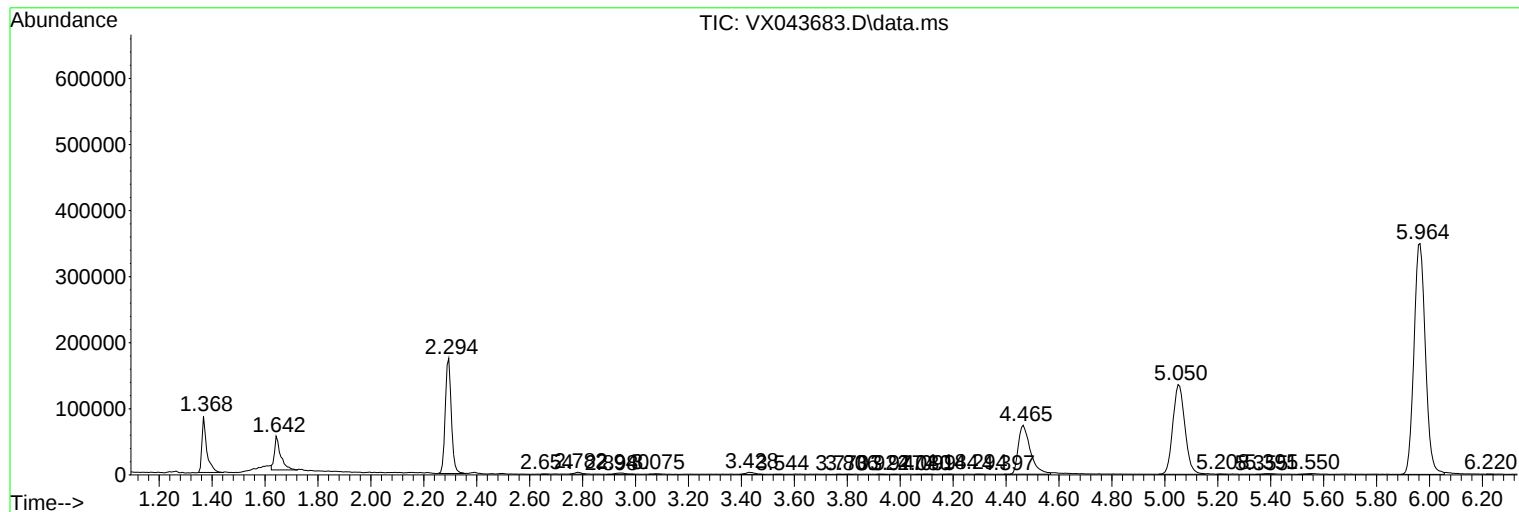

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043683.D
Acq On : 04 Nov 2024 15:32
Operator : JC/MD
Sample : PB164621TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VLEB621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043683.D
Acq On : 04 Nov 2024 15:32
Operator : JC/MD
Sample : PB164621TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VLEB621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc