

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043684.D
 Acq On : 04 Nov 2024 15:55
 Operator : JC/MD
 Sample : P4621-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043684.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	58	rBV	92947	116887	10.68%	1.375%
2	1.642	88	91	104	rVB	54818	84490	7.72%	0.994%
3	2.294	191	198	211	rBV	185933	298658	27.28%	3.512%
4	2.666	257	259	261	rVB	408	286	0.03%	0.003%
5	2.782	272	278	286	rBV3	5070	10843	0.99%	0.128%
6	2.941	298	304	319	rVB2	5701	13936	1.27%	0.164%
7	3.044	319	321	324	rVB2	328	296	0.03%	0.003%
8	3.087	324	328	330	rBV3	566	719	0.07%	0.008%
9	3.191	343	345	348	rVB2	426	302	0.03%	0.004%
10	3.215	348	349	353	rVB2	308	298	0.03%	0.004%
11	3.313	363	365	368	rBV2	425	549	0.05%	0.006%
12	3.392	375	378	379	rBV2	311	378	0.03%	0.004%
13	3.434	379	385	392	rVB4	2605	5861	0.54%	0.069%
14	3.599	409	412	415	rBV3	394	642	0.06%	0.008%
15	3.782	441	442	445	rBV	314	268	0.02%	0.003%
16	3.849	451	453	455	rBV	435	275	0.03%	0.003%
17	4.123	497	498	502	rBV	331	435	0.04%	0.005%
18	4.203	509	511	513	rBV2	465	345	0.03%	0.004%
19	4.276	521	523	526	rBV3	349	428	0.04%	0.005%
20	4.465	544	554	568	rBV	75638	243881	22.28%	2.868%
21	4.867	617	620	621	rVB2	536	463	0.04%	0.005%
22	5.050	638	650	666	rBV	141912	448824	41.00%	5.278%
23	5.385	703	705	710	rBV2	621	840	0.08%	0.010%
24	5.526	725	728	729	rBV2	696	658	0.06%	0.008%
25	5.611	741	742	744	rBV	346	336	0.03%	0.004%
26	5.654	746	749	752	rVV	309	398	0.04%	0.005%
27	5.830	775	778	780	rBV	363	432	0.04%	0.005%
28	5.891	786	788	789	rBV2	318	299	0.03%	0.004%
29	5.958	789	799	819	rBV2	365743	1094748	100.00%	12.875%
30	6.245	844	846	848	rVB	396	345	0.03%	0.004%
31	6.282	851	852	853	rBV	458	266	0.02%	0.003%
32	6.355	862	864	866	rBV2	463	363	0.03%	0.004%
33	6.458	877	881	882	rBV2	438	526	0.05%	0.006%
34	6.678	916	917	919	rBV2	523	378	0.03%	0.004%
35	6.757	921	930	946	rBV	311418	761382	69.55%	8.954%
36	7.117	983	989	998	rVB5	2660	7581	0.69%	0.089%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043684.D
 Acq On : 04 Nov 2024 15:55
 Operator : JC/MD
 Sample : P4621-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.306	1012	1020	1033	rBV	231861	514045	46.96%	6.046%
38	7.513	1052	1054	1055	rBV	499	364	0.03%	0.004%
39	7.921	1118	1121	1122	rBV2	420	452	0.04%	0.005%
40	7.958	1125	1127	1130	rVV3	708	822	0.08%	0.010%

41	7.982	1130	1131	1135	rVB2	812	619	0.06%	0.007%
42	8.324	1181	1187	1201	rBV	148777	253968	23.20%	2.987%
43	8.647	1233	1240	1259	rBV	518594	848924	77.55%	9.984%
44	8.824	1267	1269	1272	rVB3	732	589	0.05%	0.007%
45	8.952	1284	1290	1298	rBV	103243	162398	14.83%	1.910%

46	9.281	1340	1344	1347	rBV4	879	1267	0.12%	0.015%
47	9.348	1354	1355	1356	rBV	366	259	0.02%	0.003%
48	9.385	1356	1361	1385	rVV	369699	580356	53.01%	6.825%
49	9.689	1409	1411	1414	rBV2	432	475	0.04%	0.006%
50	9.726	1415	1417	1420	rVB	429	363	0.03%	0.004%

51	9.781	1424	1426	1429	rVB2	369	420	0.04%	0.005%
52	10.049	1465	1470	1485	rBV	602257	878703	80.27%	10.334%
53	10.409	1526	1529	1533	rBV4	431	715	0.07%	0.008%
54	10.537	1548	1550	1552	rBV	421	359	0.03%	0.004%
55	10.604	1557	1561	1563	rVB2	464	526	0.05%	0.006%

56	10.787	1590	1591	1594	rBV	485	451	0.04%	0.005%
57	11.049	1632	1634	1635	rVB	447	302	0.03%	0.004%
58	11.098	1641	1642	1644	rBV	505	272	0.02%	0.003%
59	11.189	1652	1657	1670	rVB	456225	584687	53.41%	6.876%
60	11.317	1674	1678	1681	rVB4	859	1337	0.12%	0.016%

61	11.445	1696	1699	1700	rBV2	339	330	0.03%	0.004%
62	11.713	1737	1743	1745	rBV4	541	1216	0.11%	0.014%
63	11.756	1748	1750	1753	rVB2	605	510	0.05%	0.006%
64	11.866	1764	1768	1771	rBV2	287	438	0.04%	0.005%
65	11.976	1782	1786	1788	rBV3	1168	1325	0.12%	0.016%

66	12.018	1788	1793	1805	rBV	601766	779887	71.24%	9.172%
67	12.171	1816	1818	1823	rBV2	447	700	0.06%	0.008%
68	12.317	1837	1842	1853	rBV	604628	769722	70.31%	9.052%
69	12.585	1884	1886	1889	rVV2	325	260	0.02%	0.003%
70	12.646	1893	1896	1898	rBV3	473	509	0.05%	0.006%

71	12.762	1912	1915	1919	rVB2	1633	2018	0.18%	0.024%
72	12.829	1923	1926	1927	rBV	366	267	0.02%	0.003%
73	12.884	1934	1935	1937	rBV	356	261	0.02%	0.003%
74	12.927	1941	1942	1945	rVB2	452	399	0.04%	0.005%
75	12.957	1945	1947	1951	rBV2	451	520	0.05%	0.006%

76	13.116	1971	1973	1976	rVV3	743	882	0.08%	0.010%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043684.D
 Acq On : 04 Nov 2024 15:55
 Operator : JC/MD
 Sample : P4621-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	13.171	1980	1982	1985	rVV3	533	425	0.04%	0.005%
78	13.201	1985	1987	1990	rVB2	355	401	0.04%	0.005%
79	13.274	1997	1999	2002	rBV2	511	524	0.05%	0.006%
80	13.323	2005	2007	2010	rVV	329	376	0.03%	0.004%
81	13.372	2013	2015	2017	rBV	398	477	0.04%	0.006%
82	13.420	2021	2023	2026	rVB	476	444	0.04%	0.005%
83	13.457	2026	2029	2032	rBV2	339	509	0.05%	0.006%
84	13.500	2034	2036	2037	rVB	463	284	0.03%	0.003%
85	13.518	2037	2039	2040	rBV	606	390	0.04%	0.005%
86	13.719	2070	2072	2074	rBV2	285	262	0.02%	0.003%
87	13.774	2079	2081	2082	rBV2	696	550	0.05%	0.006%
88	13.969	2110	2113	2115	rBV2	977	805	0.07%	0.009%
89	14.012	2117	2120	2121	rBV2	502	564	0.05%	0.007%
90	14.085	2130	2132	2134	rBV2	455	373	0.03%	0.004%
91	14.128	2135	2139	2147	rVV	2189	2679	0.24%	0.032%
92	14.201	2149	2151	2152	rBV	485	429	0.04%	0.005%
93	14.408	2182	2185	2187	rBV2	557	586	0.05%	0.007%
94	14.451	2189	2192	2194	rBV3	675	826	0.08%	0.010%
95	14.701	2231	2233	2236	rBV2	644	476	0.04%	0.006%
96	14.743	2238	2240	2241	rBV2	465	258	0.02%	0.003%
97	14.823	2251	2253	2254	rBV2	611	283	0.03%	0.003%
98	16.377	2505	2508	2509	rVB	780	609	0.06%	0.007%
99	16.402	2510	2512	2515	rVB2	648	393	0.04%	0.005%
100	16.560	2537	2538	2541	rBV2	578	431	0.04%	0.005%

Sum of corrected areas: 8502887




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043684.D
Acq On : 04 Nov 2024 15:55
Operator : JC/MD
Sample : P4621-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

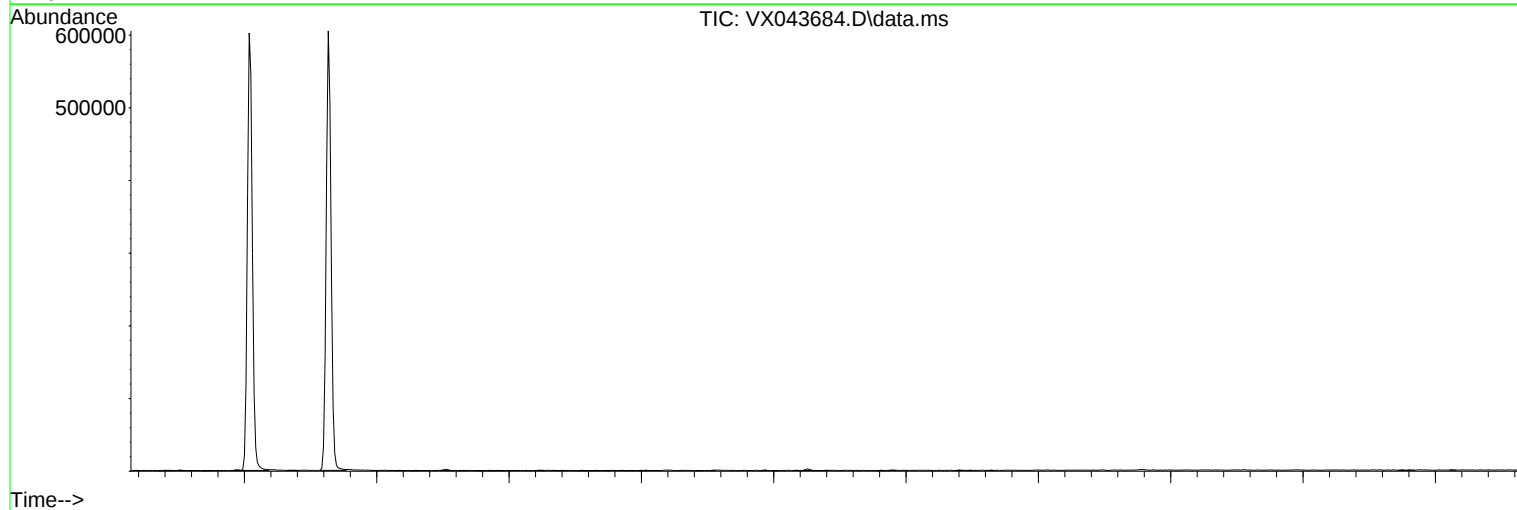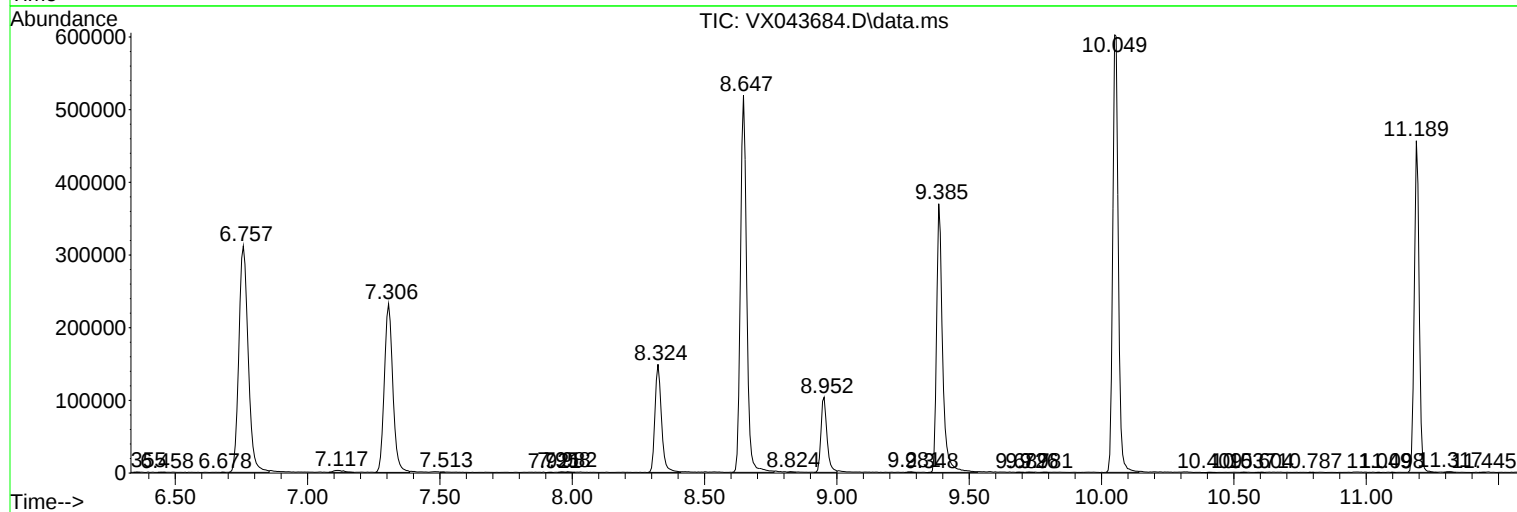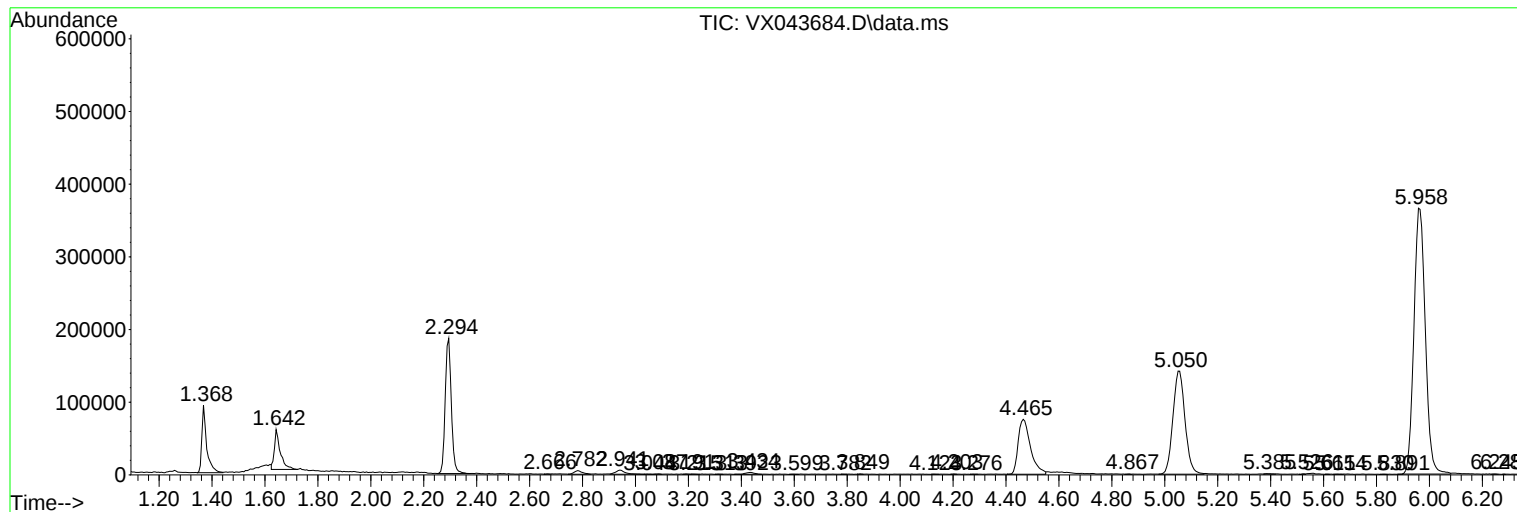

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043684.D
Acq On : 04 Nov 2024 15:55
Operator : JC/MD
Sample : P4621-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043684.D
Acq On : 04 Nov 2024 15:55
Operator : JC/MD
Sample : P4621-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
