

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043685.D
 Acq On : 04 Nov 2024 16:18
 Operator : JC/MD
 Sample : P4621-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043685.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rBV	82290	101687	10.22%	1.299%
2	1.642	88	91	102	rVB	52515	76229	7.66%	0.973%
3	2.294	192	198	209	rVB	166997	257912	25.93%	3.294%
4	2.782	273	278	287	rVB4	4951	8523	0.86%	0.109%
5	2.941	296	304	313	rBV2	5732	14491	1.46%	0.185%
6	3.130	334	335	336	rBV	489	342	0.03%	0.004%
7	3.166	339	341	343	rVV2	577	473	0.05%	0.006%
8	3.251	353	355	357	rBV	494	402	0.04%	0.005%
9	3.270	357	358	363	rVB3	452	393	0.04%	0.005%
10	3.434	379	385	391	rBV4	2155	4853	0.49%	0.062%
11	3.562	403	406	410	rVB3	268	340	0.03%	0.004%
12	3.751	434	437	439	rBV2	353	320	0.03%	0.004%
13	3.831	448	450	452	rBV2	365	416	0.04%	0.005%
14	3.922	462	465	468	rVB3	398	536	0.05%	0.007%
15	3.965	468	472	475	rBV2	426	727	0.07%	0.009%
16	4.398	542	543	545	rBV2	323	332	0.03%	0.004%
17	4.465	545	554	571	rVV	77801	244364	24.56%	3.121%
18	4.721	594	596	600	rBV3	486	407	0.04%	0.005%
19	5.056	637	651	667	rBV	133309	408600	41.07%	5.218%
20	5.202	673	675	678	rBV3	522	460	0.05%	0.006%
21	5.367	699	702	705	rBV3	485	793	0.08%	0.010%
22	5.830	777	778	781	rBV	355	399	0.04%	0.005%
23	5.964	788	800	826	rBV3	333603	994811	100.00%	12.704%
24	6.312	856	857	861	rBV	483	612	0.06%	0.008%
25	6.367	863	866	868	rBV2	413	501	0.05%	0.006%
26	6.629	906	909	911	rVB2	388	398	0.04%	0.005%
27	6.684	916	918	920	rBV2	297	331	0.03%	0.004%
28	6.757	920	930	947	rBV	270406	664101	66.76%	8.481%
29	7.025	972	974	977	rVB3	446	440	0.04%	0.006%
30	7.098	984	986	987	rBV2	1590	1217	0.12%	0.016%
31	7.190	1000	1001	1002	rBV	589	324	0.03%	0.004%
32	7.306	1011	1020	1037	rBV	206872	471148	47.36%	6.017%
33	7.580	1064	1065	1069	rVB2	477	314	0.03%	0.004%
34	7.617	1069	1071	1076	rVB2	347	476	0.05%	0.006%
35	7.836	1101	1107	1110	rBV3	786	1379	0.14%	0.018%
36	7.946	1123	1125	1127	rBV3	516	439	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043685.D
 Acq On : 04 Nov 2024 16:18
 Operator : JC/MD
 Sample : P4621-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	8.104	1150	1151	1154	rBV2	452	510	0.05%	0.007%
38	8.220	1166	1170	1172	rBV2	387	581	0.06%	0.007%
39	8.244	1172	1174	1175	rBV	485	381	0.04%	0.005%
40	8.324	1180	1187	1203	rBV	134705	234108	23.53%	2.990%
41	8.513	1216	1218	1220	rBV	708	798	0.08%	0.010%
42	8.647	1234	1240	1256	rBV	471432	756732	76.07%	9.664%
43	8.952	1284	1290	1299	rBV	97782	150906	15.17%	1.927%
44	9.256	1336	1340	1341	rBV2	536	671	0.07%	0.009%
45	9.275	1341	1343	1347	rVB3	607	709	0.07%	0.009%
46	9.385	1356	1361	1382	rBV	364000	573950	57.69%	7.330%
47	9.720	1414	1416	1417	rBV2	433	307	0.03%	0.004%
48	9.970	1454	1457	1460	rBV2	354	400	0.04%	0.005%
49	10.055	1465	1471	1485	rBV	546957	792951	79.71%	10.127%
50	10.299	1510	1511	1513	rBV2	546	527	0.05%	0.007%
51	10.378	1522	1524	1525	rBV	421	305	0.03%	0.004%
52	10.543	1549	1551	1555	rBV2	489	433	0.04%	0.006%
53	10.646	1566	1568	1570	rVB2	518	440	0.04%	0.006%
54	10.683	1570	1574	1576	rBV2	478	763	0.08%	0.010%
55	10.756	1583	1586	1588	rBV	500	530	0.05%	0.007%
56	10.963	1617	1620	1623	rVV2	466	636	0.06%	0.008%
57	11.031	1628	1631	1634	rBV2	318	425	0.04%	0.005%
58	11.098	1641	1642	1645	rBV	431	366	0.04%	0.005%
59	11.140	1647	1649	1652	rVB	378	316	0.03%	0.004%
60	11.189	1652	1657	1668	rBV	438432	573943	57.69%	7.330%
61	11.354	1683	1684	1686	rBV	489	347	0.03%	0.004%
62	11.421	1693	1695	1698	rBV2	420	315	0.03%	0.004%
63	11.451	1698	1700	1704	rBV3	626	772	0.08%	0.010%
64	11.549	1715	1716	1718	rBV	551	359	0.04%	0.005%
65	11.622	1727	1728	1732	rBV2	233	307	0.03%	0.004%
66	11.707	1740	1742	1746	rVB3	471	541	0.05%	0.007%
67	11.756	1746	1750	1752	rBV2	521	710	0.07%	0.009%
68	11.860	1765	1767	1770	rVB2	352	308	0.03%	0.004%
69	11.957	1781	1783	1784	rBV2	467	343	0.03%	0.004%
70	11.976	1784	1786	1788	rVB3	751	640	0.06%	0.008%
71	12.018	1788	1793	1805	rBV	554879	710952	71.47%	9.079%
72	12.134	1811	1812	1813	rBV	669	352	0.04%	0.004%
73	12.244	1828	1830	1832	rBV2	689	599	0.06%	0.008%
74	12.317	1837	1842	1858	rBV	573675	734029	73.79%	9.374%
75	12.610	1887	1890	1892	rBV2	321	428	0.04%	0.005%
76	12.695	1902	1904	1907	rBV2	389	307	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043685.D
 Acq On : 04 Nov 2024 16:18
 Operator : JC/MD
 Sample : P4621-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.762	1910	1915	1918	rBV3	1707	2483	0.25%	0.032%
78	12.866	1928	1932	1934	rBV2	280	435	0.04%	0.006%
79	12.927	1940	1942	1944	rBV2	491	365	0.04%	0.005%
80	12.963	1944	1948	1950	rBV2	424	519	0.05%	0.007%
81	13.122	1970	1974	1976	rBV2	624	742	0.07%	0.009%
82	13.225	1990	1991	1994	rBV2	368	337	0.03%	0.004%
83	13.311	2003	2005	2009	rVB3	294	322	0.03%	0.004%
84	13.463	2029	2030	2033	rBV	533	433	0.04%	0.006%
85	13.597	2047	2052	2055	rVB4	585	813	0.08%	0.010%
86	13.737	2073	2075	2077	rBV	601	397	0.04%	0.005%
87	13.786	2079	2083	2090	rBV4	712	1413	0.14%	0.018%
88	13.939	2105	2108	2111	rBV3	428	688	0.07%	0.009%
89	14.042	2123	2125	2126	rBV	503	445	0.04%	0.006%
90	14.091	2130	2133	2135	rVV2	501	678	0.07%	0.009%
91	14.128	2137	2139	2142	rVV3	1694	1915	0.19%	0.024%
92	14.176	2145	2147	2149	rBV2	387	342	0.03%	0.004%
93	14.274	2161	2163	2167	rVB4	428	419	0.04%	0.005%
94	14.390	2181	2182	2185	rBV	394	374	0.04%	0.005%
95	14.530	2203	2205	2207	rVB2	419	355	0.04%	0.005%
96	14.823	2251	2253	2255	rBV2	371	315	0.03%	0.004%
97	14.920	2268	2269	2271	rBV	489	464	0.05%	0.006%
98	14.993	2276	2281	2288	rBV5	8354	12527	1.26%	0.160%
99	15.103	2298	2299	2303	rBV3	552	648	0.07%	0.008%
100	16.030	2449	2451	2452	rBV2	863	534	0.05%	0.007%

Sum of corrected areas: 7830450




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043685.D
Acq On : 04 Nov 2024 16:18
Operator : JC/MD
Sample : P4621-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

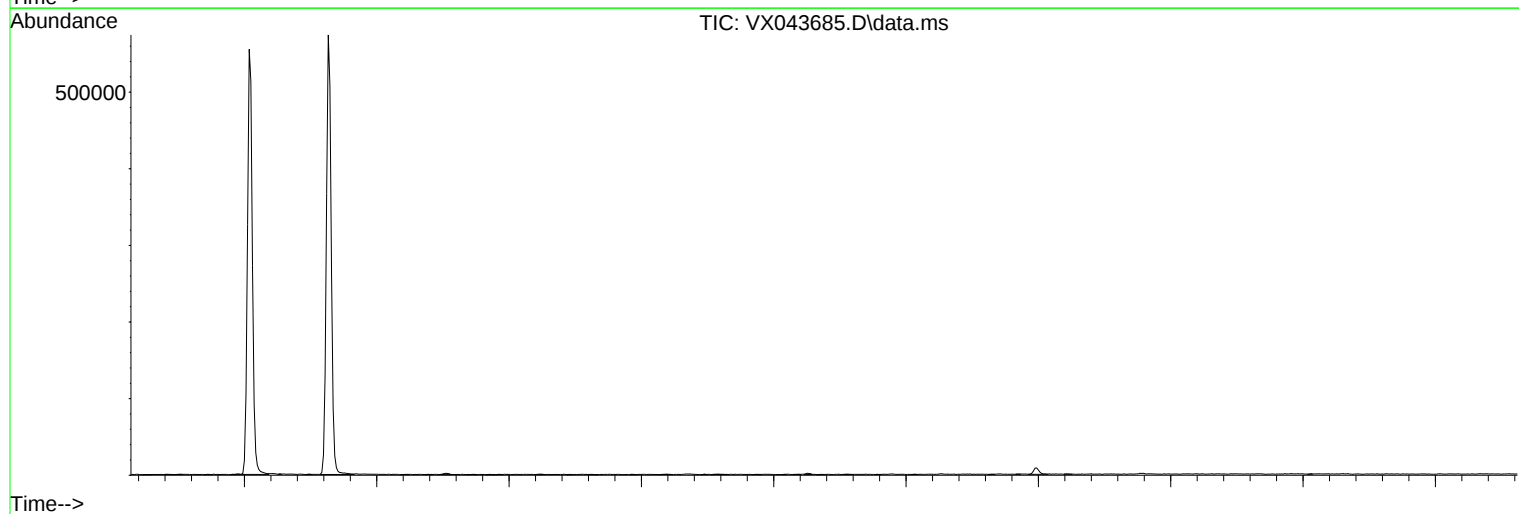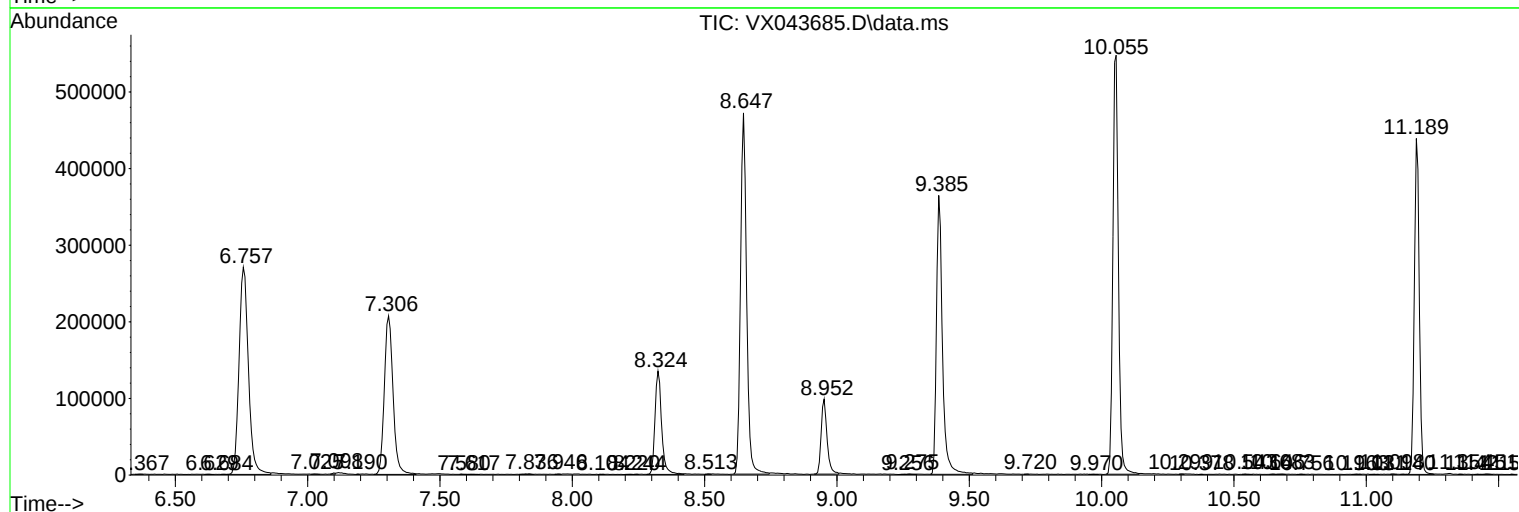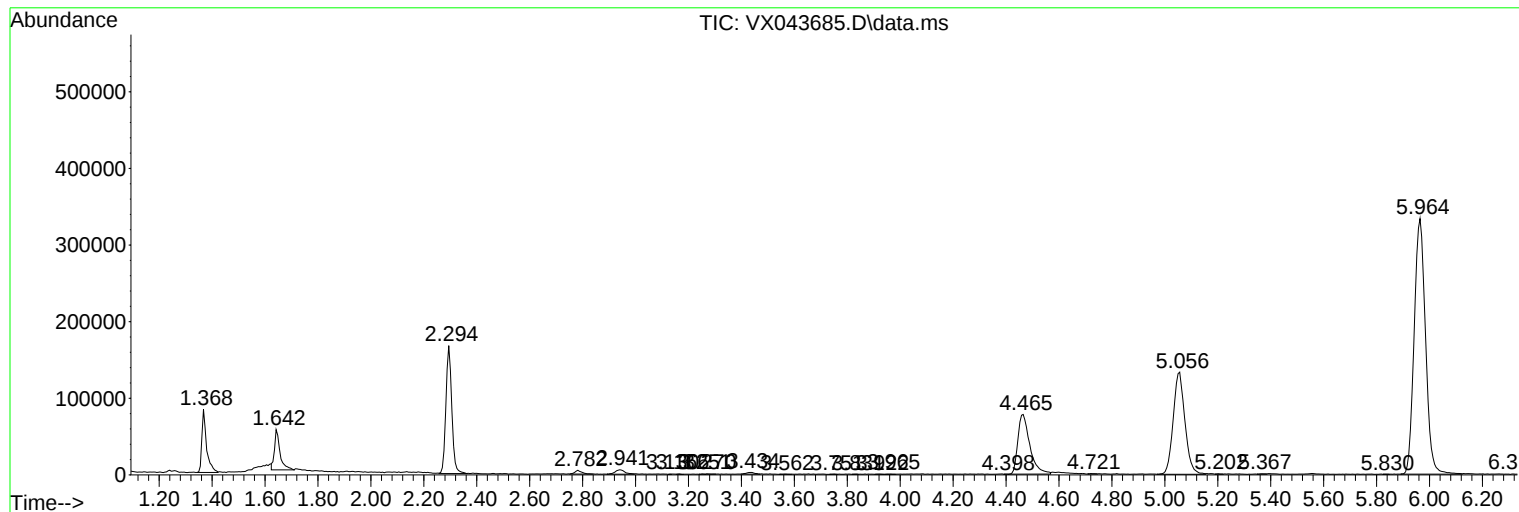

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043685.D
Acq On : 04 Nov 2024 16:18
Operator : JC/MD
Sample : P4621-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043685.D
Acq On : 04 Nov 2024 16:18
Operator : JC/MD
Sample : P4621-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
