

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043686.D
 Acq On : 04 Nov 2024 16:41
 Operator : JC/MD
 Sample : P4621-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043686.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	56	rBV	80606	98998	9.83%	1.270%
2	1.642	88	91	102	rVB	49438	76592	7.61%	0.982%
3	2.294	192	198	209	rVB	170287	262889	26.10%	3.372%
4	2.453	223	224	225	rBV	600	306	0.03%	0.004%
5	2.611	249	250	252	rBV2	577	513	0.05%	0.007%
6	2.709	264	266	267	rVB	719	388	0.04%	0.005%
7	2.727	267	269	272	rBV	383	544	0.05%	0.007%
8	2.776	273	277	283	rBV3	4023	8025	0.80%	0.103%
9	2.934	297	303	312	rBV2	5409	12966	1.29%	0.166%
10	3.233	349	352	353	rBV	294	258	0.03%	0.003%
11	3.276	357	359	362	rBV	369	372	0.04%	0.005%
12	3.440	376	386	389	rBV5	2171	5369	0.53%	0.069%
13	3.514	395	398	400	rBV3	400	425	0.04%	0.005%
14	3.544	400	403	404	rBV	414	367	0.04%	0.005%
15	3.562	404	406	407	rVB	566	290	0.03%	0.004%
16	3.605	407	413	414	rBV	442	664	0.07%	0.009%
17	3.867	453	456	459	rBV2	392	523	0.05%	0.007%
18	3.946	468	469	472	rBV	442	285	0.03%	0.004%
19	3.977	472	474	477	rBV	450	343	0.03%	0.004%
20	4.056	484	487	488	rBV	229	305	0.03%	0.004%
21	4.379	539	540	542	rBV2	358	276	0.03%	0.004%
22	4.465	545	554	572	rBV	78365	247566	24.58%	3.175%
23	5.050	639	650	666	rVV	137793	414821	41.19%	5.320%
24	5.330	694	696	698	rVV2	324	313	0.03%	0.004%
25	5.544	729	731	732	rBV2	485	312	0.03%	0.004%
26	5.635	744	746	748	rBV	491	320	0.03%	0.004%
27	5.672	751	752	755	rBV	310	300	0.03%	0.004%
28	5.739	760	763	764	rBV	294	259	0.03%	0.003%
29	5.879	782	786	787	rBV2	288	354	0.04%	0.005%
30	5.964	789	800	817	rBV3	338176	1007076	100.00%	12.916%
31	6.220	840	842	845	rVB	422	367	0.04%	0.005%
32	6.300	853	855	857	rBV3	318	262	0.03%	0.003%
33	6.330	857	860	862	rVV	306	327	0.03%	0.004%
34	6.470	881	883	886	rBV	375	367	0.04%	0.005%
35	6.605	903	905	908	rBV	213	268	0.03%	0.003%
36	6.659	912	914	917	rBV3	399	448	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043686.D
 Acq On : 04 Nov 2024 16:41
 Operator : JC/MD
 Sample : P4621-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	6.757	920	930	950	rBV	254888	634881	63.04%	8.143%
38	7.117	983	989	994	rBV5	2990	6659	0.66%	0.085%
39	7.172	996	998	1001	rBV3	450	321	0.03%	0.004%
40	7.306	1011	1020	1035	rBV	216297	474861	47.15%	6.090%
41	7.604	1068	1069	1072	rBV	579	386	0.04%	0.005%
42	7.720	1087	1088	1091	rBV3	466	540	0.05%	0.007%
43	7.775	1096	1097	1101	rVV2	432	471	0.05%	0.006%
44	7.903	1116	1118	1121	rBV3	309	435	0.04%	0.006%
45	8.190	1162	1165	1167	rBV3	418	571	0.06%	0.007%
46	8.220	1167	1170	1172	rVB2	324	322	0.03%	0.004%
47	8.324	1181	1187	1201	rBV	135816	234879	23.32%	3.012%
48	8.482	1211	1213	1216	rBV3	450	456	0.05%	0.006%
49	8.519	1216	1219	1220	rVV2	818	634	0.06%	0.008%
50	8.568	1225	1227	1229	rVB2	468	371	0.04%	0.005%
51	8.592	1229	1231	1233	rBV2	279	261	0.03%	0.003%
52	8.647	1234	1240	1259	rBV	485811	775078	76.96%	9.941%
53	8.879	1277	1278	1280	rBV2	445	272	0.03%	0.003%
54	8.952	1285	1290	1303	rVV	100204	153462	15.24%	1.968%
55	9.171	1324	1326	1329	rBV	467	589	0.06%	0.008%
56	9.269	1340	1342	1343	rBV	587	423	0.04%	0.005%
57	9.385	1356	1361	1375	rBV	370367	573962	56.99%	7.361%
58	9.799	1427	1429	1432	rVB2	566	580	0.06%	0.007%
59	9.842	1435	1436	1439	rVB	406	286	0.03%	0.004%
60	9.976	1456	1458	1460	rBV2	307	276	0.03%	0.004%
61	10.055	1465	1471	1484	rBV	520623	753910	74.86%	9.669%
62	10.183	1490	1492	1493	rBV	471	282	0.03%	0.004%
63	10.427	1530	1532	1533	rBV2	320	298	0.03%	0.004%
64	10.646	1565	1568	1570	rBV	671	640	0.06%	0.008%
65	10.701	1575	1577	1579	rVB2	494	355	0.04%	0.005%
66	10.720	1579	1580	1583	rBV2	477	390	0.04%	0.005%
67	10.842	1598	1600	1602	rBV	405	275	0.03%	0.004%
68	10.890	1607	1608	1612	rBV2	375	382	0.04%	0.005%
69	11.134	1646	1648	1652	rBV	257	348	0.03%	0.004%
70	11.189	1652	1657	1669	rVV	468061	588541	58.44%	7.548%
71	11.427	1695	1696	1698	rBV	295	273	0.03%	0.004%
72	11.457	1698	1701	1703	rVB2	555	636	0.06%	0.008%
73	11.671	1734	1736	1738	rBV2	542	481	0.05%	0.006%
74	11.707	1738	1742	1743	rBV2	333	479	0.05%	0.006%
75	11.829	1761	1762	1766	rVV	296	305	0.03%	0.004%
76	11.969	1782	1785	1788	rBV3	775	1056	0.10%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043686.D
 Acq On : 04 Nov 2024 16:41
 Operator : JC/MD
 Sample : P4621-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.018	1788	1793	1804	rBV	516930	675901	67.12%	8.669%
78	12.140	1811	1813	1818	rVB3	661	759	0.08%	0.010%
79	12.317	1837	1842	1857	rBV	584317	752650	74.74%	9.653%
80	12.768	1912	1916	1922	rBV3	1636	2448	0.24%	0.031%
81	12.902	1935	1938	1941	rBV2	304	454	0.05%	0.006%
82	13.091	1965	1969	1971	rBV2	317	563	0.06%	0.007%
83	13.207	1986	1988	1991	rBV	300	260	0.03%	0.003%
84	13.585	2048	2050	2054	rVV4	598	689	0.07%	0.009%
85	13.670	2061	2064	2069	rBV4	507	737	0.07%	0.009%
86	13.786	2081	2083	2085	rBV2	483	426	0.04%	0.005%
87	13.890	2099	2100	2104	rVB2	389	398	0.04%	0.005%
88	14.128	2137	2139	2147	rVB3	1375	1979	0.20%	0.025%
89	14.451	2189	2192	2195	rVB3	1391	1245	0.12%	0.016%
90	14.524	2202	2204	2205	rBV	429	297	0.03%	0.004%
91	14.652	2221	2225	2228	rBV3	601	669	0.07%	0.009%
92	14.780	2242	2246	2248	rBV2	867	825	0.08%	0.011%
93	14.920	2267	2269	2271	rBV2	437	321	0.03%	0.004%
94	14.993	2279	2281	2283	rBV3	644	572	0.06%	0.007%
95	15.018	2283	2285	2286	rVB	543	299	0.03%	0.004%
96	15.133	2301	2304	2305	rBV2	421	306	0.03%	0.004%
97	15.152	2305	2307	2308	rBV	437	293	0.03%	0.004%
98	15.481	2360	2361	2363	rBV	483	414	0.04%	0.005%
99	15.896	2428	2429	2432	rBV3	568	591	0.06%	0.008%
100	16.133	2466	2468	2470	rVB3	663	317	0.03%	0.004%

Sum of corrected areas: 7797098




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043686.D
Acq On : 04 Nov 2024 16:41
Operator : JC/MD
Sample : P4621-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

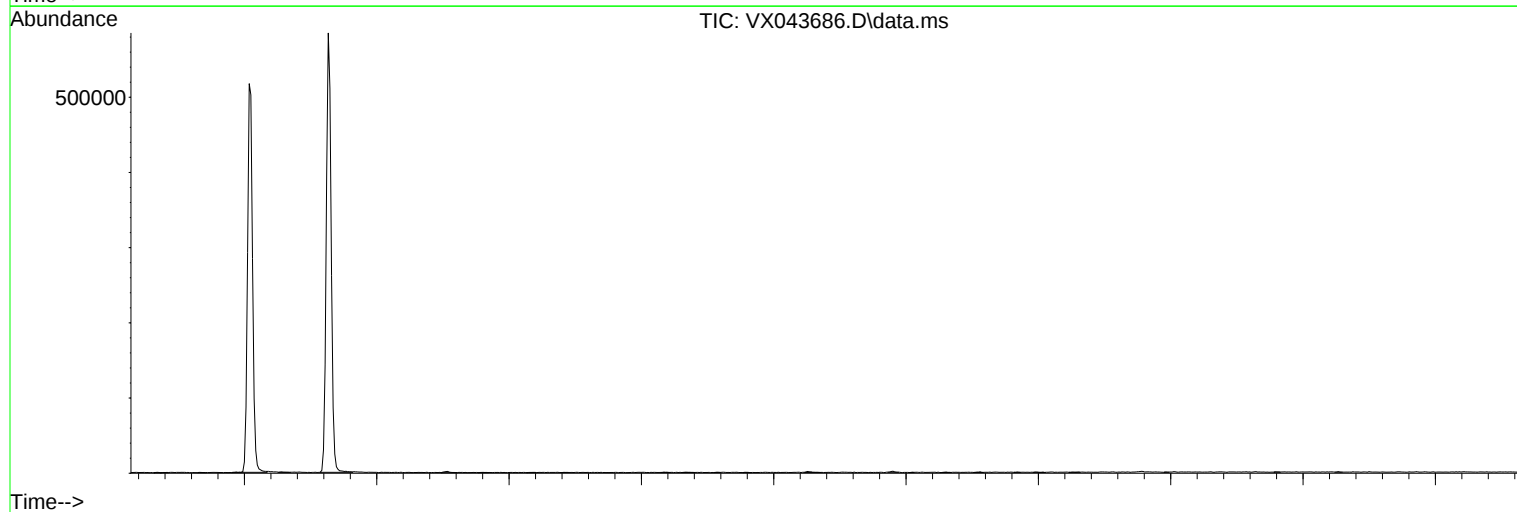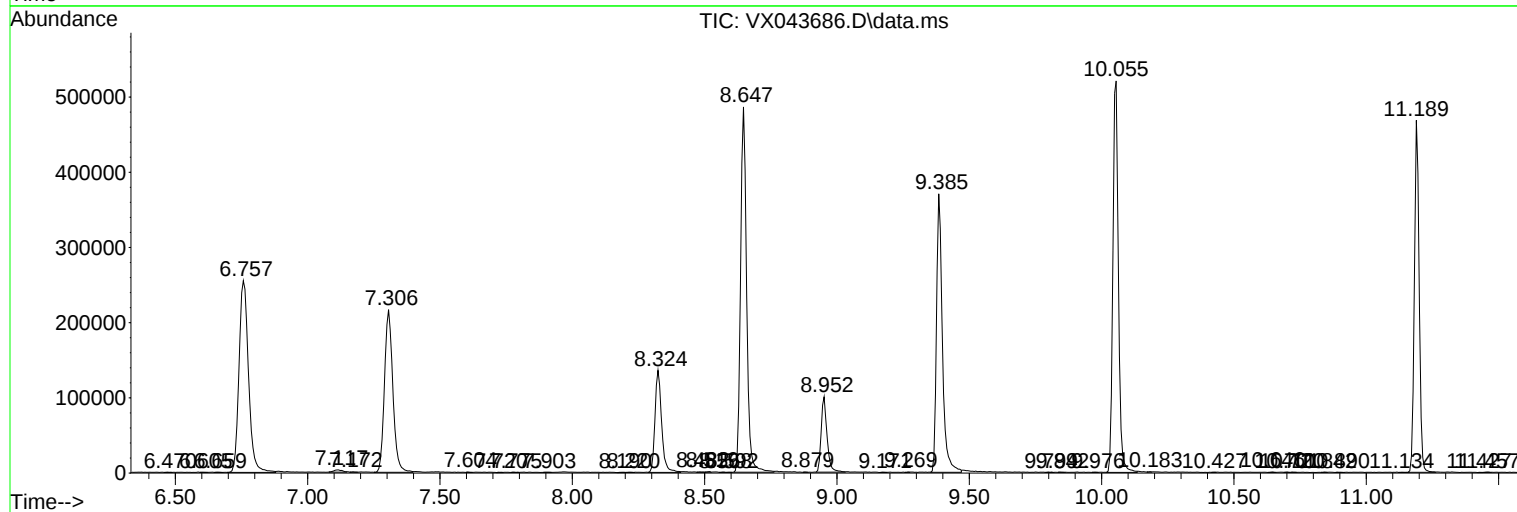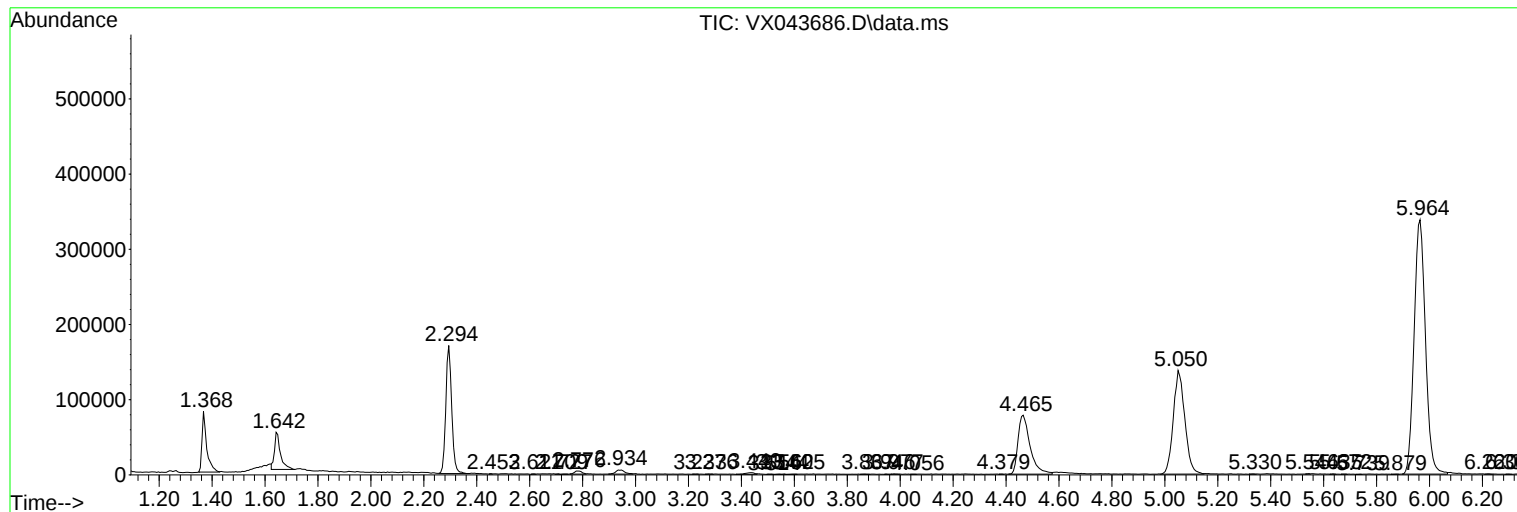

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043686.D
Acq On : 04 Nov 2024 16:41
Operator : JC/MD
Sample : P4621-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043686.D
Acq On : 04 Nov 2024 16:41
Operator : JC/MD
Sample : P4621-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
