

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043688.D
 Acq On : 04 Nov 2024 17:28
 Operator : JC/MD
 Sample : P4621-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043688.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	58	rVB	103921	128650	10.16%	1.611%
2	1.642	88	91	104	rVB	57661	96431	7.62%	1.207%
3	2.294	192	198	209	rVV	209233	328471	25.94%	4.112%
4	2.386	209	213	220	rVB3	3409	6248	0.49%	0.078%
5	2.526	234	236	238	rVB3	544	353	0.03%	0.004%
6	2.672	256	260	265	rVB2	2194	3488	0.28%	0.044%
7	2.782	274	278	284	rVB2	4552	7356	0.58%	0.092%
8	2.941	297	304	313	rBV2	7666	18851	1.49%	0.236%
9	3.075	324	326	327	rBV	463	411	0.03%	0.005%
10	3.087	327	328	330	rVB	596	293	0.02%	0.004%
11	3.190	343	345	348	rBV2	254	333	0.03%	0.004%
12	3.434	380	385	394	rVB5	1895	4639	0.37%	0.058%
13	3.703	427	429	431	rVB2	431	347	0.03%	0.004%
14	3.739	431	435	437	rBV	293	407	0.03%	0.005%
15	3.898	458	461	465	rVB2	400	537	0.04%	0.007%
16	3.928	465	466	469	rBV2	298	369	0.03%	0.005%
17	4.050	484	486	488	rBV2	384	419	0.03%	0.005%
18	4.099	492	494	497	rBV2	301	364	0.03%	0.005%
19	4.227	513	515	517	rVB2	432	346	0.03%	0.004%
20	4.367	536	538	541	rBV2	481	472	0.04%	0.006%
21	4.465	544	554	575	rBV	92595	302485	23.89%	3.787%
22	4.922	627	629	632	rBV2	340	327	0.03%	0.004%
23	5.056	638	651	669	rBV	160667	521085	41.16%	6.524%
24	5.233	678	680	682	rVB2	597	430	0.03%	0.005%
25	5.269	684	686	688	rVB	559	436	0.03%	0.005%
26	5.373	701	703	704	rBV	329	318	0.03%	0.004%
27	5.733	760	762	765	rVB2	354	399	0.03%	0.005%
28	5.757	765	766	770	rBV3	426	609	0.05%	0.008%
29	5.964	788	800	825	rBV2	424769	1266065	100.00%	15.851%
30	6.184	835	836	839	rVB2	614	411	0.03%	0.005%
31	6.361	862	865	866	rBV	508	530	0.04%	0.007%
32	6.574	897	900	901	rBV2	253	293	0.02%	0.004%
33	6.757	921	930	950	rBV	114716	293920	23.22%	3.680%
34	6.952	960	962	967	rBV2	355	392	0.03%	0.005%
35	7.110	980	988	999	rBV3	8988	23189	1.83%	0.290%
36	7.226	1004	1007	1011	rVB4	483	558	0.04%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043688.D
 Acq On : 04 Nov 2024 17:28
 Operator : JC/MD
 Sample : P4621-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.306	1011	1020	1036	rBV	264076	593371	46.87%	7.429%
38	7.452	1043	1044	1045	rBV	689	342	0.03%	0.004%
39	7.519	1053	1055	1057	rVB2	556	410	0.03%	0.005%
40	7.818	1100	1104	1109	rVV4	878	1524	0.12%	0.019%
41	7.891	1114	1116	1119	rVB2	366	310	0.02%	0.004%
42	7.915	1119	1120	1123	rBV	304	305	0.02%	0.004%
43	7.946	1123	1125	1126	rBV	647	519	0.04%	0.006%
44	8.086	1146	1148	1152	rBV3	524	814	0.06%	0.010%
45	8.165	1159	1161	1165	rVB2	365	410	0.03%	0.005%
46	8.324	1181	1187	1201	rBV	177152	293114	23.15%	3.670%
47	8.507	1216	1217	1218	rBV	682	404	0.03%	0.005%
48	8.647	1234	1240	1258	rBV	599580	959153	75.76%	12.009%
49	8.952	1285	1290	1301	rVV	122567	188200	14.86%	2.356%
50	9.275	1340	1343	1346	rVB3	772	973	0.08%	0.012%
51	9.384	1356	1361	1379	rBV	413635	651462	51.46%	8.156%
52	9.671	1406	1408	1411	rBV2	560	380	0.03%	0.005%
53	10.055	1465	1471	1484	rBV	239169	342784	27.07%	4.292%
54	10.317	1512	1514	1517	rVB2	704	548	0.04%	0.007%
55	10.415	1528	1530	1532	rVB2	438	339	0.03%	0.004%
56	10.439	1532	1534	1535	rBV	518	334	0.03%	0.004%
57	10.665	1570	1571	1574	rVB2	535	437	0.03%	0.005%
58	10.799	1588	1593	1594	rBV	255	374	0.03%	0.005%
59	10.902	1608	1610	1614	rVB2	328	370	0.03%	0.005%
60	11.189	1652	1657	1670	rVV	542526	698404	55.16%	8.744%
61	11.762	1749	1751	1753	rVB3	365	351	0.03%	0.004%
62	11.793	1753	1756	1757	rBV2	288	301	0.02%	0.004%
63	11.975	1784	1786	1788	rBV2	471	439	0.03%	0.005%
64	12.024	1788	1794	1804	rBV	228986	305328	24.12%	3.823%
65	12.256	1827	1832	1833	rBV3	295	420	0.03%	0.005%
66	12.317	1837	1842	1856	rVV	732499	917553	72.47%	11.488%
67	12.597	1884	1888	1889	rVV2	408	454	0.04%	0.006%
68	12.628	1891	1893	1898	rVV3	481	557	0.04%	0.007%
69	12.744	1910	1912	1914	rBV3	312	308	0.02%	0.004%
70	12.762	1914	1915	1919	rVB	744	602	0.05%	0.008%
71	12.798	1919	1921	1924	rBV2	369	585	0.05%	0.007%
72	12.896	1935	1937	1938	rBV	447	299	0.02%	0.004%
73	13.030	1958	1959	1964	rBV2	230	334	0.03%	0.004%
74	13.122	1973	1974	1977	rVB2	416	322	0.03%	0.004%
75	13.164	1977	1981	1982	rBV	472	470	0.04%	0.006%
76	13.268	1997	1998	2002	rVB3	347	301	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043688.D
 Acq On : 04 Nov 2024 17:28
 Operator : JC/MD
 Sample : P4621-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	13.493	2032	2035	2036	rBV2	467	404	0.03%	0.005%
78	13.597	2048	2052	2056	rVB2	766	1074	0.08%	0.013%
79	13.634	2056	2058	2059	rBV	401	293	0.02%	0.004%
80	13.670	2062	2064	2066	rBV	362	372	0.03%	0.005%
81	13.792	2081	2084	2085	rBV2	353	315	0.02%	0.004%
82	13.835	2089	2091	2093	rVB2	498	383	0.03%	0.005%
83	13.890	2098	2100	2105	rVB3	471	680	0.05%	0.009%
84	14.030	2121	2123	2124	rBV	470	408	0.03%	0.005%
85	14.067	2128	2129	2133	rVV2	448	453	0.04%	0.006%
86	14.121	2135	2138	2139	rBV3	339	454	0.04%	0.006%
87	14.134	2139	2140	2143	rVV3	769	696	0.05%	0.009%
88	14.195	2146	2150	2151	rBV2	416	624	0.05%	0.008%
89	14.353	2173	2176	2177	rBV2	516	426	0.03%	0.005%
90	14.371	2177	2179	2180	rBV	564	382	0.03%	0.005%
91	14.451	2189	2192	2195	rVB2	1501	1406	0.11%	0.018%
92	14.493	2197	2199	2203	rVB4	561	607	0.05%	0.008%
93	14.615	2217	2219	2221	rVB3	554	356	0.03%	0.004%
94	14.993	2280	2281	2283	rBV2	517	400	0.03%	0.005%
95	15.066	2291	2293	2295	rBV2	621	389	0.03%	0.005%
96	15.103	2298	2299	2300	rBV	507	292	0.02%	0.004%
97	15.188	2311	2313	2314	rBV	551	404	0.03%	0.005%
98	15.633	2383	2386	2388	rBV2	604	932	0.07%	0.012%
99	15.963	2438	2440	2442	rVB3	862	603	0.05%	0.008%
100	16.475	2520	2524	2525	rBV3	636	781	0.06%	0.010%

Sum of corrected areas: 7987271




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043688.D
Acq On : 04 Nov 2024 17:28
Operator : JC/MD
Sample : P4621-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

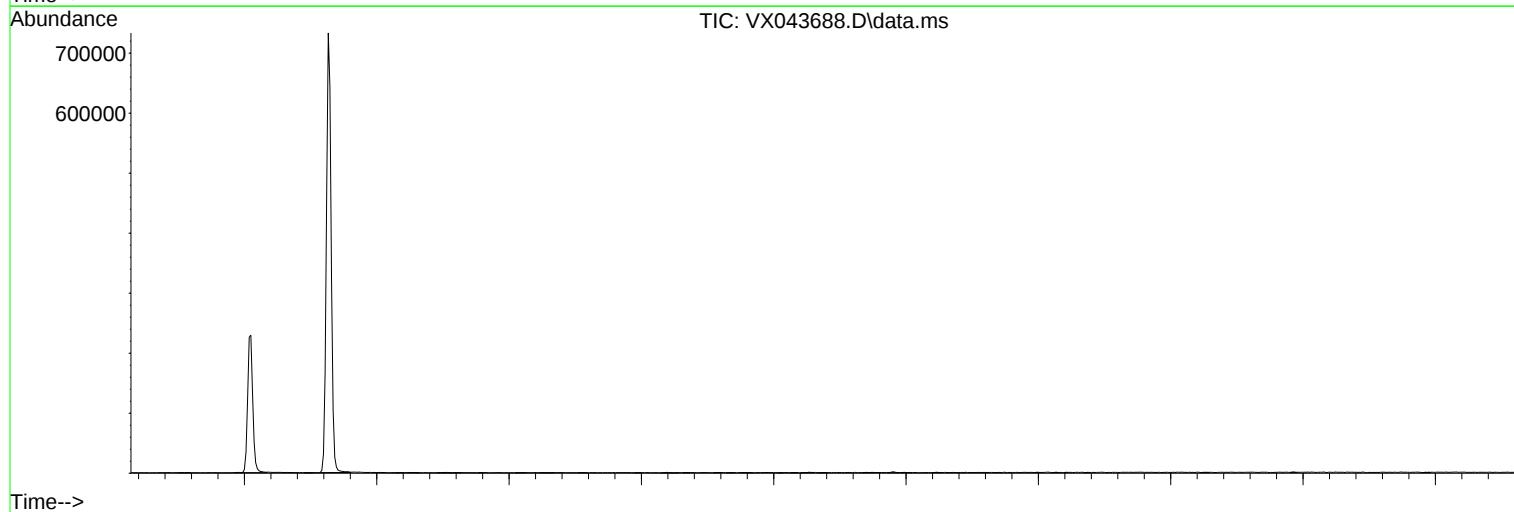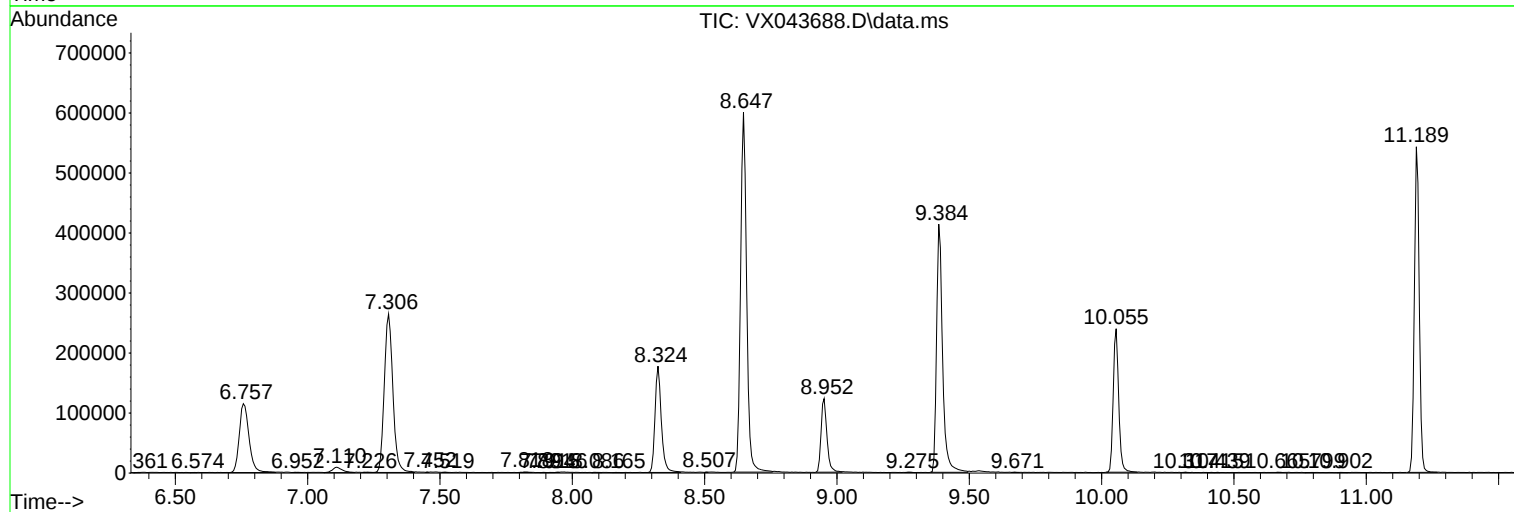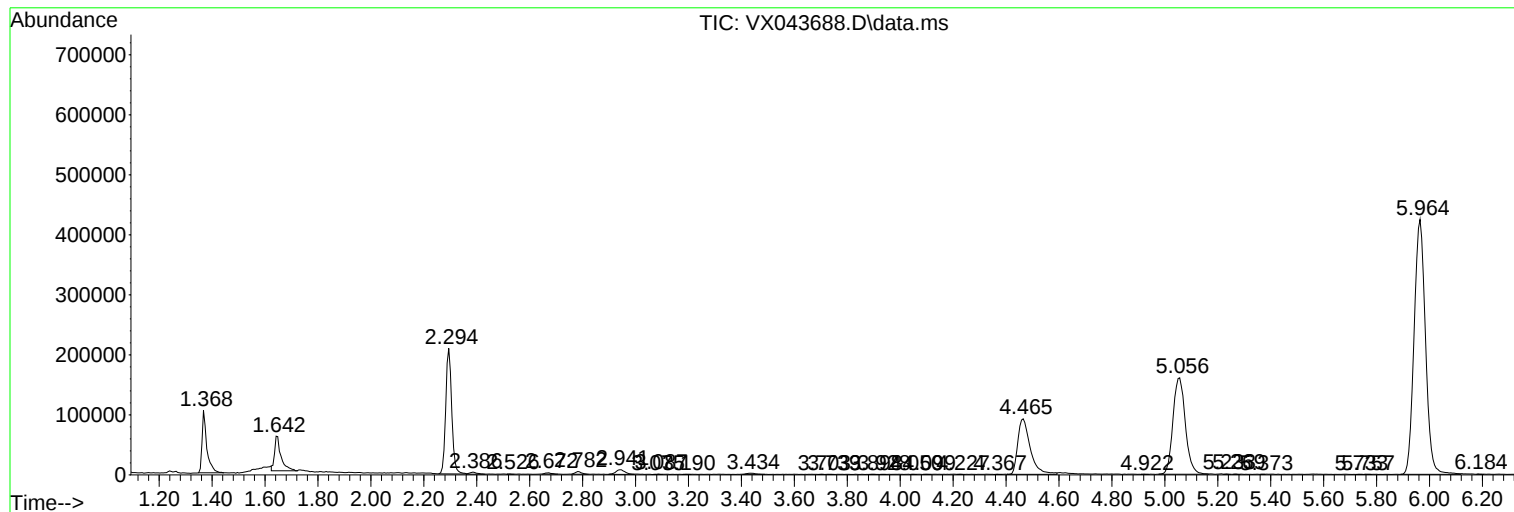

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043688.D
Acq On : 04 Nov 2024 17:28
Operator : JC/MD
Sample : P4621-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043688.D
Acq On : 04 Nov 2024 17:28
Operator : JC/MD
Sample : P4621-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
