

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043690.D
 Acq On : 04 Nov 2024 18:14
 Operator : JC/MD
 Sample : P4621-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043690.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV2	3843	4334	0.32%	0.040%
2	1.368	43	46	57	rBV	113955	140477	10.29%	1.303%
3	1.642	88	91	103	rVB	64614	99057	7.26%	0.919%
4	2.294	192	198	207	rBV	231357	356665	26.13%	3.308%
5	2.386	207	213	224	rVV	291245	487779	35.73%	4.525%
6	2.666	255	259	268	rVB	6751	12478	0.91%	0.116%
7	2.782	272	278	284	rVV2	4229	8032	0.59%	0.075%
8	2.855	287	290	293	rBV	624	954	0.07%	0.009%
9	2.941	297	304	313	rVV2	6935	16867	1.24%	0.156%
10	3.026	316	318	319	rVV	537	298	0.02%	0.003%
11	3.044	319	321	323	rVV	391	343	0.03%	0.003%
12	3.337	366	369	371	rBV2	425	407	0.03%	0.004%
13	3.367	373	374	378	rVB2	468	446	0.03%	0.004%
14	3.434	378	385	393	rBV4	3018	7372	0.54%	0.068%
15	3.654	417	421	422	rVB2	369	421	0.03%	0.004%
16	3.678	422	425	426	rBV	398	326	0.02%	0.003%
17	3.739	432	435	436	rVB2	544	449	0.03%	0.004%
18	3.757	436	438	440	rBV2	328	353	0.03%	0.003%
19	3.812	446	447	449	rBV	361	357	0.03%	0.003%
20	3.946	468	469	473	rBV	406	446	0.03%	0.004%
21	3.983	473	475	480	rVB3	422	505	0.04%	0.005%
22	4.050	484	486	487	rBV	459	394	0.03%	0.004%
23	4.202	507	511	515	rBV3	331	519	0.04%	0.005%
24	4.294	521	526	529	rBV3	546	1065	0.08%	0.010%
25	4.465	545	554	572	rBV	98901	317558	23.26%	2.946%
26	5.050	637	650	665	rBV2	177686	575473	42.16%	5.338%
27	5.379	703	704	705	rBV	514	300	0.02%	0.003%
28	5.660	748	750	752	rVB2	370	361	0.03%	0.003%
29	5.964	788	800	824	rBV2	462198	1365062	100.00%	12.662%
30	6.202	837	839	842	rVB3	398	429	0.03%	0.004%
31	6.367	863	866	868	rBV3	417	578	0.04%	0.005%
32	6.574	897	900	903	rVB2	426	392	0.03%	0.004%
33	6.757	921	930	952	rBV	321238	802065	58.76%	7.440%
34	7.110	980	988	997	rBV3	14343	36930	2.71%	0.343%
35	7.306	1011	1020	1034	rBV	283498	639510	46.85%	5.932%
36	7.641	1073	1075	1077	rBV2	475	434	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043690.D
 Acq On : 04 Nov 2024 18:14
 Operator : JC/MD
 Sample : P4621-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.690	1082	1083	1085	rBV	398	320	0.02%	0.003%
38	7.830	1099	1106	1113	rVB3	2437	4736	0.35%	0.044%
39	7.891	1113	1116	1117	rBV2	359	321	0.02%	0.003%
40	7.915	1117	1120	1121	rBV2	338	308	0.02%	0.003%
41	7.952	1124	1126	1128	rBV3	736	713	0.05%	0.007%
42	8.324	1181	1187	1200	rBV	182556	312799	22.91%	2.901%
43	8.647	1233	1240	1259	rBV	666934	1062462	77.83%	9.855%
44	8.952	1284	1290	1309	rVB	130659	207116	15.17%	1.921%
45	9.104	1313	1315	1321	rBV4	449	470	0.03%	0.004%
46	9.214	1331	1333	1337	rBV	451	599	0.04%	0.006%
47	9.281	1340	1344	1348	rVB2	1335	1835	0.13%	0.017%
48	9.324	1348	1351	1352	rBV	408	383	0.03%	0.004%
49	9.384	1356	1361	1380	rBV	453970	702227	51.44%	6.514%
50	9.811	1430	1431	1434	rVB2	530	378	0.03%	0.004%
51	9.842	1434	1436	1437	rBV	379	306	0.02%	0.003%
52	9.982	1457	1459	1461	rBV2	313	331	0.02%	0.003%
53	10.055	1465	1471	1482	rBV	668400	947111	69.38%	8.785%
54	10.220	1495	1498	1499	rBV	533	391	0.03%	0.004%
55	10.238	1499	1501	1503	rVB2	667	421	0.03%	0.004%
56	10.262	1503	1505	1507	rBV3	447	477	0.03%	0.004%
57	10.317	1513	1514	1521	rVB2	351	553	0.04%	0.005%
58	10.653	1565	1569	1573	rVB2	519	697	0.05%	0.006%
59	10.683	1573	1574	1577	rBV2	422	351	0.03%	0.003%
60	10.774	1586	1589	1592	rBV2	447	530	0.04%	0.005%
61	10.811	1592	1595	1597	rVB2	362	341	0.02%	0.003%
62	10.945	1615	1617	1619	rBV	776	546	0.04%	0.005%
63	11.018	1625	1629	1631	rVB2	367	446	0.03%	0.004%
64	11.085	1638	1640	1643	rVV2	296	326	0.02%	0.003%
65	11.116	1643	1645	1648	rVV	356	361	0.03%	0.003%
66	11.189	1652	1657	1672	rVV	573890	742964	54.43%	6.892%
67	11.317	1675	1678	1682	rVB4	563	749	0.05%	0.007%
68	11.354	1682	1684	1688	rBV3	419	511	0.04%	0.005%
69	11.658	1730	1734	1735	rVB2	378	356	0.03%	0.003%
70	11.884	1768	1771	1774	rBV2	196	303	0.02%	0.003%
71	12.018	1788	1793	1804	rBV	668680	858308	62.88%	7.961%
72	12.317	1837	1842	1853	rBV	807995	1032311	75.62%	9.575%
73	12.524	1875	1876	1879	rVB2	516	420	0.03%	0.004%
74	12.549	1879	1880	1883	rBV2	531	461	0.03%	0.004%
75	12.670	1899	1900	1902	rBV2	447	386	0.03%	0.004%
76	12.762	1910	1915	1920	rVB2	1927	2525	0.18%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043690.D
 Acq On : 04 Nov 2024 18:14
 Operator : JC/MD
 Sample : P4621-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.805	1920	1922	1926	rVB2	428	337	0.02%	0.003%
78	12.859	1929	1931	1932	rVB2	613	376	0.03%	0.003%
79	12.963	1944	1948	1951	rVV2	314	454	0.03%	0.004%
80	13.097	1967	1970	1973	rBV3	331	446	0.03%	0.004%
81	13.237	1992	1993	1997	rBV	469	400	0.03%	0.004%
82	13.274	1997	1999	2002	rVB2	405	458	0.03%	0.004%
83	13.305	2002	2004	2006	rBV	397	398	0.03%	0.004%
84	13.359	2011	2013	2014	rBV	429	389	0.03%	0.004%
85	13.457	2026	2029	2032	rBV3	278	296	0.02%	0.003%
86	13.506	2032	2037	2039	rBV2	396	639	0.05%	0.006%
87	13.591	2048	2051	2055	rVV3	458	779	0.06%	0.007%
88	13.786	2081	2083	2087	rVB3	520	710	0.05%	0.007%
89	13.884	2097	2099	2100	rBV	508	330	0.02%	0.003%
90	14.067	2124	2129	2132	rBV2	608	1069	0.08%	0.010%
91	14.128	2137	2139	2145	rVB3	1706	2234	0.16%	0.021%
92	14.231	2153	2156	2158	rBV2	498	573	0.04%	0.005%
93	14.451	2188	2192	2196	rBV4	830	1160	0.08%	0.011%
94	14.487	2196	2198	2200	rBV3	433	423	0.03%	0.004%
95	14.597	2214	2216	2218	rBV2	600	457	0.03%	0.004%
96	14.670	2226	2228	2230	rVB	540	396	0.03%	0.004%
97	15.286	2328	2329	2332	rBV3	535	423	0.03%	0.004%
98	15.316	2332	2334	2335	rVB	862	433	0.03%	0.004%
99	15.780	2408	2410	2411	rBV2	807	703	0.05%	0.007%
100	16.755	2568	2570	2571	rBV2	613	368	0.03%	0.003%

Sum of corrected areas: 10780836




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043690.D
Acq On : 04 Nov 2024 18:14
Operator : JC/MD
Sample : P4621-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

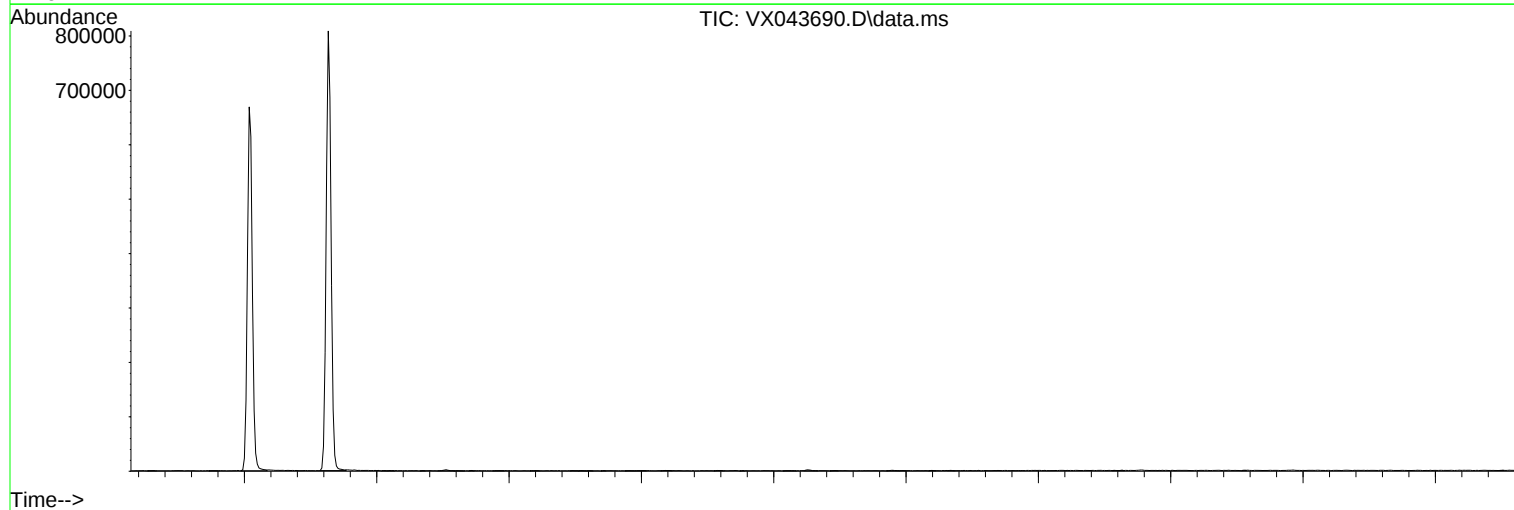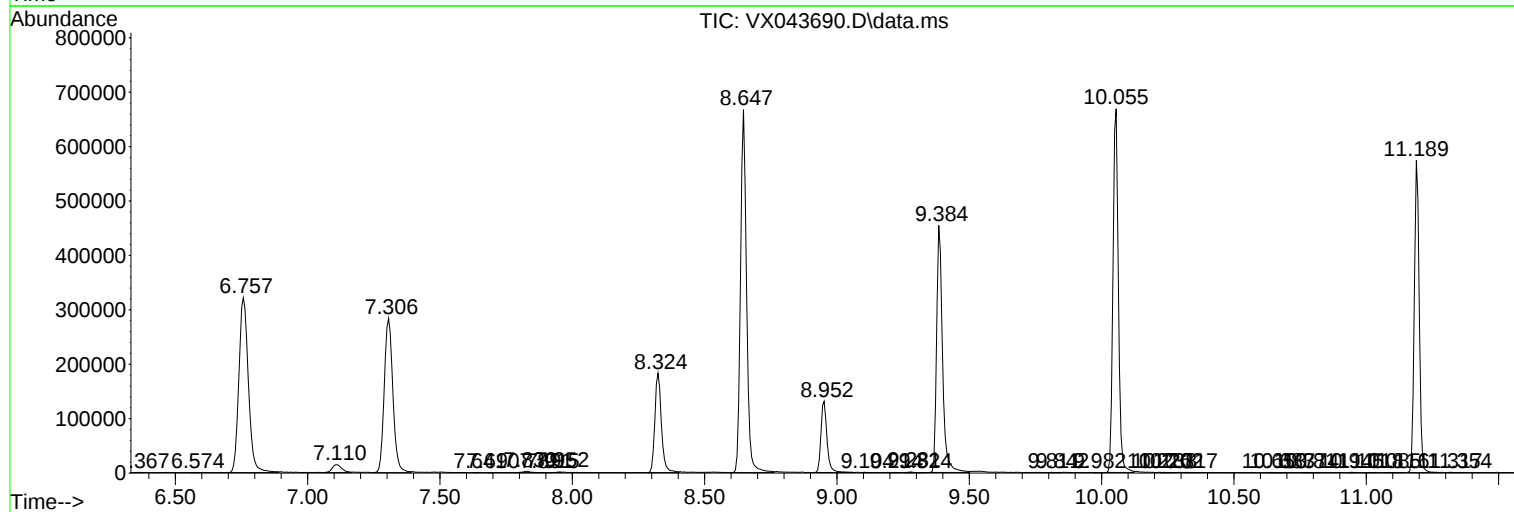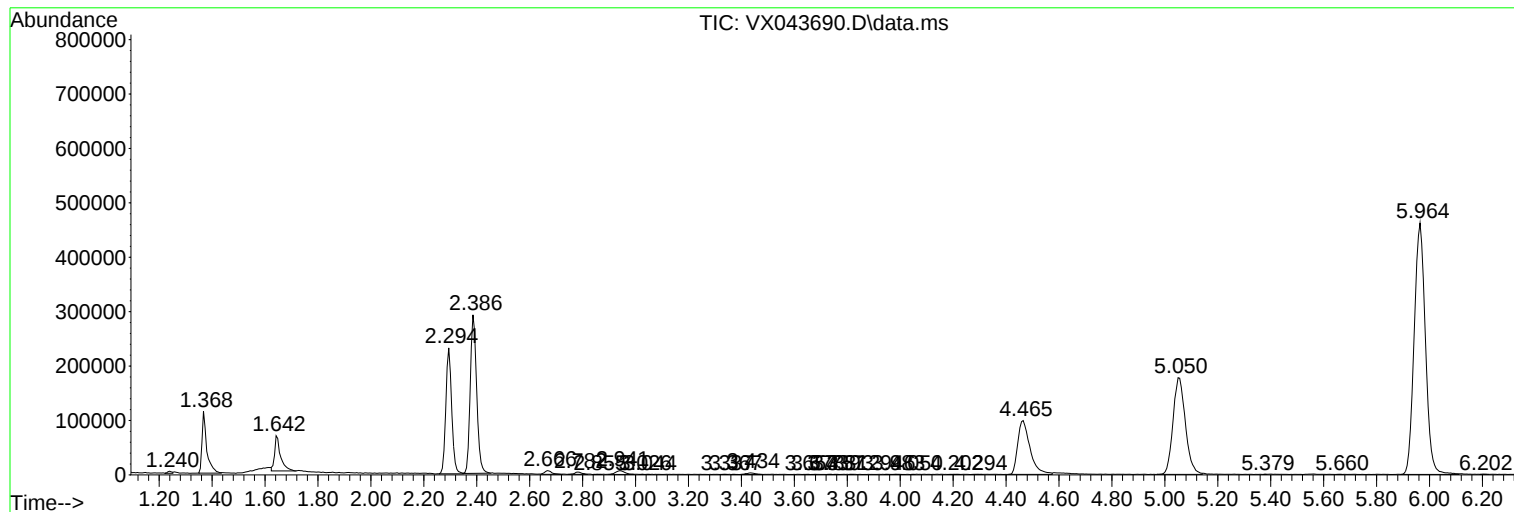

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043690.D
Acq On : 04 Nov 2024 18:14
Operator : JC/MD
Sample : P4621-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043690.D
Acq On : 04 Nov 2024 18:14
Operator : JC/MD
Sample : P4621-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
