

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043692.D
 Acq On : 04 Nov 2024 19:00
 Operator : JC/MD
 Sample : P4621-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043692.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	27	rBV2	3297	4166	0.51%	0.070%
2	1.367	43	46	59	rBV	68063	82500	10.08%	1.392%
3	1.642	89	91	103	rVB	41927	64205	7.84%	1.084%
4	2.294	192	198	210	rBV	136900	213207	26.04%	3.598%
5	2.453	221	224	225	rBV	660	507	0.06%	0.009%
6	2.507	231	233	237	rVB2	582	550	0.07%	0.009%
7	2.605	245	249	251	rBV3	400	820	0.10%	0.014%
8	2.623	251	252	255	rVV	770	677	0.08%	0.011%
9	2.672	255	260	268	rVB2	2615	5071	0.62%	0.086%
10	2.788	274	279	285	rVB4	2887	6191	0.76%	0.104%
11	2.940	297	304	312	rBV2	7267	15776	1.93%	0.266%
12	3.062	321	324	325	rVB2	409	297	0.04%	0.005%
13	3.093	328	329	332	rBV3	357	393	0.05%	0.007%
14	3.209	347	348	351	rBV	298	369	0.05%	0.006%
15	3.294	360	362	365	rVB3	467	420	0.05%	0.007%
16	3.324	365	367	370	rVB	358	307	0.04%	0.005%
17	3.379	373	376	379	rVB2	299	436	0.05%	0.007%
18	3.434	379	385	394	rBB5	1789	4133	0.50%	0.070%
19	3.599	410	412	416	rBV3	347	506	0.06%	0.009%
20	3.690	426	427	431	rVB3	479	436	0.05%	0.007%
21	3.727	431	433	434	rBV2	303	285	0.03%	0.005%
22	3.971	468	473	476	rBV2	406	768	0.09%	0.013%
23	4.349	532	535	539	rBV2	307	429	0.05%	0.007%
24	4.464	546	554	569	rBV	59039	186344	22.76%	3.145%
25	4.970	634	637	638	rBV2	225	275	0.03%	0.005%
26	5.050	638	650	667	rVV2	105367	332144	40.57%	5.605%
27	5.251	682	683	688	rVB2	370	498	0.06%	0.008%
28	5.543	726	731	732	rBV3	644	957	0.12%	0.016%
29	5.751	763	765	767	rBV	487	318	0.04%	0.005%
30	5.769	767	768	771	rBV2	372	403	0.05%	0.007%
31	5.964	789	800	826	rBV2	274308	818774	100.00%	13.818%
32	6.757	921	930	943	rBV	177485	433356	52.93%	7.314%
33	6.982	964	967	970	rBV4	506	720	0.09%	0.012%
34	7.110	979	988	996	rBV2	13734	33520	4.09%	0.566%
35	7.305	1011	1020	1034	rBV	171508	381028	46.54%	6.430%
36	7.446	1041	1043	1045	rVB2	513	315	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043692.D
 Acq On : 04 Nov 2024 19:00
 Operator : JC/MD
 Sample : P4621-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.482	1047	1049	1052	rVV3	764	786	0.10%	0.013%
38	7.531	1055	1057	1059	rBV3	341	298	0.04%	0.005%
39	7.689	1080	1083	1085	rBV	324	327	0.04%	0.006%
40	7.738	1088	1091	1092	rBV	329	306	0.04%	0.005%
41	7.769	1095	1096	1099	rBV2	253	322	0.04%	0.005%
42	8.098	1148	1150	1152	rBV	315	299	0.04%	0.005%
43	8.323	1181	1187	1203	rBV	104108	180824	22.08%	3.052%
44	8.592	1227	1231	1233	rBV4	452	631	0.08%	0.011%
45	8.647	1233	1240	1266	rBV	389766	632119	77.20%	10.668%
46	8.897	1279	1281	1283	rBV	527	580	0.07%	0.010%
47	8.951	1285	1290	1301	rVV	73496	116128	14.18%	1.960%
48	9.165	1322	1325	1328	rBV2	424	655	0.08%	0.011%
49	9.207	1330	1332	1334	rVV3	324	294	0.04%	0.005%
50	9.275	1339	1343	1345	rBV2	712	852	0.10%	0.014%
51	9.384	1356	1361	1372	rBV	259645	409079	49.96%	6.904%
52	9.927	1448	1450	1452	rBV2	252	295	0.04%	0.005%
53	10.055	1465	1471	1486	rVV	360845	511405	62.46%	8.631%
54	10.317	1510	1514	1515	rBV2	660	815	0.10%	0.014%
55	10.354	1518	1520	1523	rVB2	491	498	0.06%	0.008%
56	10.390	1523	1526	1528	rBV3	315	436	0.05%	0.007%
57	10.506	1543	1545	1547	rBV2	300	296	0.04%	0.005%
58	10.561	1552	1554	1555	rBV2	289	278	0.03%	0.005%
59	10.671	1570	1572	1575	rVB	436	289	0.04%	0.005%
60	10.713	1575	1579	1582	rBV2	309	443	0.05%	0.007%
61	10.908	1610	1611	1616	rVB2	387	445	0.05%	0.008%
62	10.945	1616	1617	1620	rBV	438	379	0.05%	0.006%
63	11.049	1632	1634	1637	rVB	321	276	0.03%	0.005%
64	11.189	1652	1657	1667	rBV	319902	423837	51.76%	7.153%
65	11.524	1710	1712	1714	rBV2	416	393	0.05%	0.007%
66	11.603	1723	1725	1728	rBV2	260	330	0.04%	0.006%
67	11.695	1737	1740	1742	rVB2	482	583	0.07%	0.010%
68	11.713	1742	1743	1746	rBV	350	302	0.04%	0.005%
69	11.866	1766	1768	1772	rBV2	258	289	0.04%	0.005%
70	11.975	1784	1786	1788	rBV2	489	591	0.07%	0.010%
71	12.018	1788	1793	1804	rBV	330302	443810	54.20%	7.490%
72	12.317	1837	1842	1853	rBV	458162	588477	71.87%	9.932%
73	12.768	1912	1916	1919	rVB2	1046	1539	0.19%	0.026%
74	12.798	1919	1921	1923	rBV	383	297	0.04%	0.005%
75	12.939	1942	1944	1946	rBV	459	295	0.04%	0.005%
76	12.981	1949	1951	1953	rBV2	328	285	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043692.D
 Acq On : 04 Nov 2024 19:00
 Operator : JC/MD
 Sample : P4621-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	13.243	1992	1994	1995	rBV	331	314	0.04%	0.005%
78	13.262	1995	1997	2002	rVB3	624	746	0.09%	0.013%
79	13.310	2002	2005	2008	rBV	279	354	0.04%	0.006%
80	13.335	2008	2009	2013	rBV2	349	491	0.06%	0.008%
81	13.597	2050	2052	2053	rBV2	486	285	0.03%	0.005%
82	13.676	2062	2065	2069	rVB2	497	576	0.07%	0.010%
83	13.731	2069	2074	2076	rBV2	533	749	0.09%	0.013%
84	13.755	2076	2078	2080	rVB2	420	297	0.04%	0.005%
85	13.786	2080	2083	2089	rVB3	643	1361	0.17%	0.023%
86	13.829	2089	2090	2094	rBV3	359	495	0.06%	0.008%
87	13.963	2110	2112	2114	rVV2	520	429	0.05%	0.007%
88	13.987	2114	2116	2117	rVV	527	278	0.03%	0.005%
89	14.030	2121	2123	2127	rVB2	651	491	0.06%	0.008%
90	14.127	2136	2139	2142	rVV2	796	899	0.11%	0.015%
91	14.255	2159	2160	2162	rBV	484	384	0.05%	0.006%
92	14.335	2172	2173	2177	rBV2	334	421	0.05%	0.007%
93	14.444	2188	2191	2194	rBV4	1000	1341	0.16%	0.023%
94	14.603	2216	2217	2222	rVB2	574	444	0.05%	0.007%
95	14.731	2235	2238	2242	rBV4	518	686	0.08%	0.012%
96	14.902	2263	2266	2267	rBV2	548	612	0.07%	0.010%
97	15.371	2341	2343	2344	rBV	612	386	0.05%	0.007%
98	15.554	2372	2373	2374	rBV	656	313	0.04%	0.005%
99	15.968	2439	2441	2445	rVB4	910	834	0.10%	0.014%
100	16.249	2486	2487	2491	rBV3	634	656	0.08%	0.011%

Sum of corrected areas: 5925326




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043692.D
Acq On : 04 Nov 2024 19:00
Operator : JC/MD
Sample : P4621-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

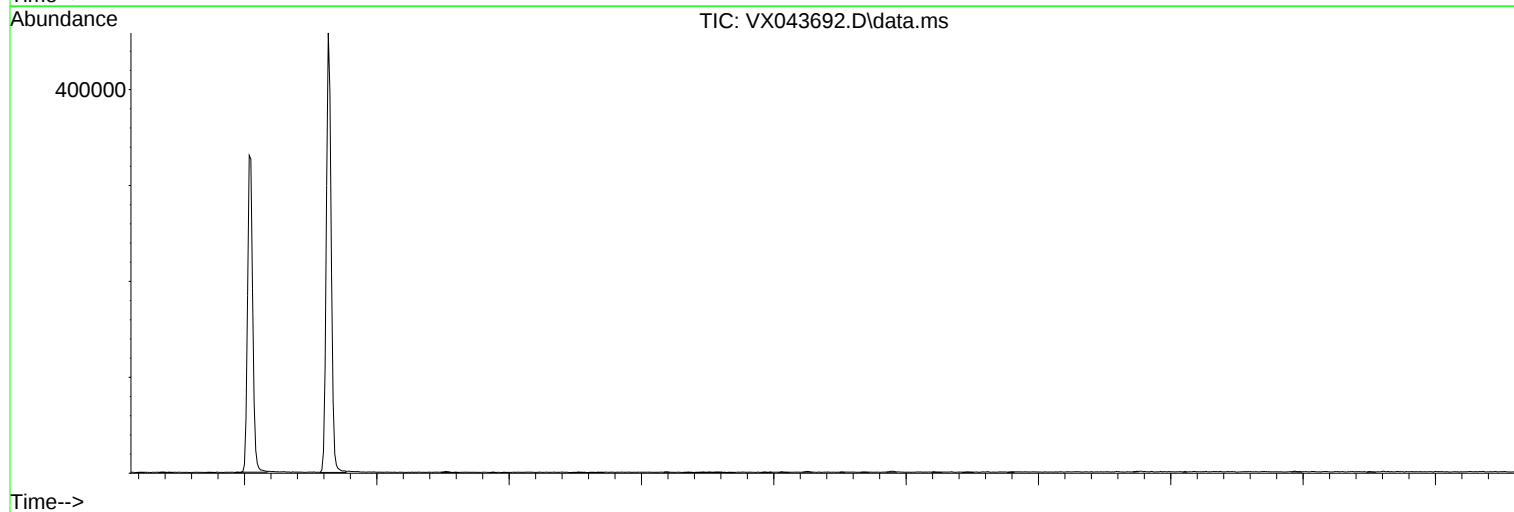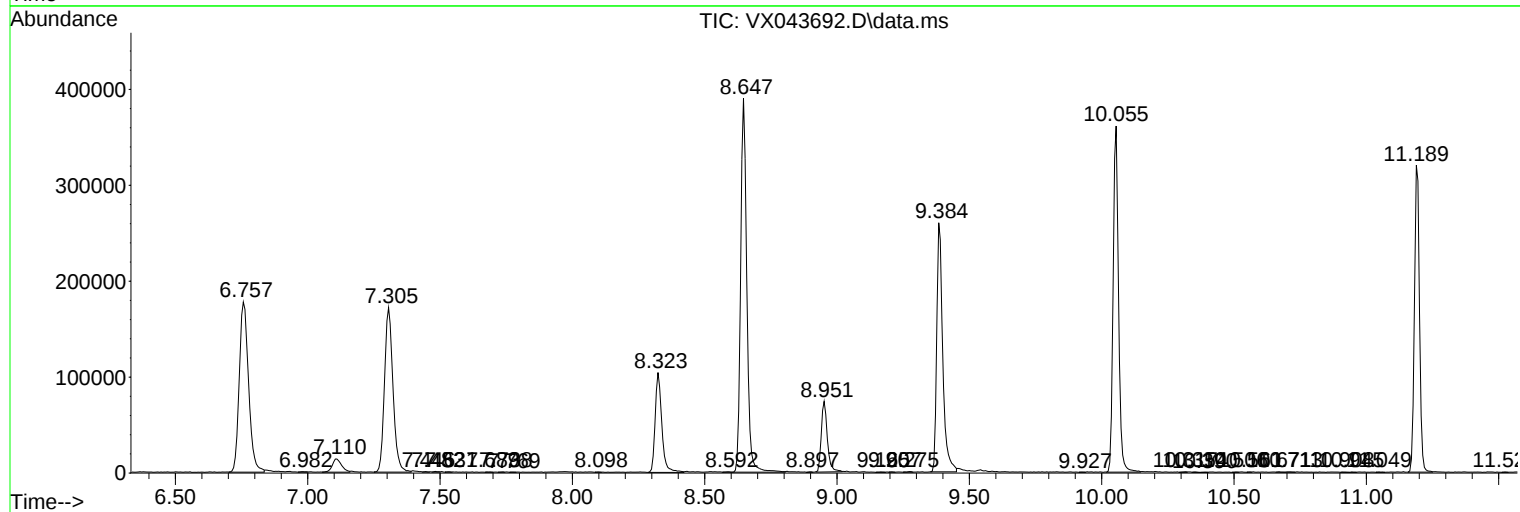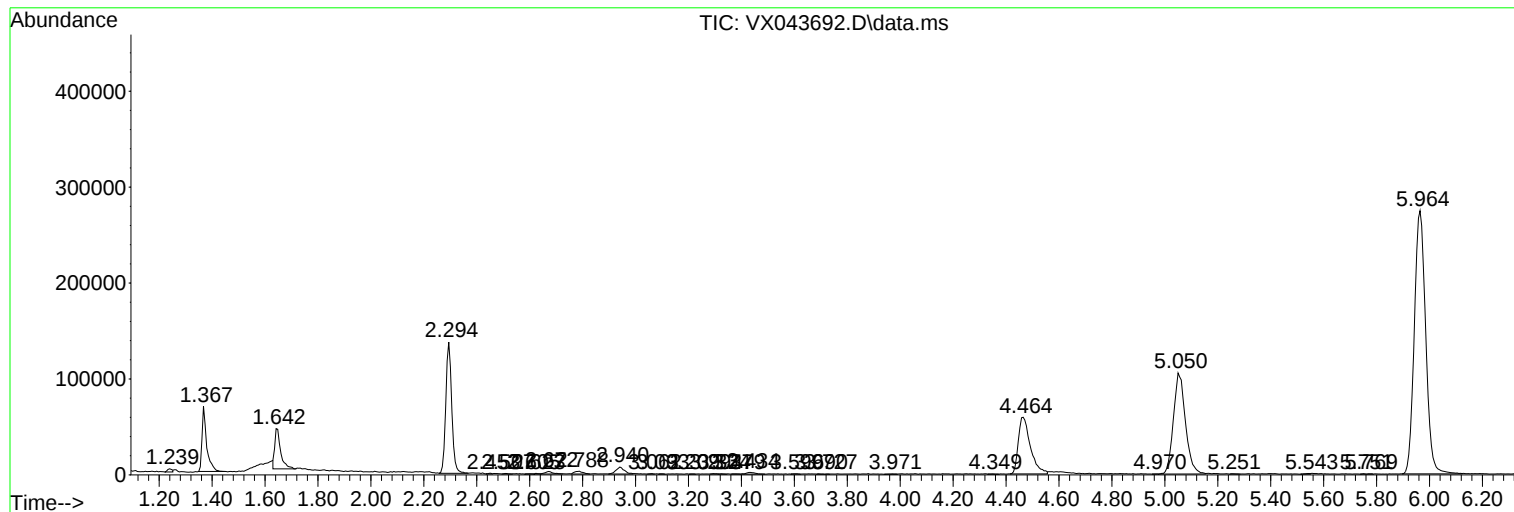

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043692.D
Acq On : 04 Nov 2024 19:00
Operator : JC/MD
Sample : P4621-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043692.D
Acq On : 04 Nov 2024 19:00
Operator : JC/MD
Sample : P4621-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
