

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043694.D
 Acq On : 04 Nov 2024 19:46
 Operator : JC/MD
 Sample : P4621-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH8M6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043694.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rVB3	3803	6188	0.61%	0.084%
2	1.368	42	46	57	rBV	76310	102486	10.12%	1.388%
3	1.642	88	91	102	rVB	47097	75652	7.47%	1.024%
4	2.294	191	198	210	rBV	163462	259678	25.65%	3.516%
5	2.563	241	242	245	rBV2	607	523	0.05%	0.007%
6	2.605	248	249	253	rBV3	490	564	0.06%	0.008%
7	2.672	253	260	268	rVB2	7502	14778	1.46%	0.200%
8	2.782	273	278	284	rVB3	5175	9677	0.96%	0.131%
9	2.941	299	304	312	rVB3	6541	13796	1.36%	0.187%
10	3.050	320	322	325	rBV2	353	404	0.04%	0.005%
11	3.087	325	328	329	rBV	451	369	0.04%	0.005%
12	3.105	329	331	334	rVV2	368	457	0.05%	0.006%
13	3.154	337	339	342	rBV	314	408	0.04%	0.006%
14	3.227	350	351	354	rBV	651	597	0.06%	0.008%
15	3.337	366	369	370	rBV	437	378	0.04%	0.005%
16	3.434	379	385	392	rVB4	2224	5122	0.51%	0.069%
17	3.520	397	399	402	rBV2	398	419	0.04%	0.006%
18	3.587	408	410	411	rVB	490	339	0.03%	0.005%
19	3.605	411	413	414	rBV2	448	352	0.03%	0.005%
20	3.867	454	456	459	rBV2	424	354	0.03%	0.005%
21	4.123	495	498	501	rBV2	286	284	0.03%	0.004%
22	4.257	517	520	523	rVB2	266	344	0.03%	0.005%
23	4.294	523	526	527	rBV	267	285	0.03%	0.004%
24	4.355	533	536	538	rVB2	305	357	0.04%	0.005%
25	4.465	546	554	574	rBV	73618	233311	23.04%	3.159%
26	4.806	608	610	613	rBV2	427	410	0.04%	0.006%
27	4.928	628	630	633	rVB2	300	313	0.03%	0.004%
28	5.056	637	651	669	rBV	128489	425279	42.00%	5.758%
29	5.208	674	676	678	rVB	544	550	0.05%	0.007%
30	5.276	685	687	691	rVB	378	435	0.04%	0.006%
31	5.367	700	702	703	rBV	458	336	0.03%	0.005%
32	5.550	728	732	734	rBV2	674	807	0.08%	0.011%
33	5.800	771	773	778	rVB2	311	459	0.05%	0.006%
34	5.879	784	786	787	rVB	541	339	0.03%	0.005%
35	5.964	787	800	821	rBV2	339133	1012530	100.00%	13.709%
36	6.275	849	851	852	rBV2	398	325	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043694.D
 Acq On : 04 Nov 2024 19:46
 Operator : JC/MD
 Sample : P4621-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH8M6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

37	6.550	894	896	900	rVB2	311	354	0.03%	0.005%
38	6.757	921	930	948	rBV	230128	563754	55.68%	7.633%
39	7.111	980	988	998	rBV2	14814	34920	3.45%	0.473%
40	7.306	1011	1020	1034	rBV	218698	478876	47.29%	6.484%
41	7.434	1039	1041	1042	rBV2	615	404	0.04%	0.005%
42	7.720	1087	1088	1091	rVB	527	289	0.03%	0.004%
43	7.830	1099	1106	1112	rBV3	2871	4959	0.49%	0.067%
44	7.964	1124	1128	1134	rBV3	831	1600	0.16%	0.022%
45	8.098	1148	1150	1153	rBV2	305	301	0.03%	0.004%
46	8.190	1164	1165	1168	rBV	308	310	0.03%	0.004%
47	8.324	1181	1187	1202	rVV	133127	225806	22.30%	3.057%
48	8.446	1206	1207	1208	rBV	512	309	0.03%	0.004%
49	8.647	1234	1240	1260	rBV	488583	785089	77.54%	10.630%
50	8.952	1285	1290	1303	rBV	92918	145539	14.37%	1.971%
51	9.068	1307	1309	1313	rBV4	487	543	0.05%	0.007%
52	9.275	1341	1343	1348	rVB3	976	891	0.09%	0.012%
53	9.385	1356	1361	1380	rBV	281992	471213	46.54%	6.380%
54	9.927	1448	1450	1452	rBV2	329	285	0.03%	0.004%
55	10.055	1465	1471	1491	rVV	455452	654834	64.67%	8.866%
56	10.317	1510	1514	1515	rBV3	759	815	0.08%	0.011%
57	10.470	1536	1539	1541	rVB2	458	454	0.04%	0.006%
58	10.537	1548	1550	1552	rBV	382	286	0.03%	0.004%
59	10.634	1565	1566	1569	rBV	412	427	0.04%	0.006%
60	10.756	1584	1586	1589	rVV	265	310	0.03%	0.004%
61	10.799	1589	1593	1594	rVV2	392	438	0.04%	0.006%
62	10.884	1606	1607	1611	rVB2	448	367	0.04%	0.005%
63	10.964	1618	1620	1621	rBV2	436	328	0.03%	0.004%
64	11.189	1652	1657	1668	rBV	408717	534209	52.76%	7.233%
65	11.305	1675	1676	1679	rVB	591	409	0.04%	0.006%
66	11.348	1682	1683	1686	rVB	487	294	0.03%	0.004%
67	11.372	1686	1687	1690	rBV2	405	306	0.03%	0.004%
68	11.451	1699	1700	1704	rBV2	386	329	0.03%	0.004%
69	11.561	1716	1718	1722	rVB	528	388	0.04%	0.005%
70	11.976	1784	1786	1788	rBV	339	296	0.03%	0.004%
71	12.018	1788	1793	1803	rBV	424651	556653	54.98%	7.537%
72	12.317	1837	1842	1856	rBV	580311	735880	72.68%	9.963%
73	12.671	1898	1900	1902	rVB	480	330	0.03%	0.004%
74	12.762	1912	1915	1919	rBV4	743	1166	0.12%	0.016%
75	12.841	1926	1928	1931	rBV	336	327	0.03%	0.004%
76	12.988	1949	1952	1953	rBV2	295	326	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
 Data File : VX043694.D
 Acq On : 04 Nov 2024 19:46
 Operator : JC/MD
 Sample : P4621-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH8M6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	13.152	1977	1979	1984	rVB3	424	533	0.05%	0.007%
78	13.305	2002	2004	2007	rVB2	283	324	0.03%	0.004%
79	13.372	2013	2015	2018	rVV	315	319	0.03%	0.004%
80	13.530	2038	2041	2043	rBV	330	314	0.03%	0.004%
81	13.695	2065	2068	2071	rBV2	409	595	0.06%	0.008%
82	13.725	2071	2073	2075	rVV2	444	386	0.04%	0.005%
83	13.762	2077	2079	2081	rBV2	361	352	0.03%	0.005%
84	13.792	2082	2084	2087	rVB3	377	384	0.04%	0.005%
85	13.914	2102	2104	2106	rBV2	356	299	0.03%	0.004%
86	13.951	2108	2110	2114	rVB2	338	410	0.04%	0.006%
87	14.000	2114	2118	2121	rVB3	464	722	0.07%	0.010%
88	14.030	2121	2123	2124	rBV	383	290	0.03%	0.004%
89	14.128	2133	2139	2140	rBV3	737	965	0.10%	0.013%
90	14.341	2171	2174	2177	rBV	650	745	0.07%	0.010%
91	14.445	2189	2191	2194	rBV2	1256	1199	0.12%	0.016%
92	14.475	2194	2196	2199	rBV3	452	358	0.04%	0.005%
93	14.591	2213	2215	2218	rBV3	281	307	0.03%	0.004%
94	14.969	2275	2277	2278	rVB	554	380	0.04%	0.005%
95	14.993	2278	2281	2282	rBV	375	481	0.05%	0.007%
96	15.469	2358	2359	2361	rBV2	632	627	0.06%	0.008%
97	15.670	2390	2392	2394	rBV2	663	512	0.05%	0.007%
98	16.079	2457	2459	2461	rBV	608	567	0.06%	0.008%
99	16.396	2509	2511	2512	rBV2	634	570	0.06%	0.008%
100	16.719	2563	2564	2568	rBV2	584	613	0.06%	0.008%

Sum of corrected areas: 7385771




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043694.D
Acq On : 04 Nov 2024 19:46
Operator : JC/MD
Sample : P4621-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH8M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

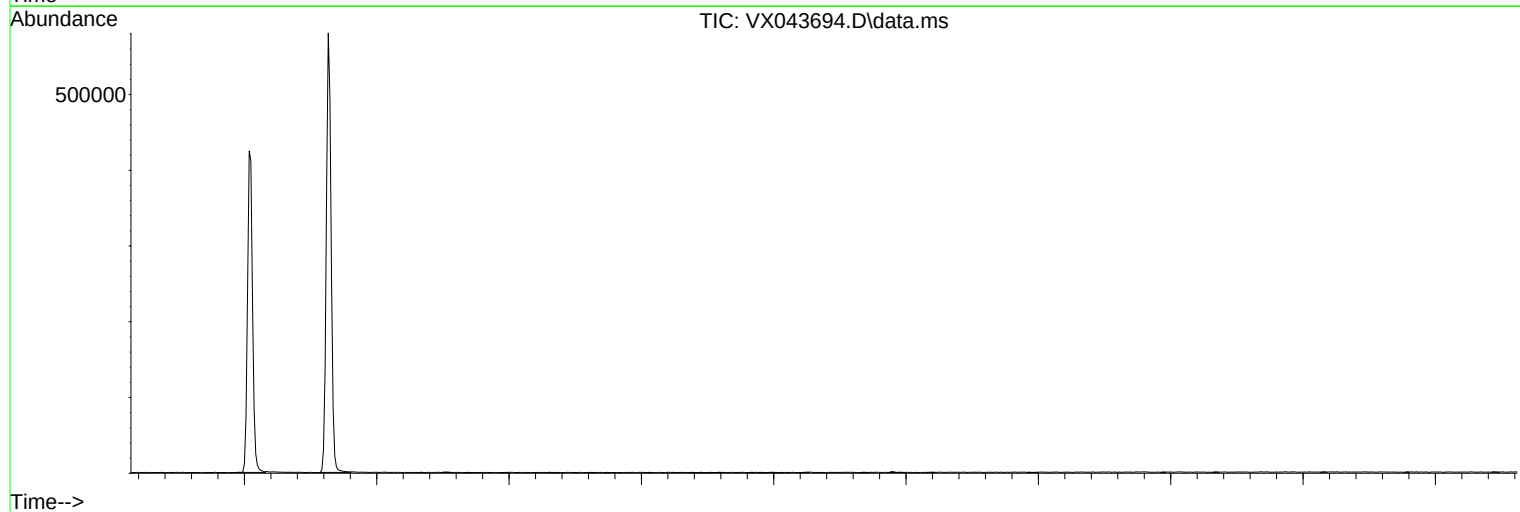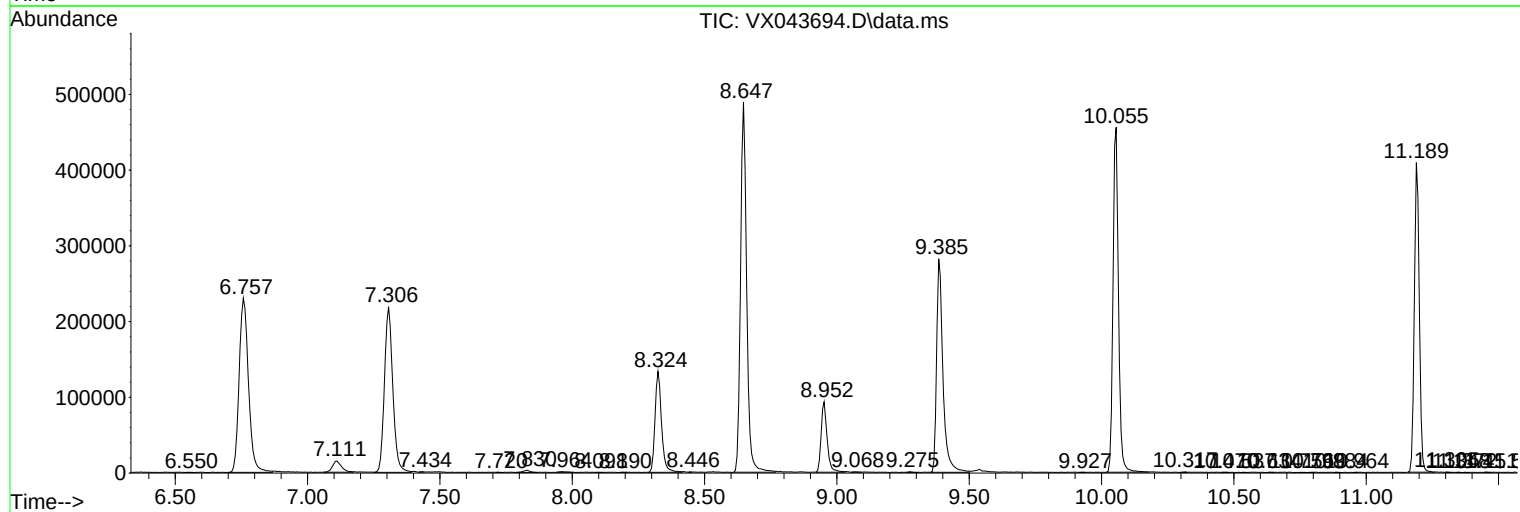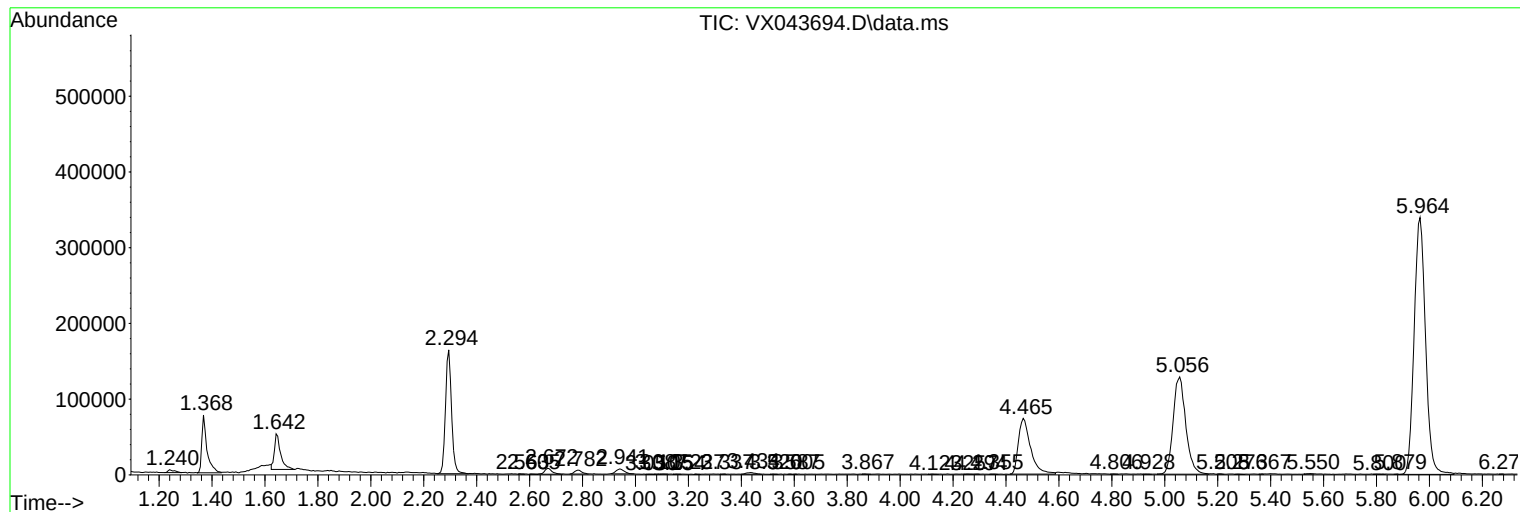

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043694.D
Acq On : 04 Nov 2024 19:46
Operator : JC/MD
Sample : P4621-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH8M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043694.D
Acq On : 04 Nov 2024 19:46
Operator : JC/MD
Sample : P4621-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH8M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
