
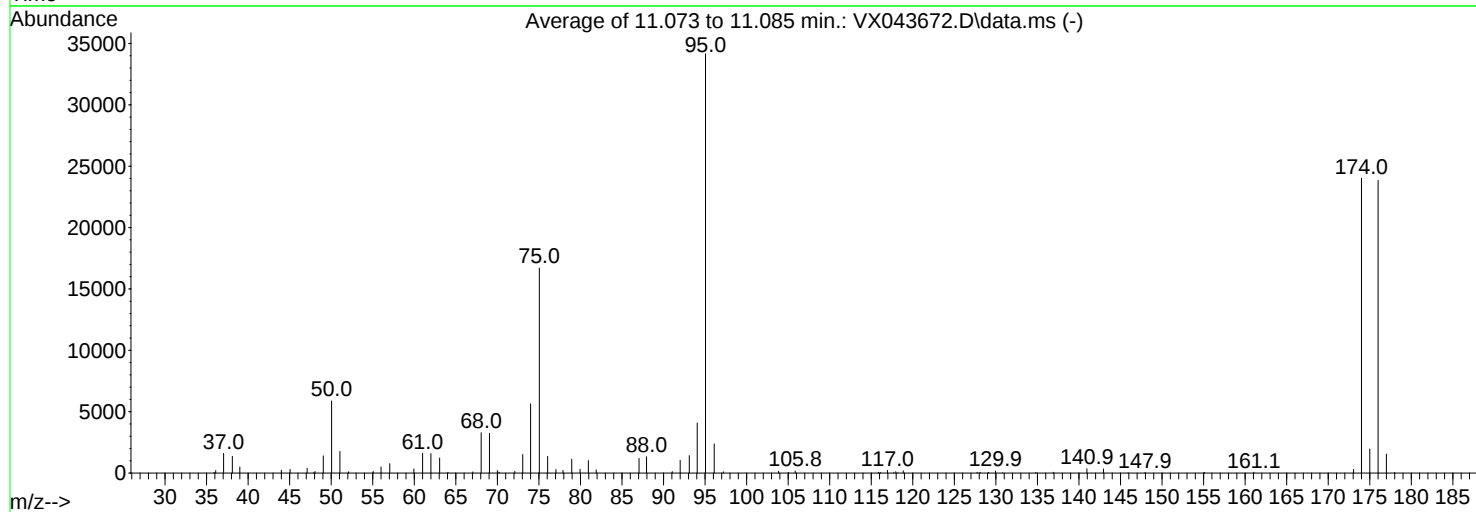


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110424\
Data File : VX043672.D
Acq On : 04 Nov 2024 09:42
Operator : JC/MD
Sample : BFB693
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB693

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Title : VOC Analysis
Last Update : Wed Nov 06 01:38:34 2024

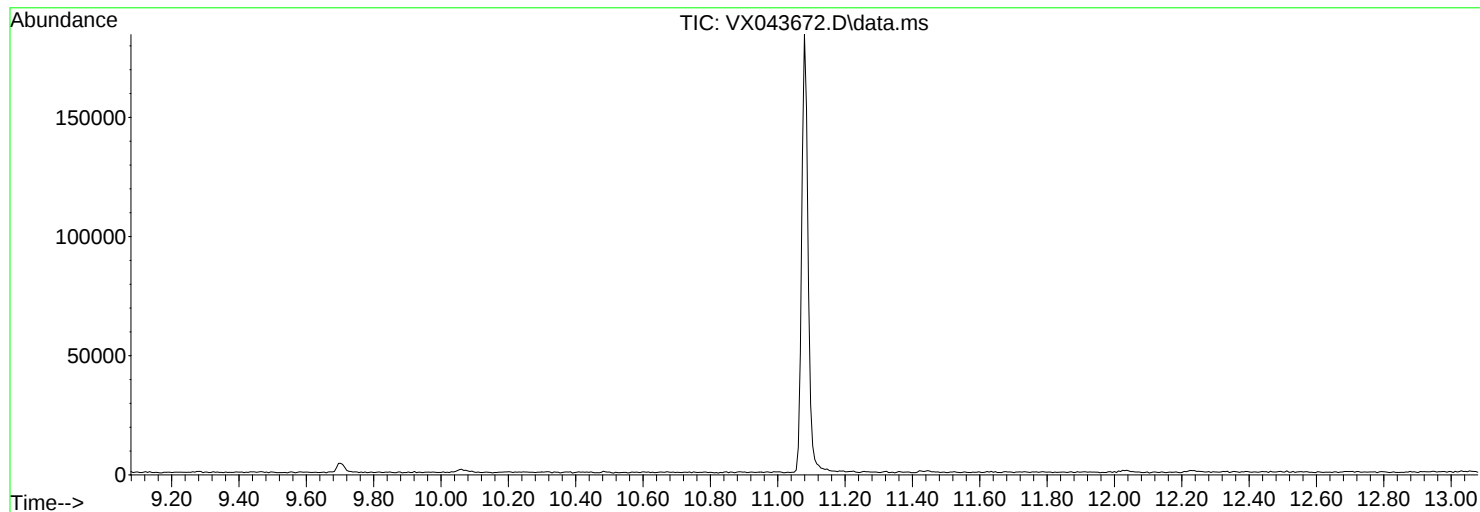

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	5877	PASS
75	95	30	80	48.9	16710	PASS
95	95	100	100	100.0	34165	PASS
96	95	5	9	7.0	2376	PASS
173	174	0.00	2	1.3	302	PASS
174	95	50	120	70.3	24024	PASS
175	174	5	9	8.1	1957	PASS
176	174	95	101	99.3	23856	PASS
177	176	5	9	6.5	1548	PASS

m/z	Abundance
39.00	74.0
40.00	717.0
44.00	321.0

Instrument :
MSVOA_X
ClientSampleId :
BFB693

m/z	Abundance
35.90	186.0
37.20	1748.0
38.10	1264.0
39.10	481.0
40.00	775.0
44.00	545.0
45.00	285.0
47.10	399.0
47.90	92.0
49.00	1187.0
50.10	5669.0
51.00	1845.0
52.00	93.0
55.10	154.0
56.10	522.0
57.10	857.0
60.00	370.0
61.00	1638.0
62.00	1518.0
63.10	1071.0
64.00	87.0
68.10	3078.0
69.00	2712.0
70.00	213.0
72.20	155.0
73.00	1408.0
74.00	5308.0
75.10	15140.0
76.00	1280.0
77.00	325.0
78.00	302.0
78.90	975.0
80.00	278.0
80.90	1018.0
81.90	150.0
87.10	1091.0
88.00	1234.0
91.00	97.0
92.00	936.0
93.10	1192.0
94.10	3340.0
95.00	29776.0
96.10	2128.0
97.20	141.0
103.80	85.0
106.00	128.0
115.80	71.0
117.00	260.0
117.70	121.0
118.20	70.0
118.80	189.0
127.70	78.0
128.10	52.0
129.10	59.0
130.00	176.0
141.10	325.0
143.00	288.0
173.10	285.0
174.00	17648.0
175.00	1475.0
176.00	17096.0
177.00	1002.0

Instrument :
MSVOA_X
ClientSampleId :
BFB693

m/z	Abundance
36.10	390.0
37.00	1620.0
38.10	1593.0
39.00	717.0
39.90	623.0
44.10	799.0
45.10	329.0
47.20	415.0
48.10	223.0
49.10	1790.0
50.10	6863.0
51.10	2055.0
52.10	119.0
55.00	159.0
55.90	557.0
57.00	919.0
60.00	343.0
61.00	1805.0
62.00	1885.0
63.00	1426.0
64.10	104.0
67.00	164.0
68.10	3868.0
69.10	4061.0
70.00	395.0
72.00	140.0
73.10	1821.0
74.00	6265.0
75.00	19544.0
76.10	1788.0
77.10	228.0
77.90	104.0
79.00	1280.0
80.00	314.0
81.00	1227.0
81.90	354.0
87.00	1380.0
87.90	1503.0
91.10	137.0
92.00	1120.0
93.10	1617.0
94.00	4876.0
95.00	40760.0
96.10	2838.0
97.20	119.0
103.80	198.0
105.10	99.0
105.80	221.0
115.90	81.0
116.90	174.0
117.90	212.0
118.80	199.0
128.10	144.0
129.10	120.0
129.80	138.0
130.80	59.0
134.80	102.0
136.90	124.0
140.90	336.0
143.00	342.0
145.90	63.0
147.90	92.0
155.10	61.0
161.10	120.0
173.00	288.0
174.00	28648.0
175.00	2228.0
176.00	28072.0
177.00	1916.0
178.00	61.0

Instrument :
MSVOA_X
ClientSampleId :
BFB693

m/z	Abundance
36.10	234.0
37.00	1448.0
38.10	1237.0
39.00	517.0
40.00	726.0
44.10	339.0
45.10	279.0
47.00	387.0
48.00	184.0
49.00	1232.0
50.00	5099.0
51.10	1388.0
52.20	134.0
55.10	94.0
56.00	434.0
57.10	542.0
59.90	297.0
61.00	1387.0
62.00	1355.0
63.10	1197.0
67.10	129.0
68.00	2924.0
69.10	2947.0
70.20	240.0
72.10	165.0
73.00	1312.0
74.00	5350.0
75.10	15445.0
76.10	1004.0
77.00	331.0
77.80	263.0
78.90	1143.0
79.80	348.0
81.00	811.0
81.90	285.0
87.10	1121.0
88.00	1267.0
91.10	128.0
92.00	1074.0
93.10	1456.0
94.10	4029.0
95.10	31960.0
96.10	2161.0
97.30	61.0
103.90	179.0
105.00	56.0
105.90	157.0
116.10	132.0
116.90	228.0
118.00	129.0
118.90	184.0
127.80	112.0
130.00	191.0
134.80	64.0
136.90	86.0
140.80	396.0
142.90	388.0
148.00	97.0
155.10	121.0
161.00	87.0
173.10	334.0
174.00	25776.0
175.00	2169.0
176.00	26400.0
177.00	1725.0
178.00	82.0

Instrument :
MSVOA_X
ClientSampleId :
BFB693