

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111823\
 Data File : VX038919.D
 Acq On : 18 Nov 2023 11:35
 Operator : JC/MD
 Sample : VX1118MBL01
 Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1118MBL01

Quant Time: Nov 20 04:31:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 16 22:59:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	108600	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	218394	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	215287	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	103309	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	82640	47.225	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	94.440%
35) Dibromofluoromethane	5.385	113	69450	44.031	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	88.060%
50) Toluene-d8	8.647	98	272248	45.113	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	90.220%#
62) 4-Bromofluorobenzene	11.079	95	111601	46.197	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	92.400%


Target Compounds			Qvalue			
3) Chloromethane	1.294	50	437	0.264	ug/l #	63
9) 1,1,2-Trichlorotrifluo...	2.331	101	303	0.226	ug/l #	51
11) Tert butyl alcohol	2.940	59	504	1.036	ug/l #	49
12) 1,1-Dichloroethene	2.319	96	296	0.219	ug/l #	67
13) Acrolein	2.209	56	102	0.396	ug/l #	1
15) Acrylonitrile	3.081	53	931	0.905	ug/l #	77
16) Acetone	2.380	43	2679	2.876	ug/l	96
17) Carbon Disulfide	2.514	76	3290	0.785	ug/l	98
20) Methylene Chloride	2.788	84	1548	0.922	ug/l #	83
21) trans-1,2-Dichloroethene	3.099	96	560	0.375	ug/l #	75
38) Carbon Tetrachloride	5.550	117	12055	5.770	ug/l #	16
44) Trichloroethene	7.135	130	756	0.465	ug/l	83
59) 2-Hexanone	9.445	43	716	0.297	ug/l	64
64) Tetrachloroethene	9.275	164	329	0.246	ug/l #	87
68) m/p-Xylenes	10.305	106	889	0.276	ug/l	82
76) 1,2,3-Trichloropropane	11.079	75	58152	22.561	ug/l #	39
78) n-propylbenzene	11.305	91	2200	0.222	ug/l	94
79) 2-Chlorotoluene	11.366	91	1192	0.203	ug/l	86
81) trans-1,4-Dichloro-2-b...	11.079	75	58152	50.043	ug/l #	5
82) 4-Chlorotoluene	11.463	91	1808	0.267	ug/l	97
85) sec-Butylbenzene	11.890	105	1761	0.202	ug/l	92
86) p-Isopropyltoluene	12.012	119	1714	0.245	ug/l #	65
87) 1,3-Dichlorobenzene	11.975	146	1072	0.303	ug/l	91
88) 1,4-Dichlorobenzene	11.975	146	1072	0.296	ug/l	90
89) n-Butylbenzene	12.335	91	3029	0.429	ug/l	86
91) 1,2-Dichlorobenzene	12.335	146	711	0.212	ug/l	85
93) 1,2,4-Trichlorobenzene	13.591	180	1295	0.575	ug/l	96
94) Hexachlorobutadiene	13.719	225	784	0.983	ug/l	91
95) Naphthalene	13.780	128	4991	0.595	ug/l	99
96) 1,2,3-Trichlorobenzene	13.963	180	1168	0.547	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111823\
Data File : VX038919.D
Acq On : 18 Nov 2023 11:35
Operator : JC/MD
Sample : VX1118MBL01
Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1118MBL01

Quant Time: Nov 20 04:31:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 16 22:59:22 2023
Response via : Initial Calibration




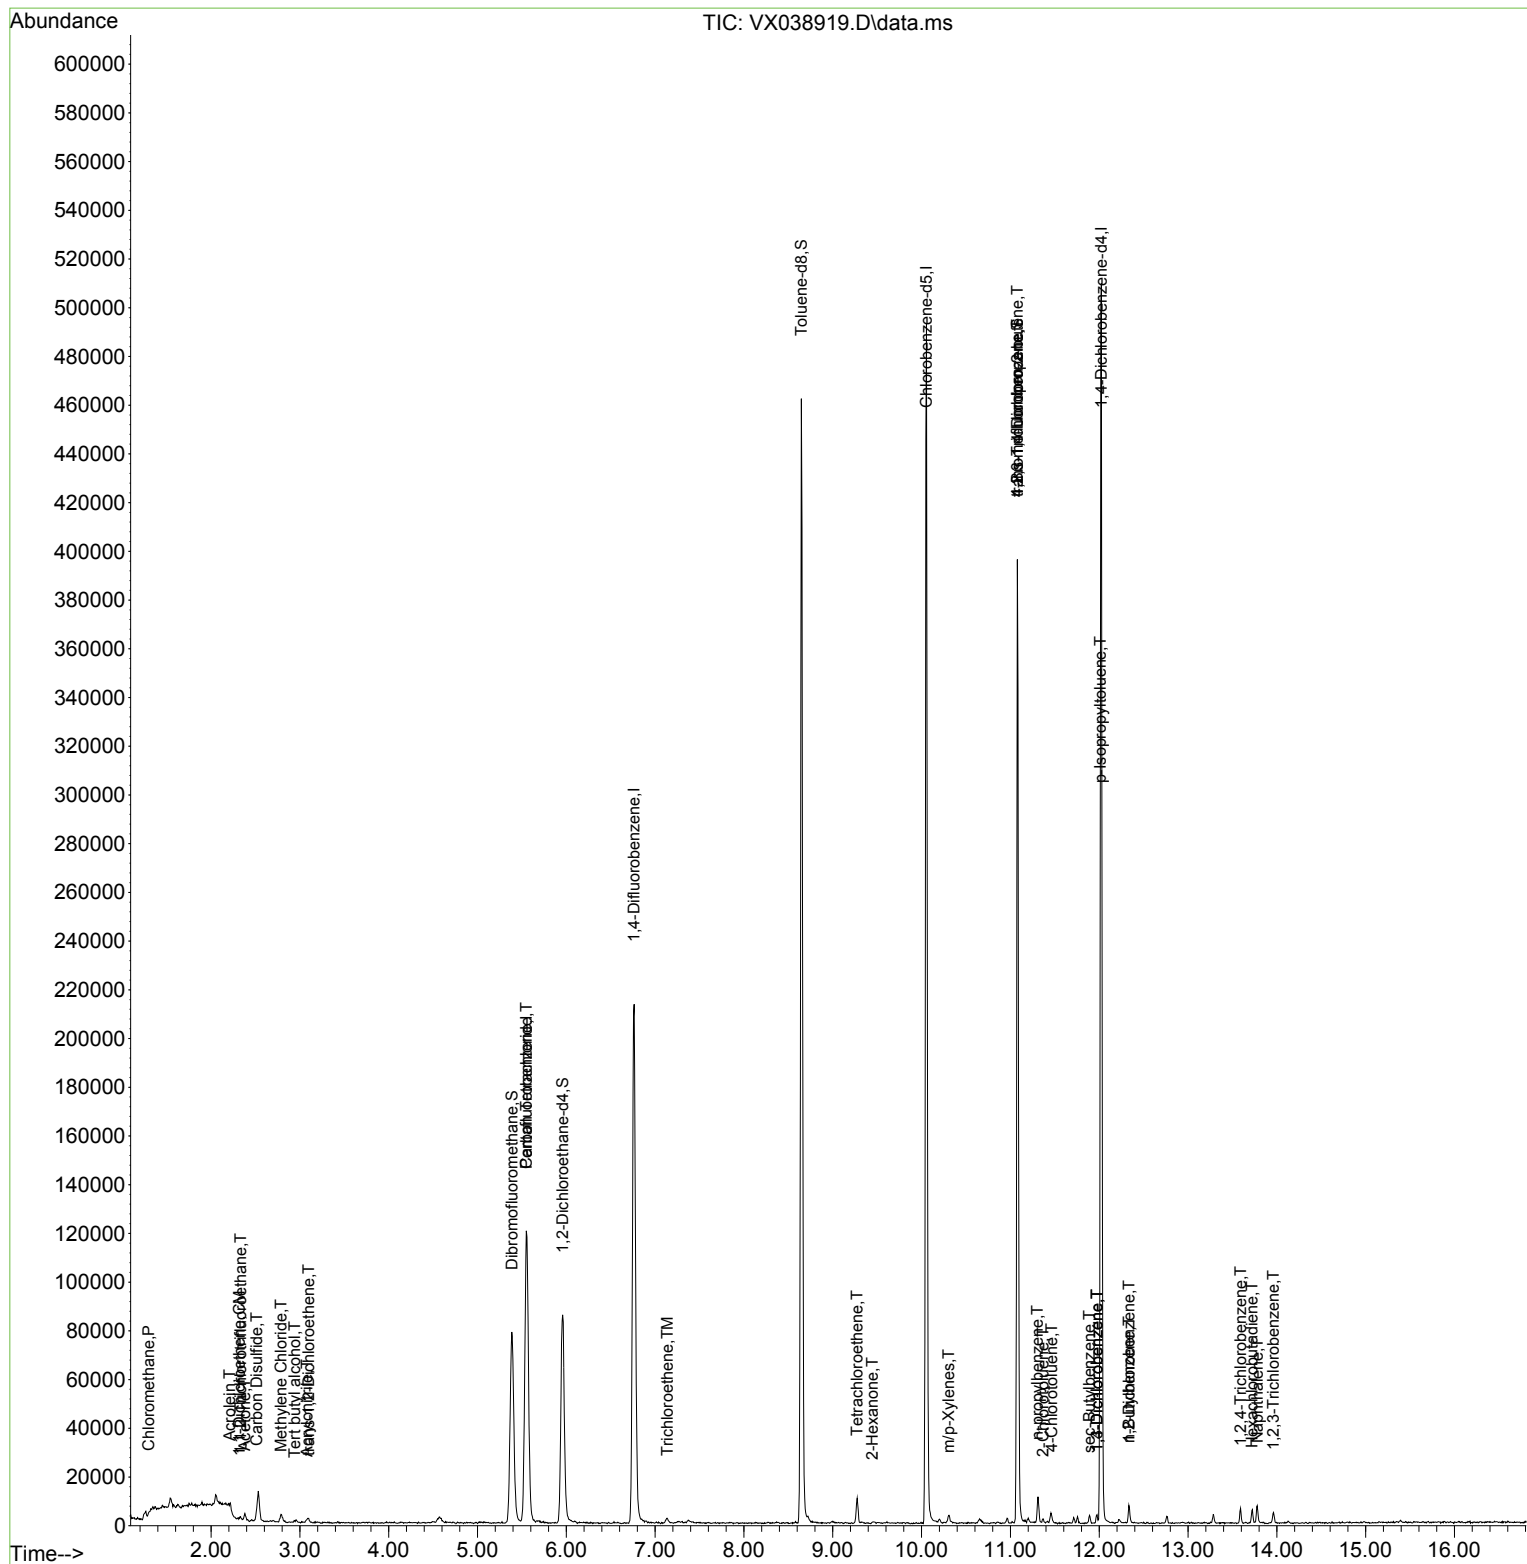




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35




Instrument :
MSVOA_X
ClientSampleId :
VX1118MBL01


Tgt Ion:168 Resp: 108600
Ion Ratio Lower Upper
168 100
99 63.0 56.6 85.0

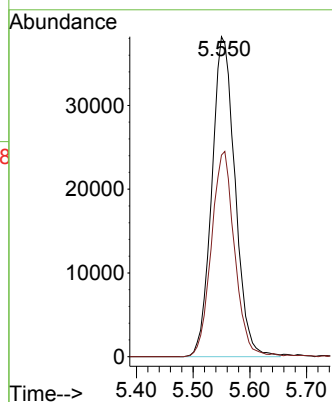

#3
Chloromethane
Concen: 0.264 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.000 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35

Tgt Ion: 50 Resp: 437
Ion Ratio Lower Upper
50 100
52 52.4 25.5 38.3#


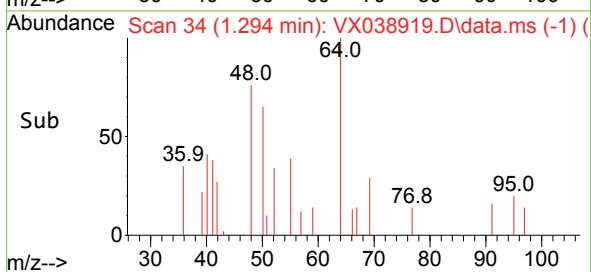
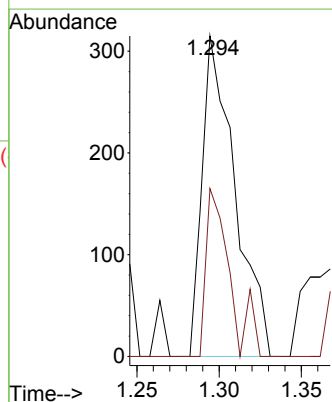



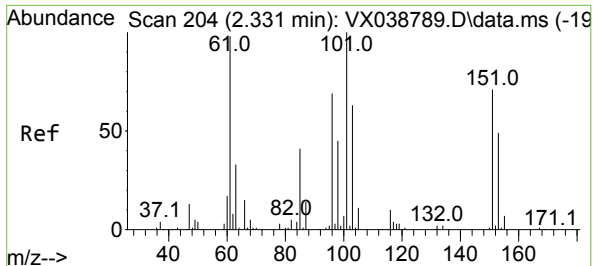

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.226 ug/l
RT: 2.331 min Scan# 204
Delta R.T. 0.000 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35




Instrument :
MSVOA_X
ClientSampleId :
VX1118MBL01


Tgt Ion:101 Resp: 303
Ion Ratio Lower Upper
101 100
85 84.2 37.0 55.6#
151 35.6 58.6 87.8#

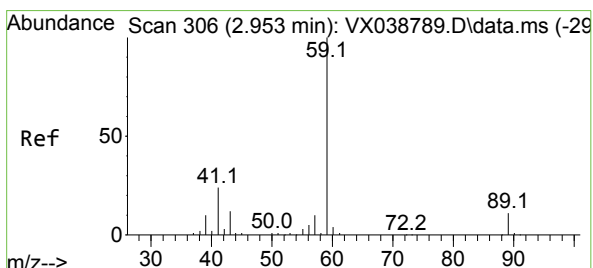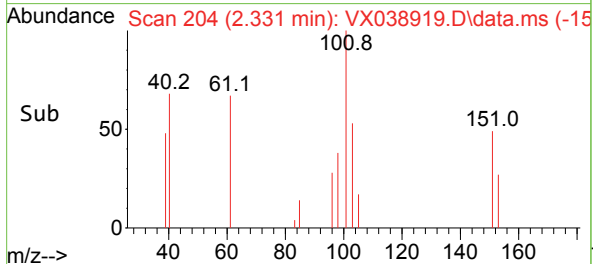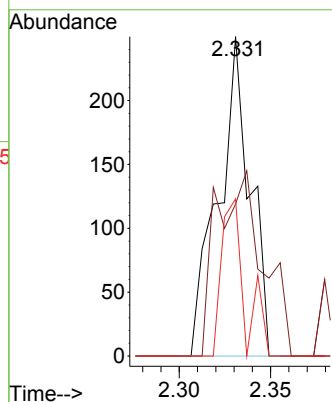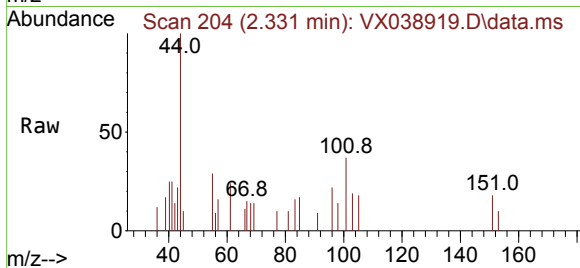

#11
Tert butyl alcohol
Concen: 1.036 ug/l
RT: 2.940 min Scan# 304
Delta R.T. -0.012 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35

Tgt Ion: 59 Resp: 504
Ion Ratio Lower Upper
59 100
57 25.2 6.0 9.0#


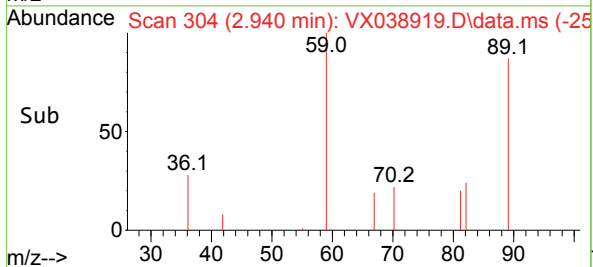
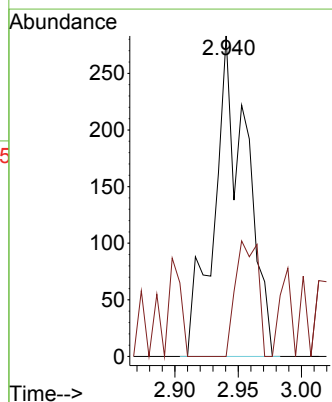
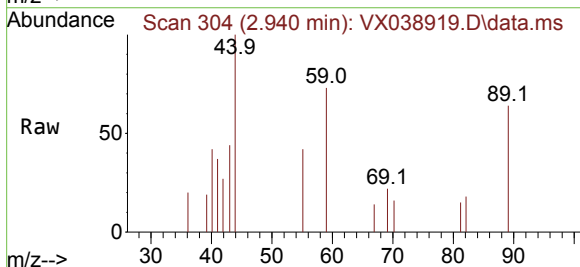




#12
1,1-Dichloroethene
Concen: 0.219 ug/l
RT: 2.319 min Scan# 20
Delta R.T. 0.000 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35




Instrument :
MSVOA_X
ClientSampleId :
VX1118MBL01


Tgt Ion: 96 Resp: 296
Ion Ratio Lower Upper
96 100
61 130.5 144.6 216.8#
98 83.8 50.4 75.6#

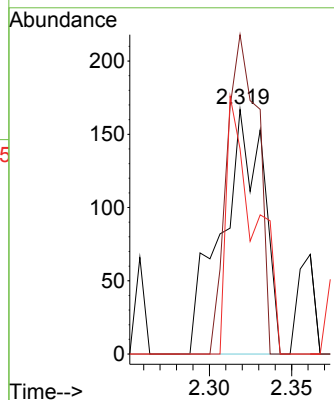

#13
Acrolein
Concen: 0.396 ug/l
RT: 2.209 min Scan# 184
Delta R.T. -0.024 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35

Tgt Ion: 56 Resp: 102
Ion Ratio Lower Upper
56 100
55 323.5 57.1 85.7#


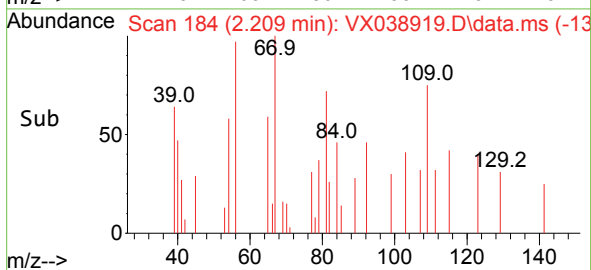
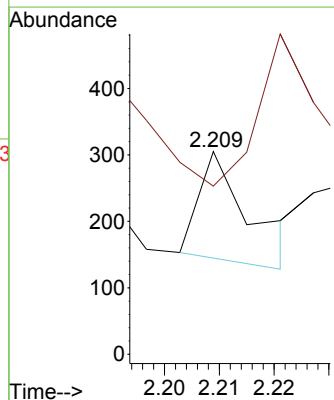





#15
Acrylonitrile
Concen: 0.905 ug/l
RT: 3.081 min Scan# 31
Delta R.T. 0.018 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35




Instrument :
MSVOA_X
ClientSampleId :
VX1118MBL01


Tgt Ion: 53 Resp: 931
Ion Ratio Lower Upper
53 100
52 57.9 66.0 99.0#
51 29.5 29.8 44.6#

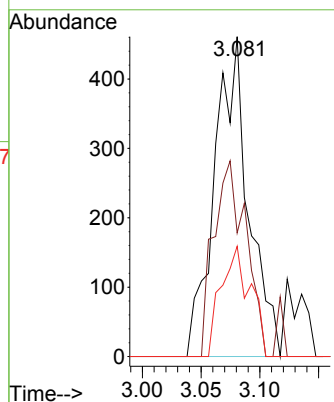

#16
Acetone
Concen: 2.876 ug/l
RT: 2.380 min Scan# 212
Delta R.T. 0.006 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35

Tgt Ion: 43 Resp: 2679
Ion Ratio Lower Upper
43 100
58 25.2 21.9 32.9


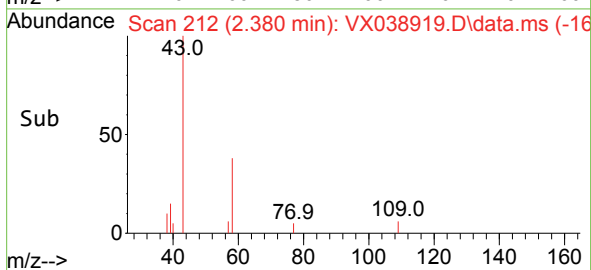
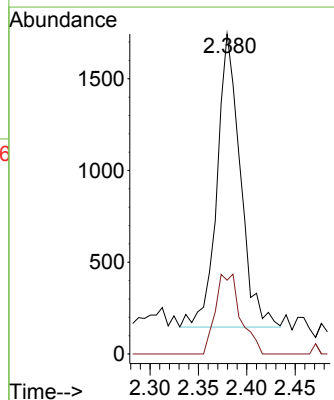





#17
Carbon Disulfide
Concen: 0.785 ug/l
RT: 2.514 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35




Instrument :
MSVOA_X
ClientSampleId :
VX1118MBL01


Tgt Ion: 76 Resp: 3290
Ion Ratio Lower Upper
76 100
78 8.2 7.0 10.6

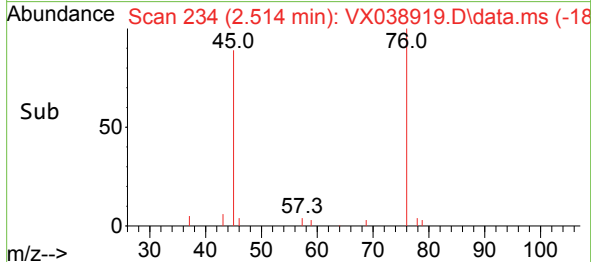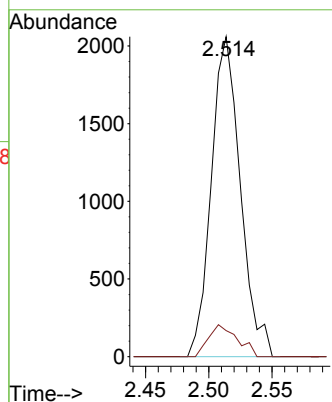

#20
Methylene Chloride
Concen: 0.922 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35

Tgt Ion: 84 Resp: 1548
Ion Ratio Lower Upper
84 100
49 104.8 103.6 155.4
51 53.2 33.8 50.6#
86 54.4 49.4 74.0


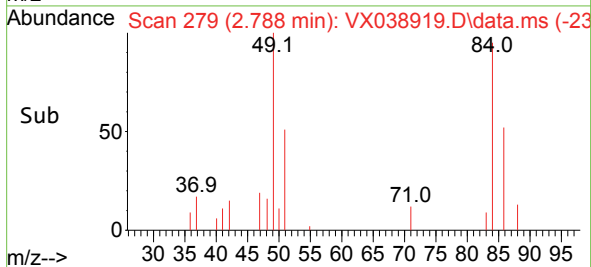
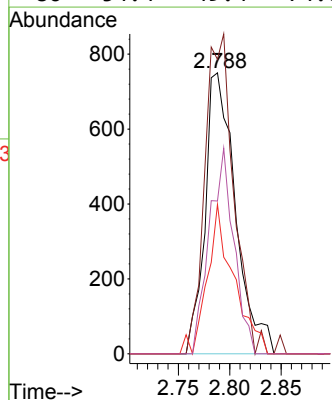
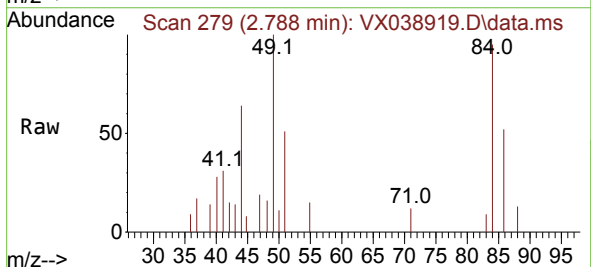




#21
trans-1,2-Dichloroethene
Concen: 0.375 ug/l
RT: 3.099 min Scan# 311
Delta R.T. 0.006 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35




Instrument :
MSVOA_X
ClientSampleId :
VX1118MBL01


Tgt Ion: 96 Resp: 560
Ion Ratio Lower Upper
96 100
61 116.0 119.2 178.8#
98 42.8 48.7 73.1#

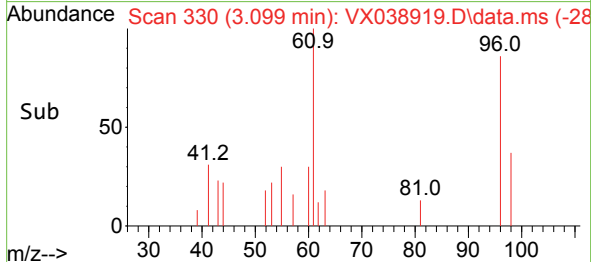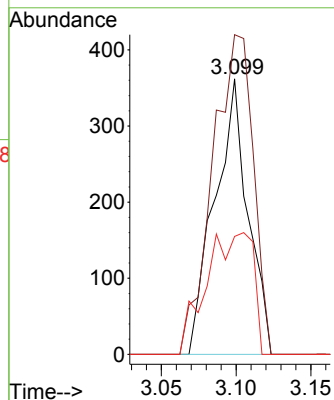

#33
1,2-Dichloroethane-d4
Concen: 47.225 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35

Tgt Ion: 65 Resp: 82640
Ion Ratio Lower Upper
65 100
67 52.3 0.0 100.2


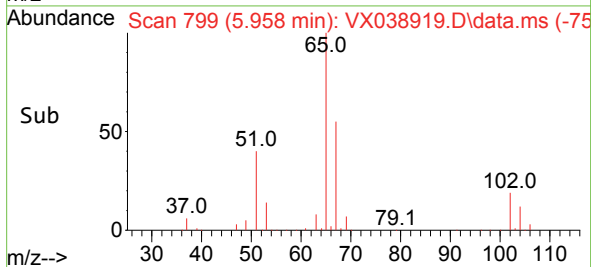
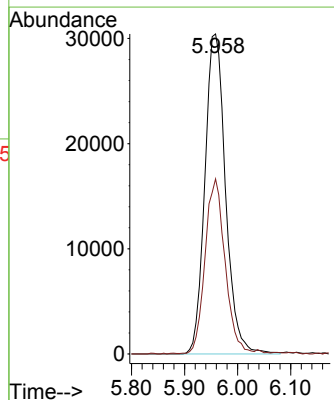
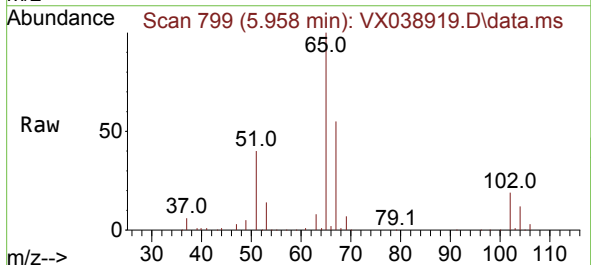




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35




Instrument :
MSVOA_X
ClientSampleId :
VX1118MBL01


Tgt Ion:114 Resp: 218394
Ion Ratio Lower Upper
114 100
63 20.5 0.0 45.0
88 16.2 0.0 36.6

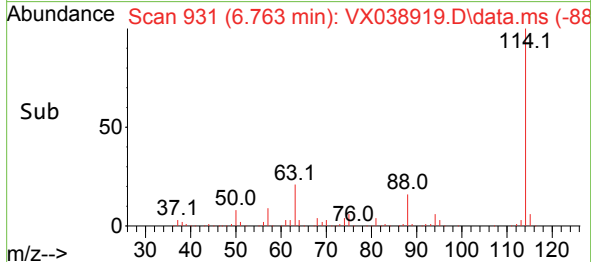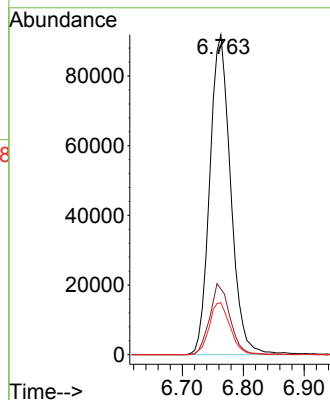

#35
Dibromofluoromethane
Concen: 44.031 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35


Tgt Ion:113 Resp: 69450
Ion Ratio Lower Upper
113 100
111 103.2 82.9 124.3
192 16.1 13.3 19.9

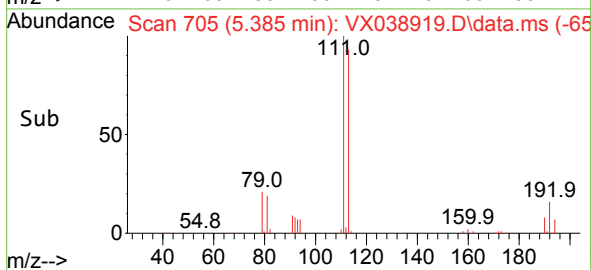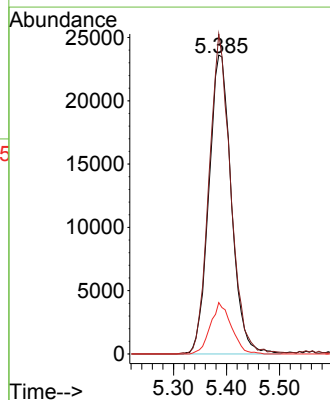






#38
Carbon Tetrachloride
Concen: 5.770 ug/l
RT: 5.550 min Scan# 711
Delta R.T. -0.128 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35

Instrument :
MSVOA_X
ClientSampleId :
VX1118MBL01



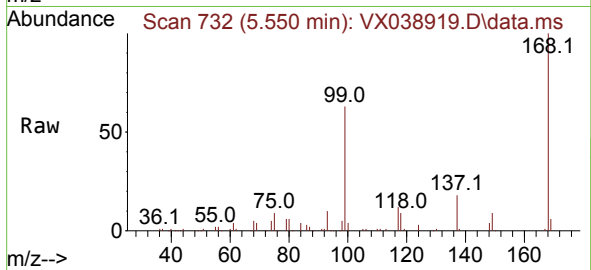



Tgt Ion:117 Resp: 12055
Ion Ratio Lower Upper
117 100
119 6.0 78.2 117.2#
121 0.0 24.4 36.6#

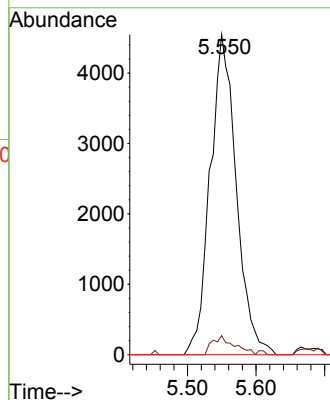

#44
Trichloroethene
Concen: 0.465 ug/l
RT: 7.135 min Scan# 992
Delta R.T. 0.012 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35

Tgt Ion:130 Resp: 756
Ion Ratio Lower Upper
130 100
95 85.2 0.0 204.4


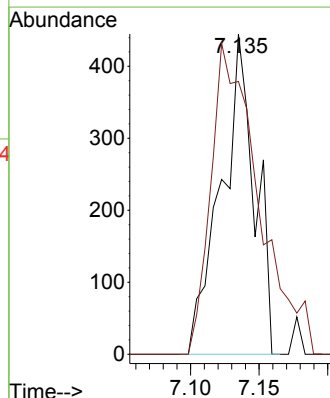

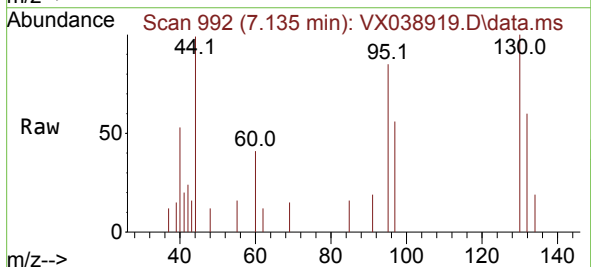




#50
Toluene-d8
Concen: 45.113 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35




Instrument :
MSVOA_X
ClientSampleId :
VX1118MBL01


Tgt Ion: 98 Resp: 272248
Ion Ratio Lower Upper
98 100
100 63.7 53.1 79.7

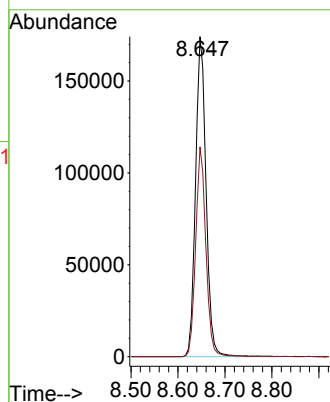

#59
2-Hexanone
Concen: 0.297 ug/l
RT: 9.445 min Scan# 1371
Delta R.T. 0.018 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35

Tgt Ion: 43 Resp: 716
Ion Ratio Lower Upper
43 100
58 27.0 26.2 78.5


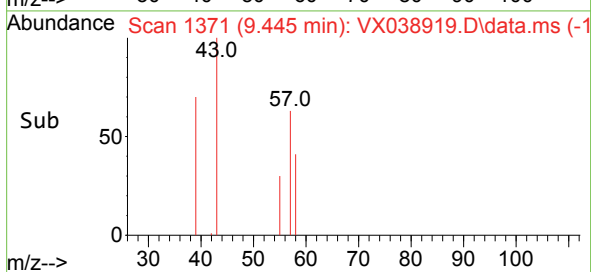
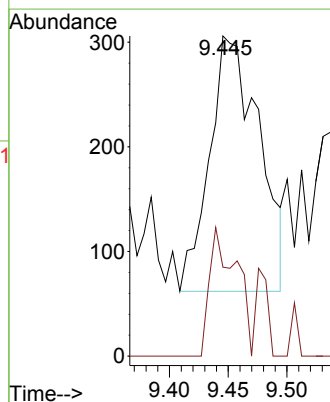





#62
4-Bromofluorobenzene
Concen: 46.197 ug/l
RT: 11.079 min Scan# 111601
Delta R.T. 0.000 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35




Instrument :
MSVOA_X
ClientSampleId :
VX1118MBL01


Tgt Ion: 95 Resp: 111601
Ion Ratio Lower Upper
95 100
174 67.3 0.0 135.6
176 65.6 0.0 131.0

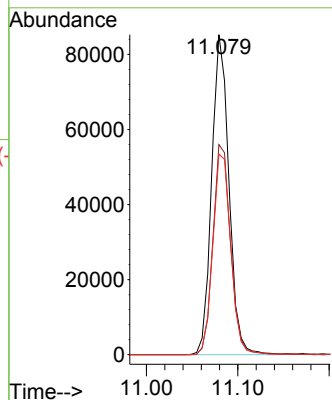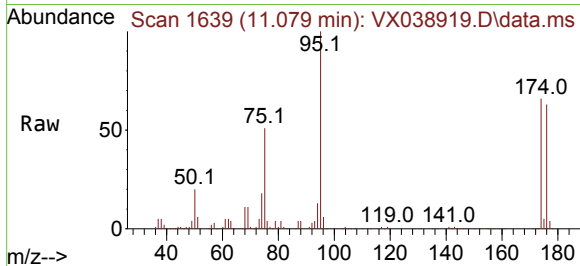

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35

Tgt Ion: 117 Resp: 215287
Ion Ratio Lower Upper
117 100
82 58.7 46.2 69.4
119 32.4 25.5 38.3


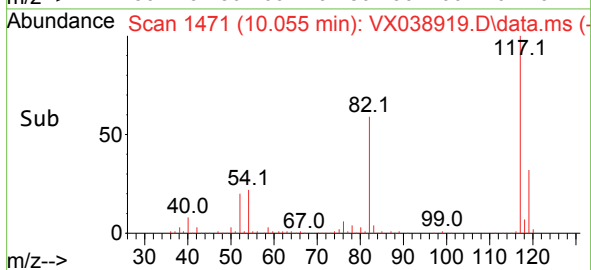
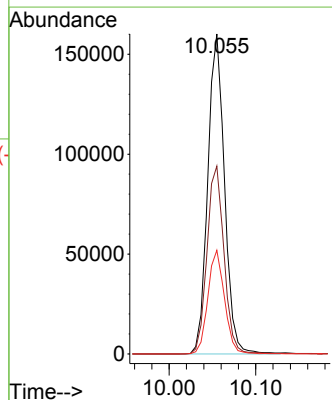
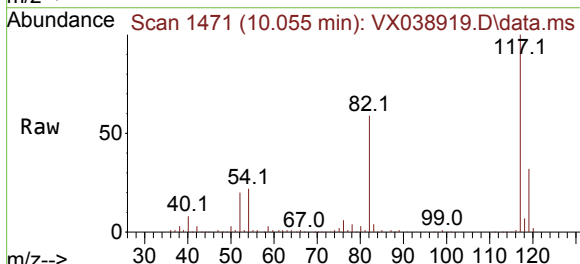




#64
Tetrachloroethene
Concen: 0.246 ug/l
RT: 9.275 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35




Instrument :
MSVOA_X
ClientSampleId :
VX1118MBL01


Tgt Ion:164 Resp: 329
Ion Ratio Lower Upper
164 100
166 117.1 102.7 154.1
129 110.7 80.4 120.6
131 116.7 76.5 114.7#

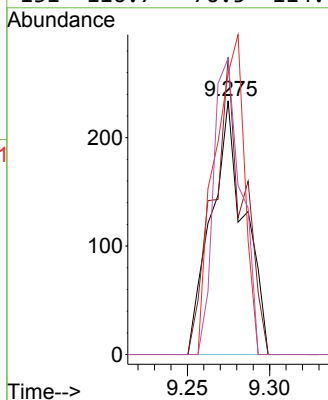

#68
m/p-Xylenes
Concen: 0.276 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35

Tgt Ion:106 Resp: 889
Ion Ratio Lower Upper
106 100
91 178.4 165.5 248.3


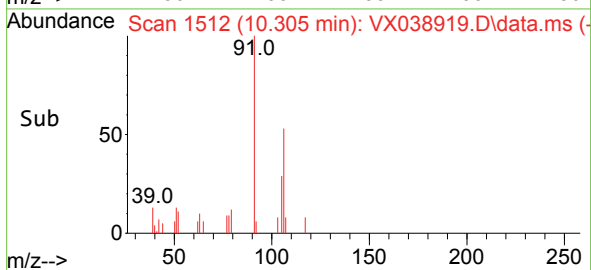
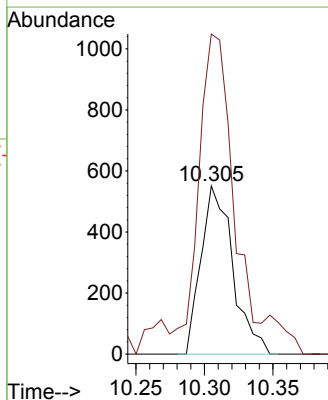
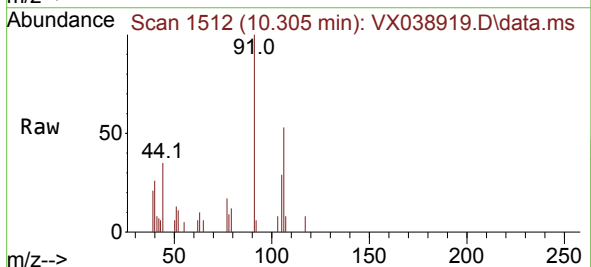




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VX038919.D
 Acq: 18 Nov 2023 11:35




Instrument :
 MSVOA_X
 ClientSampleId :
 VX1118MBL01


Tgt Ion:152 Resp: 103309
 Ion Ratio Lower Upper
 152 100
 115 66.6 43.3 129.9
 150 157.0 0.0 345.0

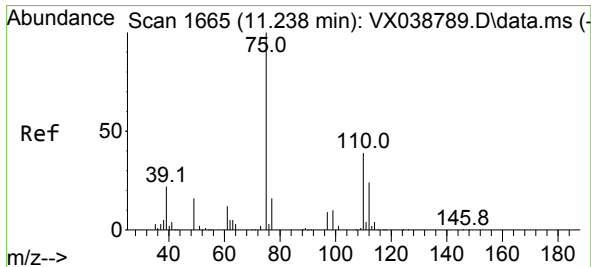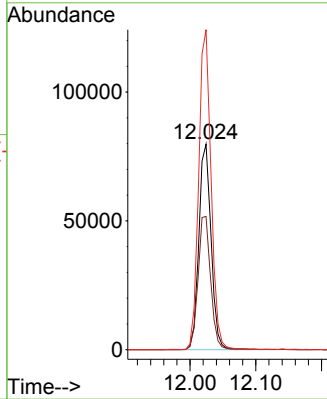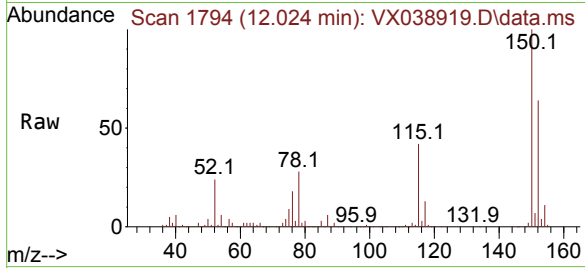

#76
 1,2,3-Trichloropropane
 Concen: 22.561 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.158 min
 Lab File: VX038919.D
 Acq: 18 Nov 2023 11:35

Tgt Ion: 75 Resp: 58152
 Ion Ratio Lower Upper
 75 100
 77 1.3 19.1 57.5#

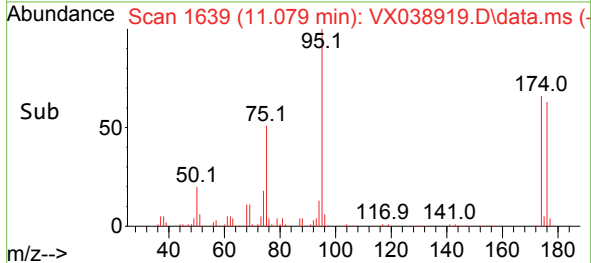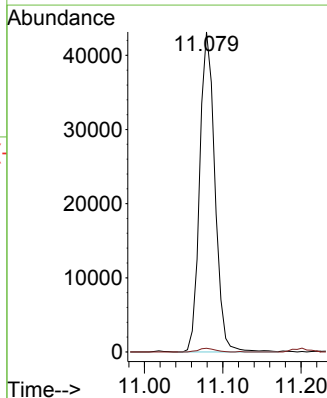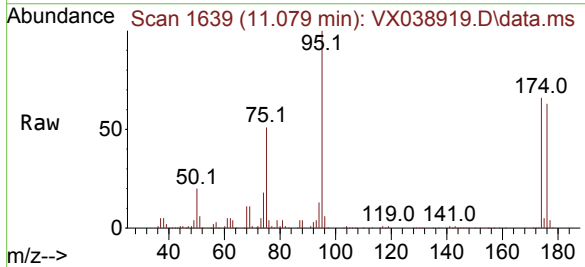



#78

n-propylbenzene

Concen: 0.222 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX038919.D

Acq: 18 Nov 2023 11:35

Instrument :

MSVOA_X

ClientSampleId :





VX1118MBL01

Tgt Ion: 91 Resp: 2200

Ion Ratio Lower Upper

91 100

120 19.9 11.5 34.4

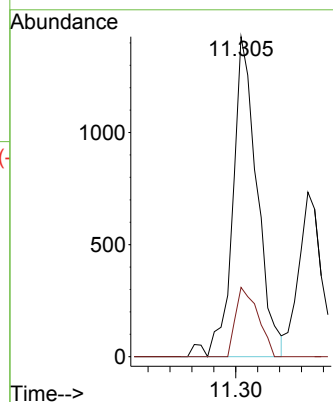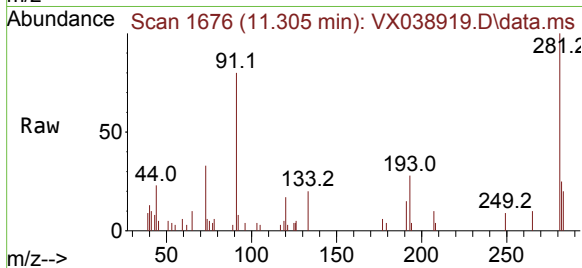

#79

2-Chlorotoluene

Concen: 0.203 ug/l

RT: 11.366 min Scan# 1686

Delta R.T. 0.000 min

Lab File: VX038919.D




Acq: 18 Nov 2023 11:35


Tgt Ion: 91 Resp: 1192

Ion Ratio Lower Upper

91 100

126 24.5 16.3 48.8


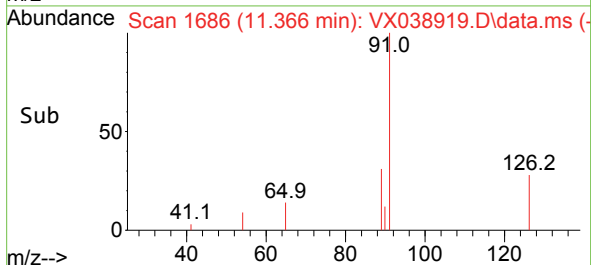
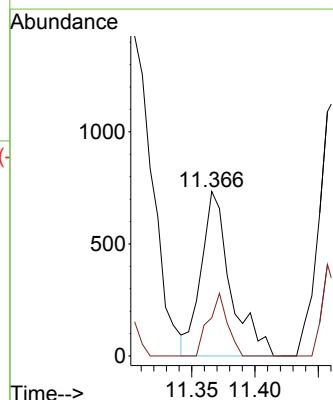
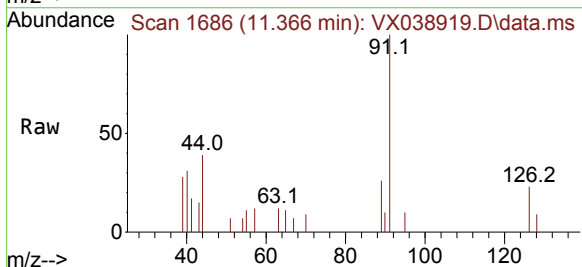




#81
trans-1,4-Dichloro-2-butene
Concen: 50.043 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35




Instrument :
MSVOA_X
ClientSampleId :
VX1118MBL01


Tgt Ion: 75 Resp: 58152
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

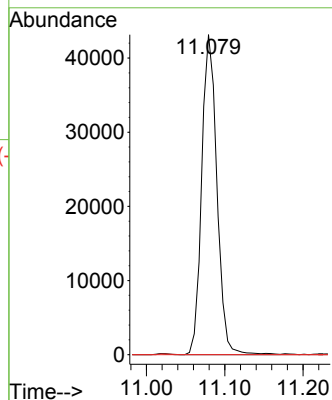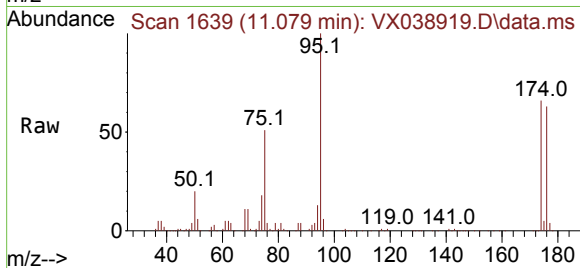

#82
4-Chlorotoluene
Concen: 0.267 ug/l
RT: 11.463 min Scan# 1702
Delta R.T. 0.012 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35

Tgt Ion: 91 Resp: 1808
Ion Ratio Lower Upper
91 100
126 27.0 14.2 42.6


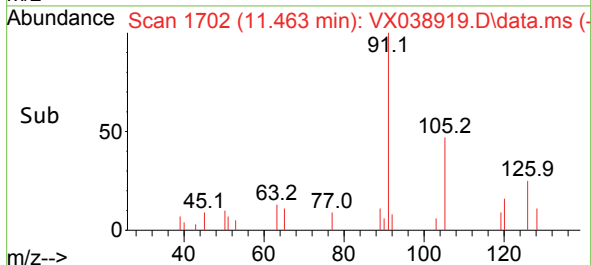
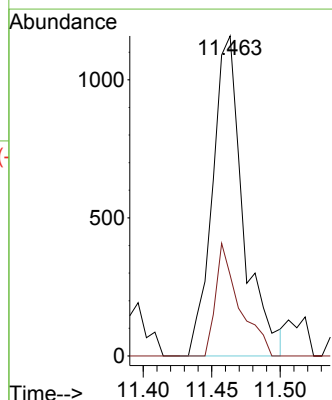
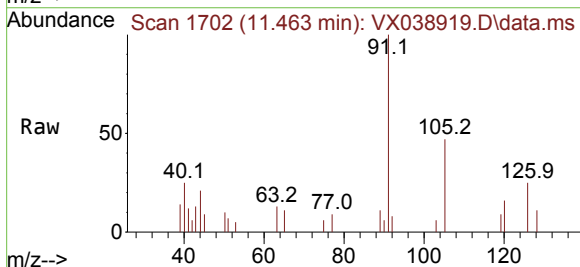




#85
 sec-Butylbenzene
 Concen: 0.202 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. 0.000 min
 Lab File: VX038919.D
 Acq: 18 Nov 2023 11:35




Instrument :
 MSVOA_X
 ClientSampleId :
 VX1118MBL01


Tgt Ion:105 Resp: 1761
 Ion Ratio Lower Upper
 105 100
 134 16.0 9.8 29.4

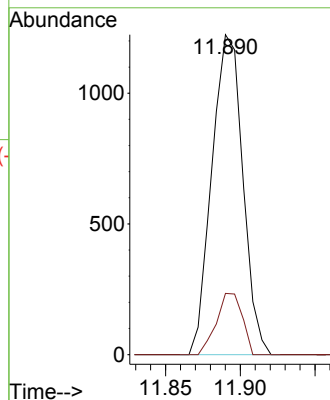

#86
 p-Isopropyltoluene
 Concen: 0.245 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. 0.006 min
 Lab File: VX038919.D
 Acq: 18 Nov 2023 11:35

Tgt Ion:119 Resp: 1714
 Ion Ratio Lower Upper
 119 100
 134 30.5 12.8 38.3
 91 56.7 13.1 39.3#

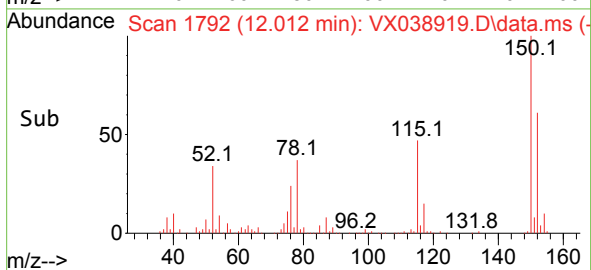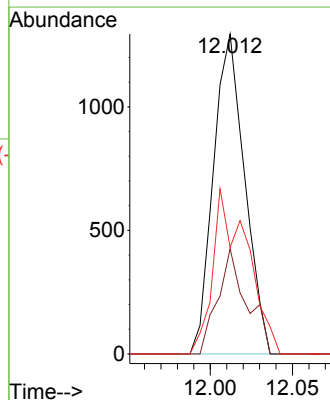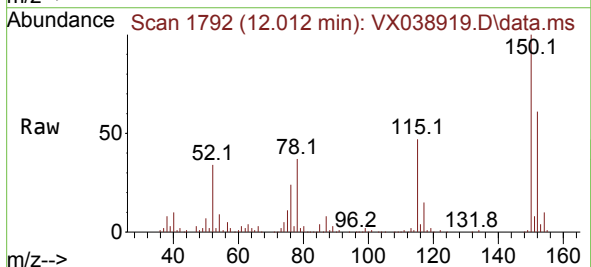



#87

1,3-Dichlorobenzene

Concen: 0.303 ug/l

RT: 11.975 min Scan# 1786

Delta R.T. 0.006 min

Lab File: VX038919.D

Acq: 18 Nov 2023 11:35

Instrument :

MSVOA_X

ClientSampleId :

VX1118MBL01





Tgt Ion:146 Resp: 1072

Ion Ratio Lower Upper

146 100

111 54.3 22.1 66.1

148 60.4 31.8 95.3

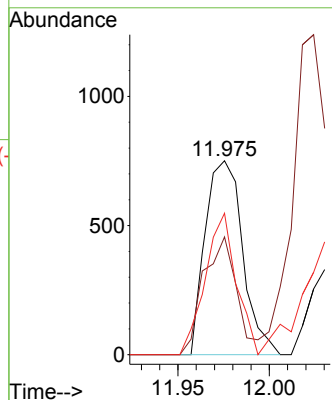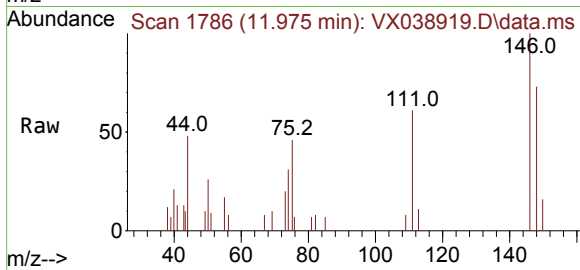

#88

1,4-Dichlorobenzene

Concen: 0.296 ug/l

RT: 11.975 min Scan# 1786

Delta R.T. -0.061 min

Lab File: VX038919.D

Acq: 18 Nov 2023 11:35




Tgt Ion:146 Resp: 1072


Ion Ratio Lower Upper

146 100

111 54.3 21.3 63.7

148 60.4 31.8 95.4

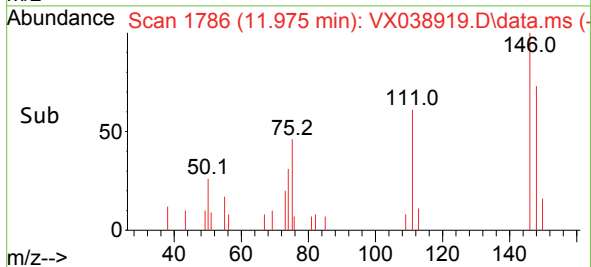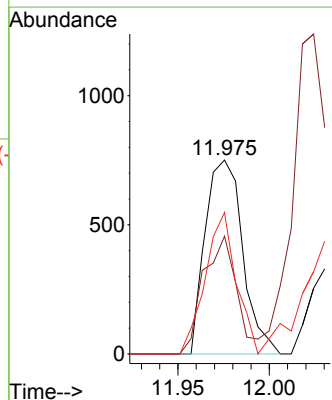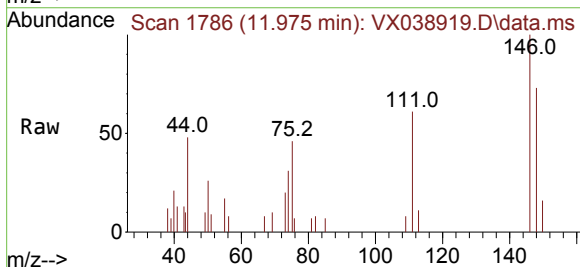



#89

n-Butylbenzene

Concen: 0.429 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.006 min

Lab File: VX038919.D

Acq: 18 Nov 2023 11:35

Instrument :

MSVOA_X

ClientSampleId :

VX1118MBL01





Tgt Ion: 91 Resp: 3029

Ion Ratio Lower Upper

91 100

92 41.3 27.4 82.0

134 22.5 12.6 37.8

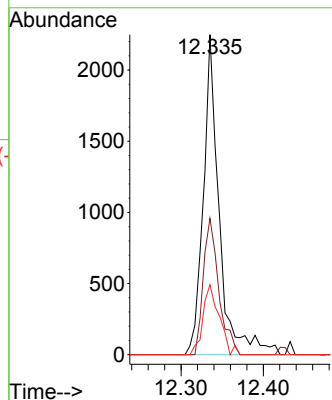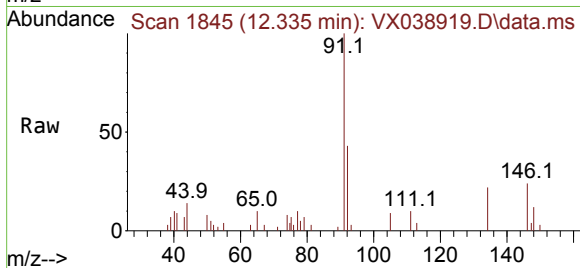

#91

1,2-Dichlorobenzene

Concen: 0.212 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.000 min

Lab File: VX038919.D

Acq: 18 Nov 2023 11:35




Tgt Ion:146 Resp: 711


Ion Ratio Lower Upper

146 100

111 55.3 22.4 67.0

148 74.1 31.6 95.0

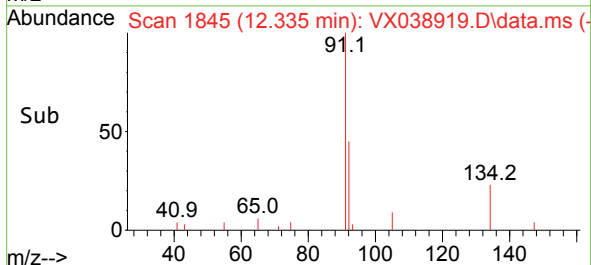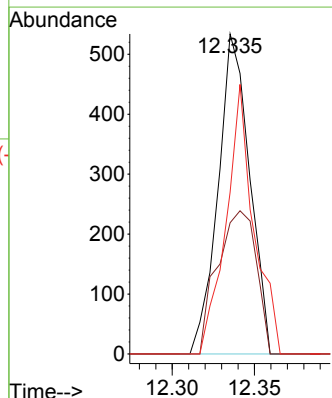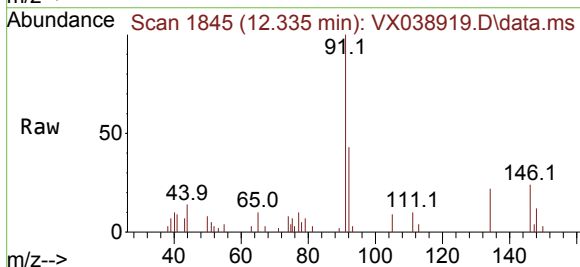



#93

1,2,4-Trichlorobenzene

Concen: 0.575 ug/l

RT: 13.591 min Scan# 2050

Delta R.T. 0.006 min

Lab File: VX038919.D

Acq: 18 Nov 2023 11:35

Instrument :

MSVOA_X

ClientSampleId :

VX1118MBL01





Tgt Ion:180 Resp: 1295

Ion Ratio Lower Upper

180 100

182 100.4 48.3 144.8

145 34.6 18.0 54.0

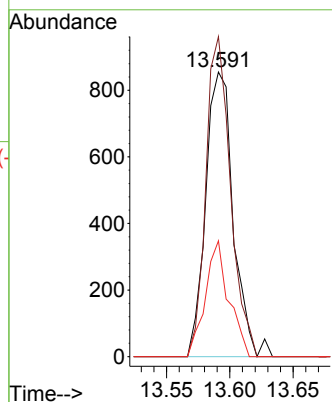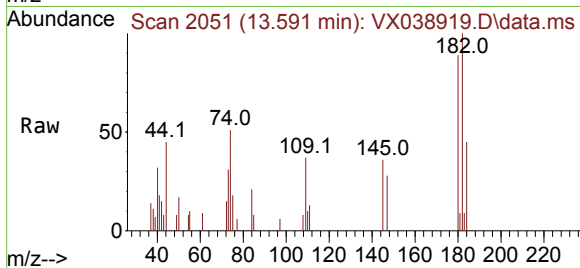

#94

Hexachlorobutadiene

Concen: 0.983 ug/l

RT: 13.719 min Scan# 2072

Delta R.T. -0.006 min

Lab File: VX038919.D

Acq: 18 Nov 2023 11:35




Tgt Ion:225 Resp: 784


Ion Ratio Lower Upper

225 100

223 55.7 31.1 93.2

227 57.5 32.5 97.5


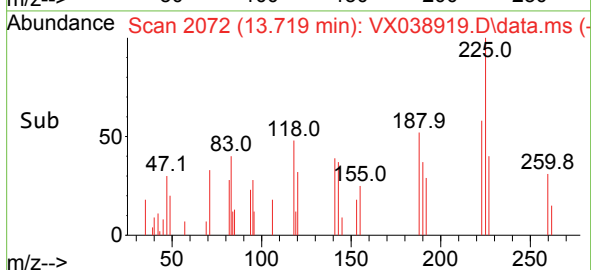
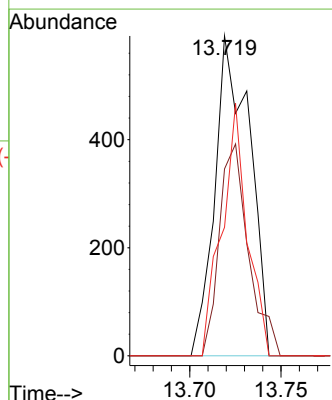
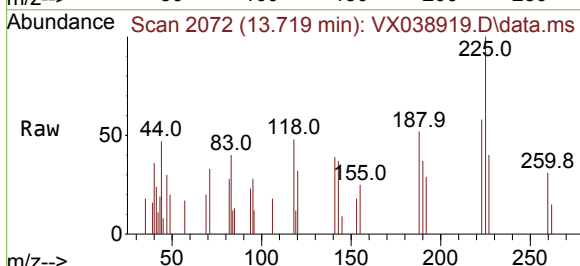




#95
Naphthalene
Concen: 0.595 ug/l
RT: 13.780 min Scan# 2081
Delta R.T. 0.006 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35

Instrument :
MSVOA_X
ClientSampleId :
VX1118MBL01

Tgt Ion:128	Resp:	4991
Ion Ratio	Lower	Upper
128	100	
127	13.2	10.3 15.5
129	11.6	8.8 13.2

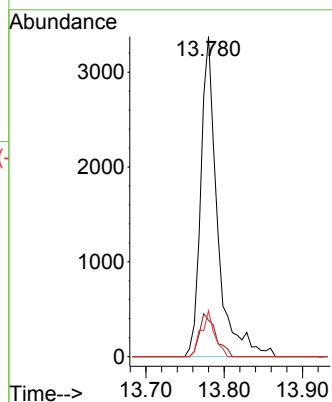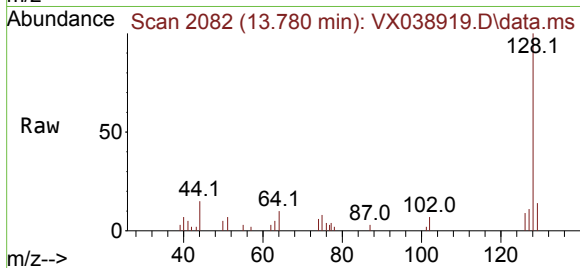

#96
1,2,3-Trichlorobenzene
Concen: 0.547 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. 0.006 min
Lab File: VX038919.D
Acq: 18 Nov 2023 11:35

Tgt Ion:180	Resp:	1168
Ion Ratio	Lower	Upper
180	100	
182	94.2	46.9 140.6
145	34.3	17.8 53.5

