

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX111823\  
 Data File : VX038923.D  
 Acq On : 18 Nov 2023 13:12  
 Operator : JC/MD  
 Sample : 05404-21DL 5X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 RE125D3-20231109DL


Quant Time: Nov 20 04:33:46 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X111623W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Nov 16 22:59:22 2023  
 Response via : Initial Calibration

| Compound                      | R.T.           | QIon | Response   | Conc    | Units  | Dev(Min) |
|-------------------------------|----------------|------|------------|---------|--------|----------|
| -----                         |                |      |            |         |        |          |
| Internal Standards            |                |      |            |         |        |          |
| 1) Pentafluorobenzene         | 5.550          | 168  | 102125     | 50.000  | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 6.763          | 114  | 202031     | 50.000  | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 10.055         | 117  | 201777     | 50.000  | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 12.024         | 152  | 97825      | 50.000  | ug/l   | 0.00     |
|                               |                |      |            |         |        |          |
| System Monitoring Compounds   |                |      |            |         |        |          |
| 33) 1,2-Dichloroethane-d4     | 5.952          | 65   | 78396      | 47.640  | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 78 - 117 |      | Recovery = | 95.280% |        |          |
| 35) Dibromofluoromethane      | 5.385          | 113  | 65614      | 44.968  | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 75 - 124 |      | Recovery = | 89.940% |        |          |
| 50) Toluene-d8                | 8.647          | 98   | 257829     | 46.184  | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 92 - 112 |      | Recovery = | 92.360% |        |          |
| 62) 4-Bromofluorobenzene      | 11.079         | 95   | 107295     | 48.012  | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 83 - 123 |      | Recovery = | 96.020% |        |          |
|                               |                |      |            |         |        |          |
| Target Compounds              |                |      |            |         | Qvalue |          |
| 6) Chloroethane               | 1.685          | 64   | 207        | 0.242   | ug/l # | 15       |
| 9) 1,1,2-Trichlorotrifluo...  | 2.331          | 101  | 35610      | 28.245  | ug/l   | 97       |
| 11) Tert butyl alcohol        | 2.941          | 59   | 1074       | 2.347   | ug/l   | 98       |
| 12) 1,1-Dichloroethene        | 2.325          | 96   | 633        | 0.497   | ug/l # | 30       |
| 13) Acrolein                  | 2.227          | 56   | 57         | 0.235   | ug/l # | 14       |
| 15) Acrylonitrile             | 3.075          | 53   | 410        | 0.424   | ug/l # | 80       |
| 16) Acetone                   | 2.374          | 43   | 752        | 0.858   | ug/l   | 95       |
| 17) Carbon Disulfide          | 2.514          | 76   | 1790       | 0.454   | ug/l   | 97       |
| 18) Methyl Acetate            | 2.703          | 43   | 849        | 0.204   | ug/l # | 66       |
| 20) Methylene Chloride        | 2.788          | 84   | 5389       | 3.413   | ug/l # | 96       |
| 27) cis-1,2-Dichloroethene    | 4.489          | 96   | 716        | 0.437   | ug/l   | 89       |
| 36) 1,1-Dichloropropene       | 5.550          | 75   | 9185       | 4.392   | ug/l # | 52       |
| 37) Ethyl Acetate             | 4.690          | 43   | 600        | 0.220   | ug/l # | 69       |
| 38) Carbon Tetrachloride      | 5.556          | 117  | 11709      | 6.058   | ug/l # | 13       |
| 44) Trichloroethene           | 7.129          | 130  | 34610      | 22.988  | ug/l   | 89       |
| 49) 1,4-Dioxane               | 7.684          | 88   | 43         | 1.052   | ug/l # | 12       |
| 60) Dibromochloromethane      | 9.275          | 129  | 3052       | 1.874   | ug/l # | 11       |
| 64) Tetrachloroethene         | 9.275          | 164  | 2974       | 2.371   | ug/l   | 98       |
| 76) 1,2,3-Trichloropropane    | 11.079         | 75   | 55578      | 22.771  | ug/l # | 39       |
| 81) trans-1,4-Dichloro-2-b... | 11.079         | 75   | 55578      | 50.509  | ug/l # | 5        |
| 89) n-Butylbenzene            | 12.335         | 91   | 1638       | 0.245   | ug/l   | 86       |
| 93) 1,2,4-Trichlorobenzene    | 13.591         | 180  | 725        | 0.340   | ug/l   | 95       |
| 94) Hexachlorobutadiene       | 13.725         | 225  | 352        | 0.466   | ug/l   | 91       |
| 95) Naphthalene               | 13.780         | 128  | 2703       | 0.340   | ug/l # | 91       |
| 96) 1,2,3-Trichlorobenzene    | 13.969         | 180  | 635        | 0.314   | ug/l   | 91       |
| -----                         |                |      |            |         |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Nov 20 04:33:46 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X111623W.M  
Quant Title : SW846 8260  
QLast Update : Thu Nov 16 22:59:22 2023  
Response via : Initial Calibration









#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 71  
Delta R.T. -0.000 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE125D3-20231109DL


Tgt Ion:168 Resp: 102125  
Ion Ratio Lower Upper  
168 100  
99 64.1 56.6 85.0

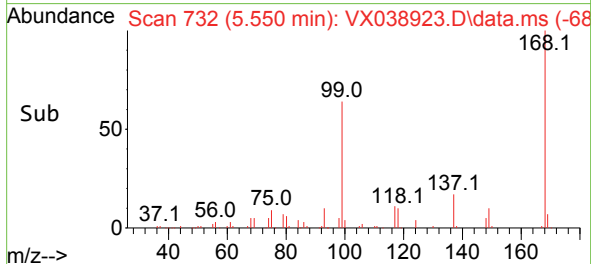

#6  
Chloroethane  
Concen: 0.242 ug/l  
RT: 1.685 min Scan# 98  
Delta R.T. -0.000 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12

Tgt Ion: 64 Resp: 207  
Ion Ratio Lower Upper  
64 100  
66 78.7 25.1 37.7#


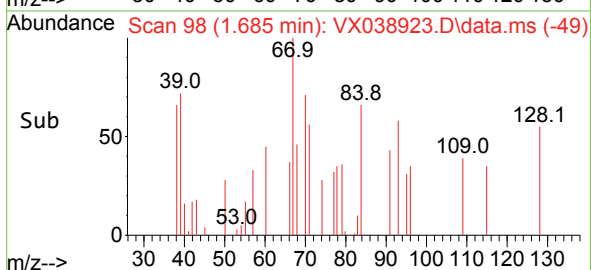




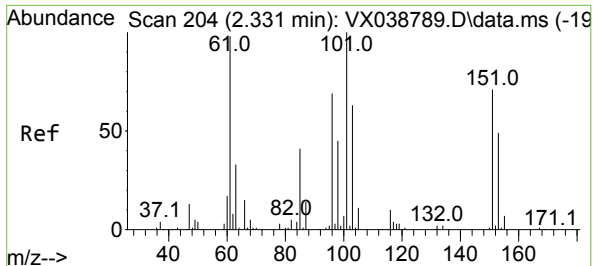

#9  
1,1,2-Trichlorotrifluoroethane  
Concen: 28.245 ug/l  
RT: 2.331 min Scan# 204  
Delta R.T. 0.000 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE125D3-20231109DL


Tgt Ion:101 Resp: 35610  
Ion Ratio Lower Upper  
101 100  
85 48.1 37.0 55.6  
151 70.4 58.6 87.8

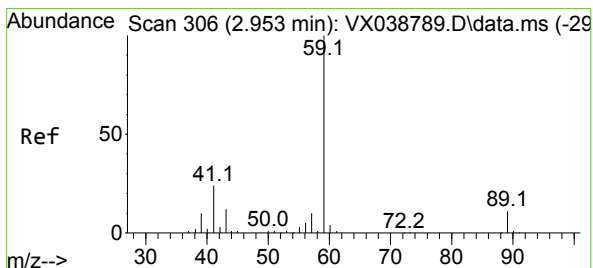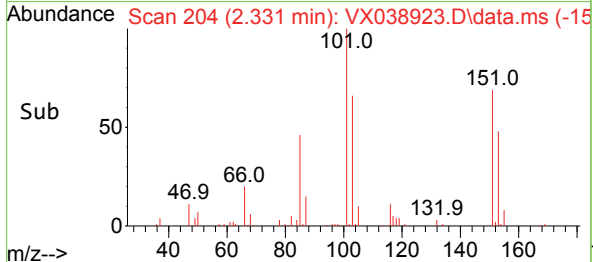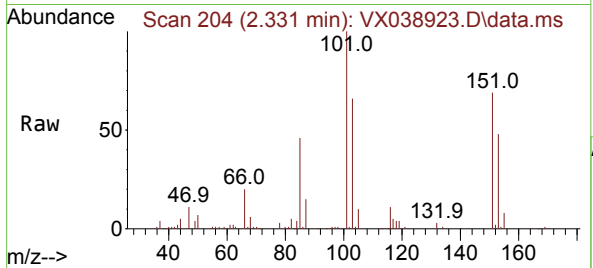

#11  
Tert butyl alcohol  
Concen: 2.347 ug/l  
RT: 2.941 min Scan# 304  
Delta R.T. -0.012 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12

Tgt Ion: 59 Resp: 1074  
Ion Ratio Lower Upper  
59 100  
57 8.1 6.0 9.0


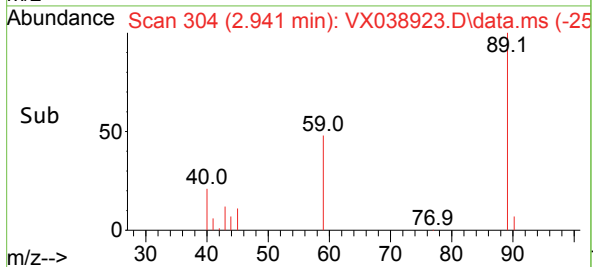

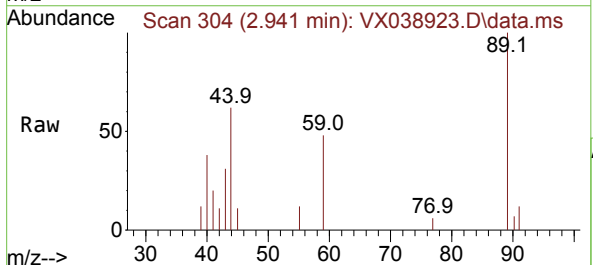


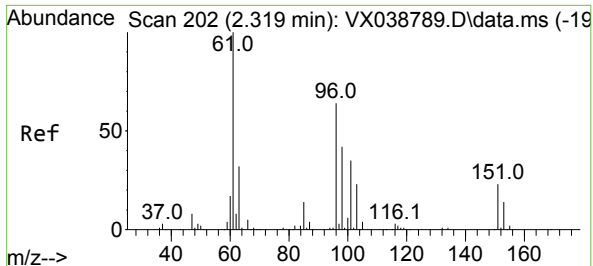

#12  
1,1-Dichloroethene  
Concen: 0.497 ug/l  
RT: 2.325 min Scan# 20  
Delta R.T. 0.006 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE125D3-20231109DL


Tgt Ion: 96 Resp: 633  
Ion Ratio Lower Upper  
96 100  
61 59.4 144.6 216.8#  
98 41.6 50.4 75.6#

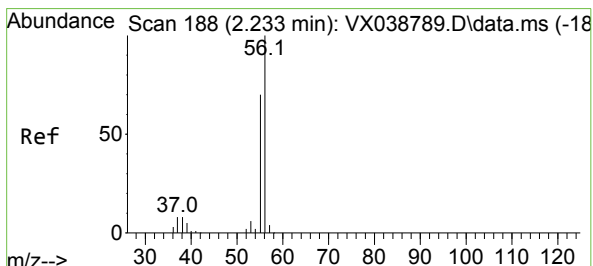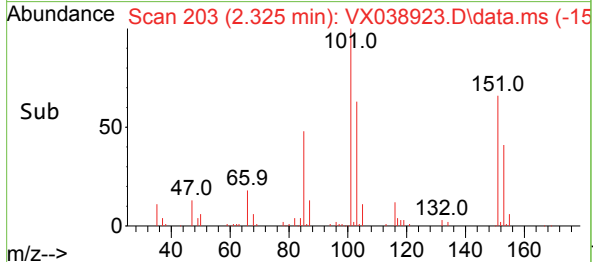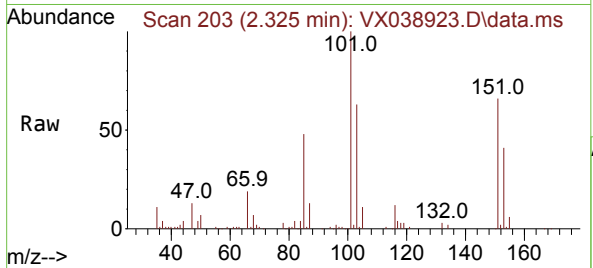

#13  
Acrolein  
Concen: 0.235 ug/l  
RT: 2.227 min Scan# 187  
Delta R.T. -0.006 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12

Tgt Ion: 56 Resp: 57  
Ion Ratio Lower Upper  
56 100  
55 0.0 57.1 85.7#

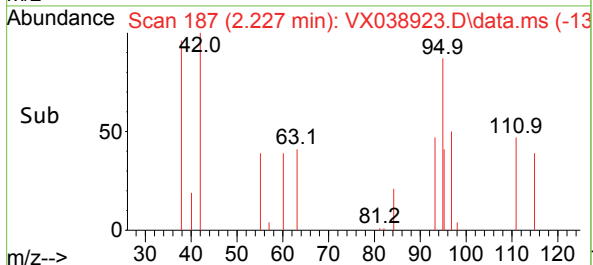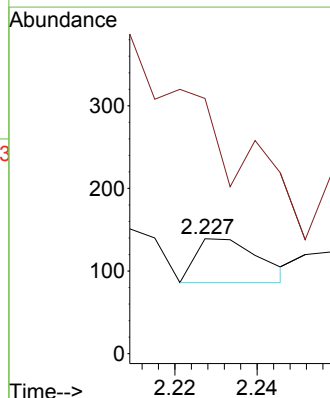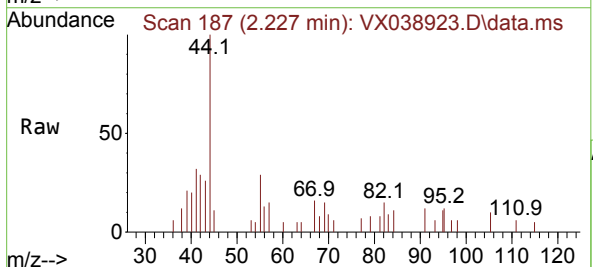



#15

Acrylonitrile

Concen: 0.424 ug/l

RT: 3.075 min Scan# 31

Delta R.T. 0.012 min

Lab File: VX038923.D

Acq: 18 Nov 2023 13:12

Instrument :

MSVOA\_X

ClientSampleId :

RE125D3-20231109DL





Tgt Ion: 53 Resp: 410

Ion Ratio Lower Upper

53 100

52 67.6 66.0 99.0

51 52.9 29.8 44.6#

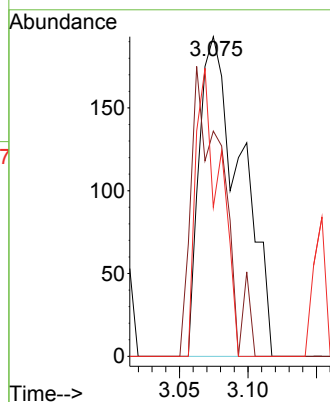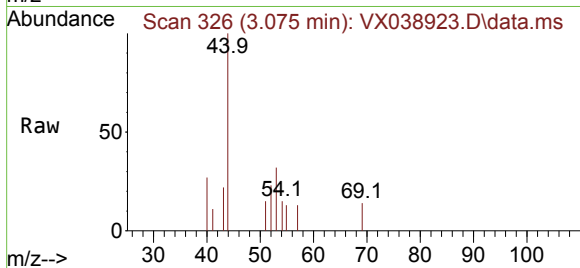

#16

Acetone

Concen: 0.858 ug/l

RT: 2.374 min Scan# 211

Delta R.T. 0.000 min

Lab File: VX038923.D




Acq: 18 Nov 2023 13:12


Tgt Ion: 43 Resp: 752

Ion Ratio Lower Upper

43 100

58 24.6 21.9 32.9

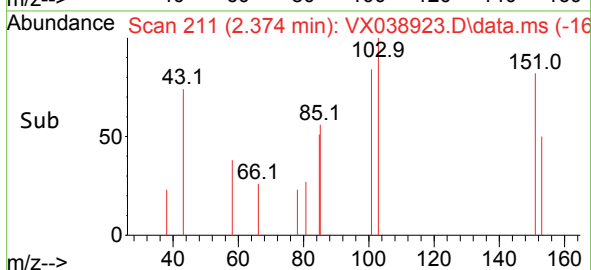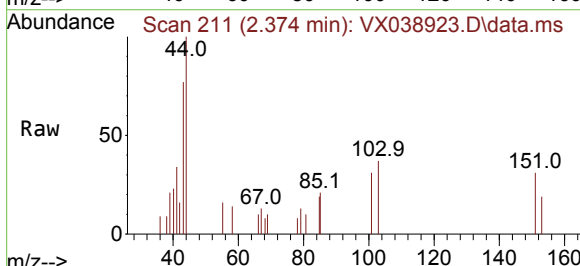

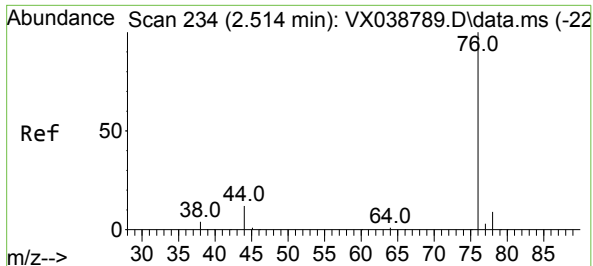

#17

Carbon Disulfide

Concen: 0.454 ug/l

RT: 2.514 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX038923.D

Acq: 18 Nov 2023 13:12

Instrument :

MSVOA\_X

ClientSampleId :





RE125D3-20231109DL

Tgt Ion: 76 Resp: 1790

Ion Ratio Lower Upper

76 100

78 10.0 7.0 10.6

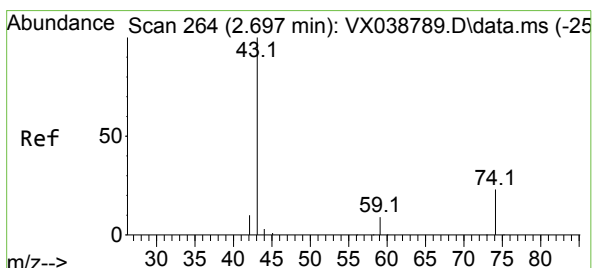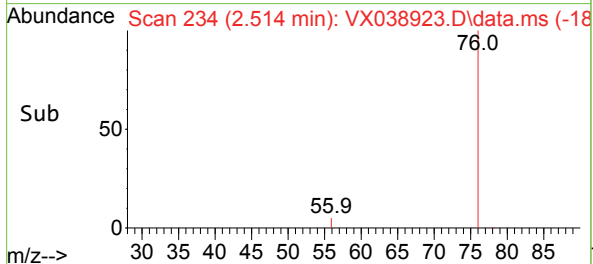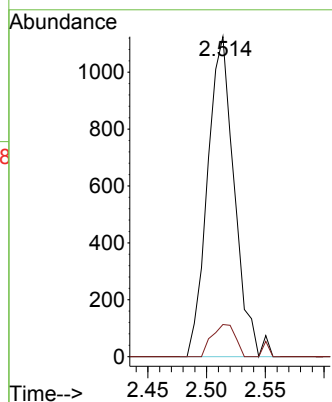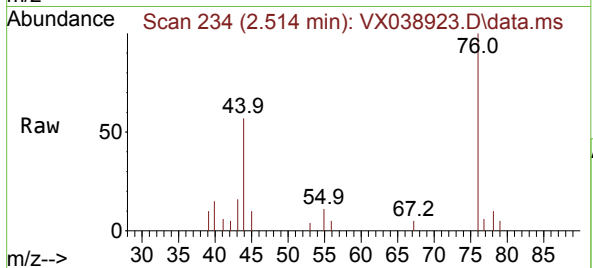

#18

Methyl Acetate

Concen: 0.204 ug/l

RT: 2.703 min Scan# 265

Delta R.T. 0.006 min

Lab File: VX038923.D




Acq: 18 Nov 2023 13:12


Tgt Ion: 43 Resp: 849

Ion Ratio Lower Upper

43 100

74 6.0 17.8 26.8#


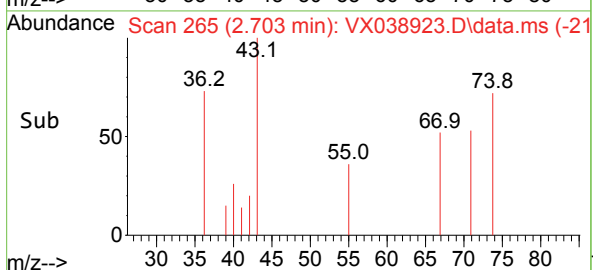
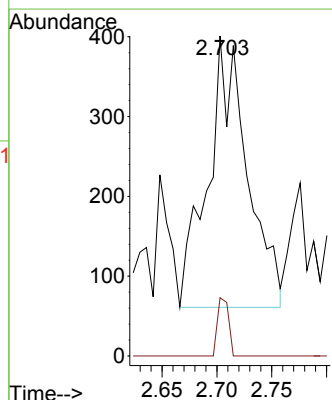
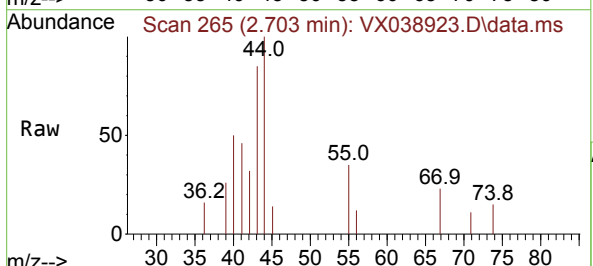




#20  
Methylene Chloride  
Concen: 3.413 ug/l  
RT: 2.788 min Scan# 21  
Delta R.T. 0.000 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE125D3-20231109DL


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 84    | Resp: | 5389  |
| Ion      | Ratio | Lower | Upper |
| 84       | 100   |       |       |
| 49       | 132.1 | 103.6 | 155.4 |
| 51       | 33.2  | 33.8  | 50.6# |
| 86       | 60.2  | 49.4  | 74.0  |

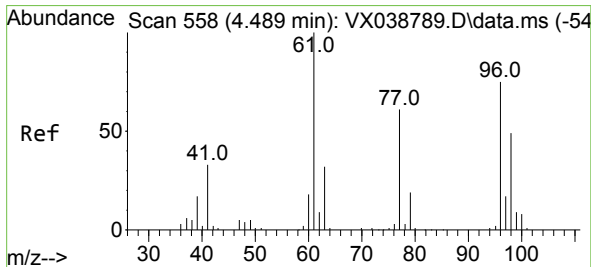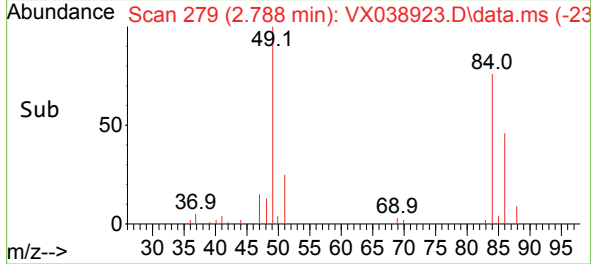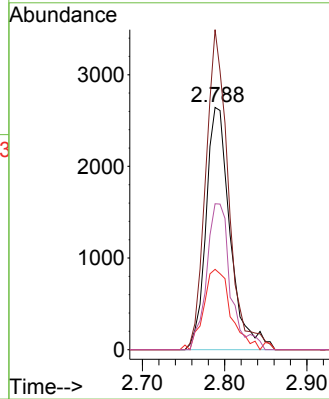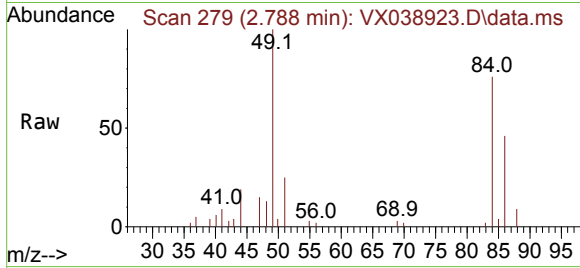

#27  
cis-1,2-Dichloroethene  
Concen: 0.437 ug/l  
RT: 4.489 min Scan# 558  
Delta R.T. 0.000 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 96    | Resp: | 716   |
| Ion      | Ratio | Lower | Upper |
| 96       | 100   |       |       |
| 61       | 149.0 | 0.0   | 312.2 |
| 98       | 45.3  | 0.0   | 129.0 |

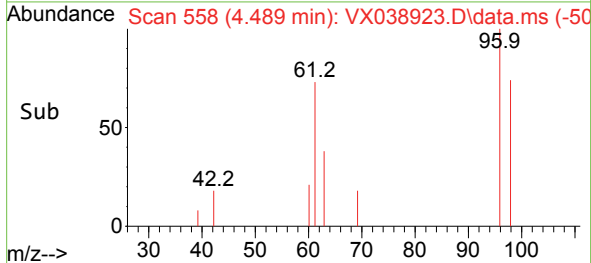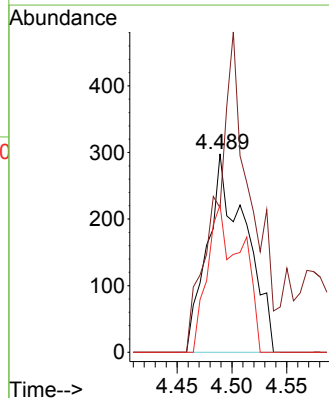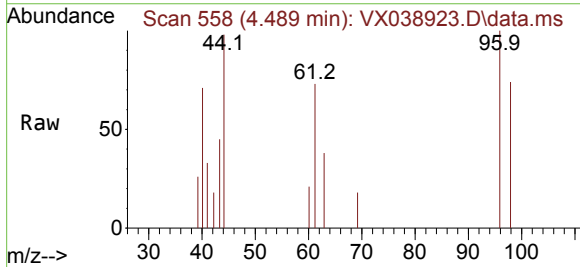



#33

1,2-Dichloroethane-d4

Concen: 47.640 ug/l

RT: 5.952 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX038923.D

Acq: 18 Nov 2023 13:12

Instrument :

MSVOA\_X

ClientSampleId :





RE125D3-20231109DL

Tgt Ion: 65 Resp: 78396

Ion Ratio Lower Upper

65 100

67 54.3 0.0 100.2

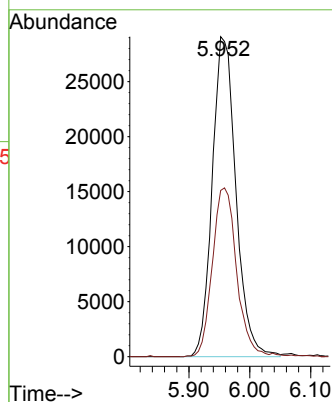

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX038923.D

Acq: 18 Nov 2023 13:12




Tgt Ion: 114 Resp: 202031


Ion Ratio Lower Upper

114 100

63 21.1 0.0 45.0

88 17.3 0.0 36.6

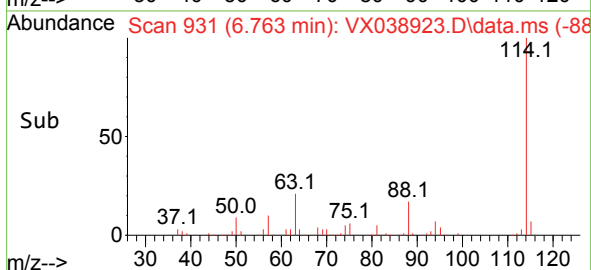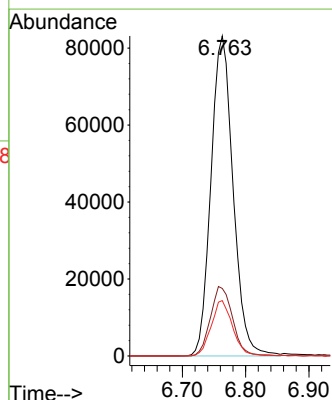

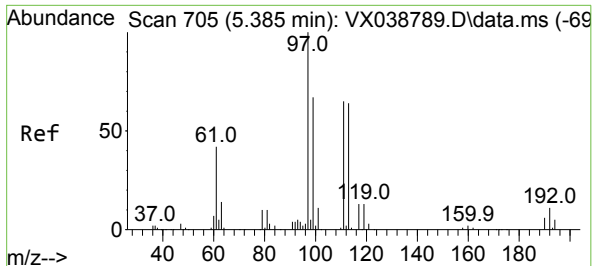

#35

Dibromofluoromethane

Concen: 44.968 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.000 min

Lab File: VX038923.D


Acq: 18 Nov 2023 13:12

Instrument :




MSVOA\_X

ClientSampleId :

RE125D3-20231109DL

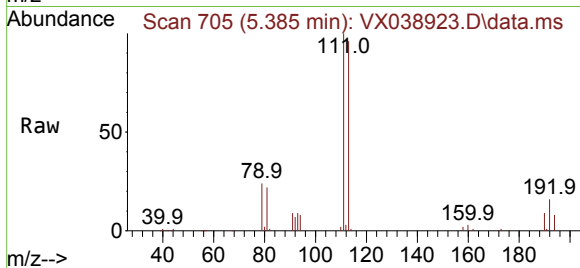

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 113   | Resp: | 65614 |
| Ion      | Ratio | Lower | Upper |
| 113      | 100   |       |       |
| 111      | 104.6 | 82.9  | 124.3 |
| 192      | 16.6  | 13.3  | 19.9  |

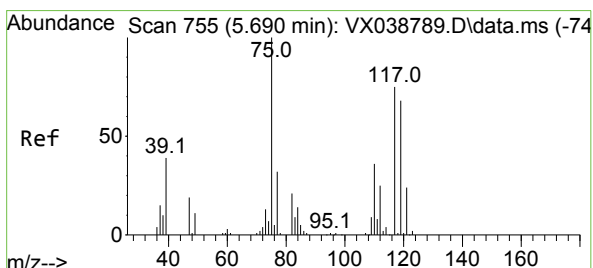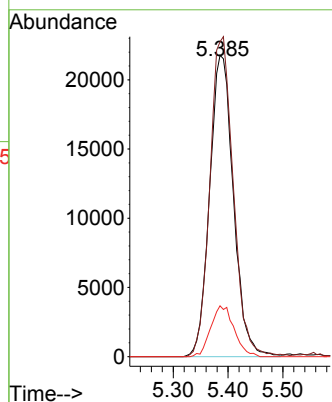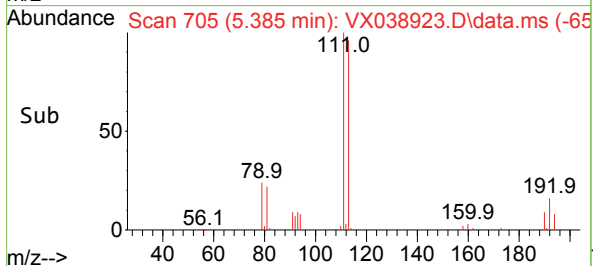

#36

1,1-Dichloropropene

Concen: 4.392 ug/l




RT: 5.550 min Scan# 732


Delta R.T. -0.140 min

Lab File: VX038923.D

Acq: 18 Nov 2023 13:12

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 75    | Resp: | 9185  |
| Ion      | Ratio | Lower | Upper |
| 75       | 100   |       |       |
| 110      | 10.5  | 17.0  | 50.9# |
| 77       | 0.2   | 24.7  | 37.1# |

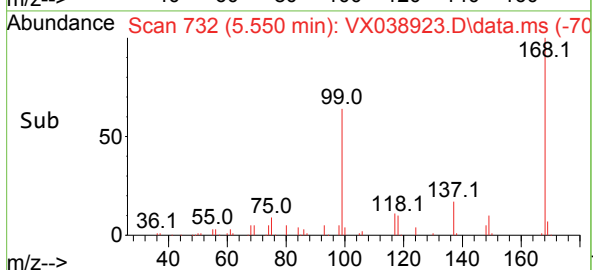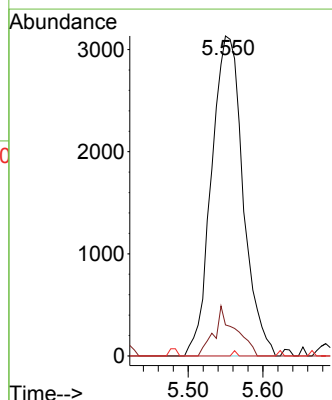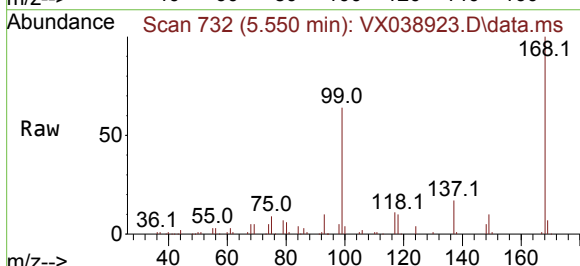



#37

Ethyl Acetate

Concen: 0.220 ug/l

RT: 4.690 min Scan# 594

Delta R.T. -0.018 min

Lab File: VX038923.D

Acq: 18 Nov 2023 13:12





Instrument :

MSVOA\_X

ClientSampleId :

RE125D3-20231109DL

|             |             |
|-------------|-------------|
| Tgt Ion: 43 | Resp: 600   |
| Ion Ratio   | Lower Upper |
| 43 100      |             |
| 61 0.0      | 10.6 16.0#  |
| 70 0.0      | 8.3 12.5#   |

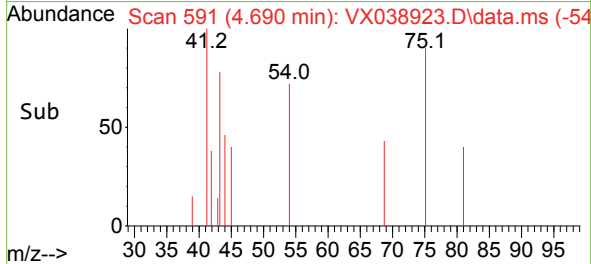

#38

Carbon Tetrachloride

Concen: 6.058 ug/l




RT: 5.556 min Scan# 733


Delta R.T. -0.122 min

Lab File: VX038923.D

Acq: 18 Nov 2023 13:12

|              |             |
|--------------|-------------|
| Tgt Ion: 117 | Resp: 11709 |
| Ion Ratio    | Lower Upper |
| 117 100      |             |
| 119 2.9      | 78.2 117.2# |
| 121 0.0      | 24.4 36.6#  |


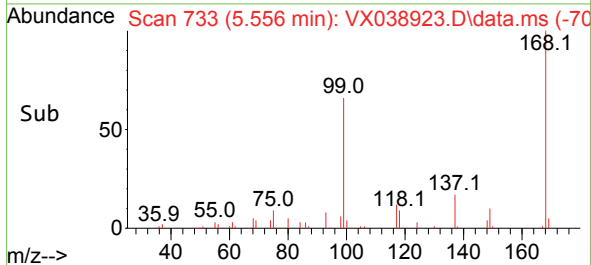

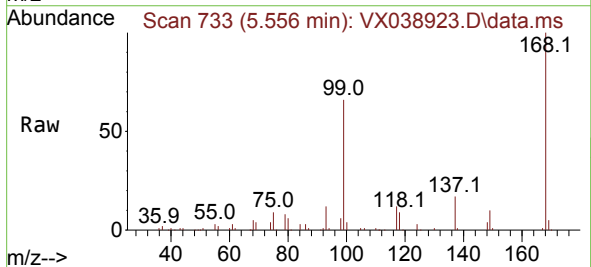


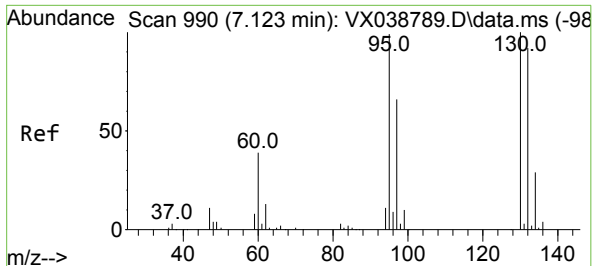

#44  
Trichloroethene  
Concen: 22.988 ug/l  
RT: 7.129 min Scan# 991  
Delta R.T. 0.006 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE125D3-20231109DL


Tgt Ion:130 Resp: 34610  
Ion Ratio Lower Upper  
130 100  
95 113.6 0.0 204.4

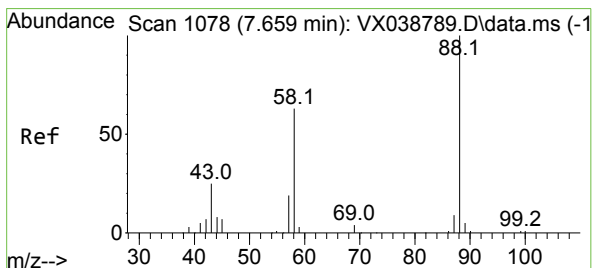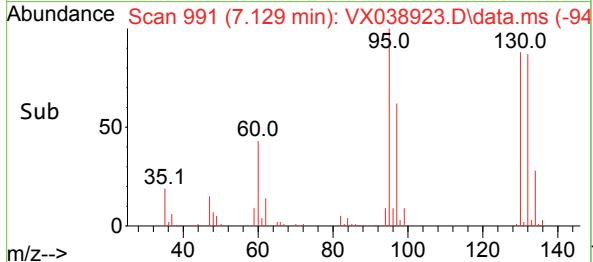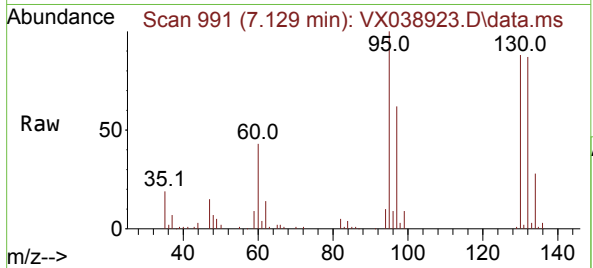

#49  
1,4-Dioxane  
Concen: 1.052 ug/l  
RT: 7.684 min Scan# 1082  
Delta R.T. 0.025 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12

Tgt Ion: 88 Resp: 43  
Ion Ratio Lower Upper  
88 100  
43 207.0 0.0 0.0#  
58 0.0 60.1 90.1#


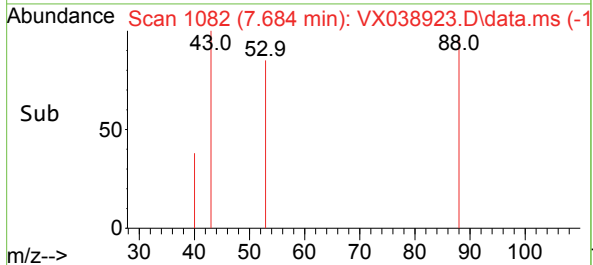

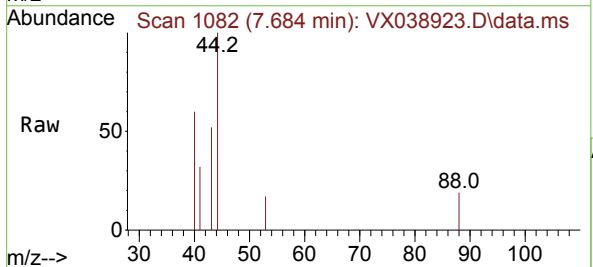




#50  
Toluene-d8  
Concen: 46.184 ug/l  
RT: 8.647 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE125D3-20231109DL


Tgt Ion: 98 Resp: 257829  
Ion Ratio Lower Upper  
98 100  
100 64.3 53.1 79.7

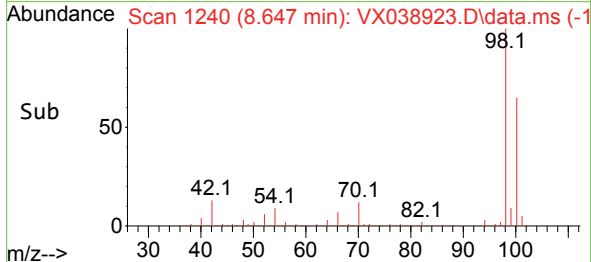

#60  
Dibromochloromethane  
Concen: 1.874 ug/l  
RT: 9.275 min Scan# 1343  
Delta R.T. -0.244 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12

Tgt Ion: 129 Resp: 3052  
Ion Ratio Lower Upper  
129 100  
127 0.0 38.8 116.4#


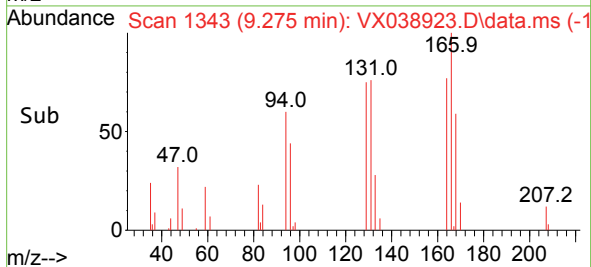

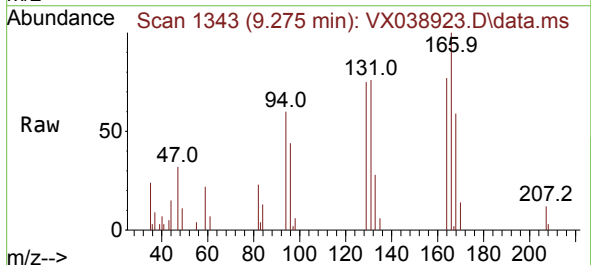




#62  
4-Bromofluorobenzene  
Concen: 48.012 ug/l  
RT: 11.079 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE125D3-20231109DL


Tgt Ion: 95 Resp: 107295  
Ion Ratio Lower Upper  
95 100  
174 67.5 0.0 135.6  
176 62.9 0.0 131.0

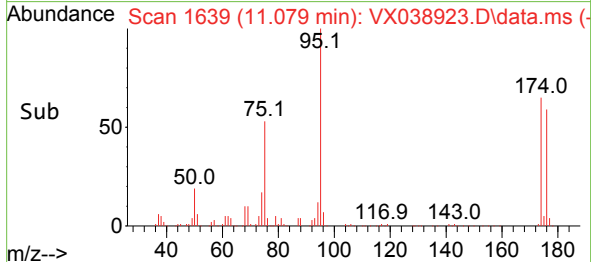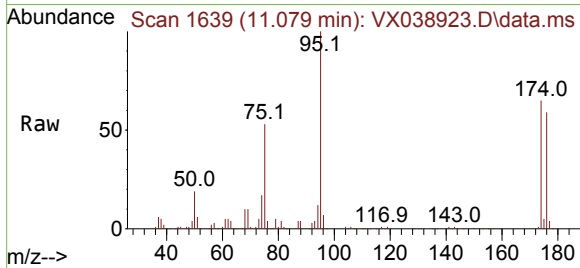

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. 0.000 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12


Tgt Ion: 117 Resp: 201777  
Ion Ratio Lower Upper  
117 100  
82 59.7 46.2 69.4  
119 32.4 25.5 38.3

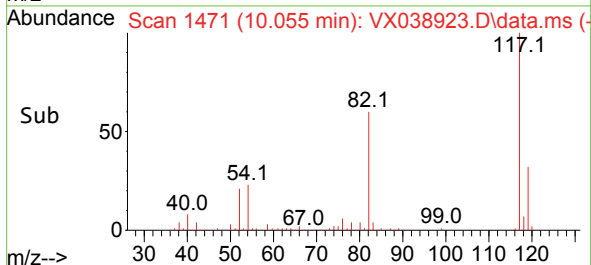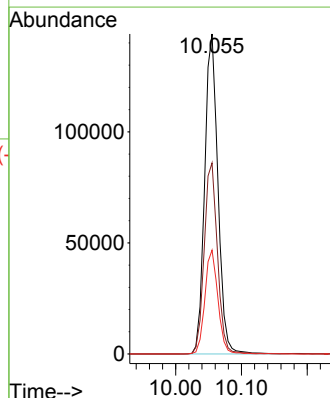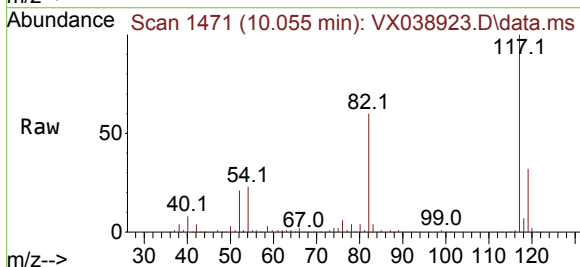






#64  
Tetrachloroethene  
Concen: 2.371 ug/l  
RT: 9.275 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12


Instrument :  
MSVOA\_X  
ClientSampleId :  
RE125D3-20231109DL

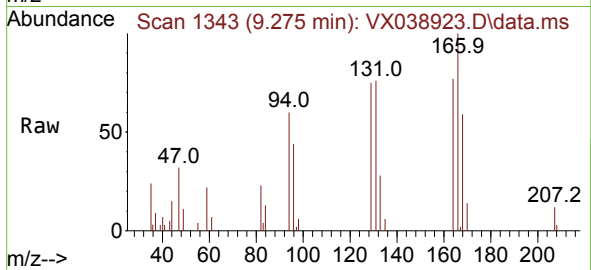



|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 164   | Resp: | 2974  |
| Ion      | Ratio | Lower | Upper |
| 164      | 100   |       |       |
| 166      | 129.2 | 102.7 | 154.1 |
| 129      | 97.4  | 80.4  | 120.6 |
| 131      | 98.6  | 76.5  | 114.7 |

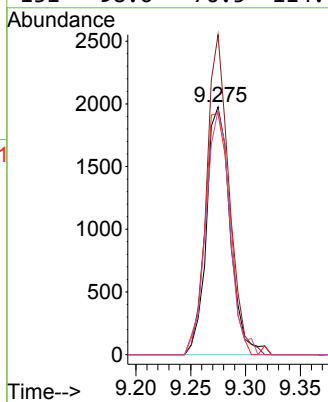


#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.024 min Scan# 1794  
Delta R.T. 0.006 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12

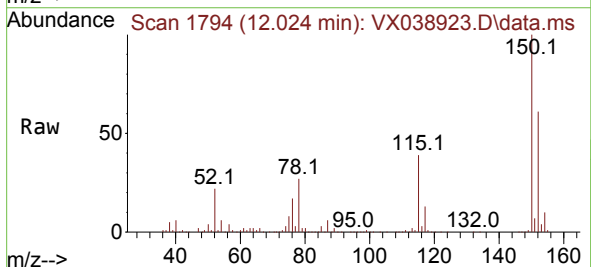

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 152   | Resp: | 97825 |
| Ion      | Ratio | Lower | Upper |
| 152      | 100   |       |       |
| 115      | 65.6  | 43.3  | 129.9 |
| 150      | 158.0 | 0.0   | 345.0 |

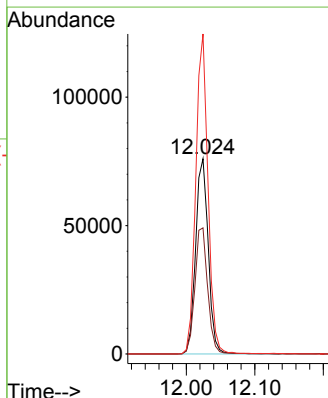



#76

1,2,3-Trichloropropane

Concen: 22.771 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.158 min

Lab File: VX038923.D

Acq: 18 Nov 2023 13:12

Instrument :

MSVOA\_X

ClientSampleId :





RE125D3-20231109DL

Tgt Ion: 75 Resp: 55578

Ion Ratio Lower Upper

75 100

77 1.2 19.1 57.5#

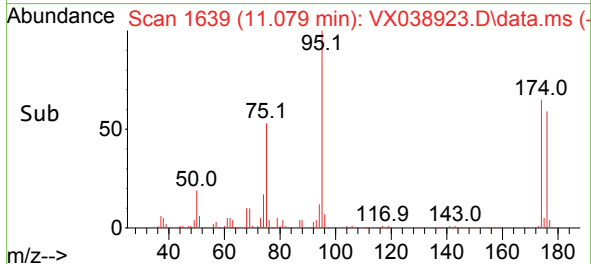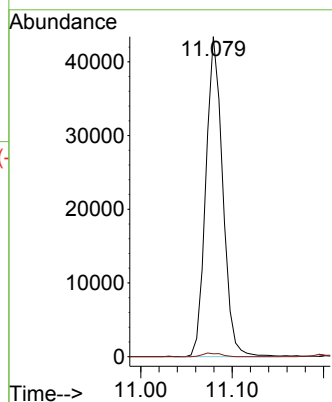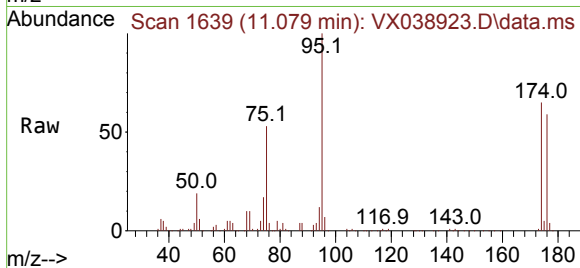

#81

trans-1,4-Dichloro-2-butene

Concen: 50.509 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX038923.D

Acq: 18 Nov 2023 13:12




Tgt Ion: 75 Resp: 55578


Ion Ratio Lower Upper

75 100

53 0.0 90.5 135.7#


89 0.0 36.9 55.3#

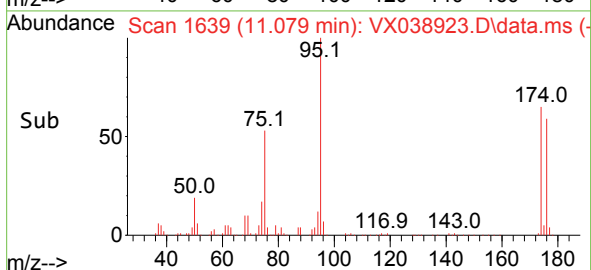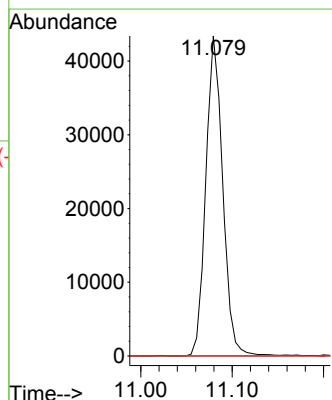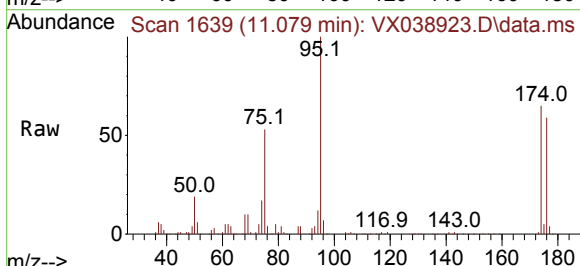






#89  
n-Butylbenzene  
Concen: 0.245 ug/l  
RT: 12.335 min Scan# 1845  
Delta R.T. 0.006 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12


Instrument :  
MSVOA\_X  
ClientSampleId :  
RE125D3-20231109DL

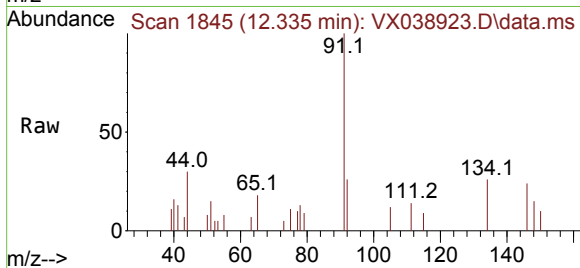



|             |       |             |
|-------------|-------|-------------|
| Tgt Ion: 91 | Resp: | 1638        |
| Ion         | Ratio | Lower Upper |
| 91          | 100   |             |
| 92          | 41.9  | 27.4 82.0   |
| 134         | 22.4  | 12.6 37.8   |

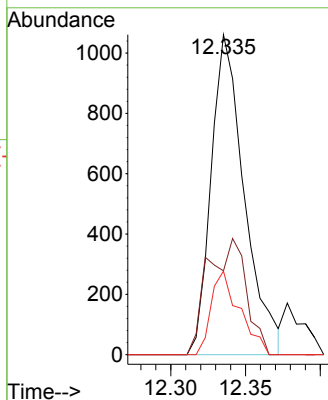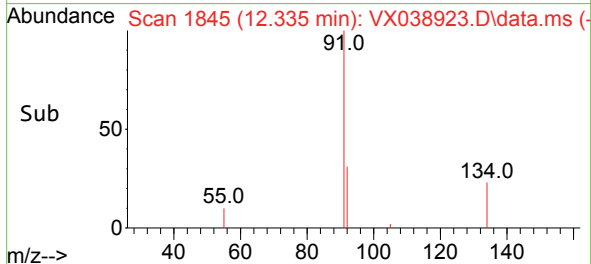


#93  
1,2,4-Trichlorobenzene  
Concen: 0.340 ug/l  
RT: 13.591 min Scan# 2051  
Delta R.T. 0.006 min  
Lab File: VX038923.D  
Acq: 18 Nov 2023 13:12

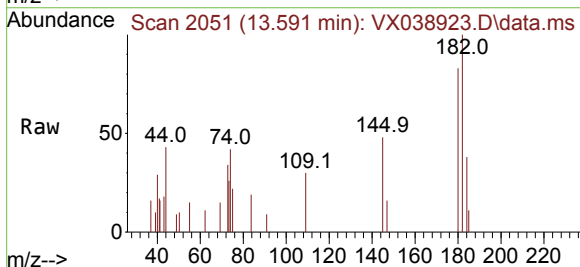

|              |       |             |
|--------------|-------|-------------|
| Tgt Ion: 180 | Resp: | 725         |
| Ion          | Ratio | Lower Upper |
| 180          | 100   |             |
| 182          | 94.8  | 48.3 144.8  |
| 145          | 45.1  | 18.0 54.0   |

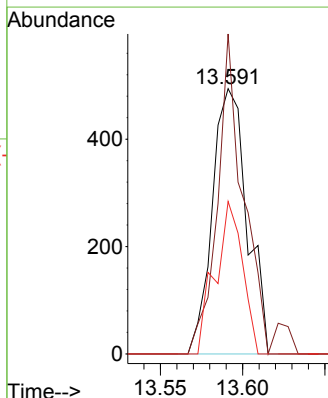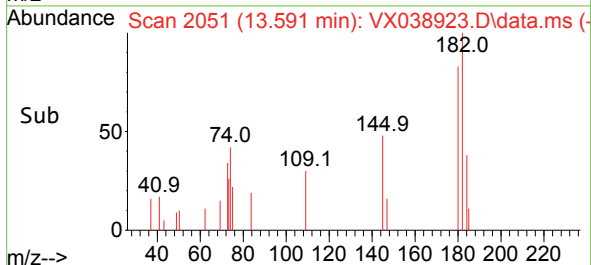



#94

Hexachlorobutadiene

Concen: 0.466 ug/l

RT: 13.725 min Scan# 2073

Delta R.T. 0.000 min

Lab File: VX038923.D

Acq: 18 Nov 2023 13:12

Instrument :

MSVOA\_X

ClientSampleId :

RE125D3-20231109DL





Tgt Ion:225 Resp: 352

Ion Ratio Lower Upper

225 100

223 62.2 31.1 93.2

227 51.4 32.5 97.5

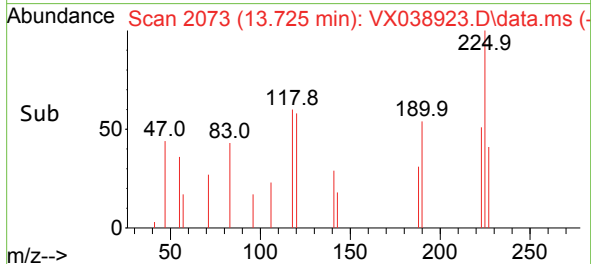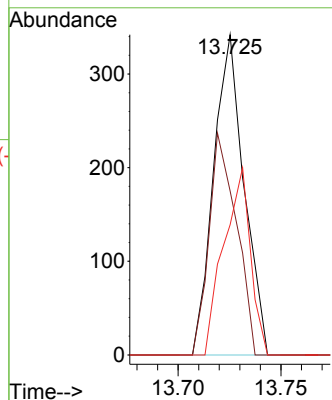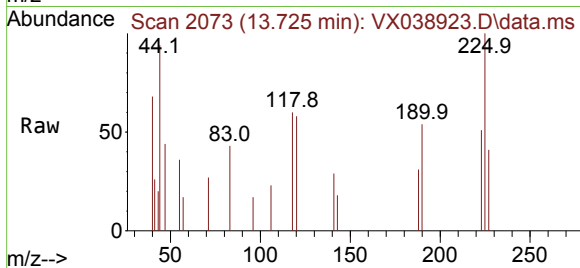

#95

Naphthalene

Concen: 0.340 ug/l

RT: 13.780 min Scan# 2082

Delta R.T. 0.006 min

Lab File: VX038923.D

Acq: 18 Nov 2023 13:12




Tgt Ion:128 Resp: 2703


Ion Ratio Lower Upper

128 100

127 10.2 10.3 15.5#


129 6.3 8.8 13.2#

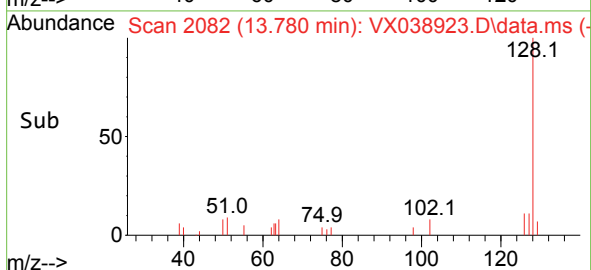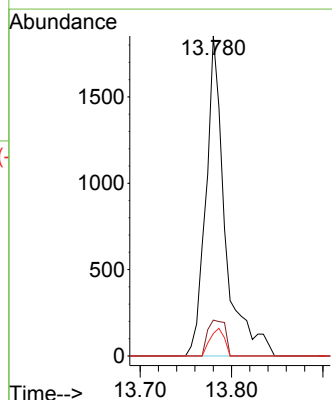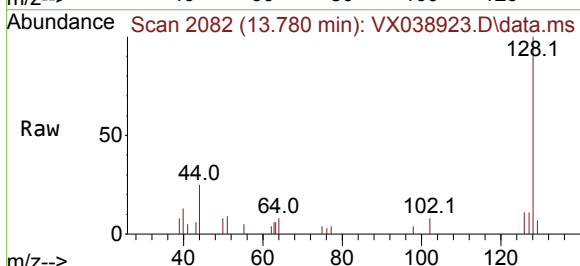



#96  
 1,2,3-Trichlorobenzene  
 Concen: 0.314 ug/l  
 RT: 13.969 min Scan# 2113  
 Delta R.T. 0.012 min  
 Lab File: VX038923.D  
 Acq: 18 Nov 2023 13:12

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 RE125D3-20231109DL



|             |       |             |
|-------------|-------|-------------|
| Tgt Ion:180 | Resp: | 635         |
| Ion         | Ratio | Lower Upper |
| 180         | 100   |             |
| 182         | 104.1 | 46.9 140.6  |
| 145         | 37.8  | 17.8 53.5   |

