

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX111823\  
 Data File : VX038938.D  
 Acq On : 18 Nov 2023 19:00  
 Operator : JC/MD  
 Sample : 05428-05  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 FB01-20231113

Quant Time: Nov 20 04:39:12 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X111623W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Nov 16 22:59:22 2023  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 5.556  | 168  | 101287   | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 6.763  | 114  | 205920   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 10.055 | 117  | 210234   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 12.024 | 152  | 104630   | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |          |
|-----------------------------|--------|-------|----------|----------|------|----------|
| System Monitoring Compounds |        |       |          |          |      |          |
| 33) 1,2-Dichloroethane-d4   | 5.958  | 65    | 83167    | 50.958   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 78 - 117 | Recovery | =    | 101.920% |
| 35) Dibromofluoromethane    | 5.385  | 113   | 66515    | 44.725   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 75 - 124 | Recovery | =    | 89.440%  |
| 50) Toluene-d8              | 8.647  | 98    | 260199   | 45.728   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 92 - 112 | Recovery | =    | 91.460%# |
| 62) 4-Bromofluorobenzene    | 11.079 | 95    | 110024   | 48.303   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 83 - 123 | Recovery | =    | 96.600%  |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX111823\  
Data File : VX038938.D  
Acq On : 18 Nov 2023 19:00  
Operator : JC/MD  
Sample : 05428-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FB01-20231113

Quant Time: Nov 20 04:39:12 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X111623W.M  
Quant Title : SW846 8260  
QLast Update : Thu Nov 16 22:59:22 2023  
Response via : Initial Calibration




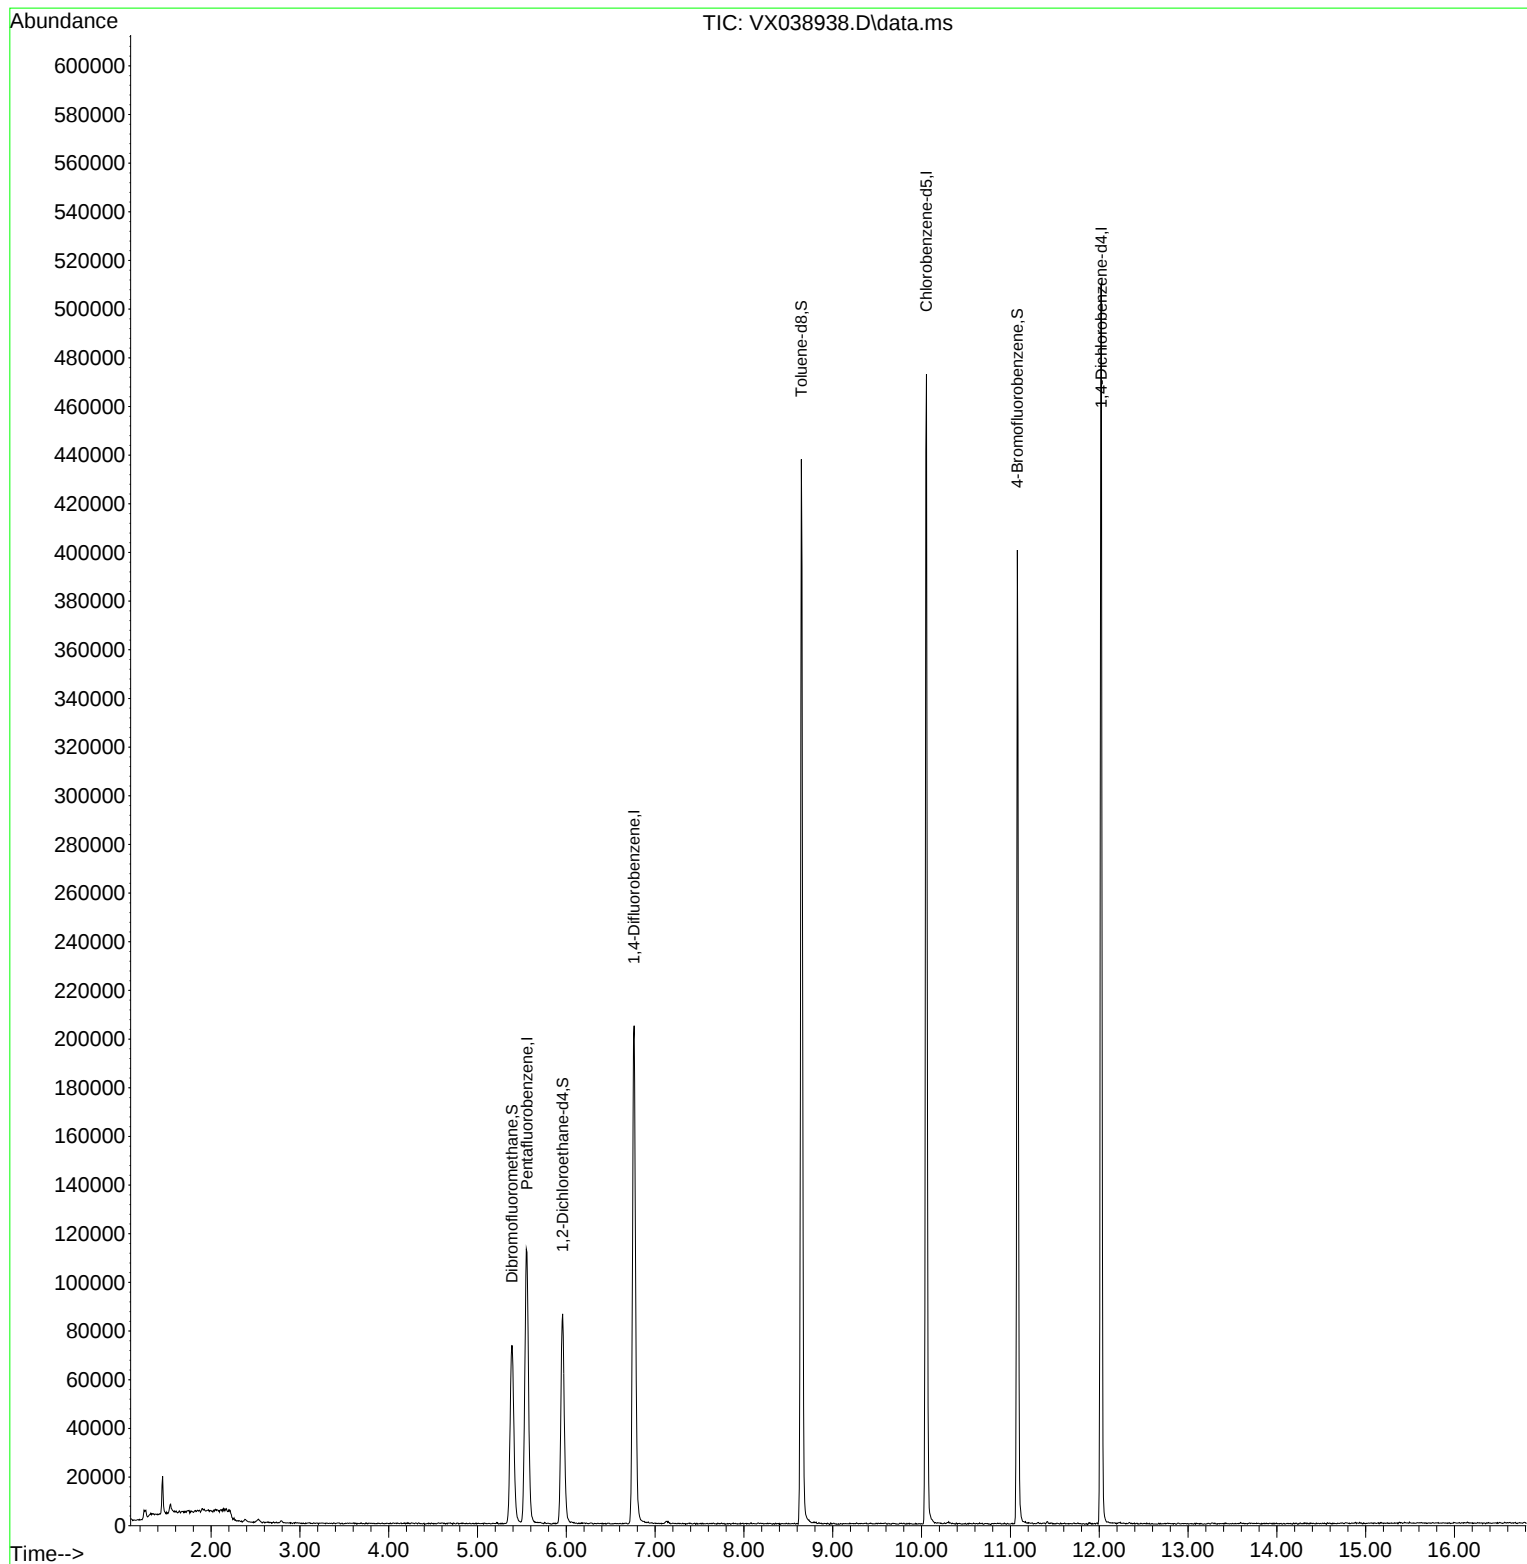




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.556 min Scan# 713  
Delta R.T. 0.006 min  
Lab File: VX038938.D  
Acq: 18 Nov 2023 19:00




Instrument :  
MSVOA\_X  
ClientSampleId :  
FB01-20231113


Tgt Ion:168 Resp: 101287  
Ion Ratio Lower Upper  
168 100  
99 61.5 56.6 85.0

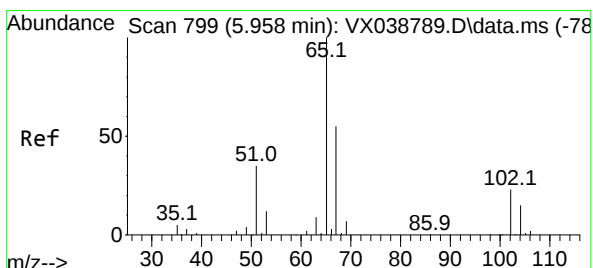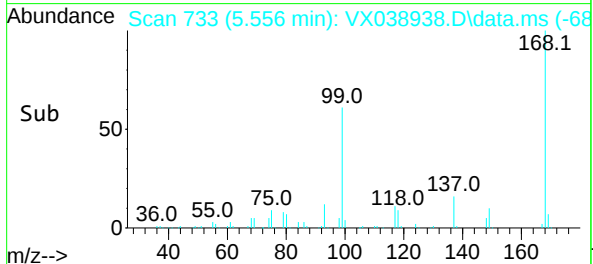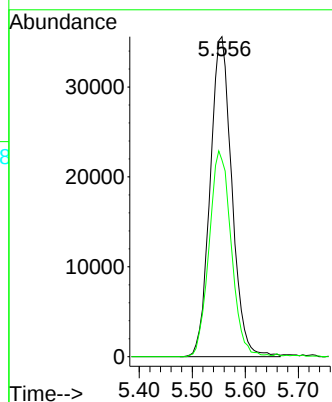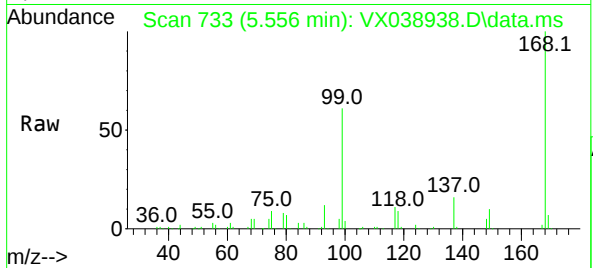

#33  
1,2-Dichloroethane-d4  
Concen: 50.958 ug/l  
RT: 5.958 min Scan# 799  
Delta R.T. 0.000 min  
Lab File: VX038938.D  
Acq: 18 Nov 2023 19:00

Tgt Ion: 65 Resp: 83167  
Ion Ratio Lower Upper  
65 100  
67 52.7 0.0 100.2


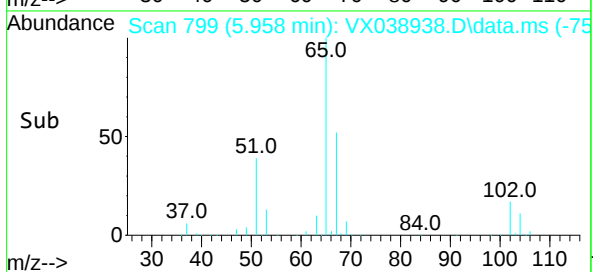
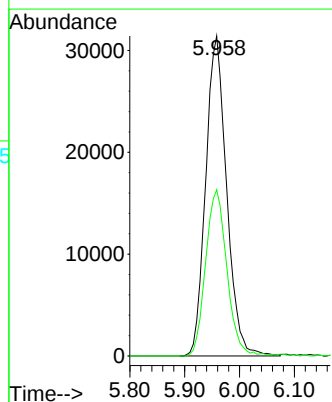
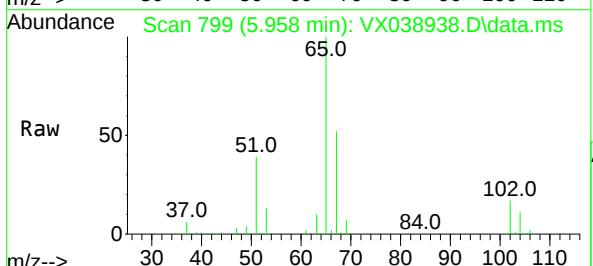


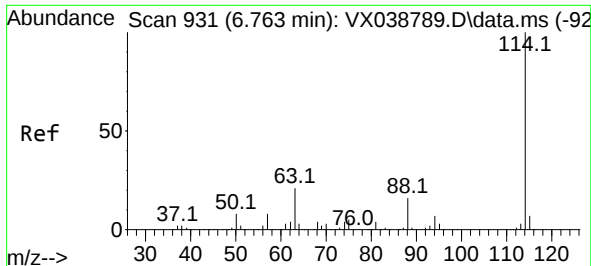

#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.763 min Scan# 911  
Delta R.T. 0.000 min  
Lab File: VX038938.D  
Acq: 18 Nov 2023 19:00




Instrument :  
MSVOA\_X  
ClientSampleId :  
FB01-20231113


Tgt Ion:114 Resp: 205920  
Ion Ratio Lower Upper  
114 100  
63 21.3 0.0 45.0  
88 17.5 0.0 36.6

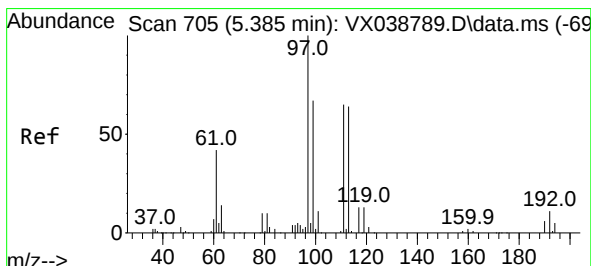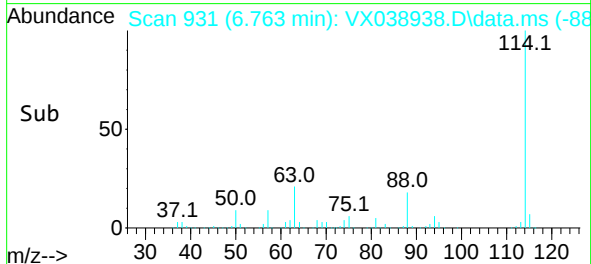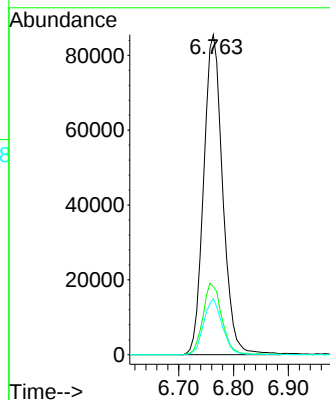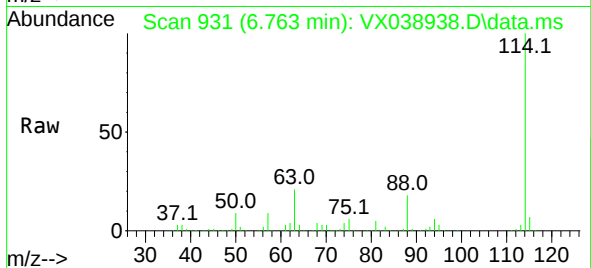

#35  
Dibromofluoromethane  
Concen: 44.725 ug/l  
RT: 5.385 min Scan# 705  
Delta R.T. 0.000 min  
Lab File: VX038938.D  
Acq: 18 Nov 2023 19:00

Tgt Ion:113 Resp: 66515  
Ion Ratio Lower Upper  
113 100  
111 102.5 82.9 124.3  
192 15.4 13.3 19.9


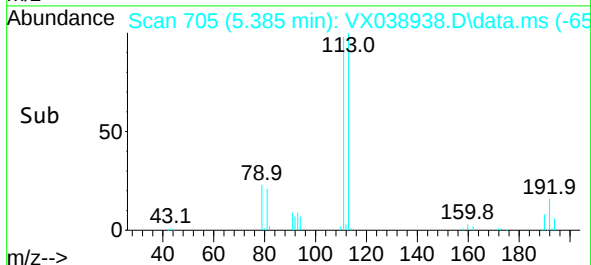
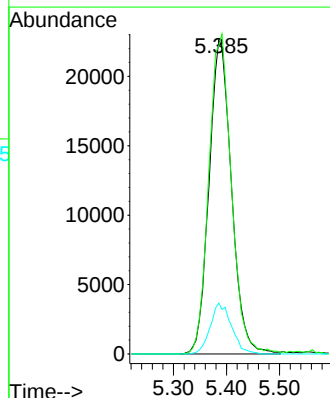
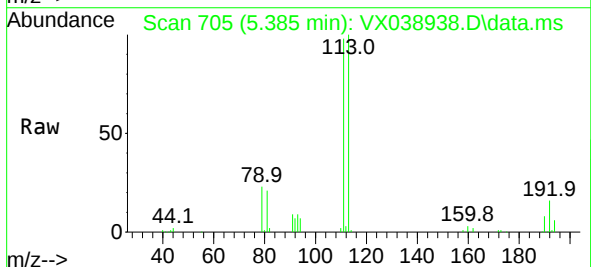


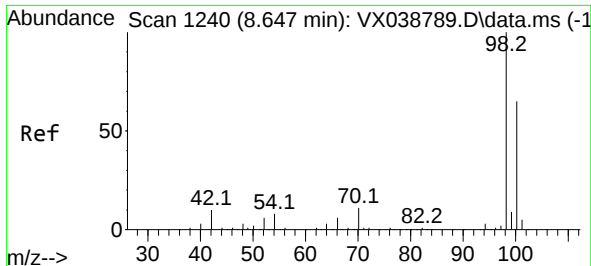

#50  
Toluene-d8  
Concen: 45.728 ug/l  
RT: 8.647 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VX038938.D  
Acq: 18 Nov 2023 19:00




Instrument :  
MSVOA\_X  
ClientSampleId :  
FB01-20231113


Tgt Ion: 98 Resp: 260199  
Ion Ratio Lower Upper  
98 100  
100 63.4 53.1 79.7

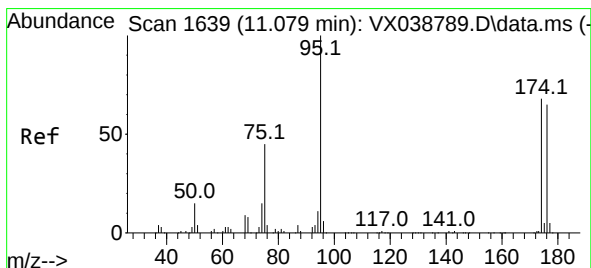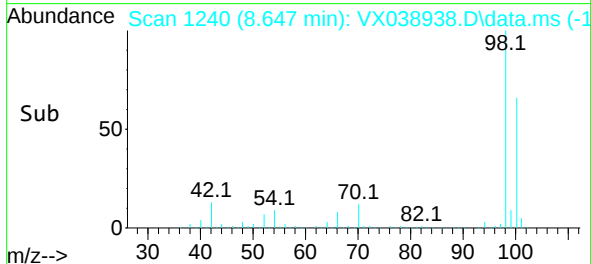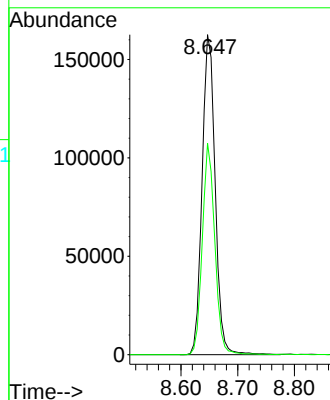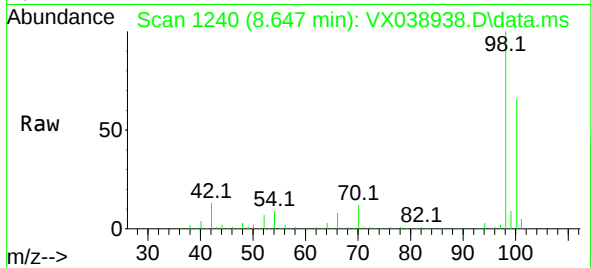

#62  
4-Bromofluorobenzene  
Concen: 48.303 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. 0.000 min  
Lab File: VX038938.D  
Acq: 18 Nov 2023 19:00

Tgt Ion: 95 Resp: 110024  
Ion Ratio Lower Upper  
95 100  
174 66.3 0.0 135.6  
176 64.1 0.0 131.0

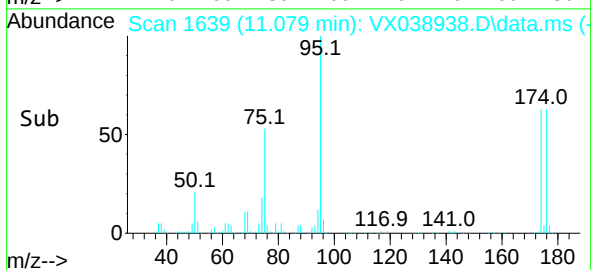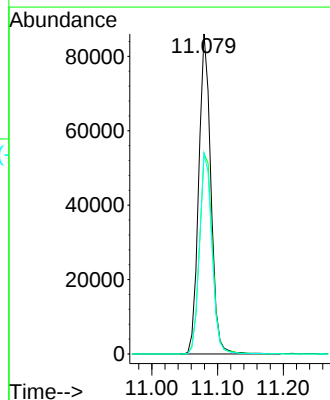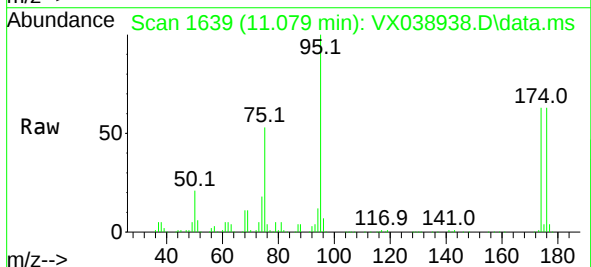

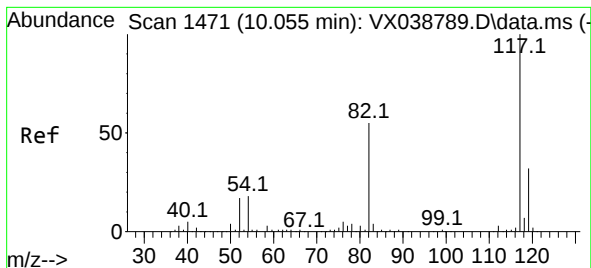

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX038938.D

Acq: 18 Nov 2023 19:00

Instrument :

MSVOA\_X

ClientSampleId :

FB01-20231113





Tgt Ion:117 Resp: 210234

Ion Ratio Lower Upper

117 100

82 58.5 46.2 69.4

119 32.2 25.5 38.3

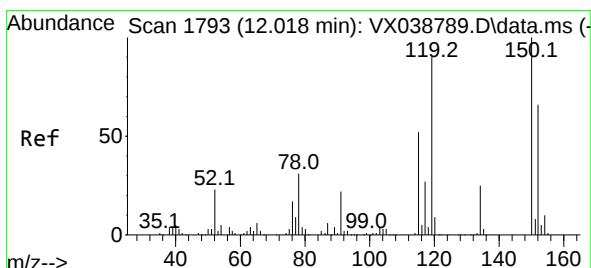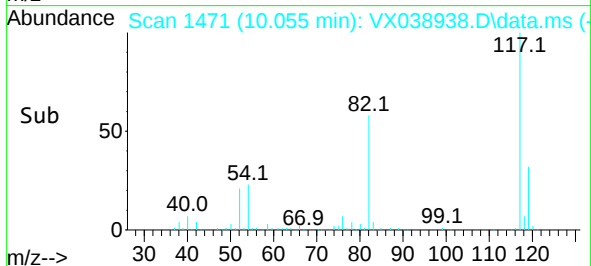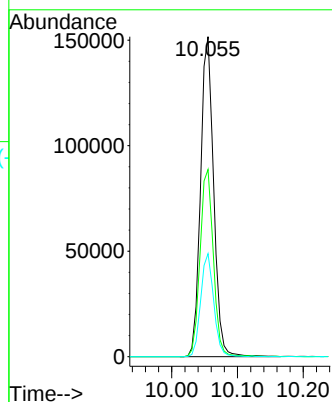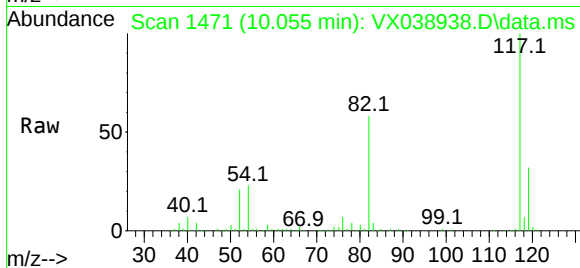

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.006 min

Lab File: VX038938.D

Acq: 18 Nov 2023 19:00

Tgt Ion:152 Resp: 104630

Ion Ratio Lower Upper

152 100

115 64.9 43.3 129.9

150 155.9 0.0 345.0

