

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111823\
 Data File : VX038935.D
 Acq On : 18 Nov 2023 17:51
 Operator : JC/MD
 Sample : 05404-07 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP06-20231109

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
 Title : SW846 8260

Signal : TIC: VX038935.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.788	272	279	290	rBV	8119	16553	2.43%	0.436%
2	4.574	562	572	581	rBV2	4364	15232	2.24%	0.401%
3	5.385	692	705	719	rBV2	73462	218216	32.05%	5.742%
4	5.550	722	732	745	rVV	111184	313378	46.03%	8.247%
5	5.958	790	799	813	rBV	85967	226743	33.30%	5.967%
6	6.763	921	931	942	rBV	197913	480398	70.56%	12.642%
7	7.129	983	991	1004	rBV3	6086	14782	2.17%	0.389%
8	8.647	1234	1240	1255	rBV	430129	680882	100.00%	17.918%
9	10.055	1465	1471	1485	rBV	455209	646718	94.98%	17.019%
10	11.079	1634	1639	1652	rBV	393003	511834	75.17%	13.469%
11	12.024	1788	1794	1812	rVB	506376	675335	99.19%	17.772%




Sum of corrected areas: 3800071

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111823\
Data File : VX038935.D
Acq On : 18 Nov 2023 17:51
Operator : JC/MD
Sample : 05404-07 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20231109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

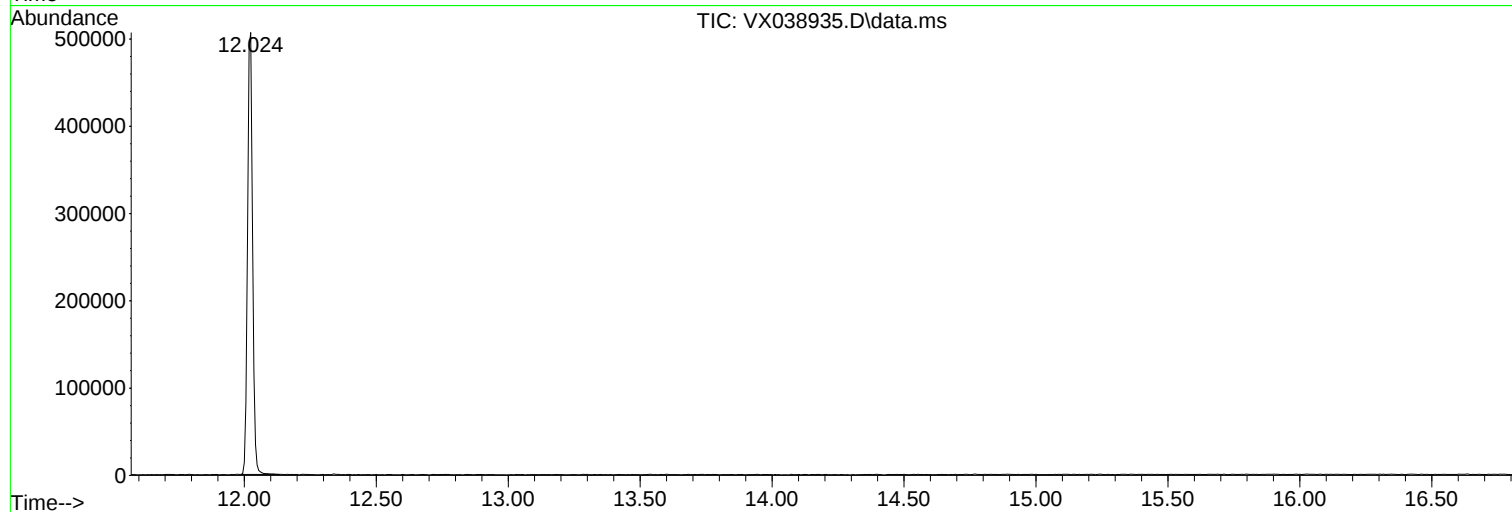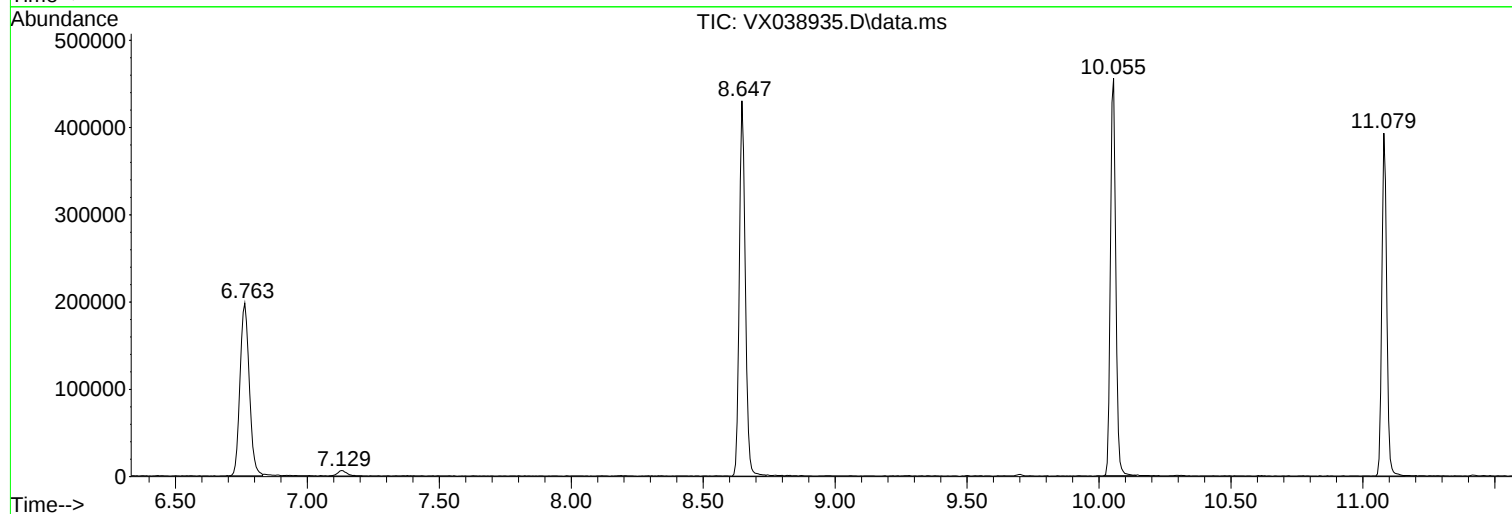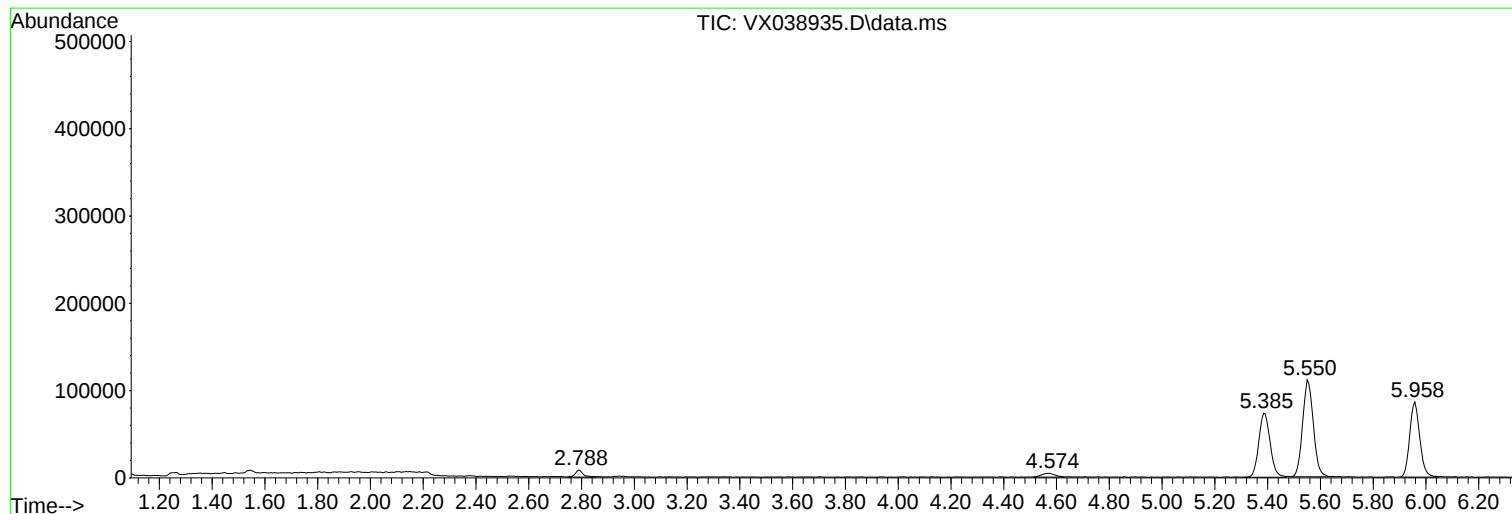

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111823\
Data File : VX038935.D
Acq On : 18 Nov 2023 17:51
Operator : JC/MD
Sample : 05404-07 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20231109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111823\
Data File : VX038935.D
Acq On : 18 Nov 2023 17:51
Operator : JC/MD
Sample : 05404-07 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20231109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------