

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112919\
Data File : VX013703.D
Acq On : 29 Nov 2019 16:00
Operator : JC/SP
Sample : K5965-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S39-0189

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 3 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	41	rBV	2106611	2424824	74.10%	11.860%
2	1.265	59	62	69	rBV	126721	163754	5.00%	0.801%
3	1.594	105	116	121	rBV9	38012	90594	2.77%	0.443%
4	2.588	273	279	287	rBV	104582	184714	5.64%	0.903%
5	4.588	599	607	615	rBV	45839	124122	3.79%	0.607%
6	5.490	744	755	766	rBV2	357054	1026719	31.37%	5.022%
7	5.654	771	782	796	rVV	653147	1820318	55.62%	8.903%
8	6.051	834	847	858	rBV	408111	1064749	32.54%	5.208%
9	6.849	969	978	990	rBV	1017414	2332695	71.28%	11.409%
10	7.209	1030	1037	1045	rBV	47177	104375	3.19%	0.510%
11	8.550	1250	1257	1262	rBV	46455	80136	2.45%	0.392%
12	8.709	1274	1283	1292	rBV	2134310	3272578	100.00%	16.006%
13	10.111	1507	1513	1522	rBV	1960978	2729975	83.42%	13.352%
14	10.355	1544	1553	1560	rBV	30533	53948	1.65%	0.264%
15	11.135	1675	1681	1688	rBV	1586809	2072782	63.34%	10.138%
16	11.940	1810	1813	1818	rVB	74562	87944	2.69%	0.430%
17	12.074	1830	1835	1842	rBV	2047496	2448358	74.81%	11.975%
18	12.361	1877	1882	1890	rBV	16149	35026	1.07%	0.171%
19	12.763	1941	1948	1954	rVB2	76189	120966	3.70%	0.592%
20	12.891	1965	1969	1974	rBV3	28891	38557	1.18%	0.189%
21	13.714	2094	2104	2109	rVB2	56397	107081	3.27%	0.524%
22	13.976	2144	2147	2151	rVB	46751	61583	1.88%	0.301%


Sum of corrected areas: 20445798

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112919\
Data File : VX013703.D
Acq On : 29 Nov 2019 16:00
Operator : JC/SP
Sample : K5965-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S39-0189

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

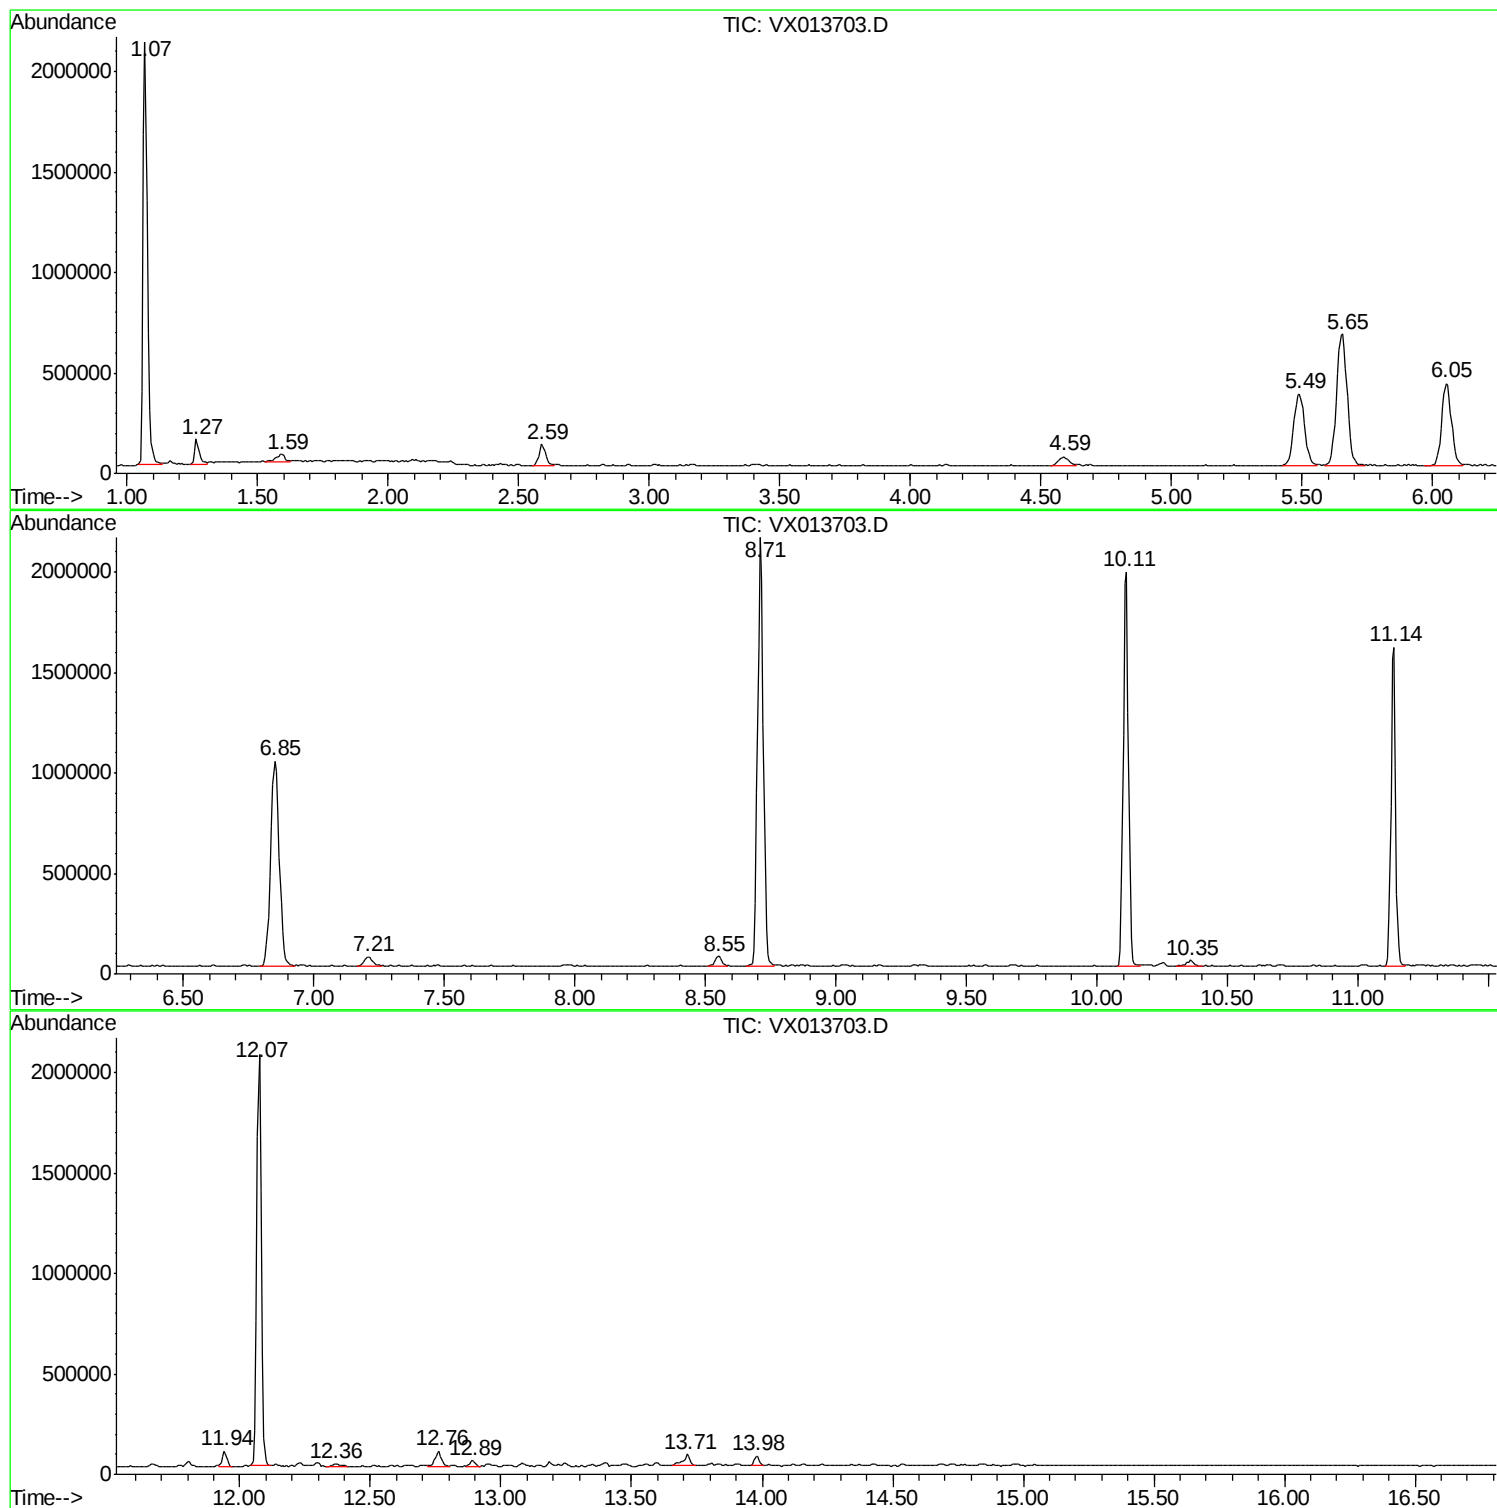

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112919\
 Data File : VX013703.D
 Acq On : 29 Nov 2019 16:00
 Operator : JC/SP
 Sample : K5965-03
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S39-0189










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
 Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
 TIC Integration Parameters: LSCINT.P

 Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	5.07 ug/l	184714	Pentafluorobenzene	5.65

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Isopropyl Alcohol	60	C3H8O	000067-63-0	72
2		Propane, 2-ethoxy-	88	C5H12O	000625-54-7	50
3		Hvdrazine, ethyl-	60	C2H8N2	000624-80-6	39
4		Formic acid, 1-methylethyl ester	88	C4H8O2	000625-55-8	39
5		Diethyl carbonate	118	C5H10O3	000105-58-8	9

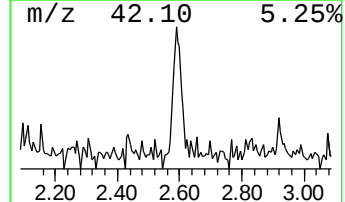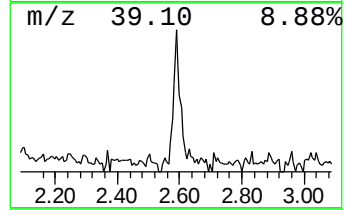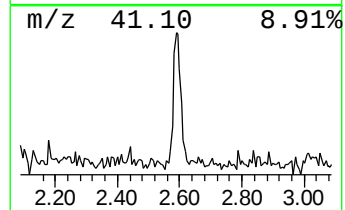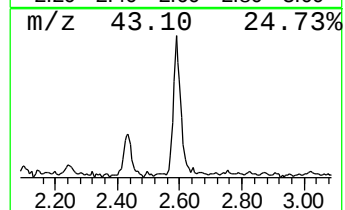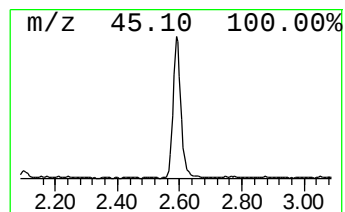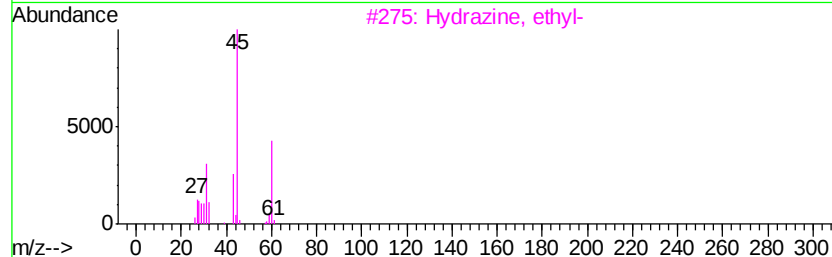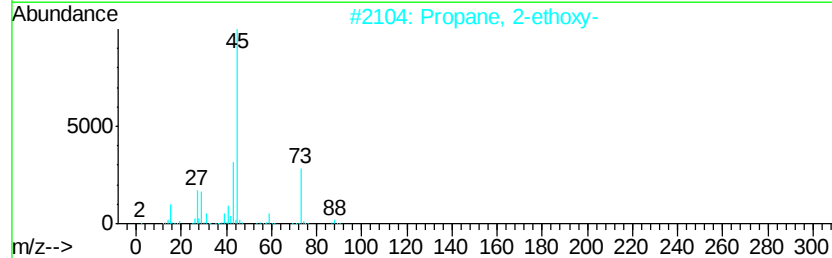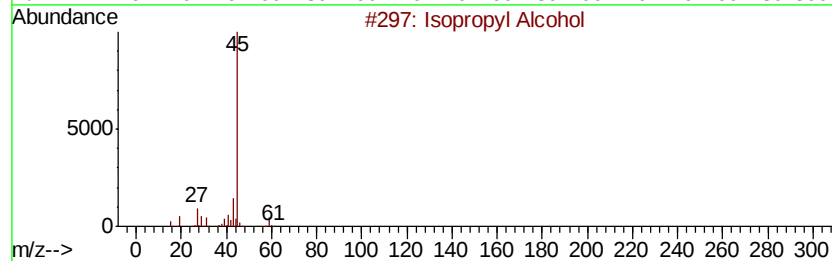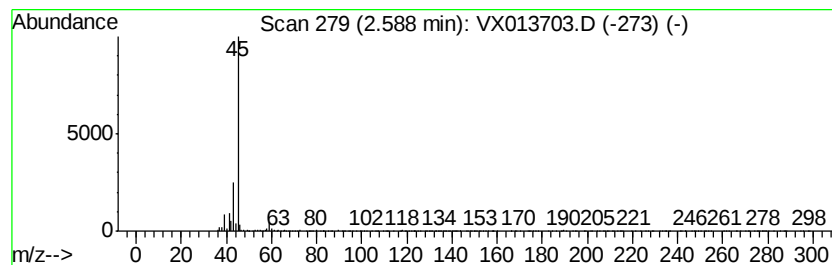

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX112919\
Data File : VX013703.D
Acq On : 29 Nov 2019 16:00
Operator : JC/SP
Sample : K5965-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S39-0189

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	5.1	ug/l	184714	1	5.65	1820320	50.0