


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112919\
 Data File : VX013691.D
 Acq On : 29 Nov 2019 08:53
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
 Title : SW846 8260
 Last Update : Tue Nov 26 15:53:00 2019

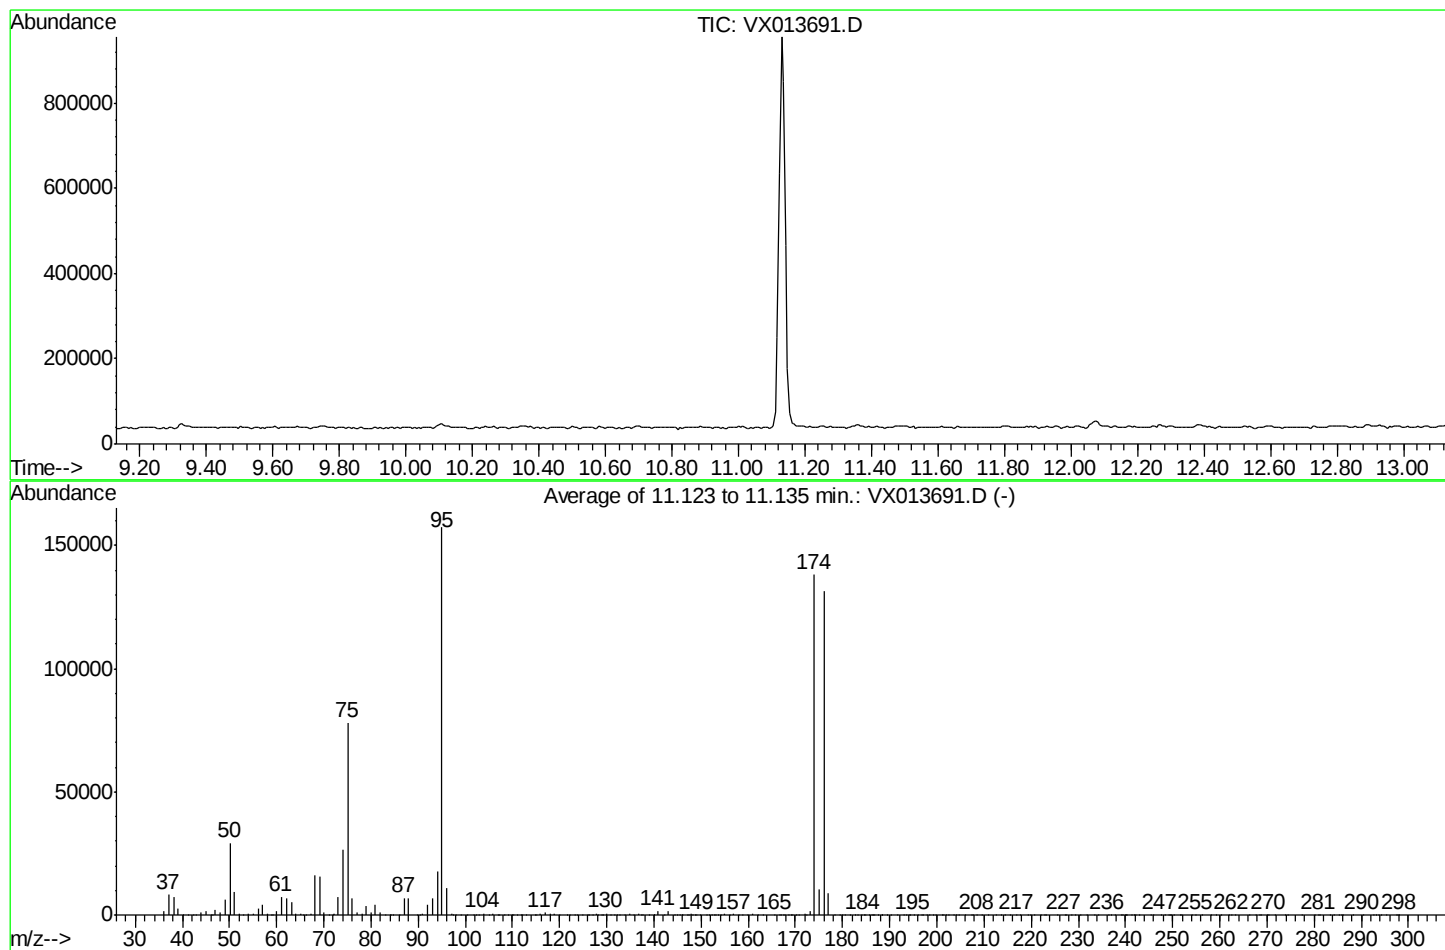

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1670

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	29274	PASS
75	95	30	60	49.6	78109	PASS
95	95	100	100	100.0	157421	PASS
96	95	5	9	7.0	11023	PASS
173	174	0.00	2	1.2	1602	PASS
174	95	50	100	87.7	138117	PASS
175	174	5	9	7.5	10325	PASS
176	174	95	101	95.3	131559	PASS
177	176	5	9	6.6	8678	PASS