

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120324\
 Data File : VX044102.D
 Acq On : 03 Dec 2024 18:46
 Operator : JC/MD
 Sample : P5006-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 04 00:15:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 22 03:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	104678	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	205665	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	184006	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	84942	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	94124	52.425	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 104.840%	
35) Dibromofluoromethane	5.379	113	52876	35.980	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 71.960%#	
50) Toluene-d8	8.647	98	254444	50.228	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 100.460%	
62) 4-Bromofluorobenzene	11.079	95	90782	52.657	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 105.320%	


Target Compounds					Qvalue	
11) Tert butyl alcohol	2.995	59	95	0.330	ug/l #	73
13) Acrolein	2.190	56	102	0.336	ug/l #	13
16) Acetone	2.386	43	14715	17.845	ug/l	93
18) Methyl Acetate	2.709	43	433	0.225	ug/l #	82
20) Methylene Chloride	2.782	84	1000	0.715	ug/l	96
25) 2-Butanone	4.586	43	2022	1.900	ug/l #	90
27) cis-1,2-Dichloroethene	4.489	96	591	0.384	ug/l	62
31) Cyclohexane	5.544	56	3397	1.698	ug/l #	65
36) 1,1-Dichloropropene	5.537	75	10342	5.647	ug/l #	46
38) Carbon Tetrachloride	5.544	117	12597	6.122	ug/l #	14
40) Benzene	6.037	78	14047	2.463	ug/l	100
51) 4-Methyl-2-Pentanone	8.580	43	1113	0.504	ug/l	95
52) Toluene	8.720	92	8797	2.577	ug/l	97
67) Ethyl Benzene	10.195	91	314227	45.886	ug/l	99
68) m/p-Xylenes	10.299	106	24707	9.675	ug/l	98
69) o-Xylene	10.640	106	26925	10.799	ug/l	96
70) Styrene	10.640	104	1917	0.465	ug/l #	1
73) Isopropylbenzene	10.963	105	28697	4.395	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	53514	28.728	ug/l #	34
78) n-propylbenzene	11.305	91	14426	1.978	ug/l	99
79) 2-Chlorotoluene	11.396	91	7751	1.681	ug/l #	45
80) 1,3,5-Trimethylbenzene	11.451	105	26719	4.974	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	53514	78.393	ug/l #	6
82) 4-Chlorotoluene	11.451	91	3657	0.702	ug/l #	46
83) tert-Butylbenzene	11.969	119	7185	1.349	ug/l	68
84) 1,2,4-Trimethylbenzene	11.750	105	97956	18.316	ug/l	98
85) sec-Butylbenzene	11.750	105	97956	15.016	ug/l #	57
86) p-Isopropyltoluene	12.012	119	5165	0.975	ug/l #	73
89) n-Butylbenzene	12.317	91	5728	1.226	ug/l #	11
90) Hexachloroethane	12.695	117	47545	52.766	ug/l #	18
92) 1,2-Dibromo-3-Chloropr...	12.957	75	570	1.272	ug/l #	4
95) Naphthalene	13.774	128	4742702	780.590	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120324\
Data File : VX044102.D
Acq On : 03 Dec 2024 18:46
Operator : JC/MD
Sample : P5006-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Dec 04 00:15:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 22 03:45:52 2024
Response via : Initial Calibration

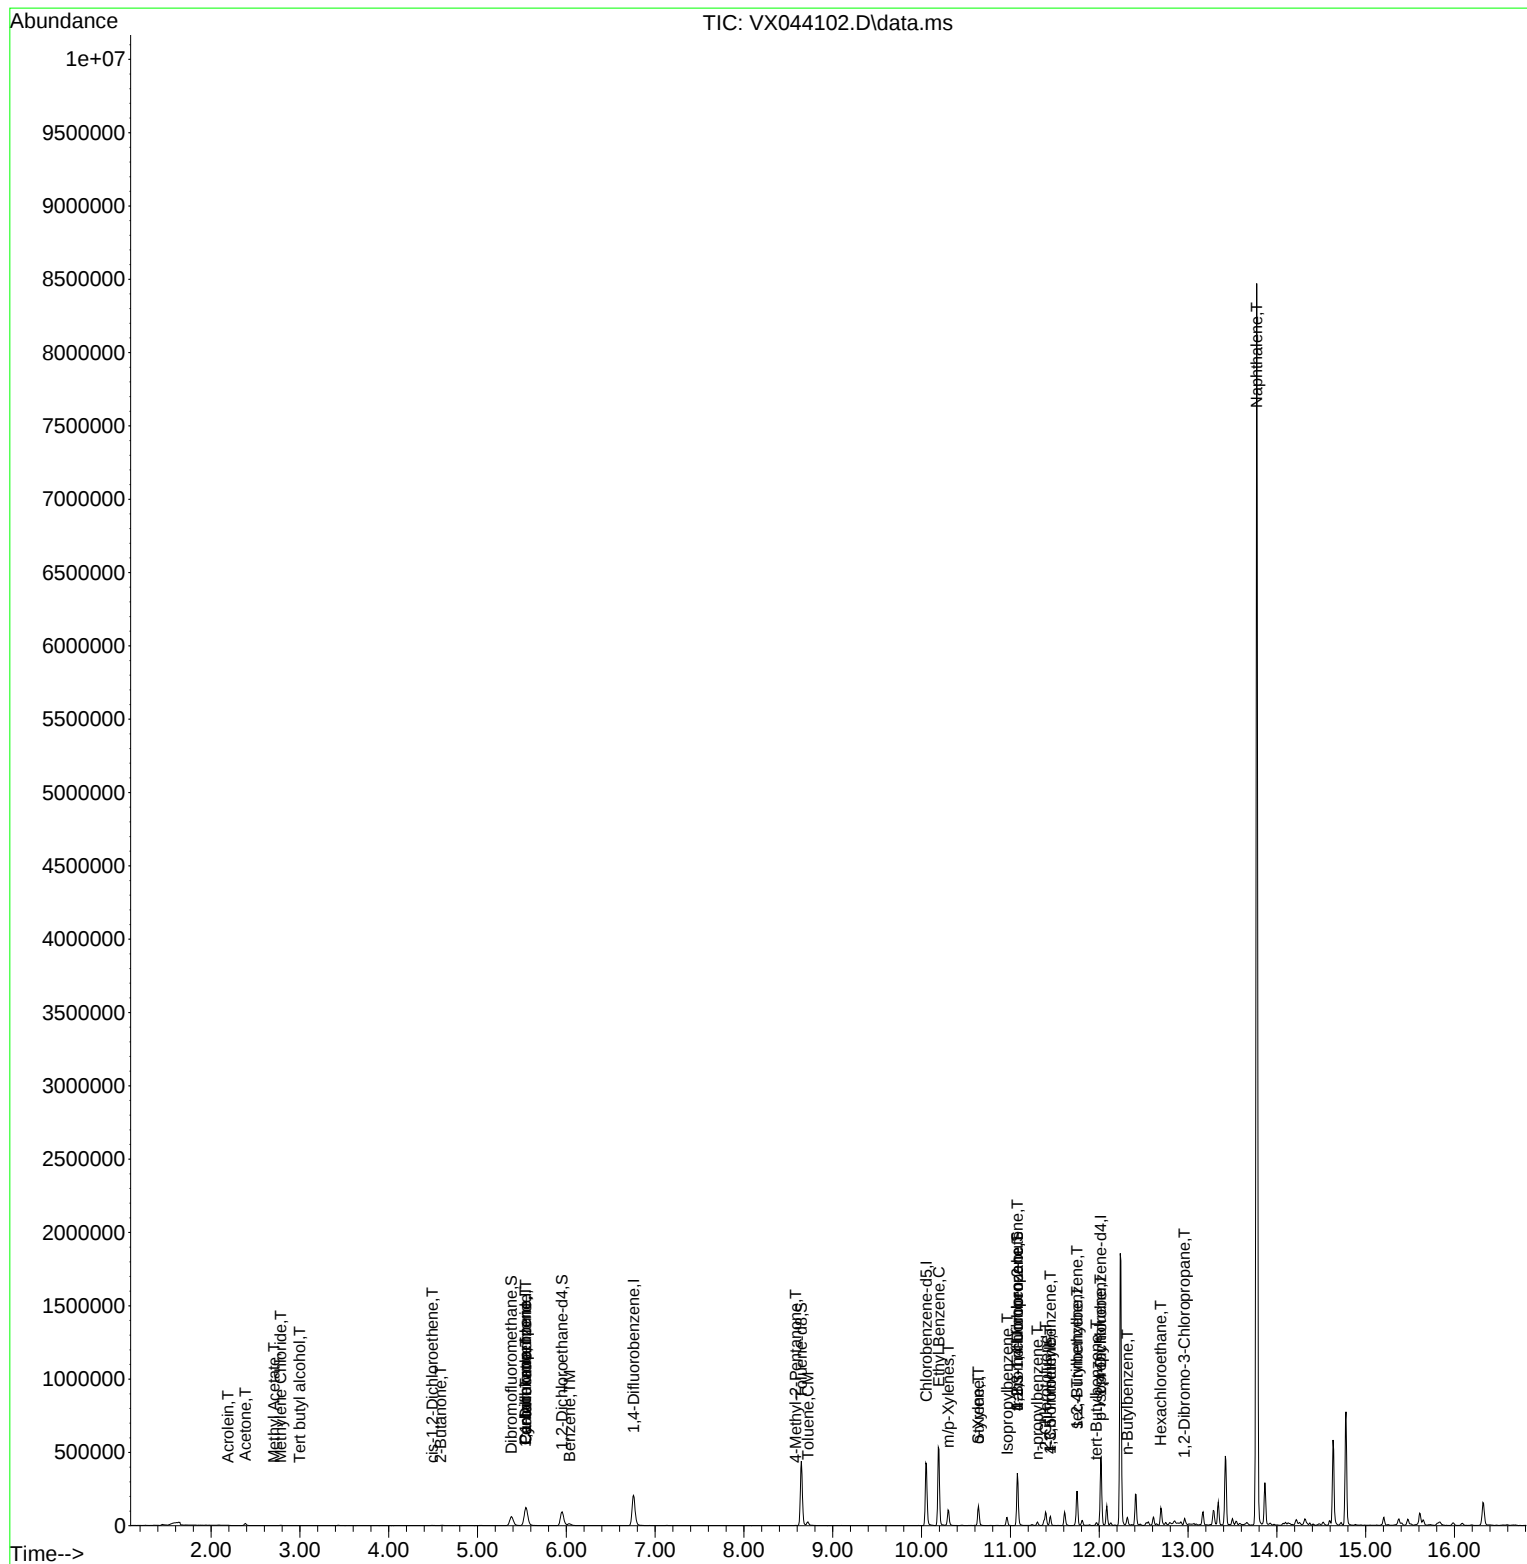



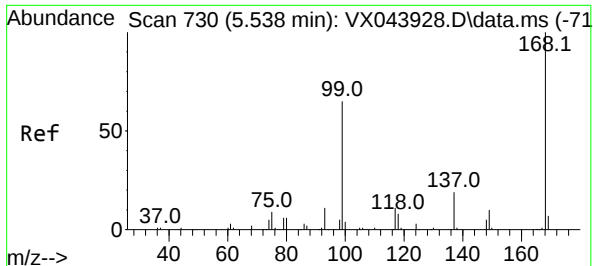


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46

Instrument :
MSVOA_X
ClientSampleId :



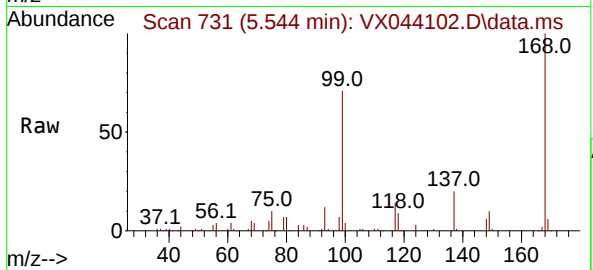



Tgt Ion:168 Resp: 104678
Ion Ratio Lower Upper
168 100
99 71.0 51.8 77.8

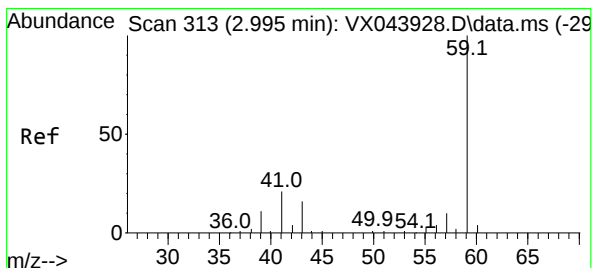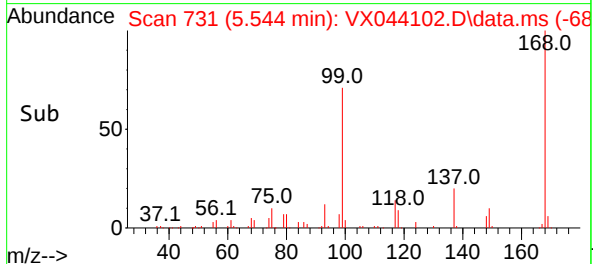

#11
Tert butyl alcohol
Concen: 0.330 ug/l
RT: 2.995 min Scan# 313
Delta R.T. -0.000 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46

Tgt Ion: 59 Resp: 95
Ion Ratio Lower Upper
59 100
57 0.0 7.9 11.9#


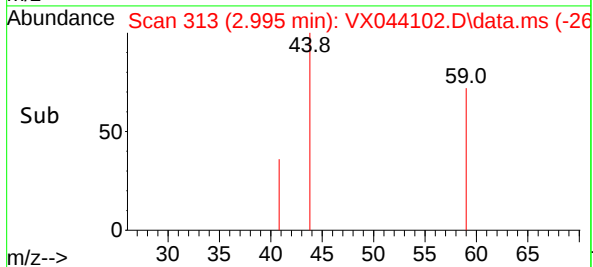

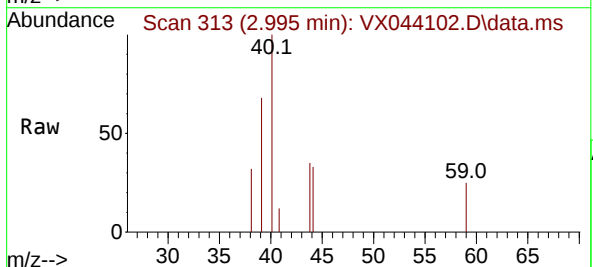


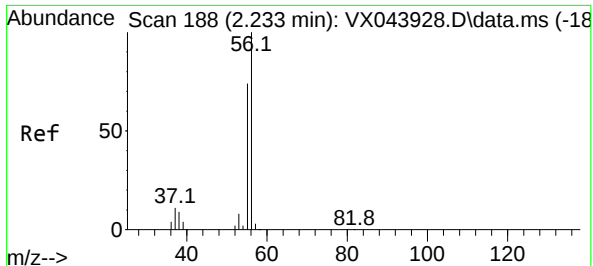

#13
Acrolein
Concen: 0.336 ug/l
RT: 2.190 min Scan# 11
Delta R.T. -0.043 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 56 Resp: 102
Ion Ratio Lower Upper
56 100
55 0.0 58.2 87.2#

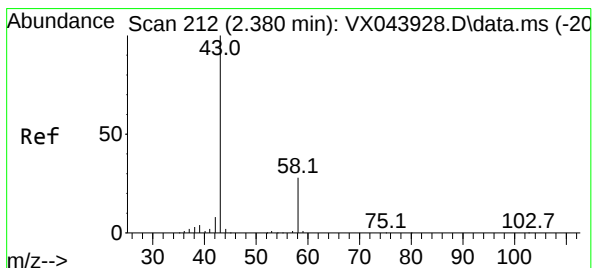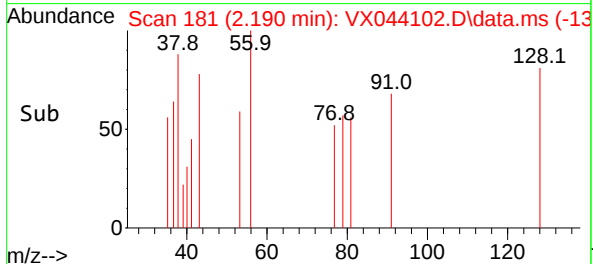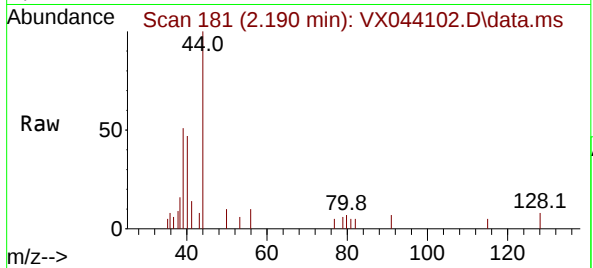

#16
Acetone
Concen: 17.845 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.006 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46

Tgt Ion: 43 Resp: 14715
Ion Ratio Lower Upper
43 100
58 24.8 22.7 34.1


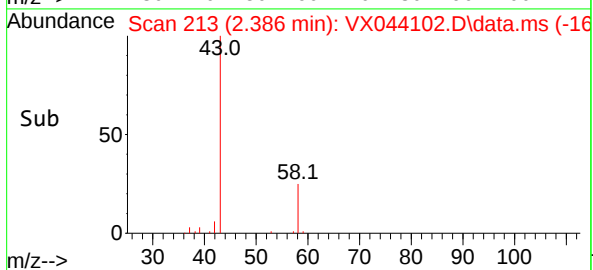

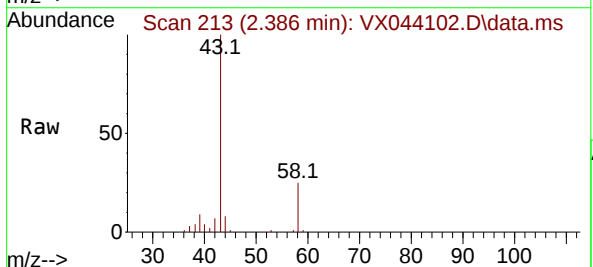




#18
Methyl Acetate
Concen: 0.225 ug/l
RT: 2.709 min Scan# 20
Delta R.T. 0.006 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 433
Ion Ratio Lower Upper
43 100
74 14.5 18.9 28.3#

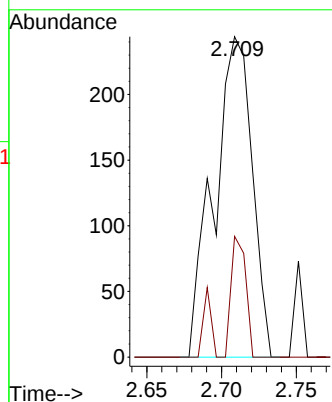

#20
Methylene Chloride
Concen: 0.715 ug/l
RT: 2.782 min Scan# 278
Delta R.T. -0.000 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46

Tgt Ion: 84 Resp: 1000
Ion Ratio Lower Upper
84 100
49 123.4 102.7 154.1
51 33.1 31.7 47.5
86 67.9 53.9 80.9









#25
2-Butanone
Concen: 1.900 ug/l
RT: 4.586 min Scan# 51
Delta R.T. 0.030 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 2022
Ion Ratio Lower Upper
43 100
72 20.0 20.2 30.2#

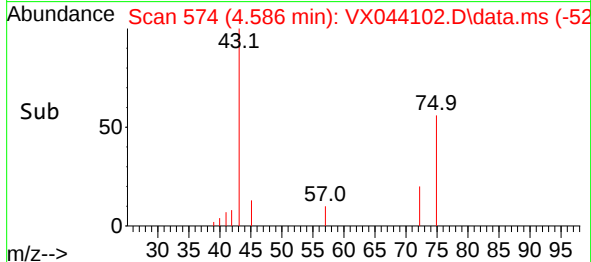

#27
cis-1,2-Dichloroethene
Concen: 0.384 ug/l
RT: 4.489 min Scan# 558
Delta R.T. 0.012 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46


Tgt Ion: 96 Resp: 591
Ion Ratio Lower Upper
96 100
61 94.4 0.0 297.4
98 84.1 0.0 127.8

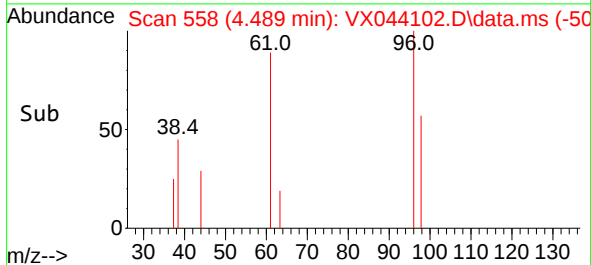






#31
Cyclohexane
Concen: 1.698 ug/l
RT: 5.544 min Scan# 717
Delta R.T. 0.085 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 3397
Ion Ratio Lower Upper
56 100
69 103.8 24.7 37.1#
84 85.8 68.7 103.1

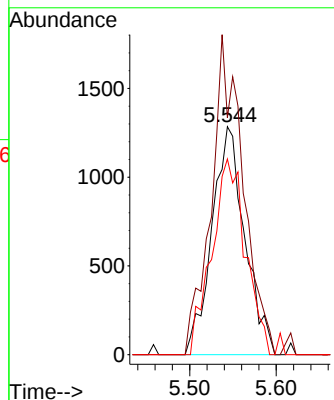

#33
1,2-Dichloroethane-d4
Concen: 52.425 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.006 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46

Tgt Ion: 65 Resp: 94124
Ion Ratio Lower Upper
65 100
67 50.9 0.0 100.8



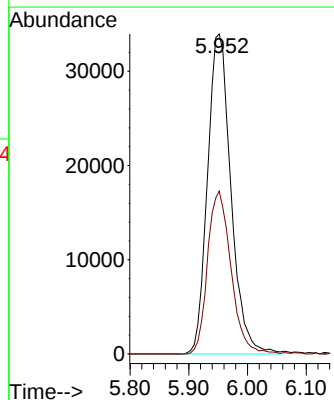
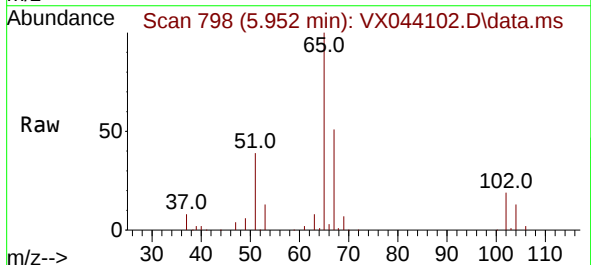




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 205665
Ion Ratio Lower Upper
114 100
63 21.6 0.0 44.0
88 16.3 0.0 32.4

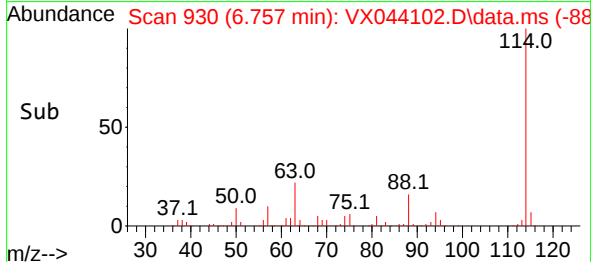

#35
Dibromofluoromethane
Concen: 35.980 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46

Tgt Ion:113 Resp: 52876
Ion Ratio Lower Upper
113 100
111 100.4 81.0 121.4
192 15.6 13.0 19.6

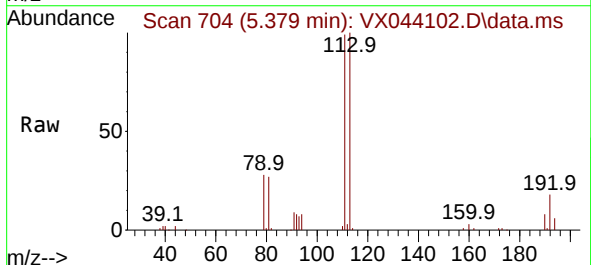



#36

1,1-Dichloropropene

Concen: 5.647 ug/l

RT: 5.537 min Scan# 711

Delta R.T. -0.141 min

Lab File: VX044102.D

Acq: 03 Dec 2024 18:46

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 75 Resp: 10342

Ion Ratio Lower Upper

75 100

110 5.3 17.4 52.2#

77 0.0 25.8 38.8#



#38

Carbon Tetrachloride

Concen: 6.122 ug/l

RT: 5.544 min Scan# 731

Delta R.T. -0.122 min

Lab File: VX044102.D

Acq: 03 Dec 2024 18:46




Tgt Ion: 117 Resp: 12597


Ion Ratio Lower Upper

117 100

119 1.9 75.2 112.8#

121 0.0 24.5 36.7#

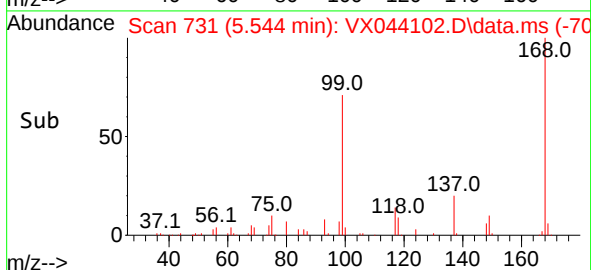

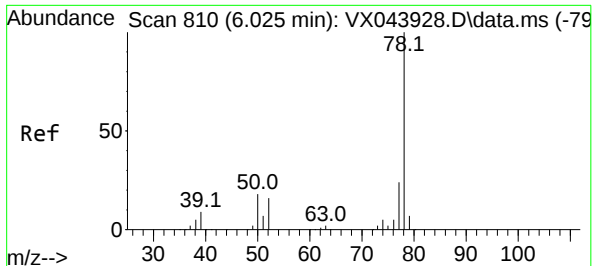

#40

Benzene

Concen: 2.463 ug/l

RT: 6.037 min Scan# 81

Delta R.T. 0.012 min

Lab File: VX044102.D

Acq: 03 Dec 2024 18:46

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 78 Resp: 14047

Ion Ratio Lower Upper

78 100

77 24.0 19.2 28.8

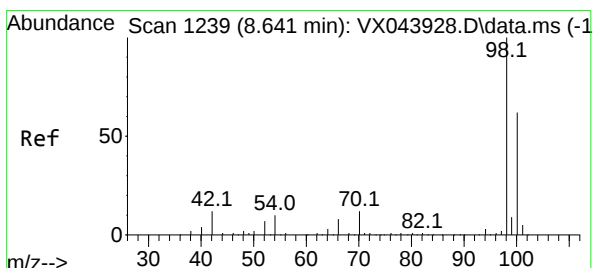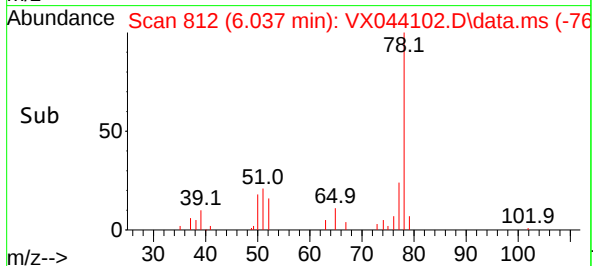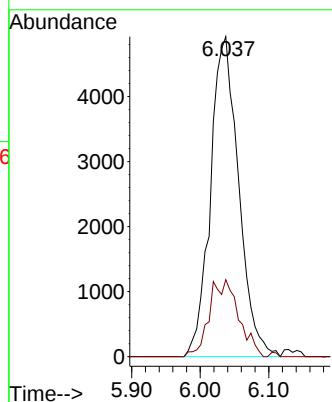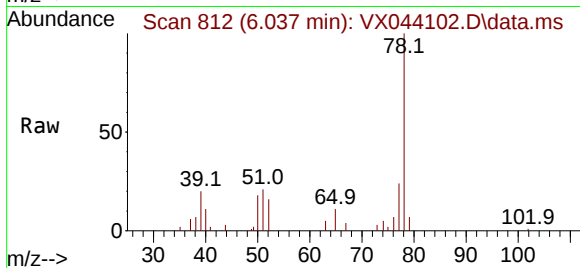

#50

Toluene-d8

Concen: 50.228 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.006 min

Lab File: VX044102.D




Acq: 03 Dec 2024 18:46


Tgt Ion: 98 Resp: 254444

Ion Ratio Lower Upper

98 100

100 65.2 52.6 79.0

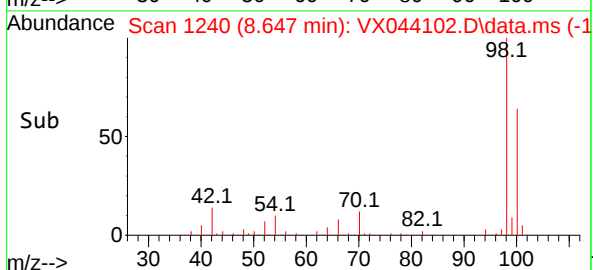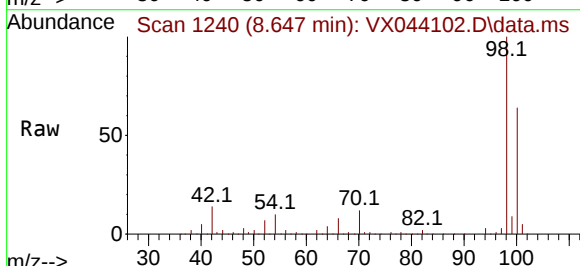



#51

4-Methyl-2-Pentanone

Concen: 0.504 ug/l

RT: 8.580 min Scan# 1113

Delta R.T. 0.006 min

Lab File: VX044102.D

Acq: 03 Dec 2024 18:46





Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 43 Resp: 1113

Ion	Ratio	Lower	Upper
43	100		
58	34.4	30.0	45.0

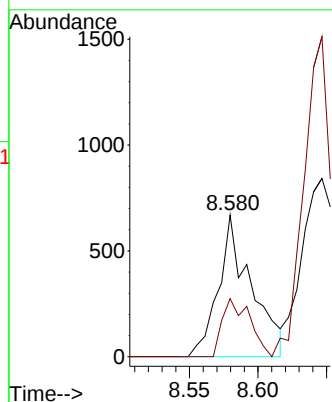

#52

Toluene

Concen: 2.577 ug/l

RT: 8.720 min Scan# 1252




Delta R.T. 0.006 min


Lab File: VX044102.D

Acq: 03 Dec 2024 18:46

Tgt Ion: 92 Resp: 8797

Ion	Ratio	Lower	Upper
92	100		
91	178.1	139.7	209.5


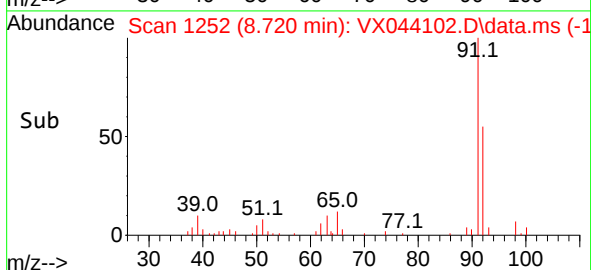






#62
4-Bromofluorobenzene
Concen: 52.657 ug/l
RT: 11.079 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 90782
Ion Ratio Lower Upper
95 100
174 71.2 0.0 150.4
176 67.8 0.0 146.0

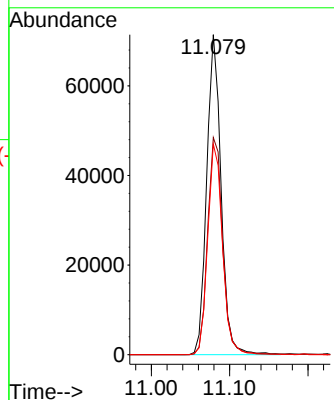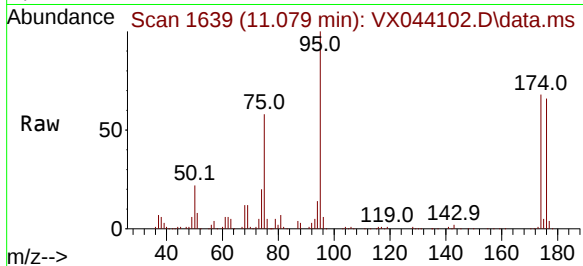

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.006 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46

Tgt Ion: 117 Resp: 184006
Ion Ratio Lower Upper
117 100
82 56.7 46.4 69.6
119 31.3 24.6 37.0

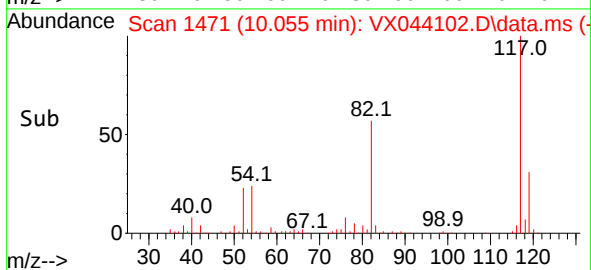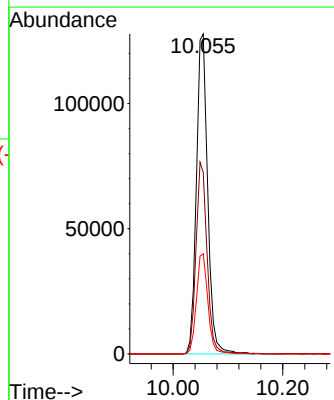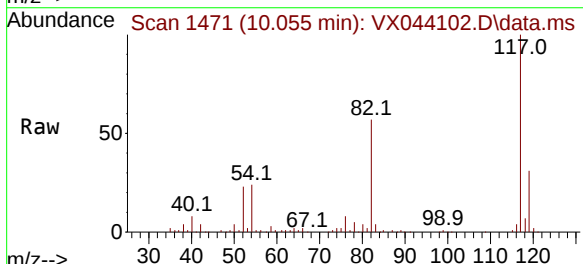



#67

Ethyl Benzene

Concen: 45.886 ug/l

RT: 10.195 min Scan# 1493

Delta R.T. 0.006 min

Lab File: VX044102.D

Acq: 03 Dec 2024 18:46

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 314227

Ion Ratio Lower Upper

91 100

106 30.0 23.6 35.4



#68

m/p-Xylenes

Concen: 9.675 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.000 min

Lab File: VX044102.D




Acq: 03 Dec 2024 18:46


Tgt Ion:106 Resp: 24707

Ion Ratio Lower Upper

106 100

91 207.3 168.1 252.1





#69

o-Xylene

Concen: 10.799 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. -0.000 min

Lab File: VX044102.D

Acq: 03 Dec 2024 18:46

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:106 Resp: 26925

Ion Ratio Lower Upper

106 100

91 226.9 110.2 330.6

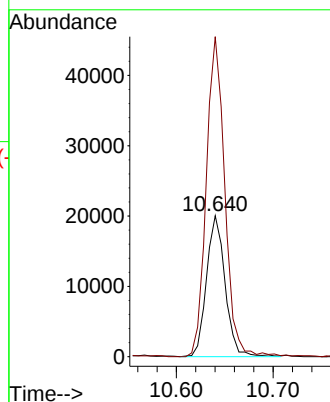

#70

Styrene

Concen: 0.465 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. -0.012 min

Lab File: VX044102.D

Acq: 03 Dec 2024 18:46




Tgt Ion:104 Resp: 1917


Ion Ratio Lower Upper

104 100

78 251.0 42.2 63.2#

103 211.4 44.7 67.1#

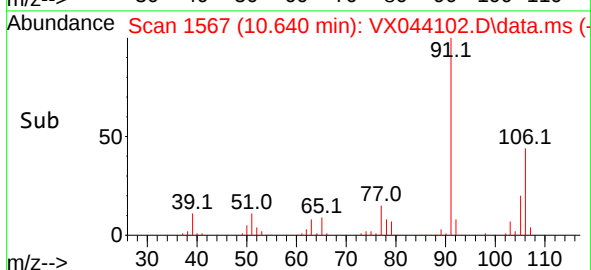

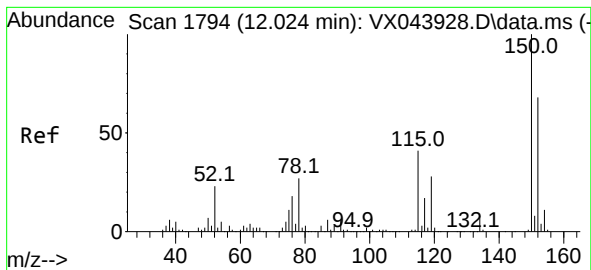

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX044102.D

Acq: 03 Dec 2024 18:46

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:152 Resp: 84942

Ion Ratio Lower Upper

152 100

115 62.9 45.4 136.2

150 153.5 0.0 353.0

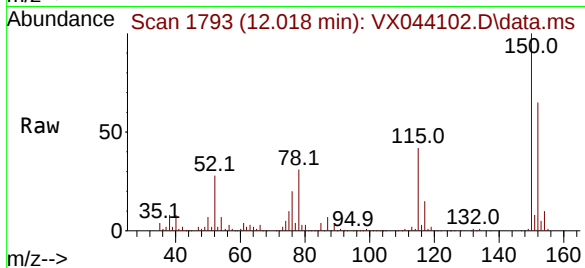

#73

Isopropylbenzene

Concen: 4.395 ug/l

RT: 10.963 min Scan# 1620

Delta R.T. 0.006 min

Lab File: VX044102.D




Acq: 03 Dec 2024 18:46


Tgt Ion:105 Resp: 28697

Ion Ratio Lower Upper

105 100

120 26.2 13.0 38.9


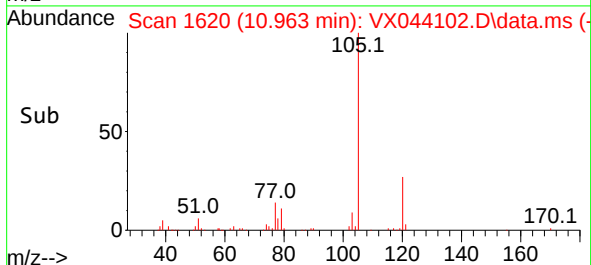
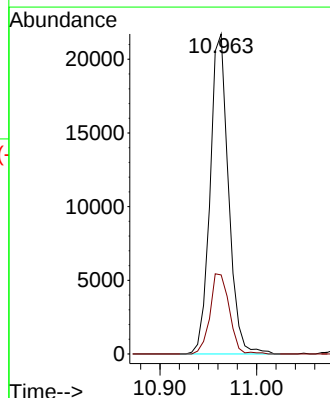
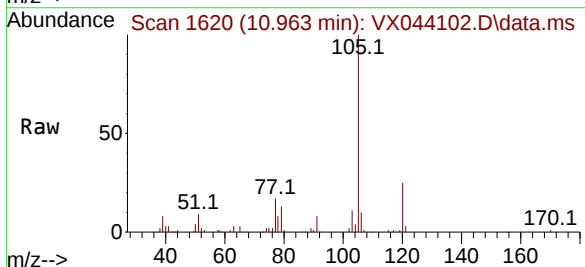




#76
1,2,3-Trichloropropane
Concen: 28.728 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 53514
Ion Ratio Lower Upper
75 100
77 1.3 21.8 65.3#

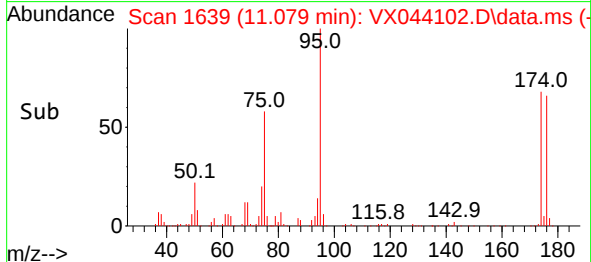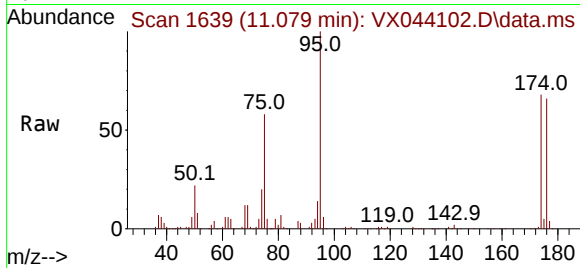

#78
n-propylbenzene
Concen: 1.978 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.006 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46

Tgt Ion: 91 Resp: 14426
Ion Ratio Lower Upper
91 100
120 22.4 11.5 34.4




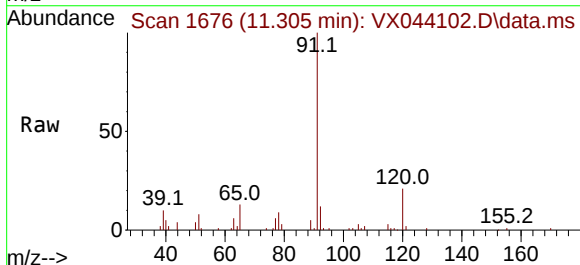




#79
2-Chlorotoluene
Concen: 1.681 ug/l
RT: 11.396 min Scan# 1
Delta R.T. 0.036 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 7751
Ion Ratio Lower Upper
91 100
126 1.8 16.6 49.8#

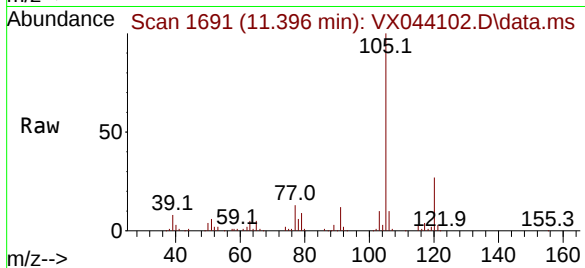

#80
1,3,5-Trimethylbenzene
Concen: 4.974 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46

Tgt Ion: 105 Resp: 26719
Ion Ratio Lower Upper
105 100
120 46.7 23.3 69.8




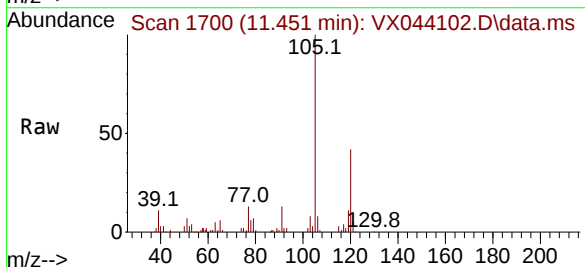




#81
trans-1,4-Dichloro-2-butene
Concen: 78.393 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 53514
Ion Ratio Lower Upper
75 100
53 0.0 86.7 130.1#
89 0.0 38.2 57.2#

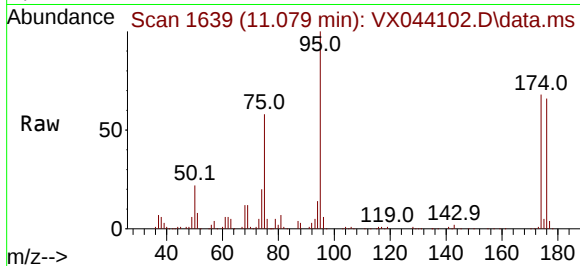

#82
4-Chlorotoluene
Concen: 0.702 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46

Tgt Ion: 91 Resp: 3657
Ion Ratio Lower Upper
91 100
126 0.0 14.3 42.9#

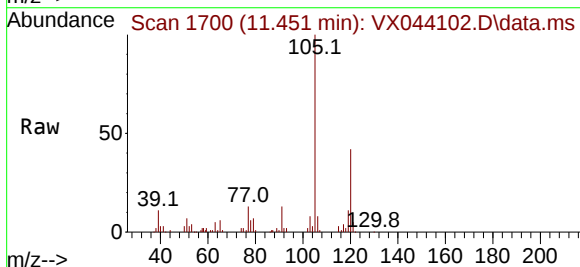



#83

tert-Butylbenzene

Concen: 1.349 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. 0.256 min

Lab File: VX044102.D

Acq: 03 Dec 2024 18:46

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:119 Resp: 7185

Ion Ratio Lower Upper

119 100

91 32.4 31.0 93.0

134 29.7 11.6 34.8

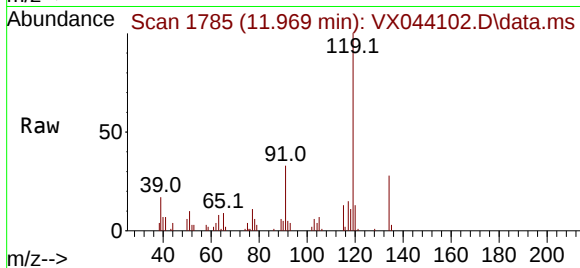

#84

1,2,4-Trimethylbenzene

Concen: 18.316 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX044102.D




Acq: 03 Dec 2024 18:46


Tgt Ion:105 Resp: 97956

Ion Ratio Lower Upper

105 100

120 42.5 21.9 65.7




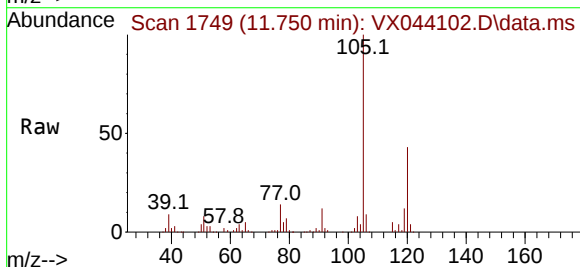




#85
 sec-Butylbenzene
 Concen: 15.016 ug/l
 RT: 11.750 min Scan# 1749
 Delta R.T. -0.140 min
 Lab File: VX044102.D
 Acq: 03 Dec 2024 18:46




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:105 Resp: 97956
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.7 29.1#



#86
 p-Isopropyltoluene
 Concen: 0.975 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. 0.006 min
 Lab File: VX044102.D
 Acq: 03 Dec 2024 18:46

Tgt Ion:119 Resp: 5165
 Ion Ratio Lower Upper
 119 100
 134 27.9 13.0 38.9
 91 0.0 13.0 38.9#

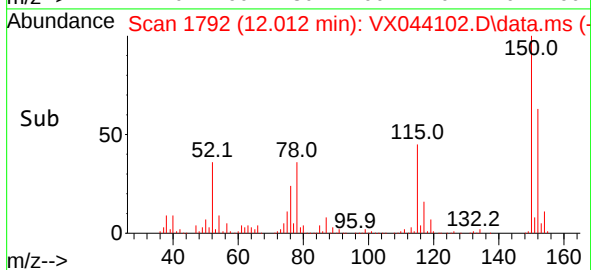



#89

n-Butylbenzene

Concen: 1.226 ug/l

RT: 12.317 min Scan# 11

Delta R.T. -0.012 min

Lab File: VX044102.D





Acq: 03 Dec 2024 18:46

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 91	Resp: 5728
Ion Ratio	Lower Upper
91	100
92	21.1 26.6 79.8#
134	116.0 12.4 37.2#

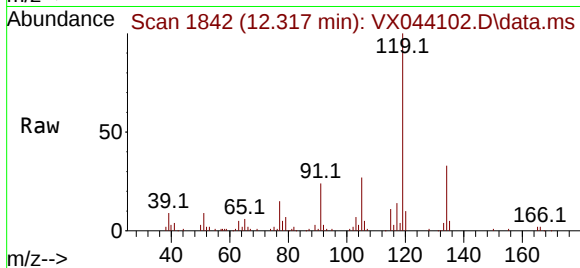

#90

Hexachloroethane

Concen: 52.766 ug/l




RT: 12.695 min Scan# 1904


Delta R.T. 0.158 min

Lab File: VX044102.D

Acq: 03 Dec 2024 18:46

Tgt Ion: 117	Resp: 47545
Ion Ratio	Lower Upper
117	100
201	0.0 32.4 97.0#


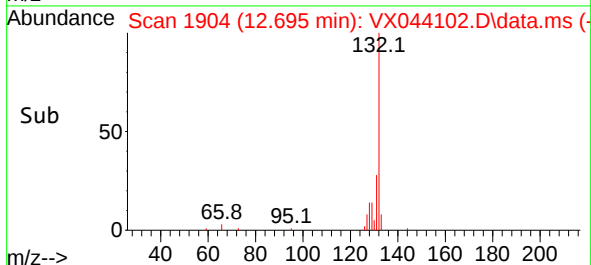
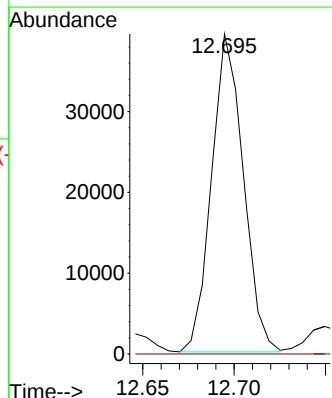
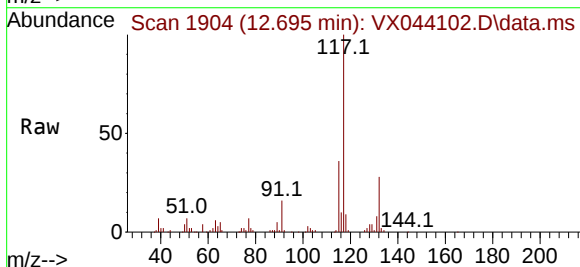




#92
1,2-Dibromo-3-Chloropropane
Concen: 1.272 ug/l
RT: 12.957 min Scan# 1944
Delta R.T. 0.018 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 75 Resp: 570
Ion Ratio Lower Upper
75 100
155 0.0 40.1 120.2#
157 0.0 49.6 149.0#

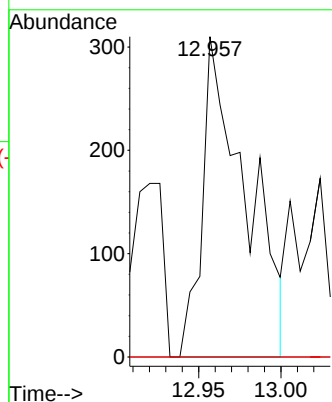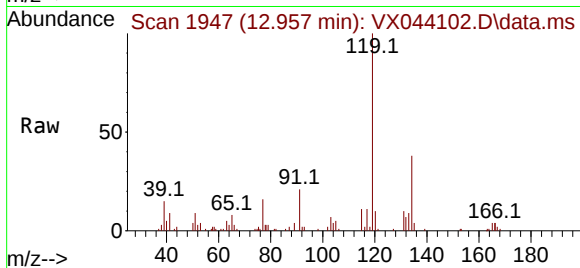

#95
Naphthalene
Concen: 780.590 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX044102.D
Acq: 03 Dec 2024 18:46

Tgt Ion:128 Resp: 4742702
Ion Ratio Lower Upper
128 100
127 13.2 10.2 15.2
129 11.4 8.6 12.8

