

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120324\
 Data File : VX044089.D
 Acq On : 03 Dec 2024 13:47
 Operator : JC/MD
 Sample : P5006-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SPLP-C4-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
 Title : SW846 8260

Signal : TIC: VX044089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.612	69	86	88	rBV6	16207	72353	3.08%	0.956%
2	2.380	206	212	221	rBV	15089	27324	1.16%	0.361%
3	5.379	694	704	720	rBV	66758	204479	8.71%	2.703%
4	5.544	720	731	749	rVV	131888	379019	16.15%	5.010%
5	5.946	786	797	808	rBV2	102304	282639	12.05%	3.736%
6	6.757	920	930	953	rBV	217050	548088	23.36%	7.244%
7	8.647	1233	1240	1249	rBV	453825	743677	31.69%	9.830%
8	10.049	1464	1470	1483	rBV	467459	657582	28.03%	8.692%
9	10.195	1489	1494	1501	rVB	35411	49874	2.13%	0.659%
10	11.079	1634	1639	1654	rBV	377693	488556	20.82%	6.458%
11	11.750	1744	1749	1754	rBV	26553	35855	1.53%	0.474%
12	12.018	1788	1793	1801	rBV	481311	605470	25.80%	8.003%
13	12.238	1821	1829	1839	rBV	310154	411118	17.52%	5.434%
14	13.164	1977	1981	1987	rBV	17754	24396	1.04%	0.322%
15	13.426	2018	2024	2032	rBV	62844	86185	3.67%	1.139%
16	13.774	2076	2081	2091	rBV	1948057	2346358	100.00%	31.013%
17	13.865	2091	2096	2103	rVB	52129	70011	2.98%	0.925%
18	14.634	2218	2222	2233	rVB	88518	116564	4.97%	1.541%
19	14.780	2240	2246	2258	rVB	207930	279198	11.90%	3.690%
20	15.615	2374	2383	2387	rBV	14433	26721	1.14%	0.353%
21	16.328	2492	2500	2514	rBV	58256	110193	4.70%	1.456%




Sum of corrected areas: 7565660

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120324\
Data File : VX044089.D
Acq On : 03 Dec 2024 13:47
Operator : JC/MD
Sample : P5006-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPLP-C4-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

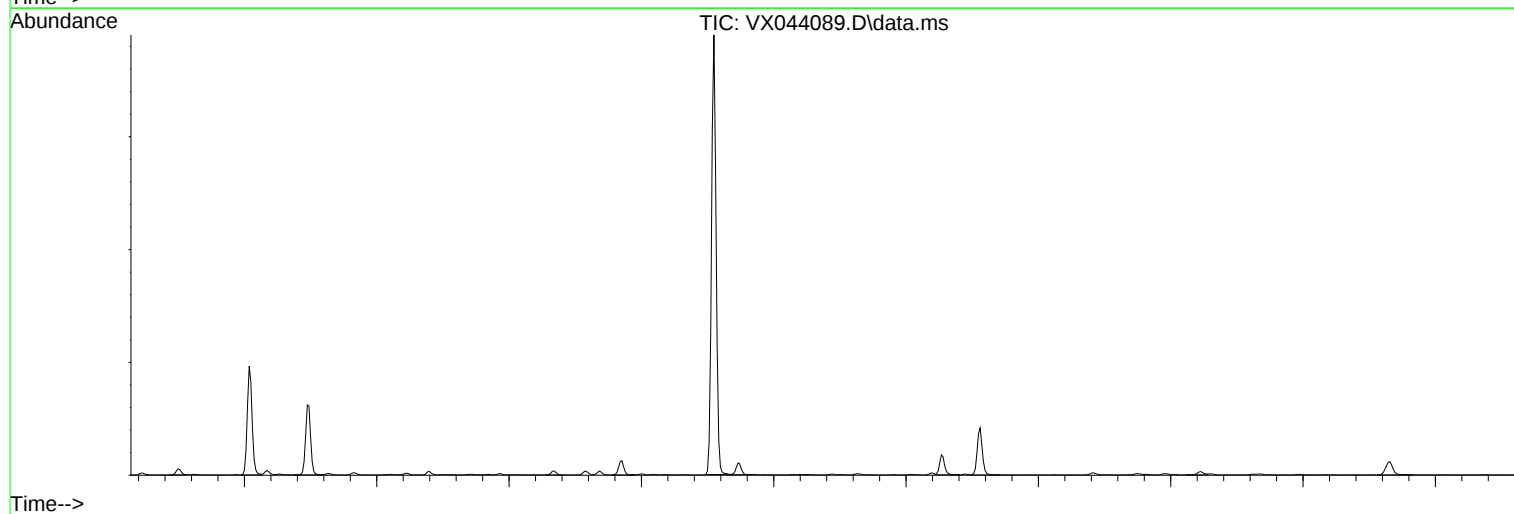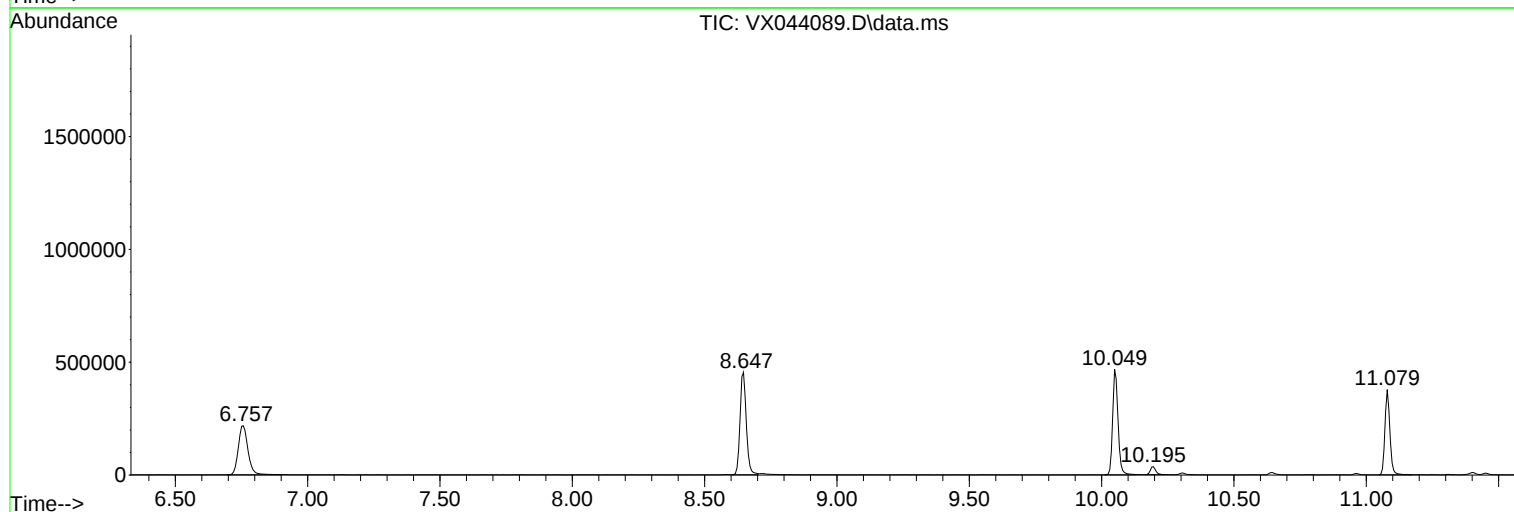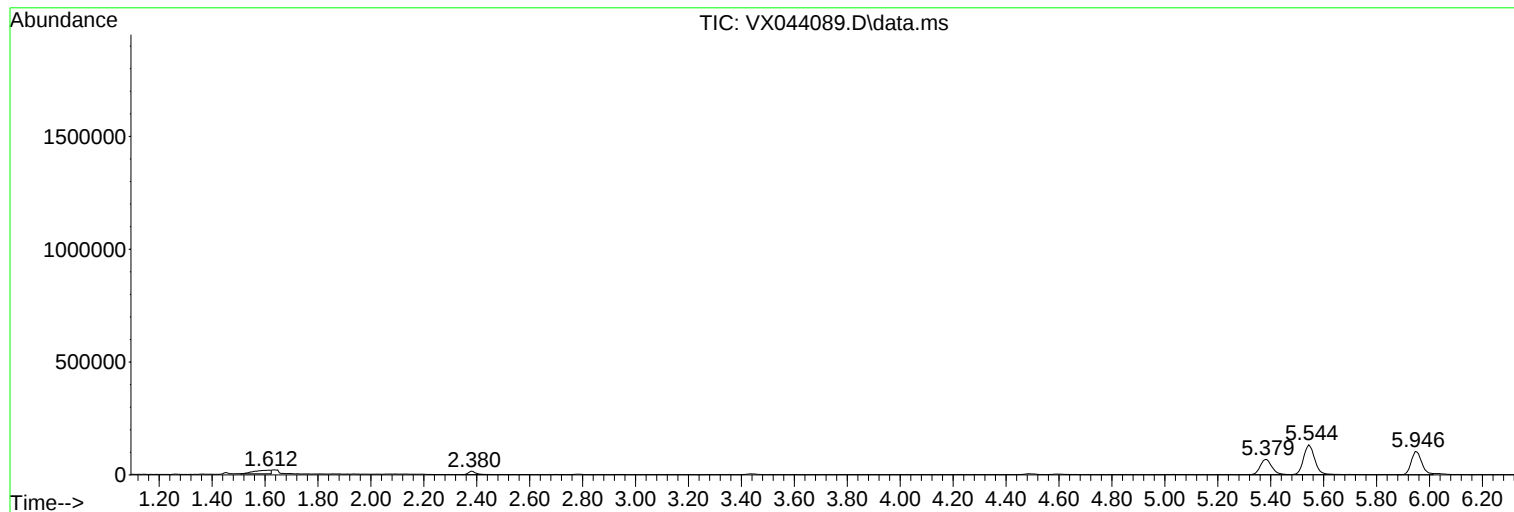

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120324\
Data File : VX044089.D
Acq On : 03 Dec 2024 13:47
Operator : JC/MD
Sample : P5006-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPLP-C4-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120324\
Data File : VX044089.D
Acq On : 03 Dec 2024 13:47
Operator : JC/MD
Sample : P5006-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPLP-C4-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------