

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
 Data File : VX044433.D
 Acq On : 19 Dec 2024 14:02
 Operator : JC/MD
 Sample : P5258-12ME
 Misc : 5.99g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 20 02:31:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 18 04:40:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	226586	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	198648	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	79907	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	95175	45.900	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.800%
7) Chloroethane-d5	1.648	69	78989	49.176	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.360%
11) 1,1-Dichloroethene-d2	2.294	65	37033	41.761	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.520%
21) 2-Butanone-d5	4.458	46	105691	83.253	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	83.250%
24) Chloroform-d	5.050	84	161326	40.977	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.960%
26) 1,2-Dichloroethane-d4	5.946	65	111482	40.041	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.080%
32) Benzene-d6	5.964	84	312669	45.553	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.100%
36) 1,2-Dichloropropane-d6	7.299	67	96263	45.166	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.340%
41) Toluene-d8	8.647	98	272672	42.964	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.920%
43) trans-1,3-Dichloroprop...	8.945	79	37397	36.513	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.020%
47) 2-Hexanone-d5	9.384	63	69931	84.152	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.150%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	121688	42.581	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.160%
66) 1,2-Dichlorobenzene-d4	12.317	152	87210	46.842	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.680%
Target Compounds						
61) 1,2,3-Trichloropropane	12.018	75	11498	6.213	ug/L	Qvalue # 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
Data File : VX044433.D
Acq On : 19 Dec 2024 14:02
Operator : JC/MD
Sample : P5258-12ME
Misc : 5.99g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Dec 20 02:31:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 04:40:20 2024
Response via : Initial Calibration

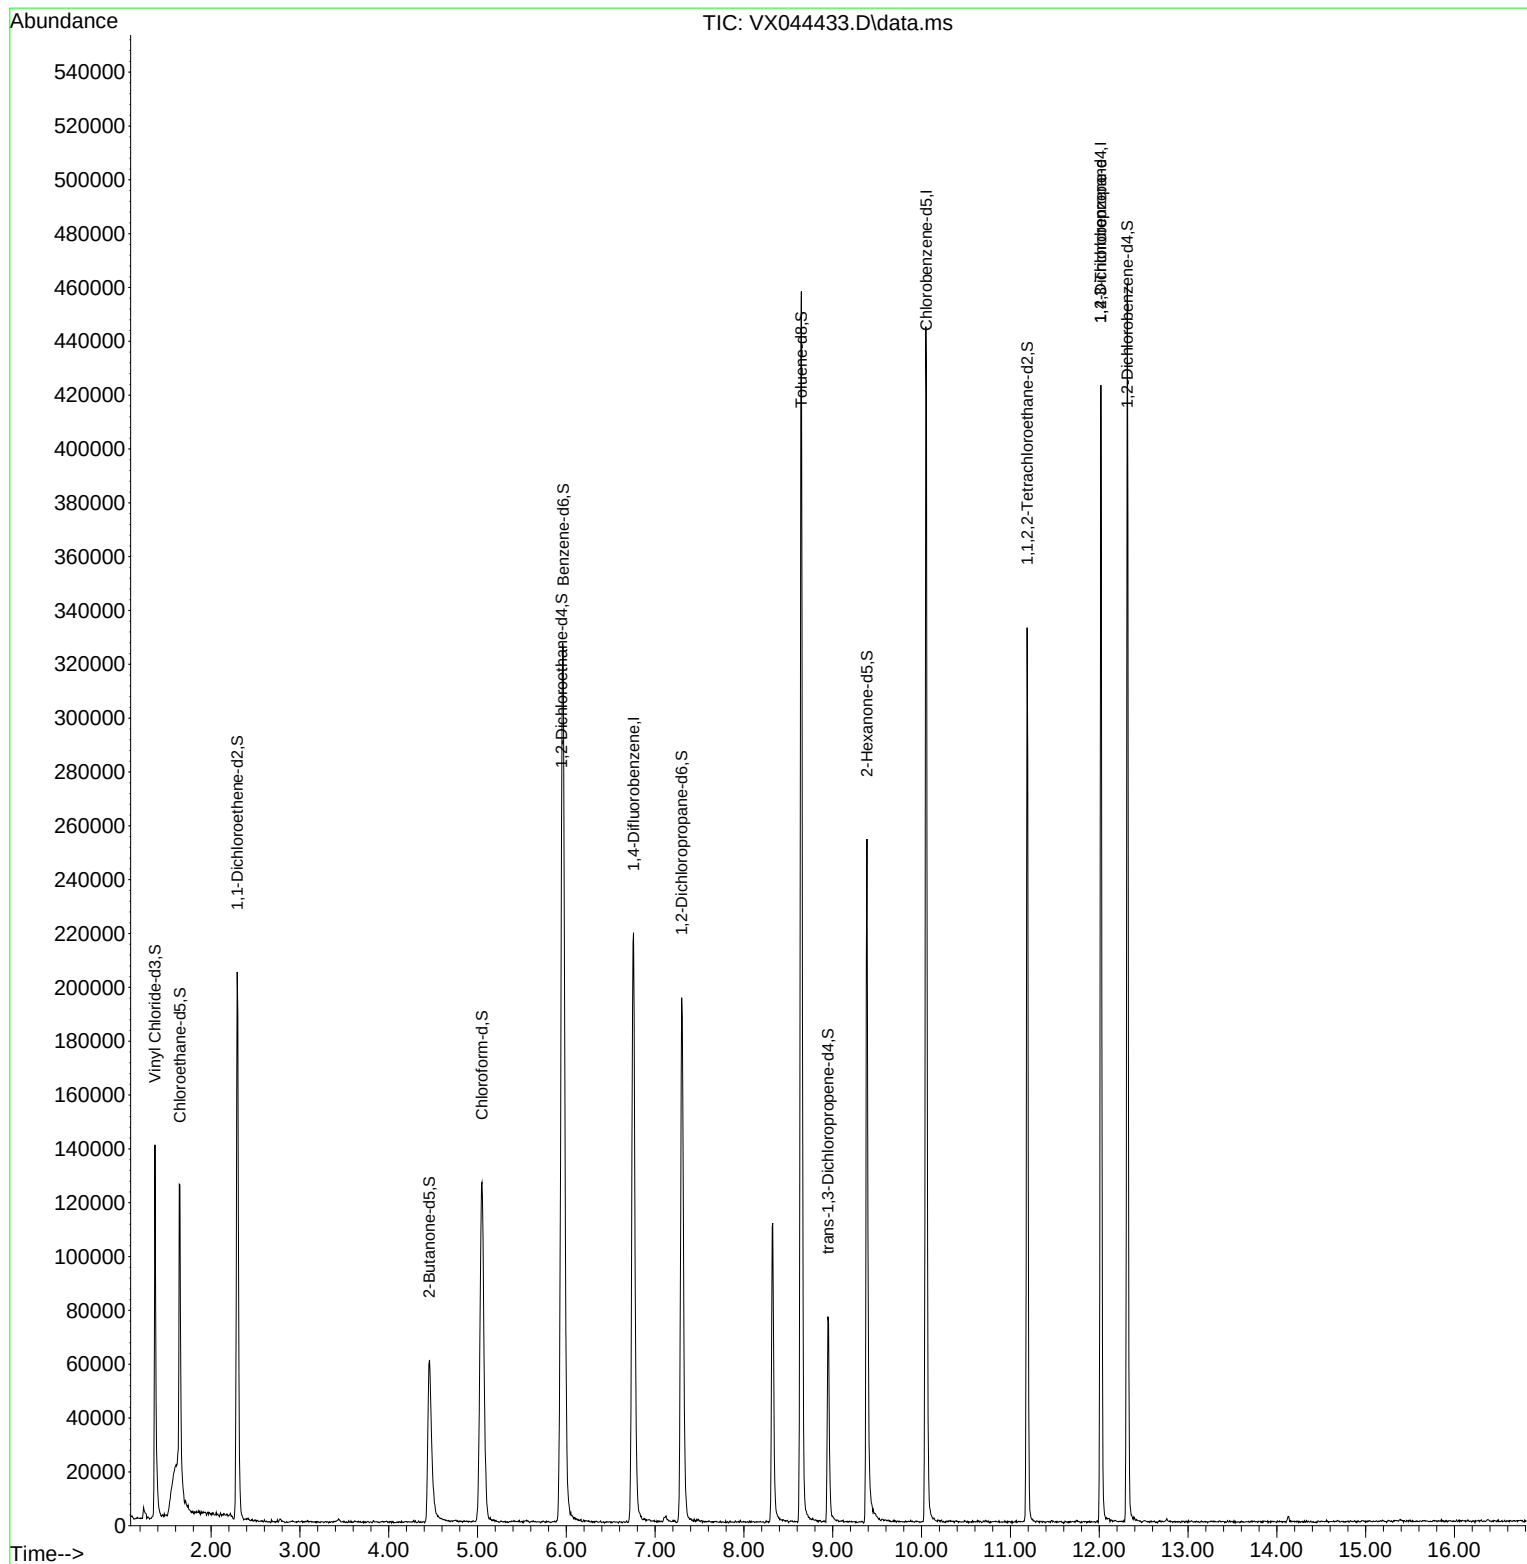

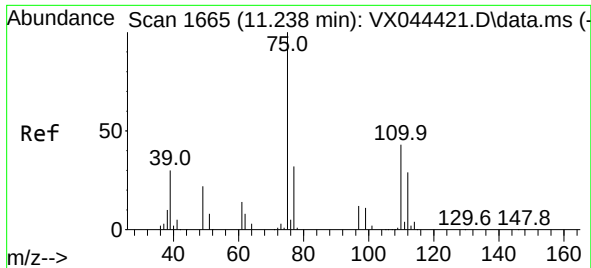

#61
 1,2,3-Trichloropropane
 Concen: 6.213 ug/L
 RT: 12.018 min Scan# 11
 Delta R.T. 0.780 min
 Lab File: VX044433.D
 Acq: 19 Dec 2024 14:02

Instrument :
 MSVOA_X
 ClientSampleId :

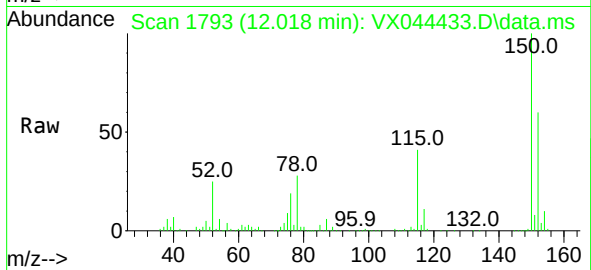

Tgt Ion:	75	Resp:	11498
Ion	Ratio	Lower	Upper
75	100		
77	31.0	25.8	38.6
110	4.7	33.3	49.9#

