




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
Data File : VX044428.D
Acq On : 19 Dec 2024 11:56
Operator : JC/MD
Sample : P5265-01ME
Misc : 3.40g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E28Y6ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
Supervised By :Mahesh Dadoda 12/23/2024

Quant Time: Dec 20 02:30:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 04:40:20 2024
Response via : Initial Calibration

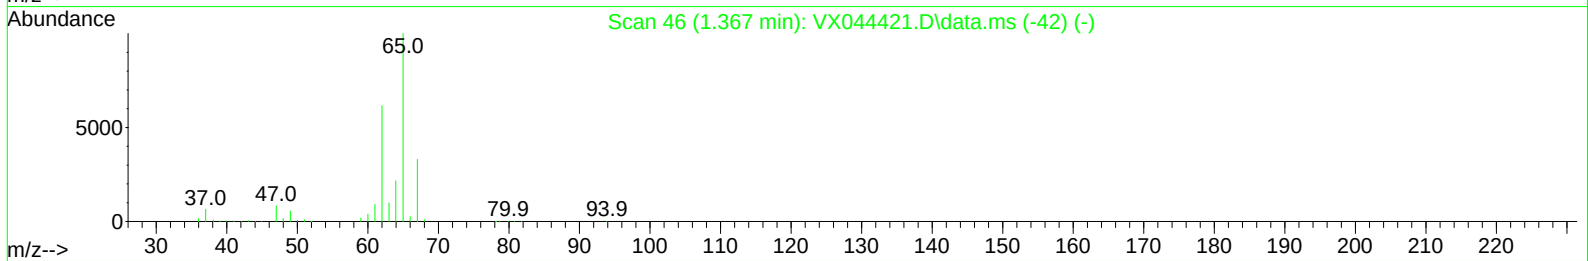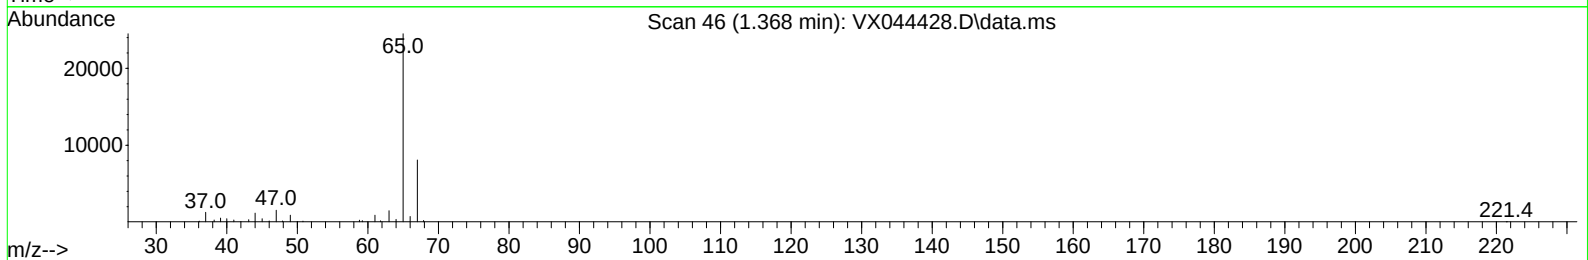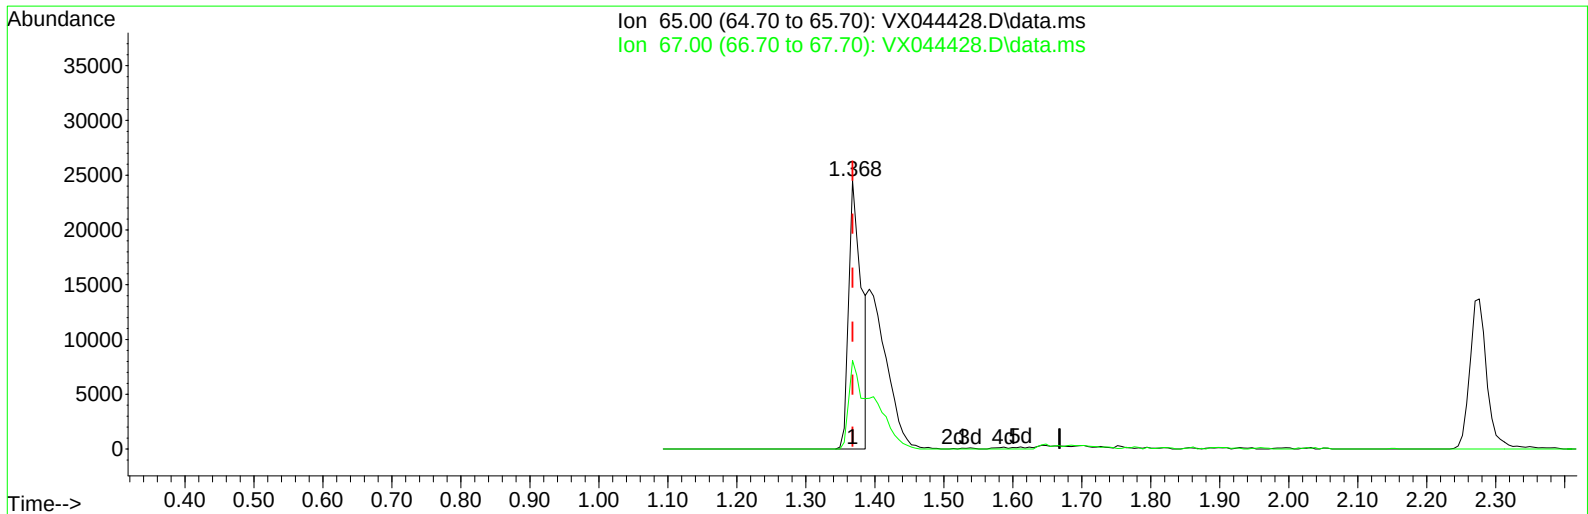

TIC: VX044428.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.368min (+ 0.000) 16.43 ug/L

response 32117

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	32.10	32.97
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
Data File : VX044428.D
Acq On : 19 Dec 2024 11:56
Operator : JC/MD
Sample : P5265-01ME
Misc : 3.40g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E28Y6ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
Supervised By :Mahesh Dadoda 12/23/2024

Quant Time: Dec 20 02:30:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 04:40:20 2024
Response via : Initial Calibration

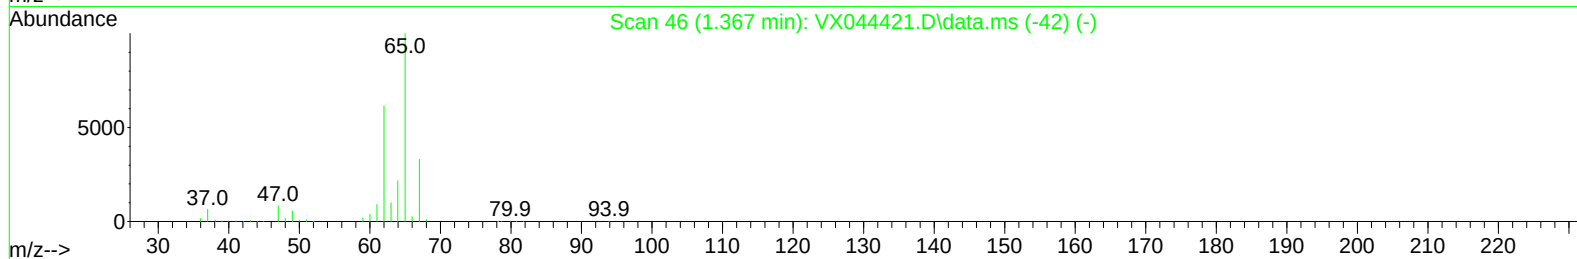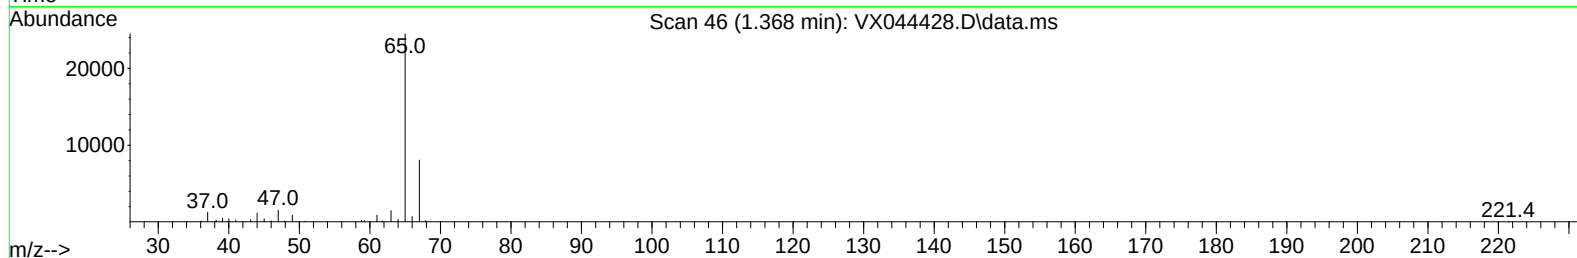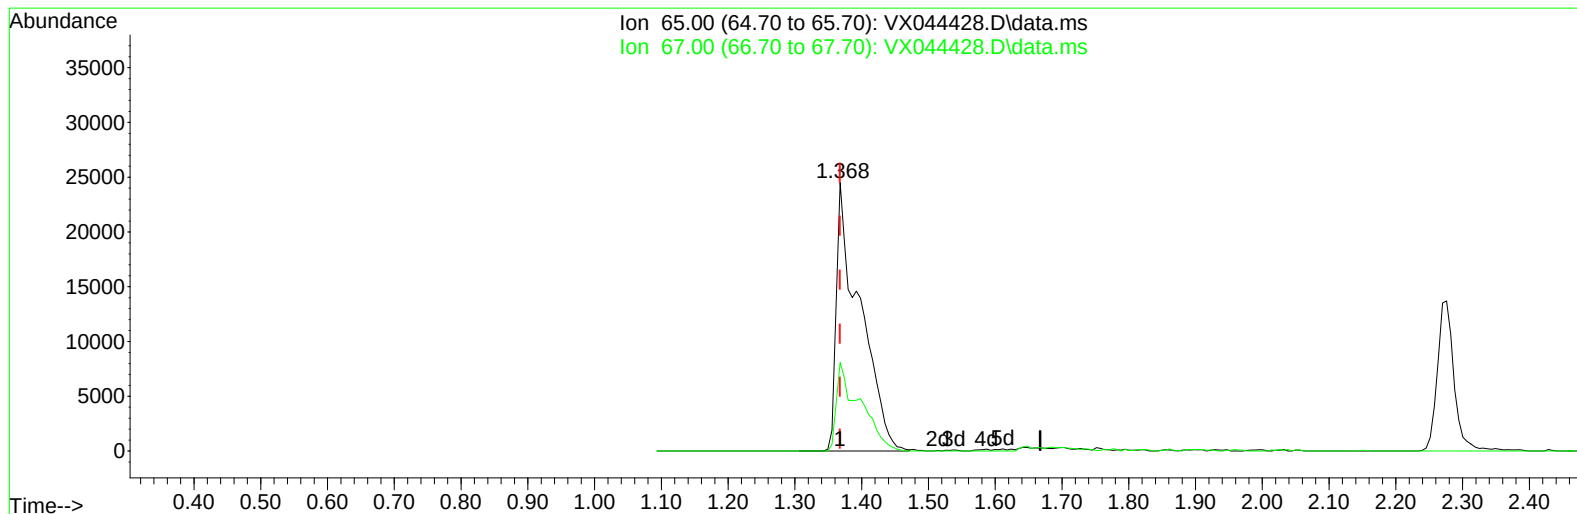

TIC: VX044428.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.368min (+ 0.000) 30.57 ug/L m

response 59755

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	32.10	17.72#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
Data File : VX044428.D
Acq On : 19 Dec 2024 11:56
Operator : JC/MD
Sample : P5265-01ME
Misc : 3.40g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E28Y6ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
Supervised By :Mahesh Dadoda 12/23/2024

Quant Time: Dec 20 02:30:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 04:40:20 2024
Response via : Initial Calibration

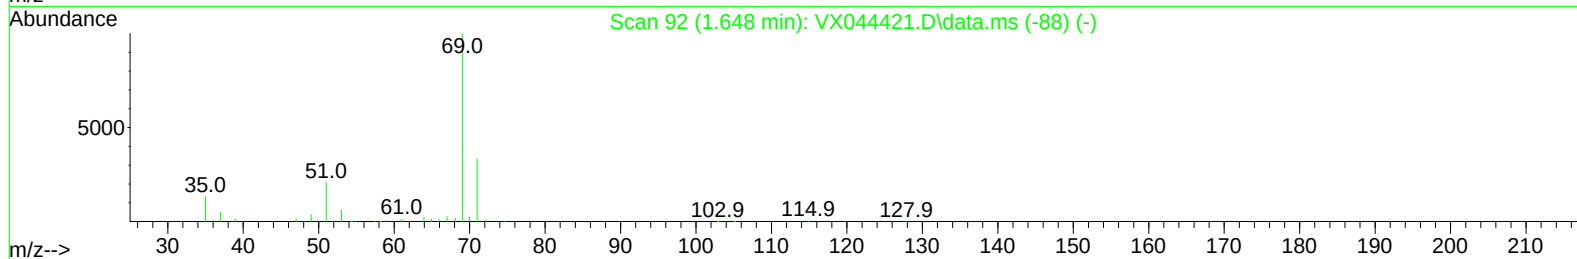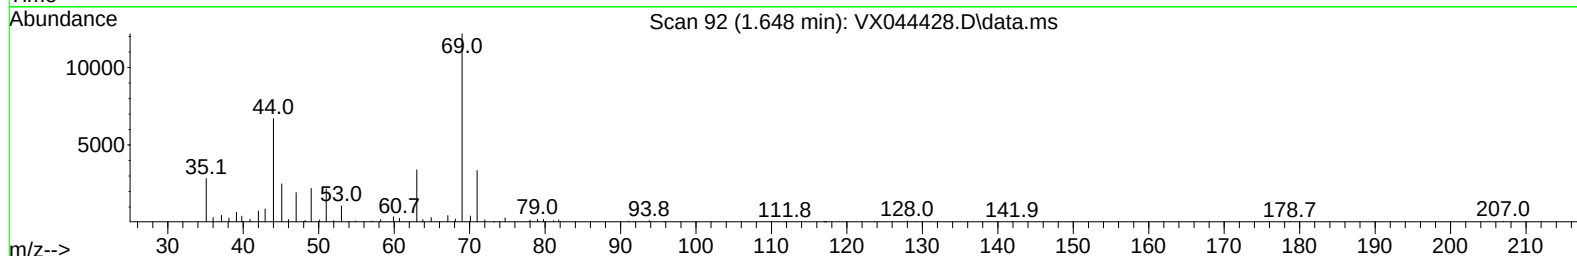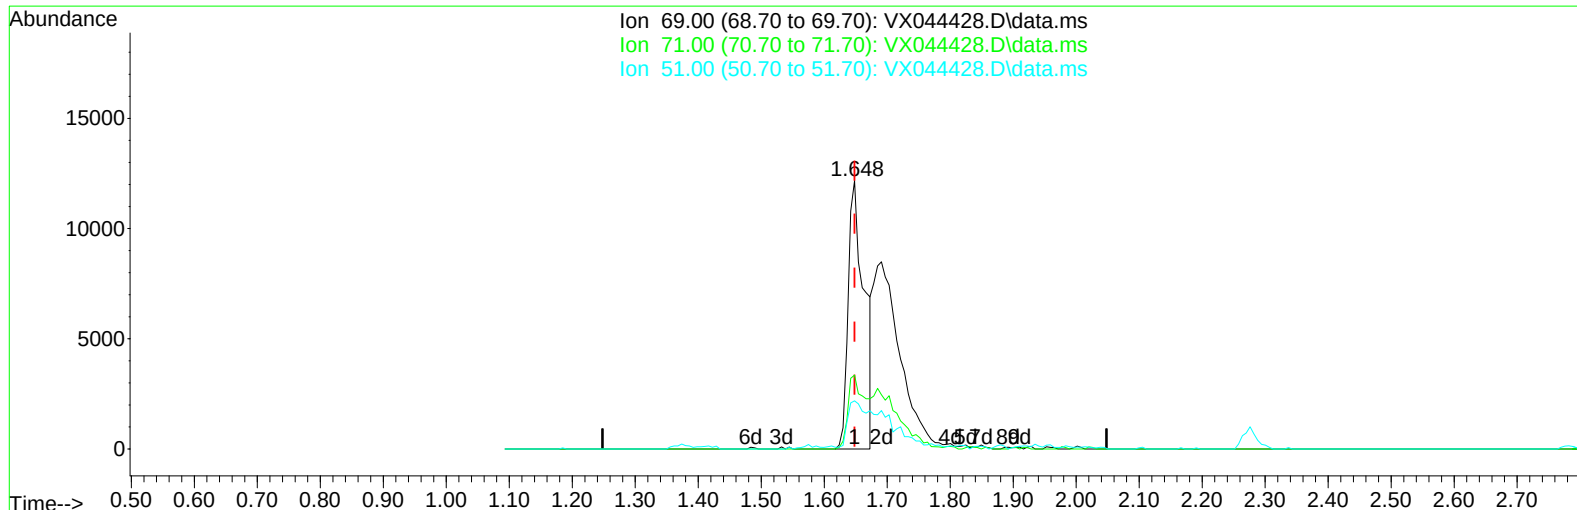

TIC: VX044428.D\data.ms

(7) Chloroethane-d5 (S)

1.648min (+ 0.000) 14.19 ug/L

response 21478

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	30.31
51.00	28.20	17.73#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
Data File : VX044428.D
Acq On : 19 Dec 2024 11:56
Operator : JC/MD
Sample : P5265-01ME
Misc : 3.40g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E28Y6ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
Supervised By :Mahesh Dadoda 12/23/2024

Quant Time: Dec 20 02:30:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 04:40:20 2024
Response via : Initial Calibration

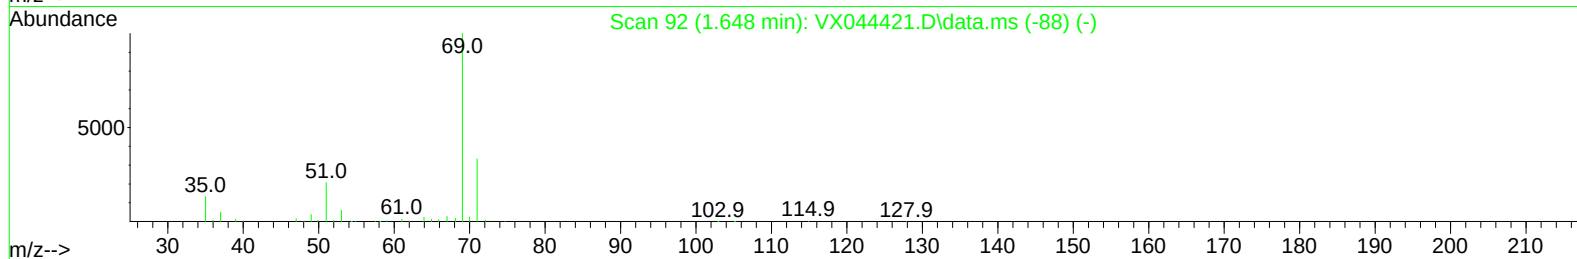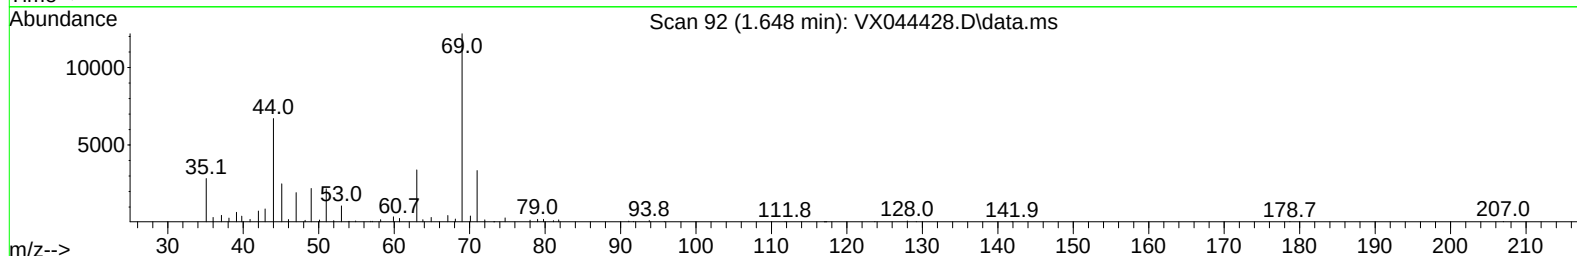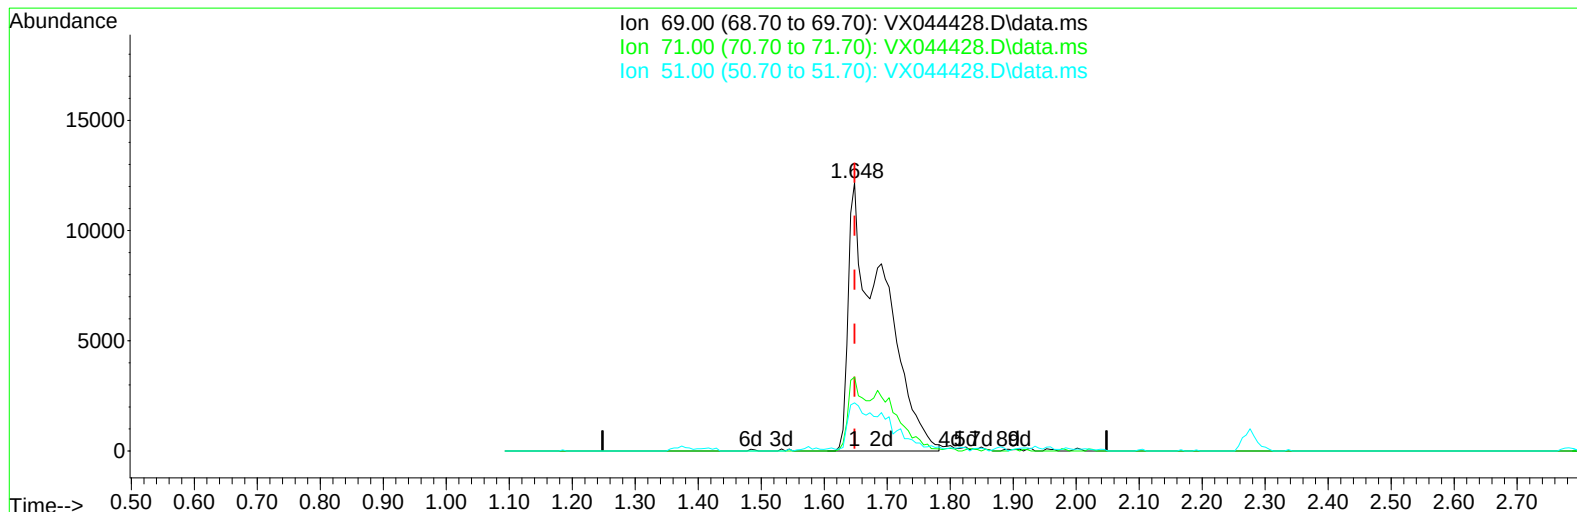

TIC: VX044428.D\data.ms

(7) Chloroethane-d5 (S)

1.648min (+ 0.000) 30.65 ug/L m

response 46407

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	14.03#
51.00	28.20	8.21#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
 Data File : VX044428.D
 Acq On : 19 Dec 2024 11:56
 Operator : JC/MD
 Sample : P5265-01ME
 Misc : 3.40g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E28Y6ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
 Supervised By :Mahesh Dadoda 12/23/2024

Quant Time: Dec 20 02:30:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 18 04:40:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	213576	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	187319	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	83663	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	59755m	30.573	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	61.140%		
7) Chloroethane-d5	1.648	69	46407m	30.652	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	61.300%#		
11) 1,1-Dichloroethene-d2	2.276	65	23603	28.238	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	56.480%#		
21) 2-Butanone-d5	4.483	46	101799	85.072	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	85.070%		
24) Chloroform-d	5.050	84	137725	37.113	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	74.220%		
26) 1,2-Dichloroethane-d4	5.952	65	98738	37.624	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	75.240%		
32) Benzene-d6	5.964	84	256526	39.634	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	79.260%		
36) 1,2-Dichloropropane-d6	7.306	67	83603	41.599	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	83.200%		
41) Toluene-d8	8.647	98	222922	37.249	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	74.500%#		
43) trans-1,3-Dichloroprop...	8.952	79	31971	33.103	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.200%		
47) 2-Hexanone-d5	9.391	63	70115	89.476	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	89.480%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	120794	44.824	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.640%		
66) 1,2-Dichlorobenzene-d4	12.317	152	85954	44.095	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.180%		
Target Compounds						Qvalue
15) Methyl Acetate	2.721	43	17445	10.103	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
Data File : VX044428.D
Acq On : 19 Dec 2024 11:56
Operator : JC/MD
Sample : P5265-01ME
Misc : 3.40g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E28Y6ME

Manual IntegrationsAPPROVED

Quant Time: Dec 20 02:30:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 04:40:20 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/23/2024
Supervised By :Mahesh Dadoda 12/23/2024

