

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
 Data File : VX044428.D
 Acq On : 19 Dec 2024 11:56
 Operator : JC/MD
 Sample : P5265-01ME
 Misc : 3.40g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E28Y6ME

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
 Supervised By :Mahesh Dadoda 12/23/2024

Quant Time: Dec 20 02:30:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 18 04:40:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	213576	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	187319	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	83663	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	59755m	30.573	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	61.140%
7) Chloroethane-d5	1.648	69	46407m	30.652	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	61.300%#
11) 1,1-Dichloroethene-d2	2.276	65	23603	28.238	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	56.480%#
21) 2-Butanone-d5	4.483	46	101799	85.072	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.070%
24) Chloroform-d	5.050	84	137725	37.113	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	74.220%
26) 1,2-Dichloroethane-d4	5.952	65	98738	37.624	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.240%
32) Benzene-d6	5.964	84	256526	39.634	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.260%
36) 1,2-Dichloropropane-d6	7.306	67	83603	41.599	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	83.200%
41) Toluene-d8	8.647	98	222922	37.249	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	74.500%#
43) trans-1,3-Dichloroprop...	8.952	79	31971	33.103	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.200%
47) 2-Hexanone-d5	9.391	63	70115	89.476	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.480%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	120794	44.824	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.640%
66) 1,2-Dichlorobenzene-d4	12.317	152	85954	44.095	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.180%
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.721	43	17445	10.103	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
Data File : VX044428.D
Acq On : 19 Dec 2024 11:56
Operator : JC/MD
Sample : P5265-01ME
Misc : 3.40g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
E28Y6ME

Quant Time: Dec 20 02:30:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 04:40:20 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 12/23/2024
Supervised By : Mahesh Dadoda 12/23/2024

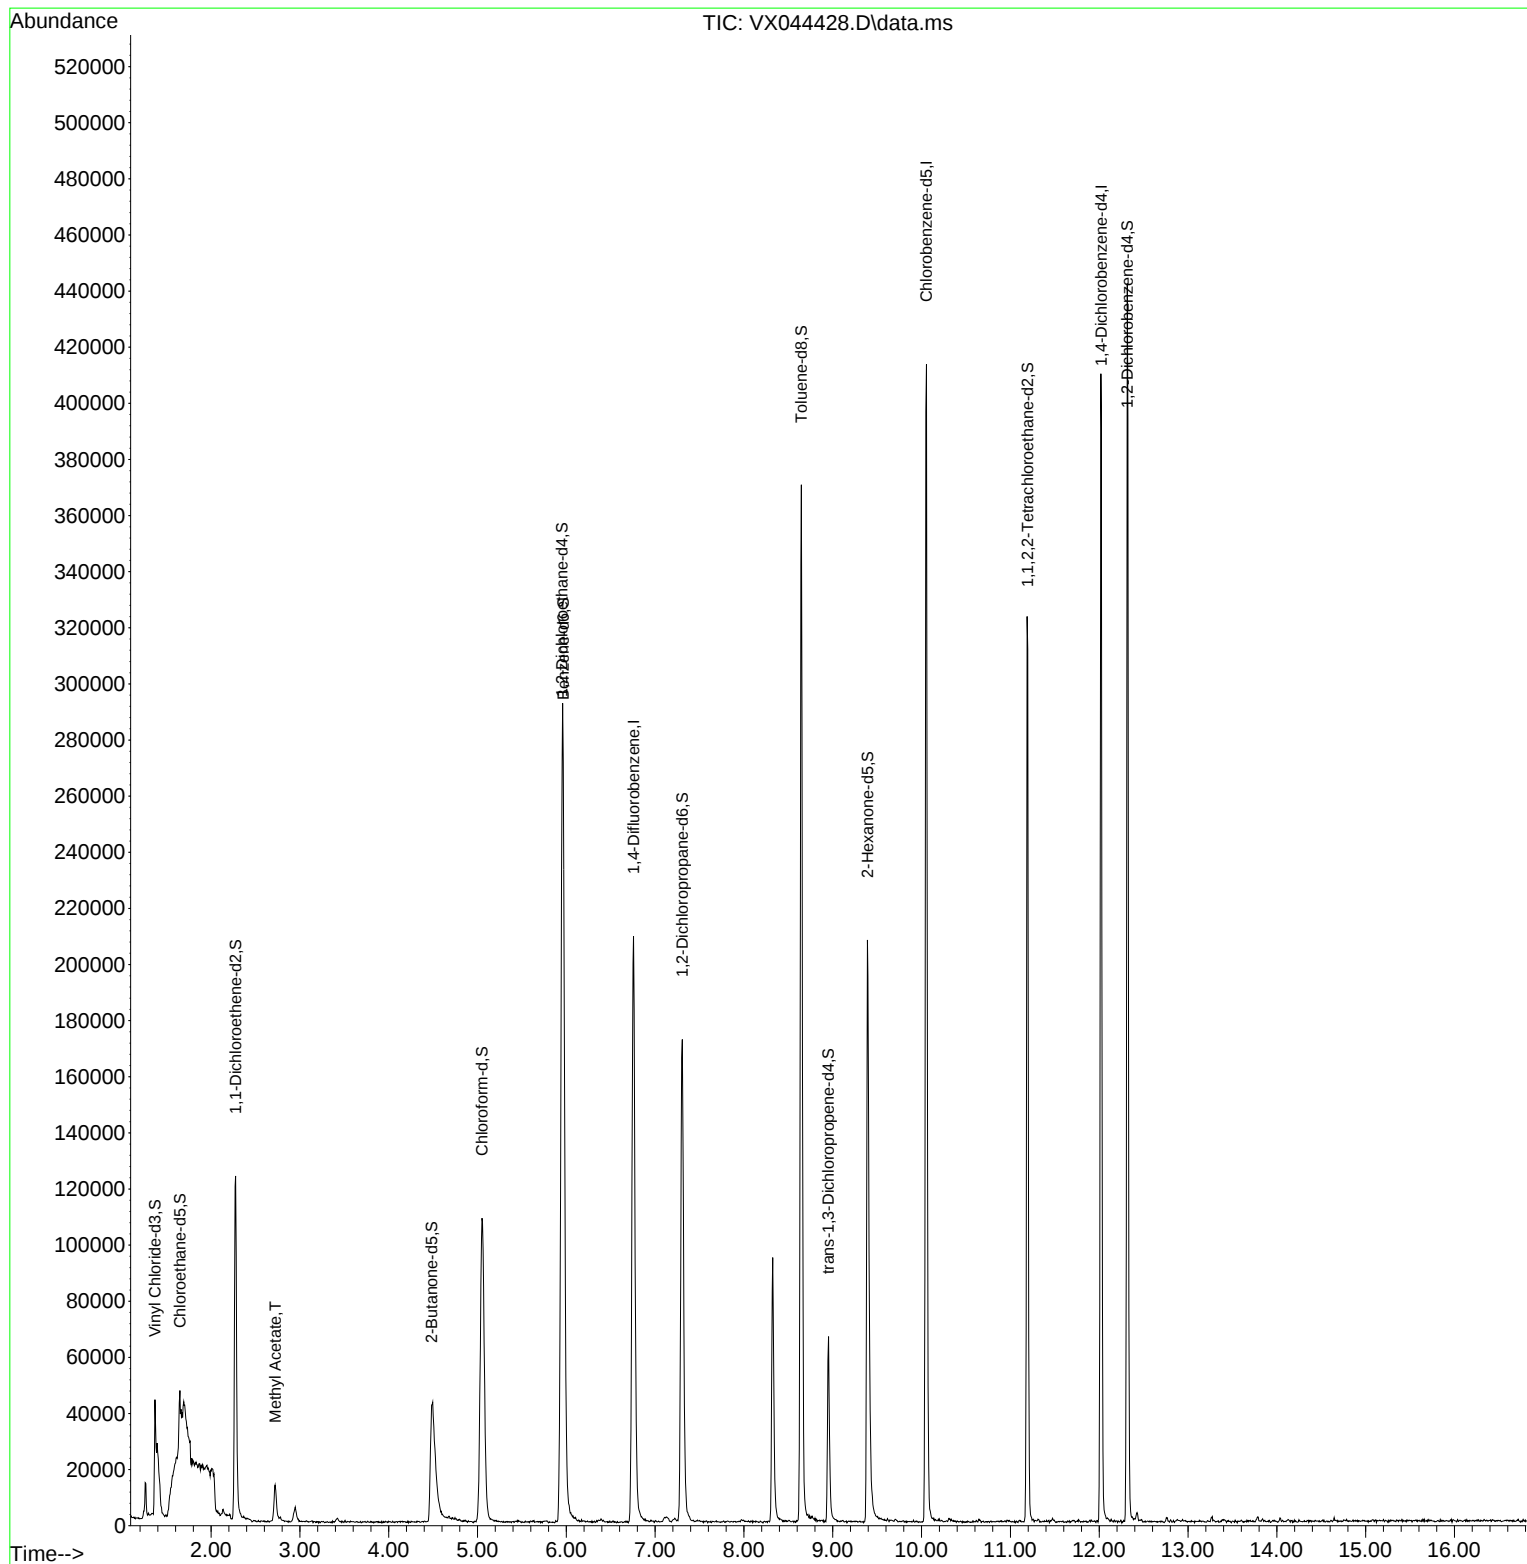

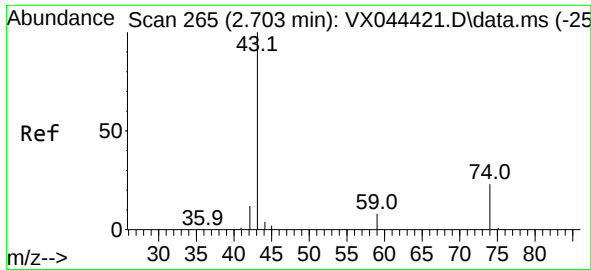

#15
Methyl Acetate
Concen: 10.103 ug/L
RT: 2.721 min Scan# 20
Delta R.T. 0.018 min
Lab File: VX044428.D
Acq: 19 Dec 2024 11:56

Instrument :
MSVOA_X
ClientSampleId :
E28Y6ME

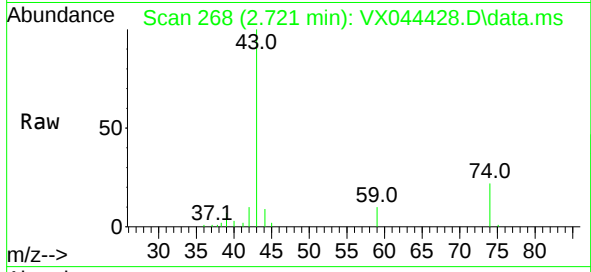

Tgt Ion: 43 Resp: 1744
Ion Ratio Lower Upper
43 100
74 22.4 19.4 29.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
Supervised By :Mahesh Dadoda 12/23/2024

