

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
 Data File : VX044424.D
 Acq On : 19 Dec 2024 10:26
 Operator : JC/MD
 Sample : P5235-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV2	5810	5633	0.58%	0.084%
2	1.368	42	46	56	rBV	132239	151207	15.59%	2.247%
3	1.648	88	92	101	rVB	114984	159699	16.47%	2.373%
4	2.294	192	198	208	rVB	206981	321801	33.19%	4.782%
5	2.496	228	231	234	rBV2	940	1430	0.15%	0.021%
6	2.654	255	257	259	rBV3	851	610	0.06%	0.009%
7	2.776	275	277	283	rBV4	1298	2410	0.25%	0.036%
8	2.947	296	305	314	rBV	12819	30626	3.16%	0.455%
9	3.392	376	378	380	rVV3	575	575	0.06%	0.009%
10	3.441	381	386	391	rVV4	1540	3148	0.32%	0.047%
11	3.514	395	398	400	rBV3	564	637	0.07%	0.009%
12	3.788	440	443	447	rVB3	499	667	0.07%	0.010%
13	3.916	461	464	467	rBV3	409	464	0.05%	0.007%
14	4.001	476	478	480	rBV2	506	475	0.05%	0.007%
15	4.044	482	485	488	rBV	583	951	0.10%	0.014%
16	4.245	514	518	522	rVV3	769	925	0.10%	0.014%
17	4.312	527	529	531	rBV3	634	561	0.06%	0.008%
18	4.465	546	554	571	rBV	58663	182509	18.82%	2.712%
19	4.843	614	616	620	rVB3	649	693	0.07%	0.010%
20	4.873	620	621	623	rBV2	663	469	0.05%	0.007%
21	4.916	627	628	630	rBV	771	502	0.05%	0.007%
22	4.959	633	635	637	rVB2	708	597	0.06%	0.009%
23	5.050	637	650	666	rBV	126371	394134	40.65%	5.857%
24	5.245	680	682	683	rVB2	899	538	0.06%	0.008%
25	5.276	685	687	690	rVB3	611	487	0.05%	0.007%
26	5.306	690	692	695	rBV3	521	643	0.07%	0.010%
27	5.361	697	701	702	rBV2	673	917	0.09%	0.014%
28	5.654	746	749	752	rBV4	765	1265	0.13%	0.019%
29	5.800	772	773	775	rBV2	706	484	0.05%	0.007%
30	5.855	779	782	783	rVB2	911	743	0.08%	0.011%
31	5.964	789	800	820	rBV2	324025	969663	100.00%	14.411%
32	6.184	834	836	837	rBV	669	474	0.05%	0.007%
33	6.757	922	930	947	rBV	214514	518917	53.52%	7.712%
34	7.123	986	990	998	rVB8	2994	6830	0.70%	0.102%
35	7.306	1012	1020	1034	rBV	194387	432692	44.62%	6.430%
36	7.617	1069	1071	1074	rVB3	555	573	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
 Data File : VX044424.D
 Acq On : 19 Dec 2024 10:26
 Operator : JC/MD
 Sample : P5235-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

37	7.659	1074	1078	1080	rBB2	634	624	0.06%	0.009%
38	7.720	1086	1088	1090	rVB2	746	590	0.06%	0.009%
39	7.824	1103	1105	1107	rVB2	913	865	0.09%	0.013%
40	7.842	1107	1108	1111	rBV2	404	525	0.05%	0.008%
41	7.964	1126	1128	1130	rBV2	494	546	0.06%	0.008%
42	8.135	1154	1156	1158	rBV2	782	601	0.06%	0.009%
43	8.324	1182	1187	1199	rBV	115864	194032	20.01%	2.884%
44	8.495	1213	1215	1218	rBV2	579	466	0.05%	0.007%
45	8.562	1224	1226	1227	rVB	844	559	0.06%	0.008%
46	8.586	1227	1230	1233	rBV4	1495	2375	0.24%	0.035%
47	8.647	1234	1240	1249	rBV	465504	716589	73.90%	10.649%
48	8.952	1285	1290	1301	rBV	80594	127384	13.14%	1.893%
49	9.055	1306	1307	1309	rBV	709	655	0.07%	0.010%
50	9.159	1322	1324	1329	rVB3	1057	1618	0.17%	0.024%
51	9.269	1340	1342	1348	rVB3	1594	2462	0.25%	0.037%
52	9.311	1348	1349	1354	rBV3	594	811	0.08%	0.012%
53	9.385	1356	1361	1372	rBV	245619	377157	38.90%	5.605%
54	9.696	1410	1412	1416	rBV4	1823	2342	0.24%	0.035%
55	10.049	1465	1470	1482	rBV	420053	607515	62.65%	9.028%
56	10.208	1492	1496	1499	rVB4	1087	1462	0.15%	0.022%
57	10.293	1508	1510	1511	rBV2	784	696	0.07%	0.010%
58	10.415	1528	1530	1534	rVB3	534	592	0.06%	0.009%
59	10.451	1534	1536	1538	rVB	727	491	0.05%	0.007%
60	10.793	1589	1592	1593	rBV2	915	726	0.07%	0.011%
61	10.964	1616	1620	1623	rBV4	1271	1804	0.19%	0.027%
62	11.189	1651	1657	1668	rBV	335829	430223	44.37%	6.394%
63	11.390	1688	1690	1692	rVB	843	657	0.07%	0.010%
64	11.451	1696	1700	1704	rBV5	1448	2590	0.27%	0.038%
65	11.652	1731	1733	1737	rVB3	818	911	0.09%	0.014%
66	11.707	1737	1742	1744	rBV3	1054	1645	0.17%	0.024%
67	11.756	1746	1750	1753	rVB4	1018	1282	0.13%	0.019%
68	11.805	1756	1758	1759	rVB	958	505	0.05%	0.008%
69	11.829	1759	1762	1763	rBV2	568	616	0.06%	0.009%
70	11.976	1782	1786	1788	rVV3	1465	2099	0.22%	0.031%
71	12.018	1788	1793	1806	rVV	377897	486069	50.13%	7.224%
72	12.128	1809	1811	1812	rVB2	1142	689	0.07%	0.010%
73	12.317	1837	1842	1853	rVV	429193	541561	55.85%	8.048%
74	12.847	1926	1929	1931	rVB2	912	793	0.08%	0.012%
75	12.872	1931	1933	1936	rBV2	575	690	0.07%	0.010%
76	12.945	1941	1945	1948	rVB3	1074	1600	0.17%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
 Data File : VX044424.D
 Acq On : 19 Dec 2024 10:26
 Operator : JC/MD
 Sample : P5235-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	12.969	1948	1949	1951	rBV	673	597	0.06%	0.009%
78	13.042	1958	1961	1964	rBV2	846	663	0.07%	0.010%
79	13.195	1983	1986	1987	rVV2	647	659	0.07%	0.010%
80	13.262	1994	1997	1999	rBV2	564	560	0.06%	0.008%
81	13.372	2009	2015	2016	rBV4	545	732	0.08%	0.011%
82	13.786	2078	2083	2084	rBV3	1725	1410	0.15%	0.021%
83	13.884	2096	2099	2103	rVB3	534	650	0.07%	0.010%
84	13.920	2103	2105	2106	rBV	671	509	0.05%	0.008%
85	14.036	2123	2124	2128	rVB2	547	465	0.05%	0.007%
86	14.128	2135	2139	2142	rBV2	2154	2969	0.31%	0.044%
87	14.195	2147	2150	2154	rBV3	694	773	0.08%	0.011%
88	14.280	2162	2164	2167	rVB2	717	744	0.08%	0.011%
89	14.365	2176	2178	2181	rBV4	495	637	0.07%	0.009%
90	14.396	2181	2183	2185	rVB2	654	490	0.05%	0.007%
91	14.573	2211	2212	2215	rVB2	835	552	0.06%	0.008%
92	14.609	2215	2218	2220	rBV2	771	849	0.09%	0.013%
93	14.676	2226	2229	2230	rVB2	589	504	0.05%	0.007%
94	14.695	2230	2232	2233	rBV2	634	459	0.05%	0.007%
95	14.859	2257	2259	2262	rBV3	707	669	0.07%	0.010%
96	15.182	2309	2312	2313	rBV2	720	609	0.06%	0.009%
97	15.377	2342	2344	2346	rBV2	725	722	0.07%	0.011%
98	15.566	2373	2375	2378	rBV3	639	717	0.07%	0.011%
99	15.932	2433	2435	2437	rBV2	701	597	0.06%	0.009%
100	16.706	2561	2562	2566	rBV2	707	959	0.10%	0.014%


Sum of corrected areas: 6728861

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
Data File : VX044424.D
Acq On : 19 Dec 2024 10:26
Operator : JC/MD
Sample : P5235-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

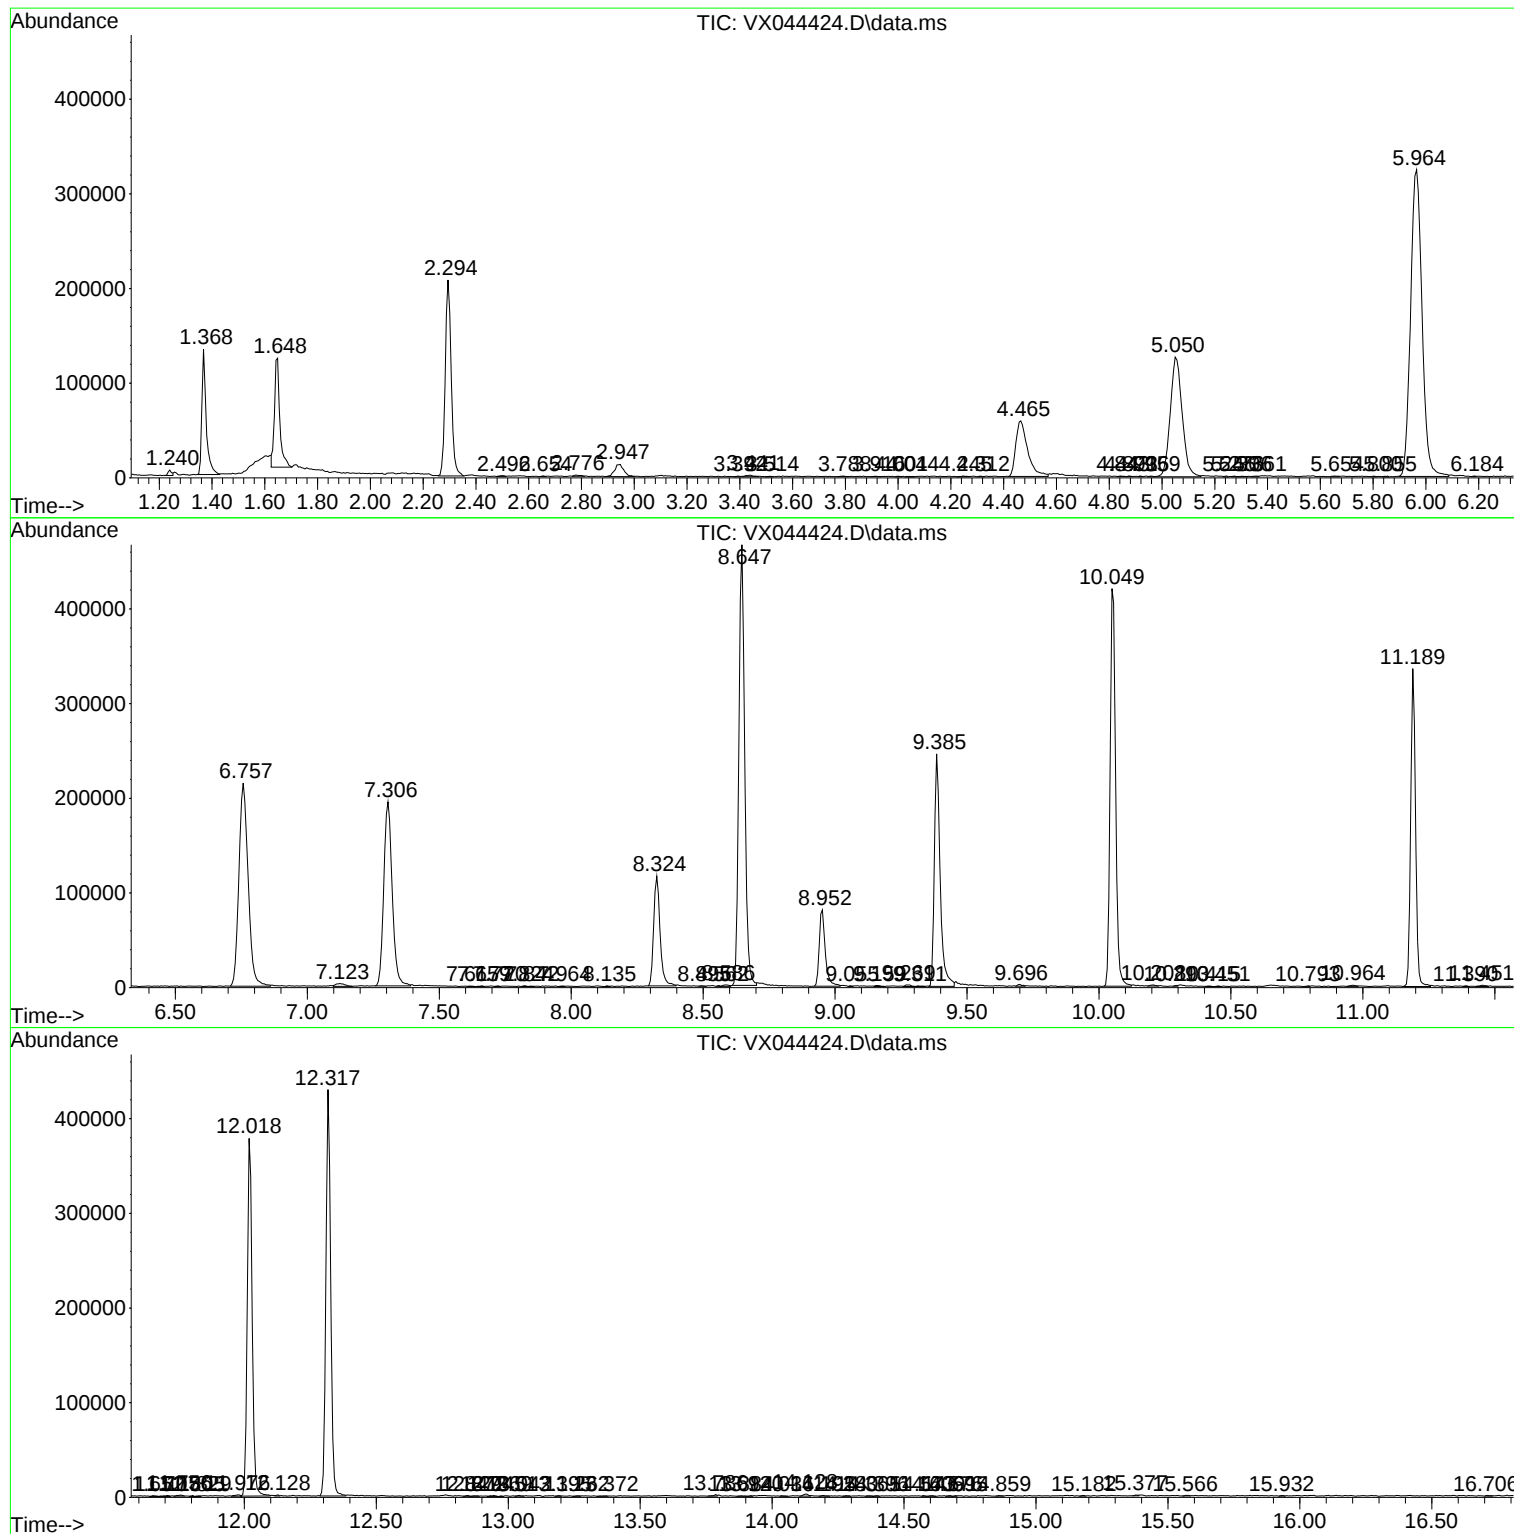

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
Data File : VX044424.D
Acq On : 19 Dec 2024 10:26
Operator : JC/MD
Sample : P5235-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
Data File : VX044424.D
Acq On : 19 Dec 2024 10:26
Operator : JC/MD
Sample : P5235-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc