

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
 Data File : VX044432.D
 Acq On : 19 Dec 2024 13:27
 Operator : JC/MD
 Sample : P5263-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M

Title : VOC Analysis

Signal : TIC: VX044432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	4483	5349	0.54%	0.077%
2	1.368	43	46	55	rVB	140443	158481	15.88%	2.285%
3	1.642	88	91	102	rVB	127589	174212	17.46%	2.511%
4	2.294	192	198	209	rVB	217748	339704	34.04%	4.897%
5	2.684	260	262	265	rBV2	512	631	0.06%	0.009%
6	2.770	274	276	278	rBV2	990	1048	0.11%	0.015%
7	3.001	311	314	315	rBV	605	591	0.06%	0.009%
8	3.184	342	344	346	rBV2	686	536	0.05%	0.008%
9	3.227	349	351	354	rVV2	557	508	0.05%	0.007%
10	3.367	373	374	378	rBV4	456	496	0.05%	0.007%
11	3.428	382	384	386	rBV3	808	665	0.07%	0.010%
12	3.635	415	418	421	rBV3	639	819	0.08%	0.012%
13	3.666	421	423	425	rVV3	565	576	0.06%	0.008%
14	3.684	425	426	428	rVV	591	484	0.05%	0.007%
15	3.727	432	433	438	rVV3	580	671	0.07%	0.010%
16	3.928	465	466	469	rBV	552	527	0.05%	0.008%
17	3.983	473	475	477	rBV2	746	559	0.06%	0.008%
18	4.093	491	493	495	rBV	557	556	0.06%	0.008%
19	4.178	503	507	508	rBV2	404	494	0.05%	0.007%
20	4.196	508	510	512	rVB2	597	456	0.05%	0.007%
21	4.458	545	553	571	rBV	56965	182385	18.28%	2.629%
22	4.739	597	599	601	rVB2	804	541	0.05%	0.008%
23	4.934	629	631	636	rVB3	513	739	0.07%	0.011%
24	5.056	638	651	665	rBV	127991	398424	39.93%	5.744%
25	5.190	670	673	677	rVV4	752	883	0.09%	0.013%
26	5.239	679	681	684	rBV3	563	605	0.06%	0.009%
27	5.452	714	716	718	rBV2	448	489	0.05%	0.007%
28	5.550	728	732	733	rBV3	516	644	0.06%	0.009%
29	5.629	742	745	747	rBV4	356	476	0.05%	0.007%
30	5.794	770	772	774	rVB	846	587	0.06%	0.008%
31	5.964	789	800	820	rBV2	330887	997925	100.00%	14.386%
32	6.196	837	838	844	rBV4	651	627	0.06%	0.009%
33	6.294	852	854	856	rBV2	585	712	0.07%	0.010%
34	6.391	868	870	872	rVB2	729	550	0.06%	0.008%
35	6.556	895	897	899	rBV	615	677	0.07%	0.010%
36	6.604	902	905	907	rBV3	450	666	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
 Data File : VX044432.D
 Acq On : 19 Dec 2024 13:27
 Operator : JC/MD
 Sample : P5263-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

37	6.757	921	930	947	rBV	227253	558396	55.96%	8.050%
38	7.117	984	989	995	rBV6	2268	6372	0.64%	0.092%
39	7.306	1011	1020	1033	rBV	198337	442439	44.34%	6.378%
40	7.635	1072	1074	1075	rBV2	551	528	0.05%	0.008%
41	7.915	1118	1120	1122	rBV2	612	507	0.05%	0.007%
42	7.940	1122	1124	1129	rVV2	466	658	0.07%	0.009%
43	7.982	1129	1131	1133	rVB2	544	455	0.05%	0.007%
44	8.153	1157	1159	1162	rVV2	590	628	0.06%	0.009%
45	8.324	1181	1187	1198	rBV	112694	190645	19.10%	2.748%
46	8.561	1224	1226	1230	rVB3	616	863	0.09%	0.012%
47	8.647	1233	1240	1251	rBV	480633	759143	76.07%	10.944%
48	8.781	1260	1262	1267	rVB4	1211	1057	0.11%	0.015%
49	8.952	1285	1290	1300	rBV	77453	119280	11.95%	1.720%
50	9.336	1350	1353	1356	rBV4	617	773	0.08%	0.011%
51	9.384	1356	1361	1375	rBV	247371	381693	38.25%	5.503%
52	9.738	1417	1419	1423	rBV4	721	990	0.10%	0.014%
53	9.878	1440	1442	1445	rVB2	770	608	0.06%	0.009%
54	10.049	1465	1470	1483	rVV	447715	639259	64.06%	9.216%
55	10.201	1494	1495	1499	rVB3	1399	1003	0.10%	0.014%
56	10.488	1538	1542	1544	rBV3	597	966	0.10%	0.014%
57	10.561	1551	1554	1555	rBV2	453	521	0.05%	0.008%
58	10.774	1587	1589	1590	rBV2	861	658	0.07%	0.009%
59	11.055	1632	1635	1636	rBV2	431	467	0.05%	0.007%
60	11.189	1652	1657	1668	rBV	342687	429998	43.09%	6.199%
61	11.421	1693	1695	1698	rBV2	563	665	0.07%	0.010%
62	11.622	1725	1728	1729	rBV3	652	675	0.07%	0.010%
63	11.713	1741	1743	1746	rBV3	356	456	0.05%	0.007%
64	11.774	1751	1753	1754	rVB2	754	496	0.05%	0.007%
65	11.969	1782	1785	1788	rBV2	628	852	0.09%	0.012%
66	12.018	1788	1793	1804	rBV	401984	525902	52.70%	7.581%
67	12.317	1837	1842	1851	rVV	444577	569709	57.09%	8.213%
68	12.573	1880	1884	1885	rBV3	818	1016	0.10%	0.015%
69	12.585	1885	1886	1891	rVV3	1084	975	0.10%	0.014%
70	12.725	1906	1909	1913	rBV5	566	1037	0.10%	0.015%
71	12.762	1913	1915	1917	rVB3	1545	1216	0.12%	0.018%
72	12.926	1940	1942	1944	rVV2	701	500	0.05%	0.007%
73	12.994	1950	1953	1957	rBV3	515	805	0.08%	0.012%
74	13.097	1968	1970	1975	rVB3	844	941	0.09%	0.014%
75	13.219	1987	1990	1991	rBV2	464	465	0.05%	0.007%
76	13.298	2000	2003	2008	rBV3	531	843	0.08%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
 Data File : VX044432.D
 Acq On : 19 Dec 2024 13:27
 Operator : JC/MD
 Sample : P5263-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.378	2012	2016	2017	rVV2	733	798	0.08%	0.012%
78	13.463	2028	2030	2032	rBV2	621	557	0.06%	0.008%
79	13.493	2032	2035	2038	rVV4	504	614	0.06%	0.009%
80	13.524	2038	2040	2043	rVB2	503	484	0.05%	0.007%
81	13.640	2056	2059	2060	rBV2	462	463	0.05%	0.007%
82	13.670	2062	2064	2067	rVB4	662	609	0.06%	0.009%
83	13.701	2067	2069	2071	rBV3	748	617	0.06%	0.009%
84	13.725	2071	2073	2076	rVB2	645	477	0.05%	0.007%
85	13.993	2115	2117	2119	rVB3	838	587	0.06%	0.008%
86	14.018	2119	2121	2122	rBV	733	576	0.06%	0.008%
87	14.134	2135	2140	2145	rVV4	1926	3613	0.36%	0.052%
88	14.445	2190	2191	2193	rBV	620	460	0.05%	0.007%
89	14.755	2240	2242	2245	rVB2	721	551	0.06%	0.008%
90	14.975	2276	2278	2279	rBV2	725	638	0.06%	0.009%
91	15.011	2282	2284	2287	rVV3	902	698	0.07%	0.010%
92	15.079	2293	2295	2297	rVV3	750	749	0.08%	0.011%
93	15.572	2374	2376	2377	rVB	908	482	0.05%	0.007%
94	15.639	2384	2387	2388	rBV2	596	686	0.07%	0.010%
95	15.920	2431	2433	2435	rVB2	600	481	0.05%	0.007%
96	15.938	2435	2436	2441	rBV4	820	1000	0.10%	0.014%
97	16.072	2455	2458	2461	rBV3	721	732	0.07%	0.011%
98	16.261	2487	2489	2493	rVV3	997	988	0.10%	0.014%
99	16.481	2523	2525	2526	rVB	893	548	0.05%	0.008%
100	16.761	2570	2571	2573	rBV	634	523	0.05%	0.008%




Sum of corrected areas: 6936684

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
Data File : VX044432.D
Acq On : 19 Dec 2024 13:27
Operator : JC/MD
Sample : P5263-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

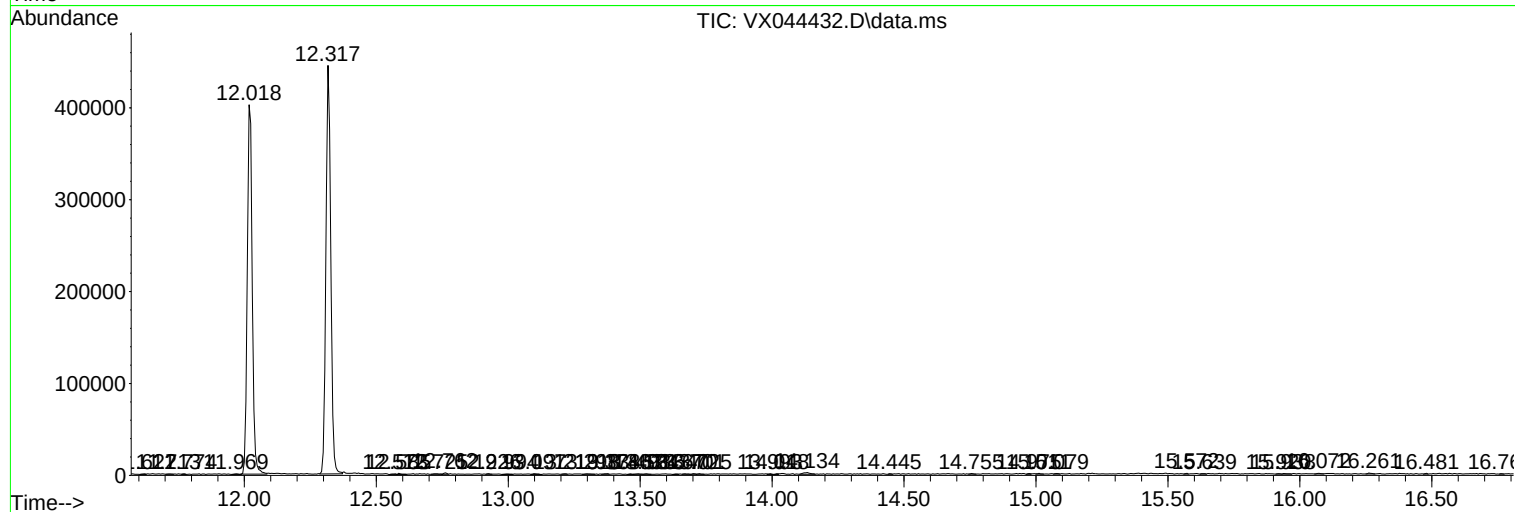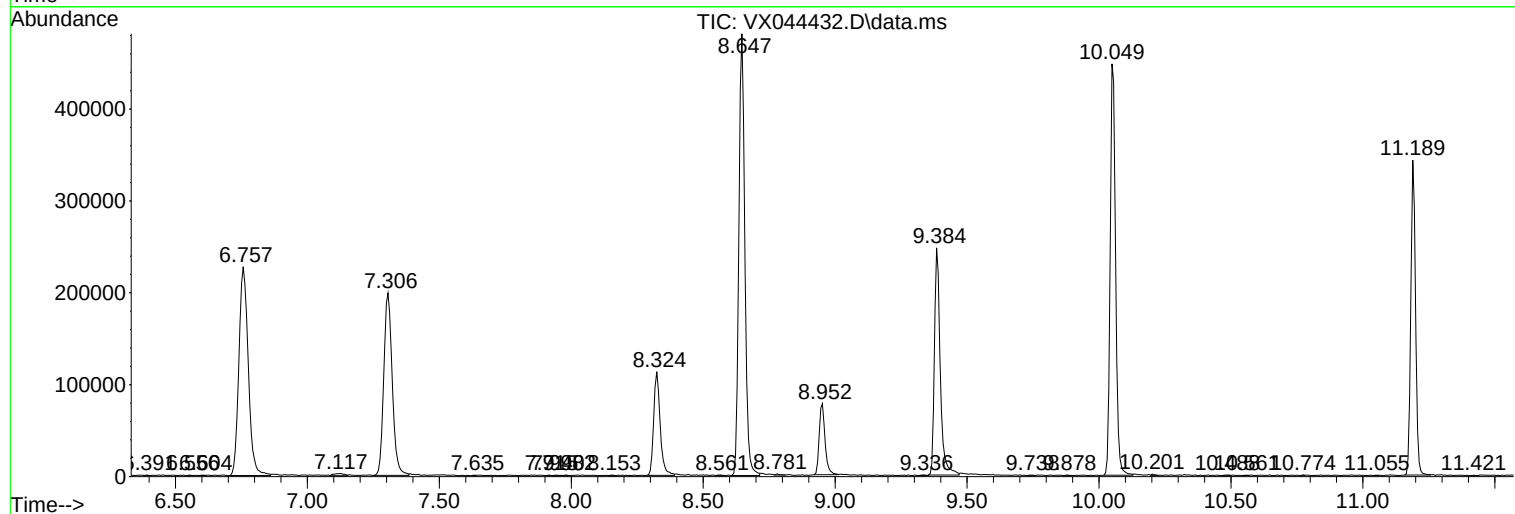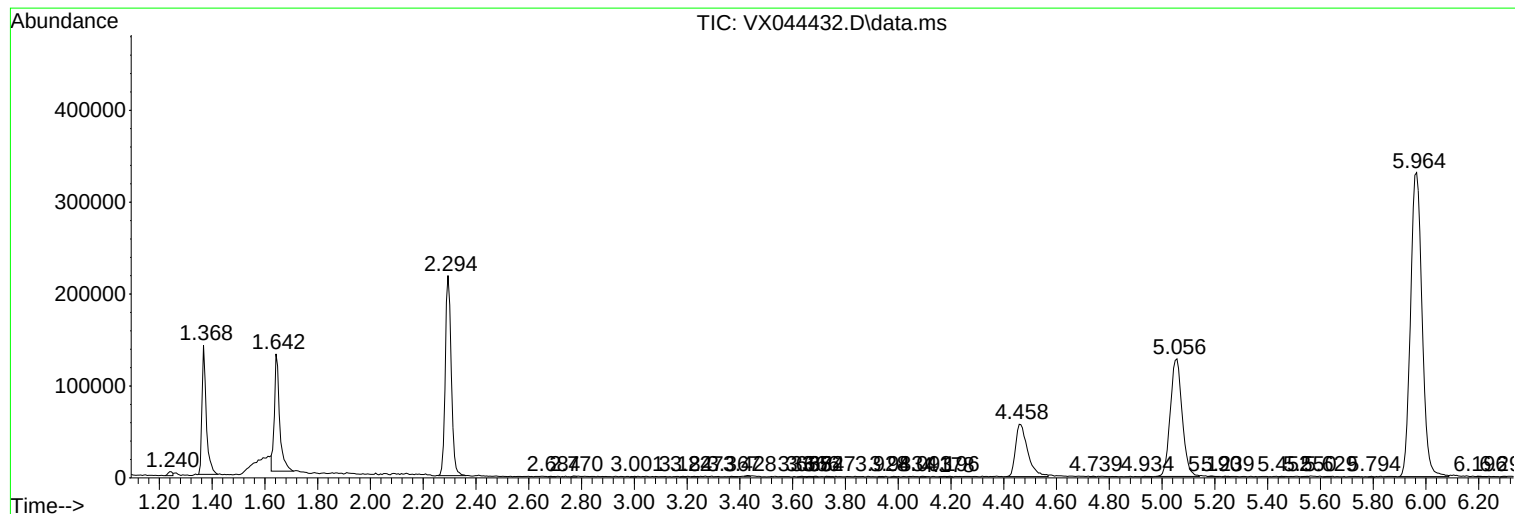

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
Data File : VX044432.D
Acq On : 19 Dec 2024 13:27
Operator : JC/MD
Sample : P5263-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
Data File : VX044432.D
Acq On : 19 Dec 2024 13:27
Operator : JC/MD
Sample : P5263-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------